

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081823\
 Data File : VX037086.D
 Acq On : 18 Aug 2023 15:55
 Operator : JC/MD
 Sample : 04024-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP05-20230815

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Title : SW846 8260

Signal : TIC: VX037086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.325	196	203	211	rBV2	64659	127577	4.71%	1.592%
2	5.385	693	705	721	rBV	90081	263245	9.72%	3.285%
3	5.556	721	733	746	rVV	145635	415096	15.33%	5.180%
4	5.958	787	799	815	rBV	91839	244684	9.04%	3.053%
5	6.763	921	931	947	rBV	238294	572192	21.13%	7.140%
6	7.129	980	991	1008	rBV	1224191	2707819	100.00%	33.788%
7	8.647	1234	1240	1259	rBV	497933	786966	29.06%	9.820%
8	10.055	1465	1471	1486	rBV	546790	736353	27.19%	9.188%
9	11.079	1634	1639	1652	rBV	462675	597346	22.06%	7.454%
10	12.024	1788	1794	1802	rBV	566469	728506	26.90%	9.090%
11	12.823	1906	1925	1945	rBV	28735	172441	6.37%	2.152%
12	13.774	2075	2081	2090	rBV	54111	73486	2.71%	0.917%
13	14.633	2210	2222	2233	rBV	61500	86155	3.18%	1.075%
14	14.780	2241	2246	2256	rVB	57650	75119	2.77%	0.937%
15	15.371	2336	2343	2354	rVB	37165	61307	2.26%	0.765%
16	15.475	2354	2360	2370	rBV	39556	64249	2.37%	0.802%
17	15.615	2377	2383	2386	rBV	50640	81758	3.02%	1.020%
18	15.645	2386	2388	2395	rVB	27223	39182	1.45%	0.489%
19	15.834	2408	2419	2430	rBV2	16280	48086	1.78%	0.600%
20	16.328	2489	2500	2508	rBV2	48856	102435	3.78%	1.278%
21	16.657	2549	2554	2568	rVB4	11810	30140	1.11%	0.376%




Sum of corrected areas: 8014142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081823\
Data File : VX037086.D
Acq On : 18 Aug 2023 15:55
Operator : JC/MD
Sample : 04024-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20230815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

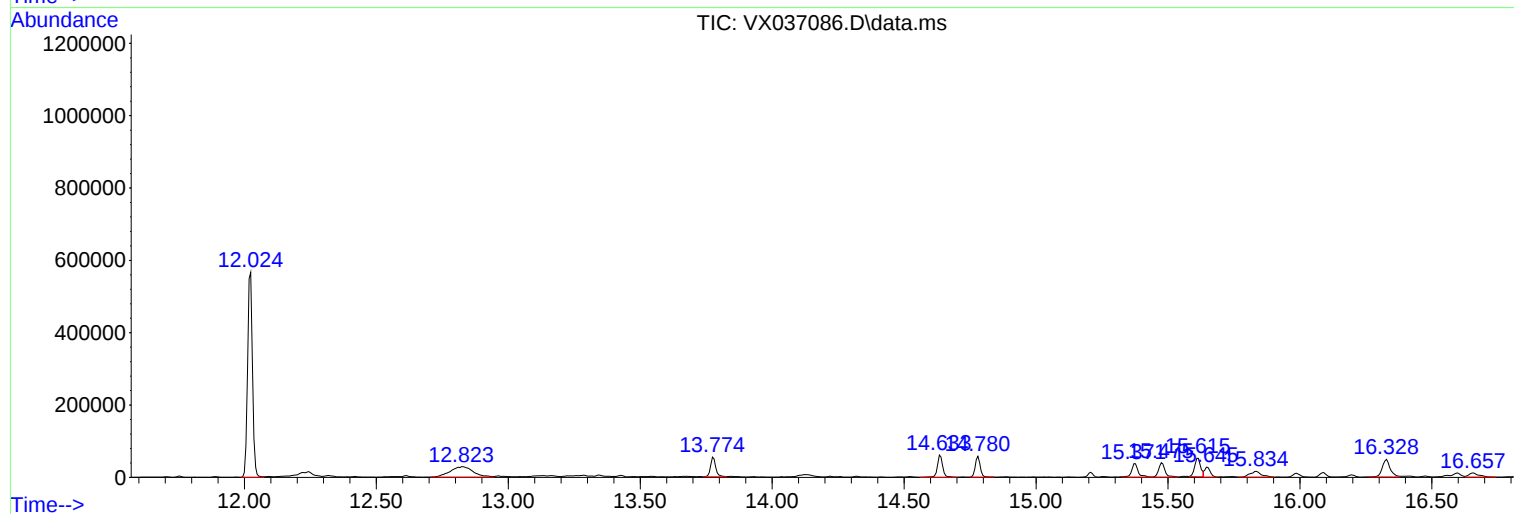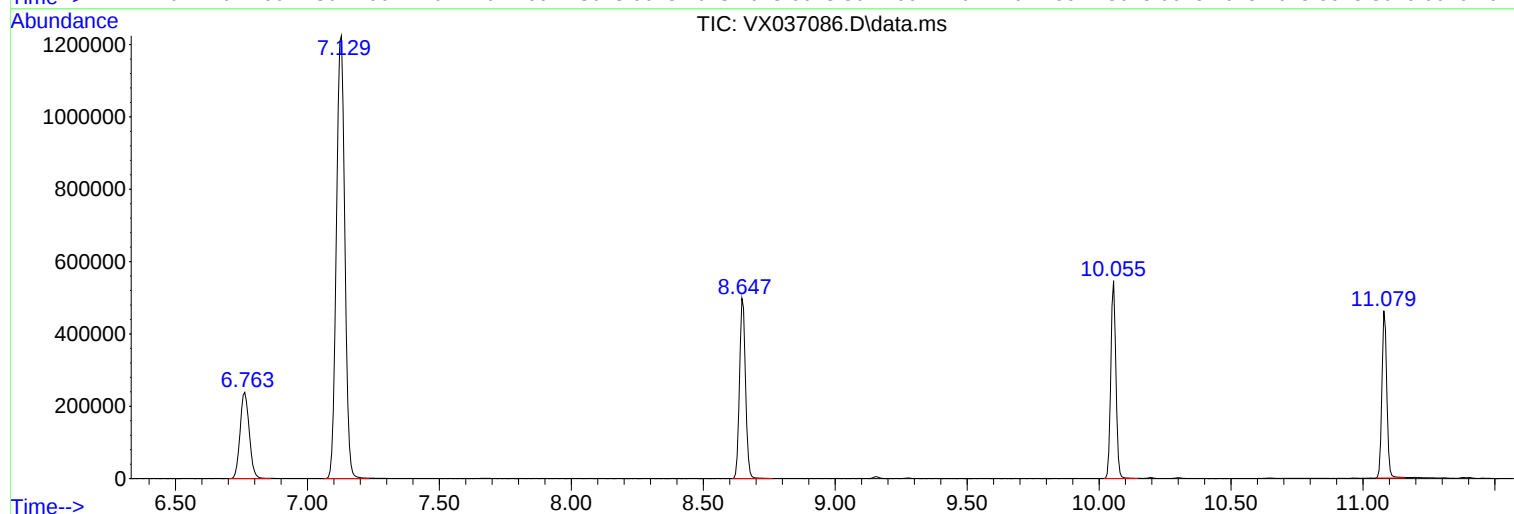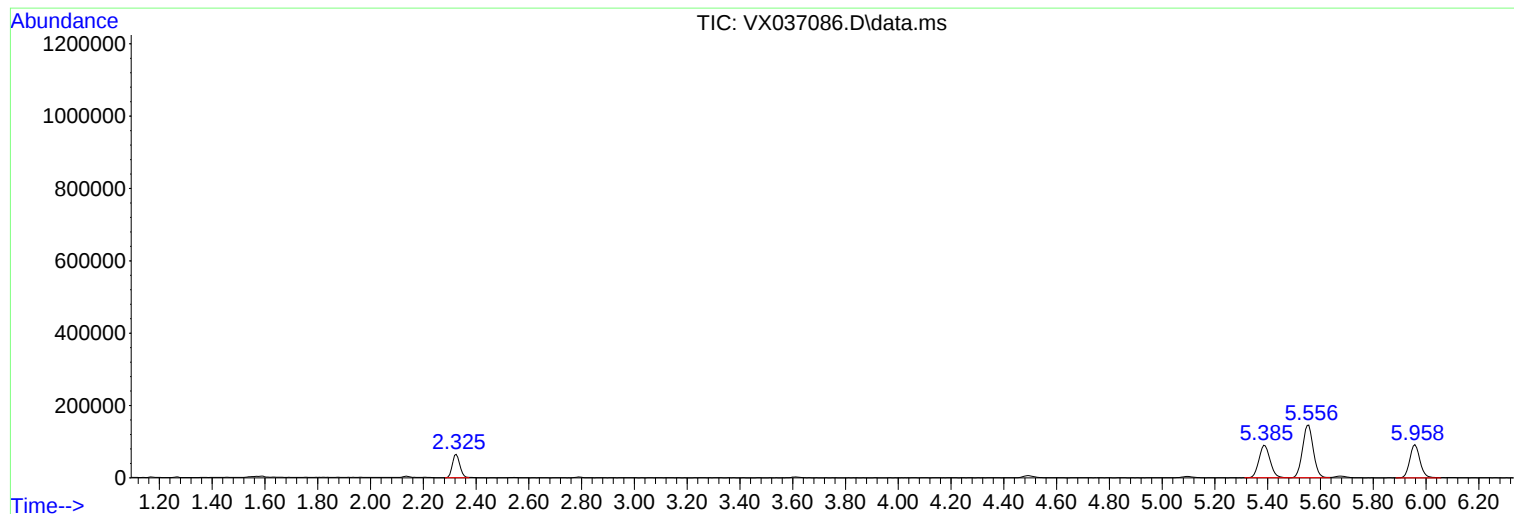

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081823\
Data File : VX037086.D
Acq On : 18 Aug 2023 15:55
Operator : JC/MD
Sample : 04024-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20230815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081823\
Data File : VX037086.D
Acq On : 18 Aug 2023 15:55
Operator : JC/MD
Sample : 04024-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP05-20230815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------