
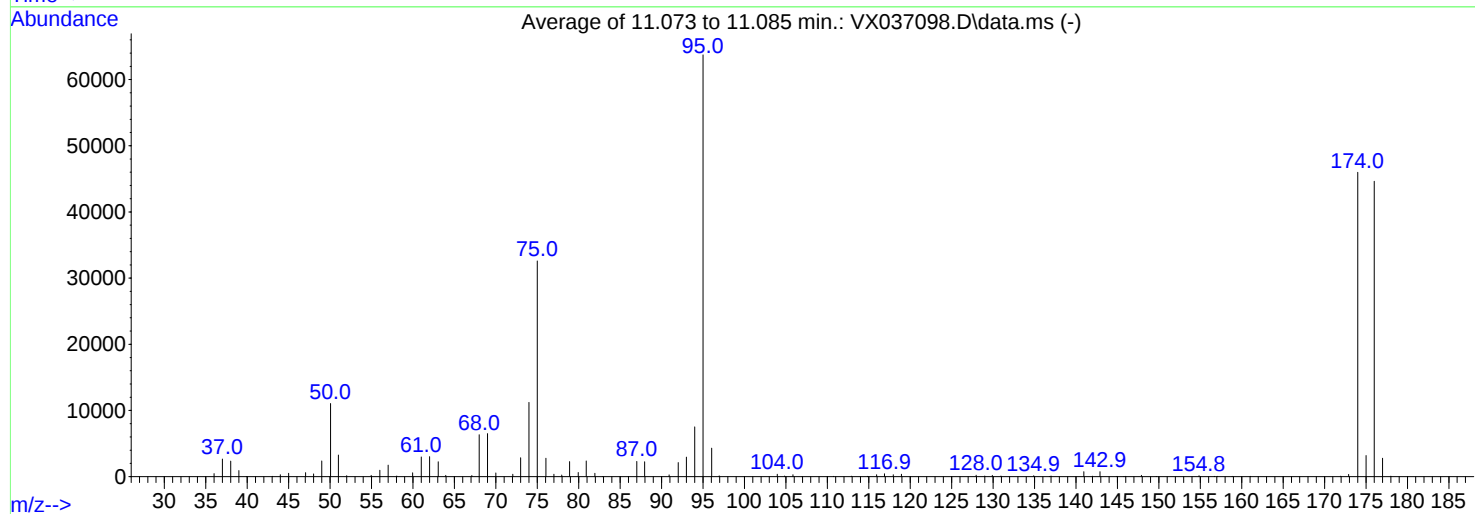


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081823\
Data File : VX037098.D
Acq On : 18 Aug 2023 23:55
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Title : SW846 8260
Last Update : Fri Aug 18 09:30:38 2023

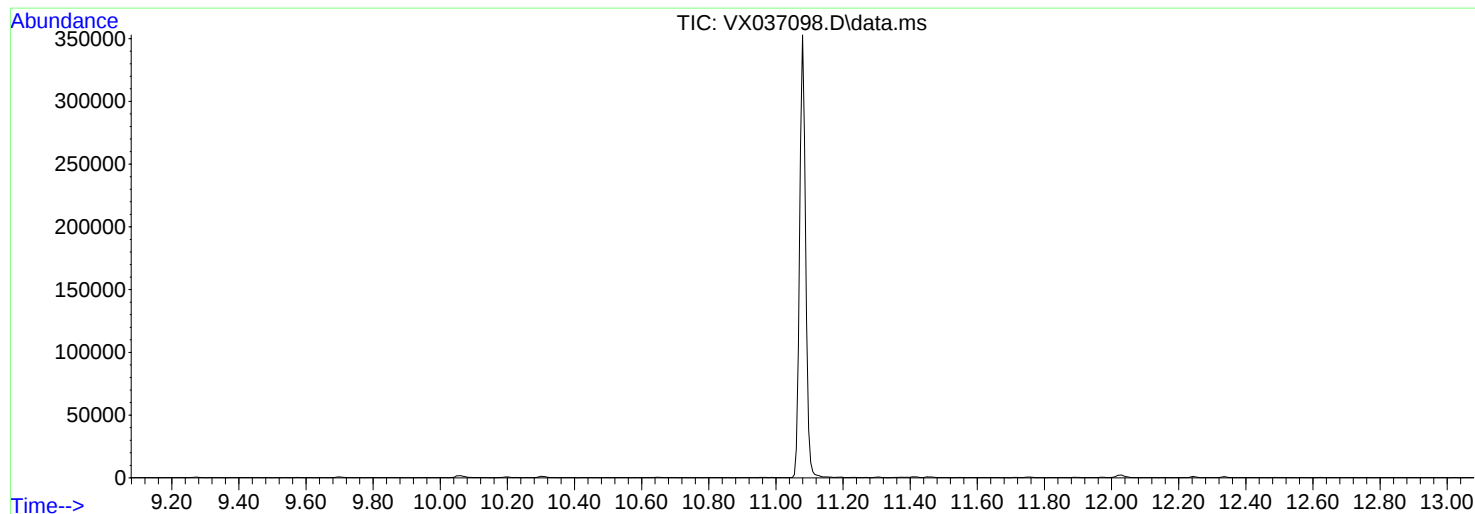

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	11057	PASS
75	95	30	60	51.2	32603	PASS
95	95	100	100	100.0	63739	PASS
96	95	5	9	6.8	4308	PASS
173	174	0.00	2	0.7	331	PASS
174	95	50	100	72.1	45984	PASS
175	174	5	9	6.9	3190	PASS
176	174	95	101	97.1	44629	PASS
177	176	5	9	6.3	2793	PASS