

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX081919\
 Data File : VX011628.D
 Acq On : 19 Aug 2019 13:45
 Operator : JC/SP
 Sample : K4351-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PH2-0135

Quant Time: Aug 20 09:38:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 04:15:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	429340	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	594959	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	520787	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	258989	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	207149	52.03	ug/l	0.00
Spiked Amount						
			Recovery	=	104.06%	
35) Dibromofluoromethane	5.49	113	175648	45.14	ug/l	0.00
Spiked Amount						
			Recovery	=	90.28%	
50) Toluene-d8	8.71	98	676599	55.80	ug/l	0.00
Spiked Amount						
			Recovery	=	111.60%	
62) 4-Bromofluorobenzene	11.13	95	235401	46.00	ug/l	0.00
Spiked Amount						
			Recovery	=	92.00%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	3.01	59	2124	2.174	ug/l #	94
13) Acrolein	2.30	56	483	13.713	ug/l #	75
16) Acetone	2.43	43	2299	1.148	ug/l #	74
31) Cyclohexane	5.57	56	2327	0.394	ug/l #	94
36) 1,1-Dichloropropene	5.66	75	24211	4.760	ug/l #	51
38) Carbon Tetrachloride	5.65	117	36543	6.521	ug/l #	17
39) Methylcyclohexane	7.46	83	4803	0.765	ug/l	92
49) 1,4-Dioxane	7.74	88	147	1.222	ug/l #	1
52) Toluene	8.79	92	2263	0.225	ug/l	77
59) 2-Hexanone	9.44	43	1319	0.286	ug/l	89
67) Ethyl Benzene	10.25	91	17443	0.941	ug/l	95
68) m/p-Xylenes	10.35	106	26045	3.660	ug/l	95
69) o-Xylene	10.69	106	2635	0.378	ug/l	88
71) Bromoform	10.66	173	129	3.321	ug/l #	28
76) 1,2,3-Trichloropropane	11.13	75	108239	22.040	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.13	75	108239	58.834	ug/l #	11
84) 1,2,4-Trimethylbenzene	11.80	105	6277	0.443	ug/l	97
95) Naphthalene	13.83	128	3668	0.202	ug/l #	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX081919\
Data File : VX011628.D
Acq On : 19 Aug 2019 13:45
Operator : JC/SP
Sample : K4351-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PH2-0135

Quant Time: Aug 20 09:38:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 04:15:26 2019
Response via : Initial Calibration

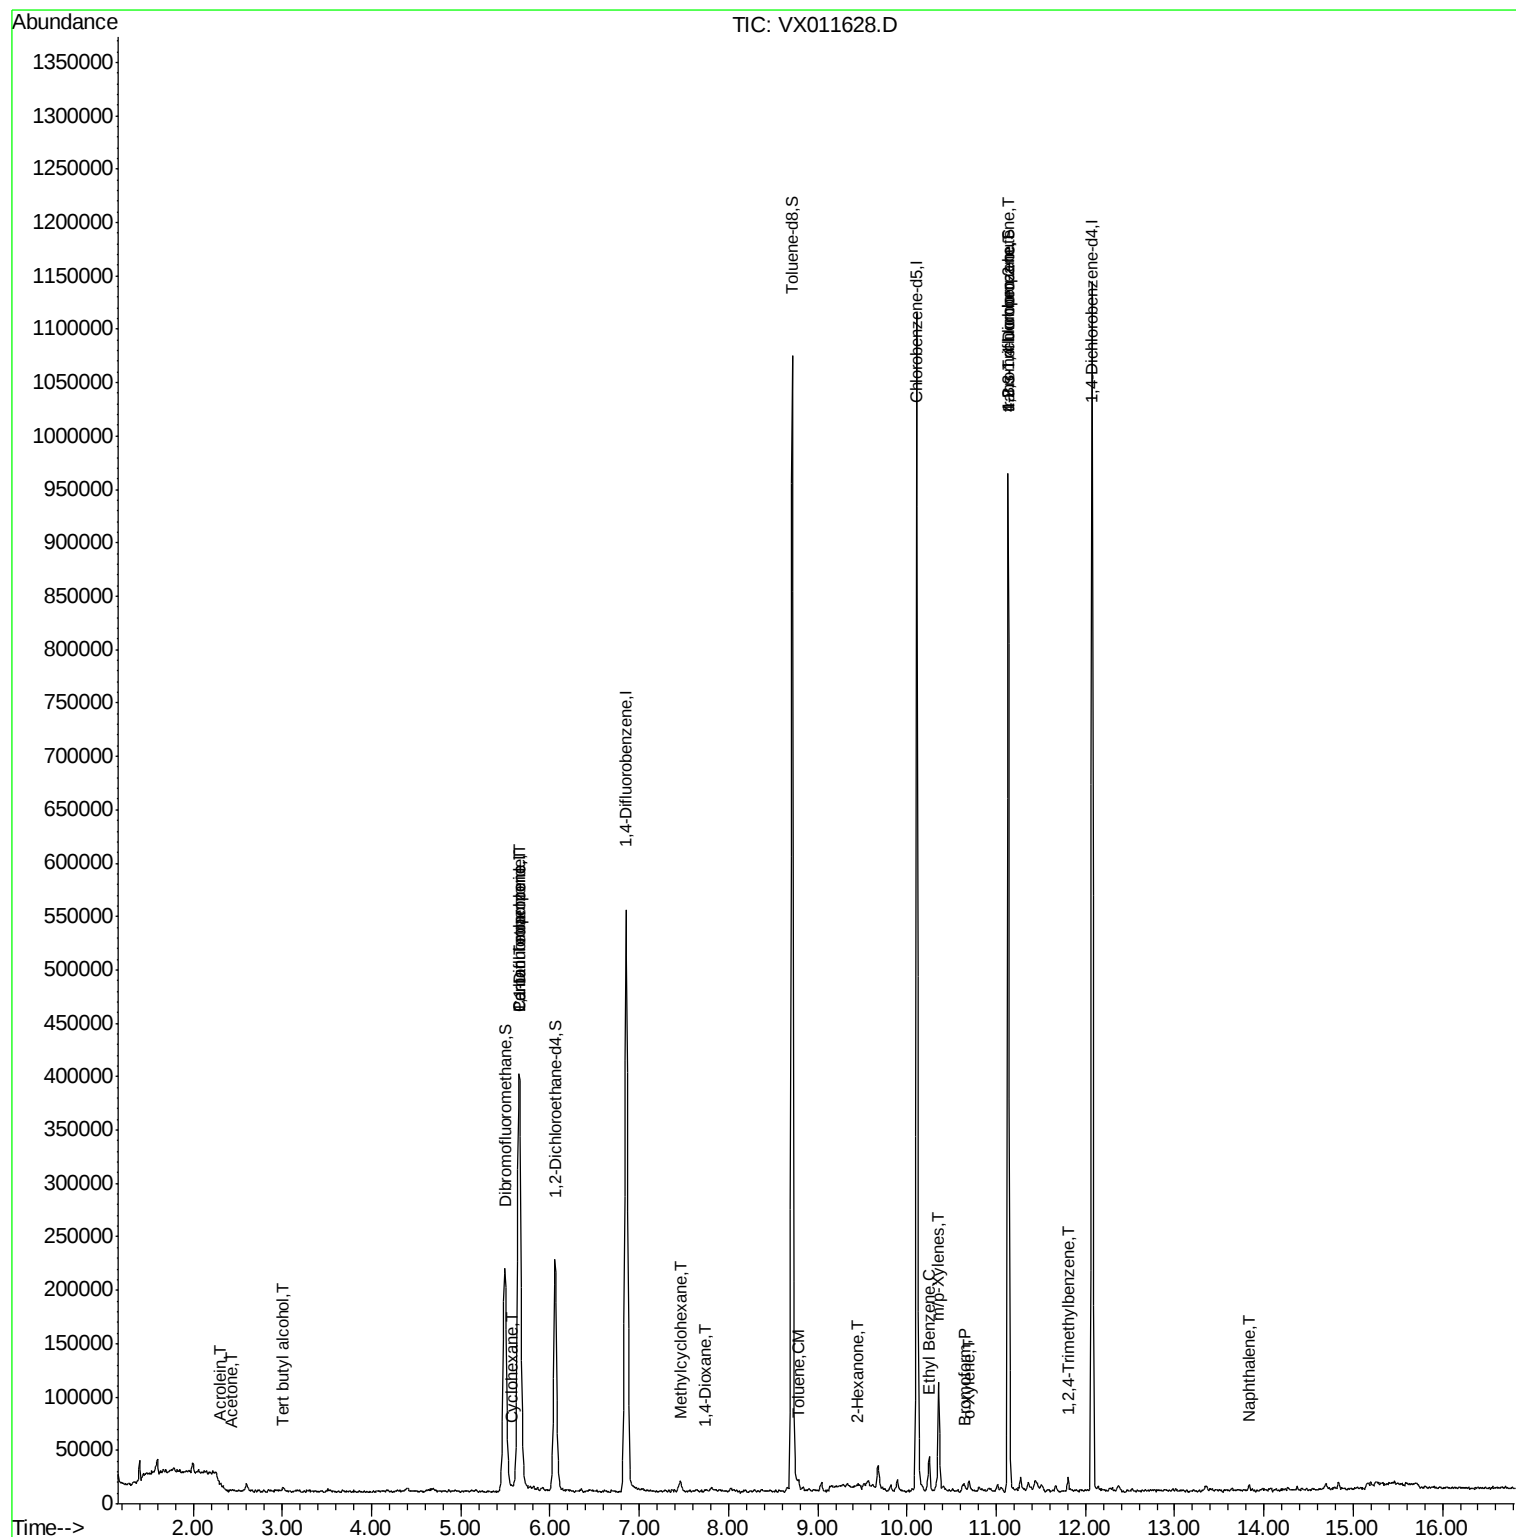



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. 0.01 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45

Instrument :

MSVOA_X

ClientSampleId :


PH2-0135

Tgt Ion:168 Resp: 429340

Ion Ratio Lower Upper

168 100

99 46.4 37.3 55.9



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0


150000

100000


50000

0

5.50 5.60 5.70 5.80



Time-->



#11

Tert butyl alcohol

Concen: 2.174 ug/l

RT: 3.01 min Scan# 304

Delta R.T. -0.03 min

Lab File: VX011628.D


Acq: 19 Aug 2019 13:45

Tgt Ion: 59 Resp: 2124

Ion Ratio Lower Upper

59 100

57 13.3 8.7 13.1#



Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

1000

800


600

400


200

0

2.95 3.00 3.05 3.10



Time-->



#13

Acrolein

Concen: 13.713 ug/l

RT: 2.30 min Scan# 188

Delta R.T. 0.01 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45

Instrument :

MSVOA_X

ClientSampleId :





PH2-0135

Tgt Ion: 56 Resp: 483

Ion Ratio Lower Upper

56 100

55 48.9 55.5 83.3#

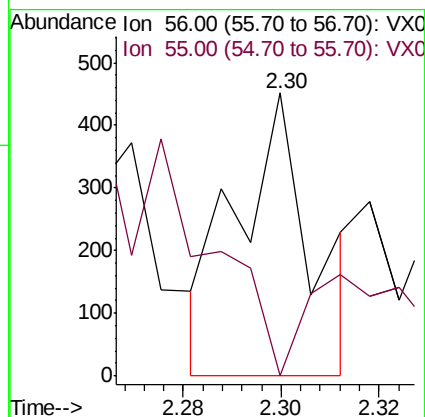

#16

Acetone

Concen: 1.148 ug/l

RT: 2.43 min Scan# 210

Delta R.T. 0.00 min

Lab File: VX011628.D




Acq: 19 Aug 2019 13:45


Tgt Ion: 43 Resp: 2299

Ion Ratio Lower Upper

43 100

58 17.3 25.2 37.8#

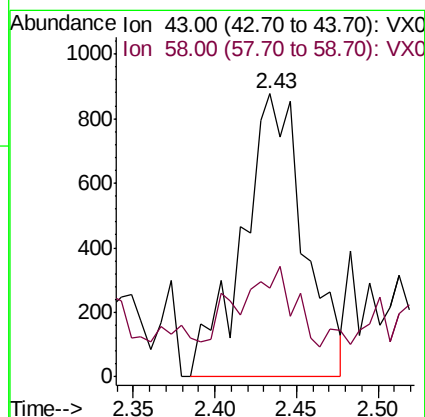

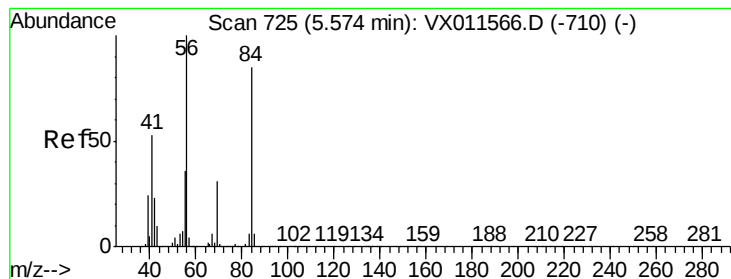

#31

Cyclohexane

Concen: 0.394 ug/l

RT: 5.57 min Scan# 725

Delta R.T. 0.00 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45

Instrument :

MSVOA_X

ClientSampleId :

PH2-0135





Tgt Ion: 56 Resp: 2327

Ion Ratio Lower Upper

56 100

69 22.7 24.8 37.2#

84 86.7 67.9 101.9

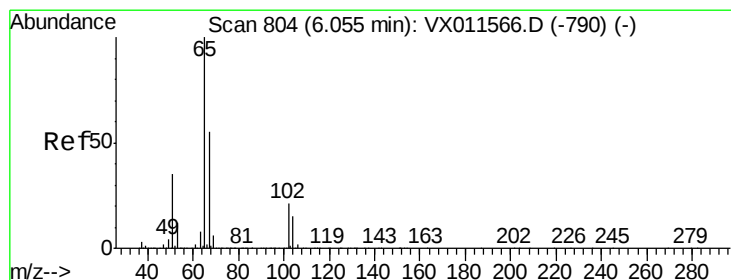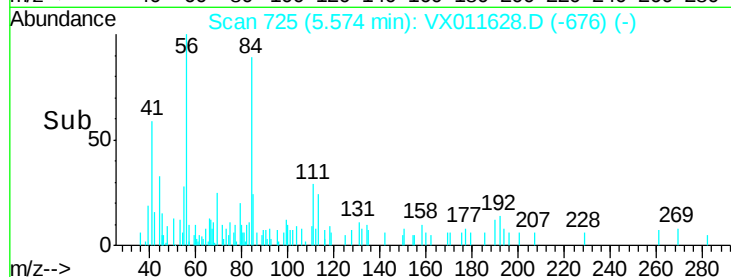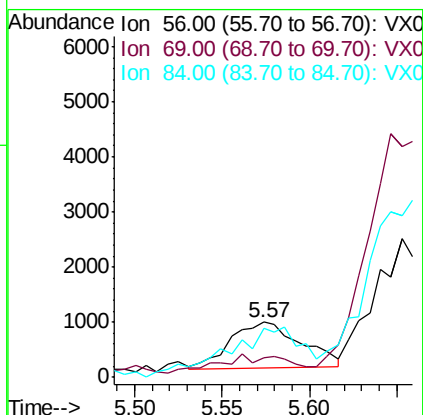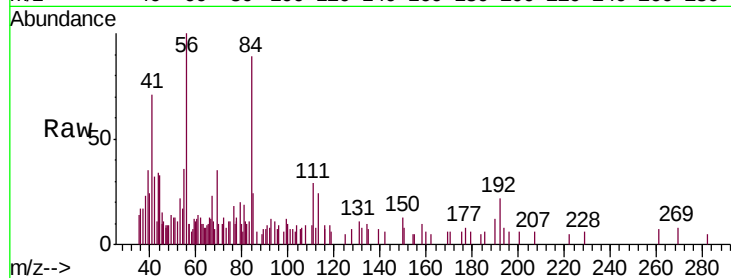

#33

1,2-Dichloroethane-d4

Concen: 52.027 ug/l

RT: 6.06 min Scan# 804

Delta R.T. 0.00 min

Lab File: VX011628.D




Acq: 19 Aug 2019 13:45


Tgt Ion: 65 Resp: 207149

Ion Ratio Lower Upper

65 100

67 52.8 0.0 107.6

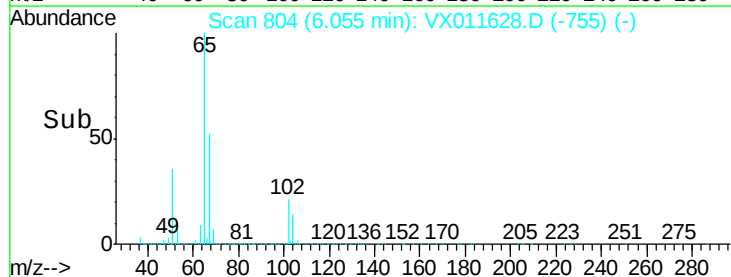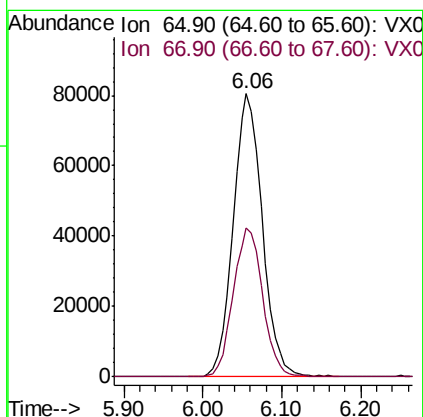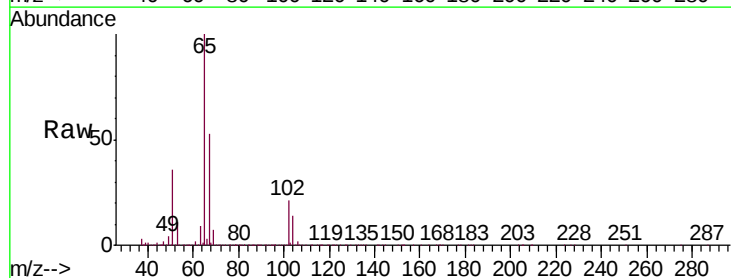

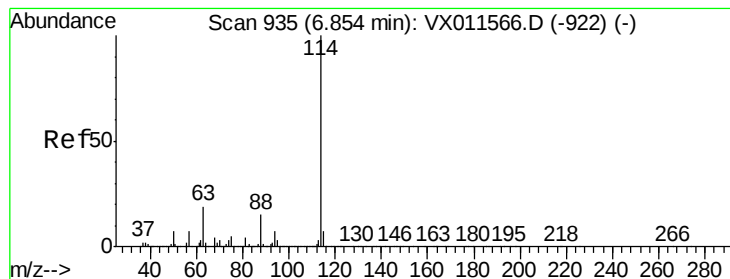

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 935

Delta R.T. 0.00 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45

Instrument :

MSVOA_X

ClientSampleId :

PH2-0135


Tgt Ion:114 Resp: 594959

Ion Ratio Lower Upper

114 100

63 18.4 0.0 37.8




88 15.0 0.0 30.2



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

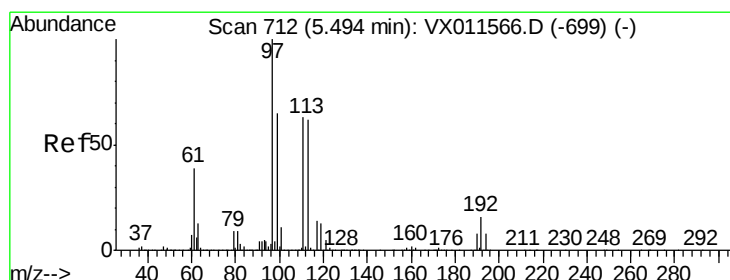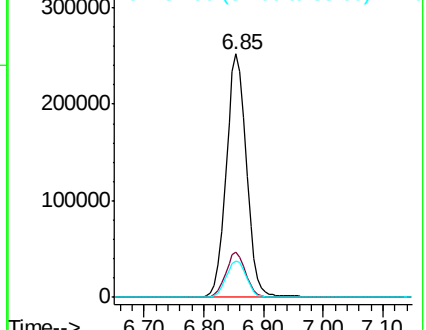

#35

Dibromofluoromethane

Concen: 45.137 ug/l

RT: 5.49 min Scan# 712

Delta R.T. 0.00 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45


Tgt Ion:113 Resp: 175648

Ion Ratio Lower Upper

113 100

111 102.2 81.1 121.7



192 25.9 20.8 31.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

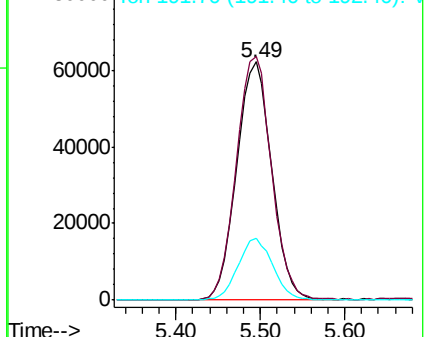

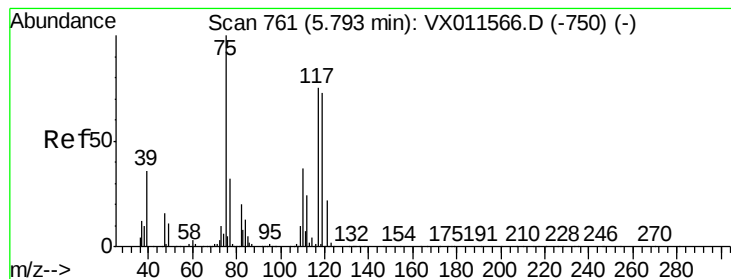

#36

1,1-Dichloropropene

Concen: 4.760 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.13 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45

Instrument :

MSVOA_X

ClientSampleId :

PH2-0135





Tgt Ion: 75 Resp: 24211

Ion Ratio Lower Upper

75 100

110 12.4 19.4 58.1#

77 0.7 25.1 37.7#

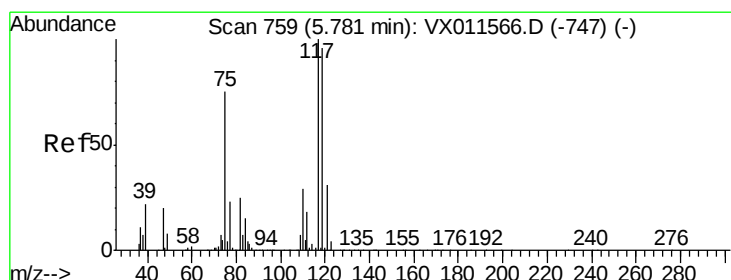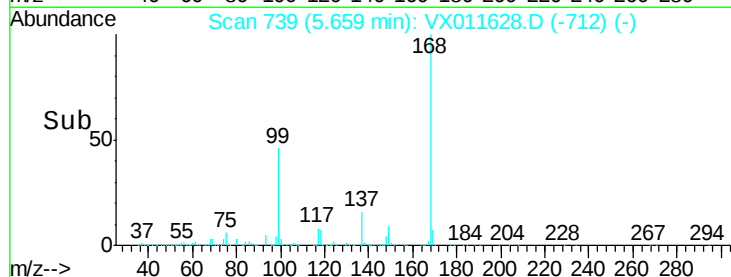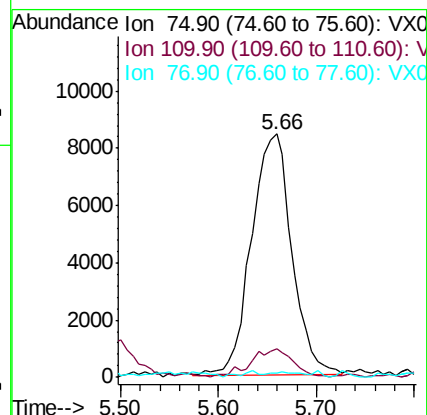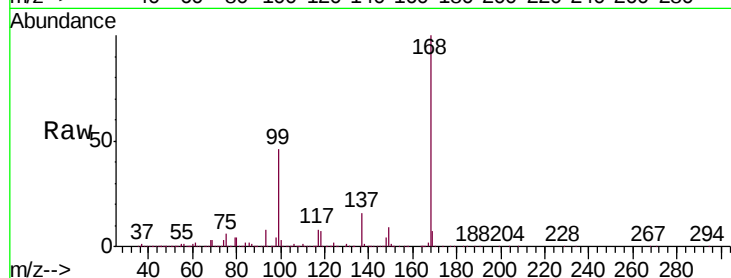

#38

Carbon Tetrachloride

Concen: 6.521 ug/l

RT: 5.65 min Scan# 738

Delta R.T. -0.13 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45




Tgt Ion: 117 Resp: 36543


Ion Ratio Lower Upper

117 100

119 6.3 76.9 115.3#

121 0.0 24.8 37.2#

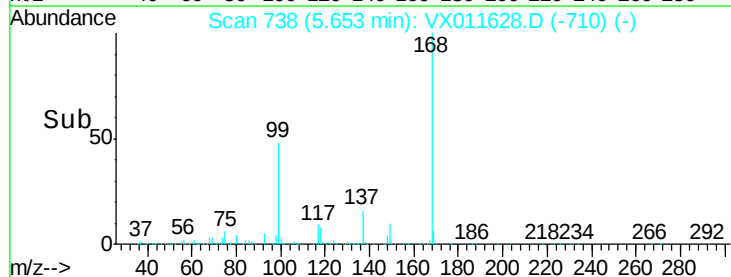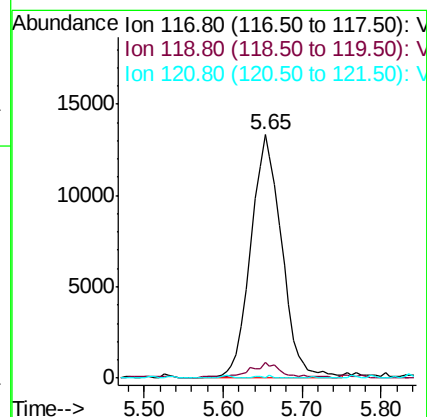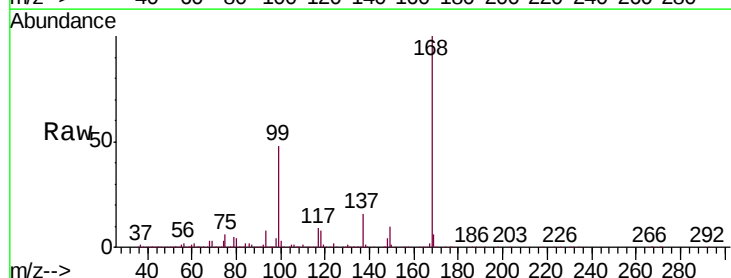

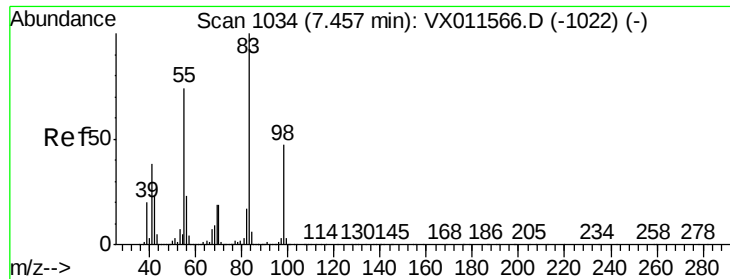

#39

Methylcyclohexane

Concen: 0.765 ug/l

RT: 7.46 min Scan# 1035

Delta R.T. 0.01 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45

Instrument :

MSVOA_X

ClientSampleId :

PH2-0135





Tgt Ion: 83 Resp: 4803

Ion Ratio Lower Upper

83 100

55 70.2 58.8 88.2

98 38.1 37.8 56.6

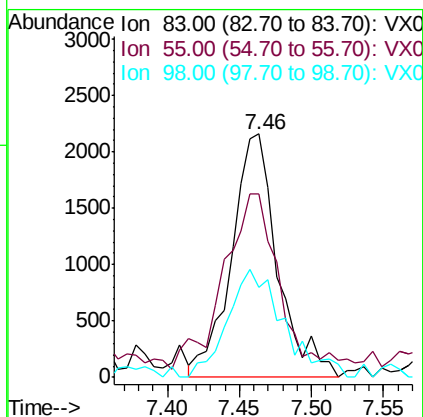

#49

1,4-Dioxane

Concen: 1.222 ug/l

RT: 7.74 min Scan# 1080

Delta R.T. 0.00 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45




Tgt Ion: 88 Resp: 147


Ion Ratio Lower Upper

88 100

43 76.2 23.4 35.0#

58 159.9 54.3 81.5#



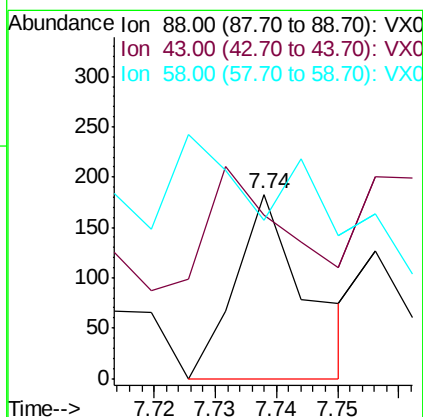





#50
Toluene-d8
Concen: 55.801 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. 0.00 min
Lab File: VX011628.D
Acq: 19 Aug 2019 13:45




Instrument :
MSVOA_X
ClientSampleId :
PH2-0135


Tgt Ion: 98 Resp: 676599
Ion Ratio Lower Upper
98 100
100 64.1 52.4 78.6

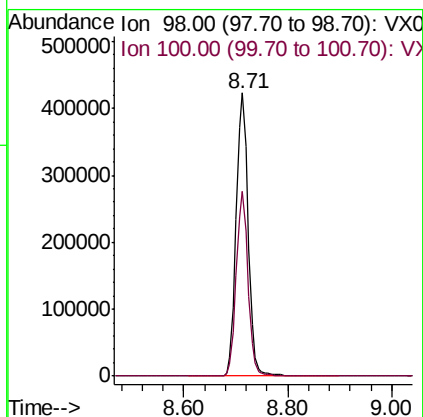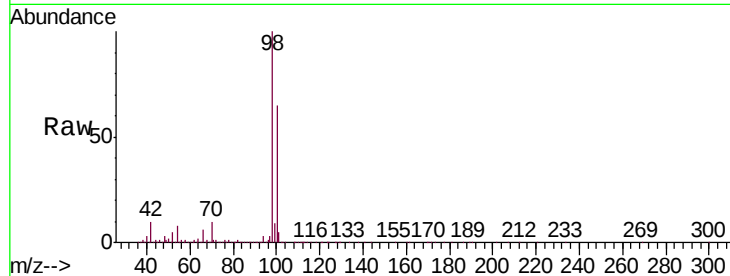

#52
Toluene
Concen: 0.225 ug/l
RT: 8.79 min Scan# 1252
Delta R.T. 0.01 min
Lab File: VX011628.D
Acq: 19 Aug 2019 13:45

Tgt Ion: 92 Resp: 2263
Ion Ratio Lower Upper
92 100
91 204.9 138.0 207.0



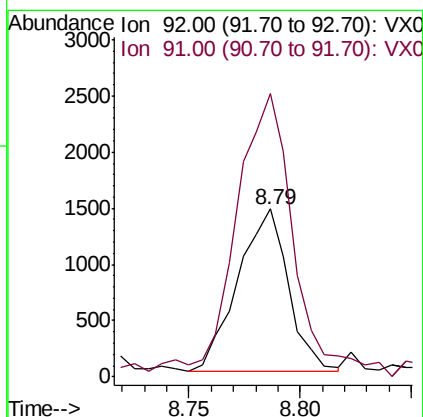



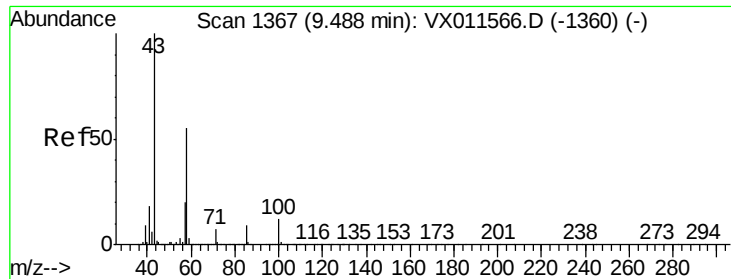

#59
2-Hexanone
Concen: 0.286 ug/l
RT: 9.44 min Scan# 1359
Delta R.T. -0.05 min
Lab File: VX011628.D
Acq: 19 Aug 2019 13:45




Instrument :
MSVOA_X
ClientSampleId :
PH2-0135


Tgt Ion: 43 Resp: 1319
Ion Ratio Lower Upper
43 100
58 47.1 27.5 82.4

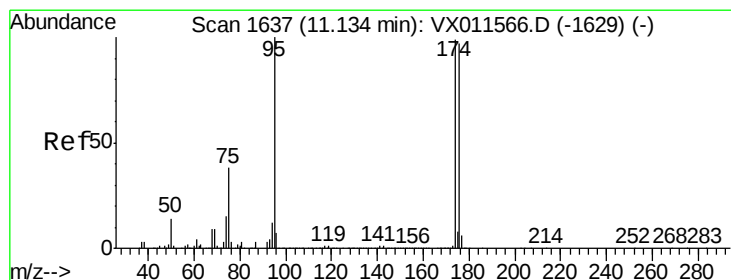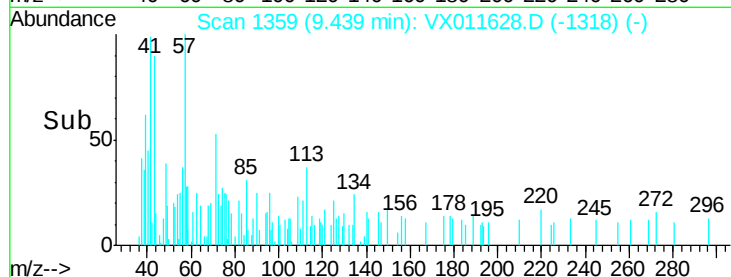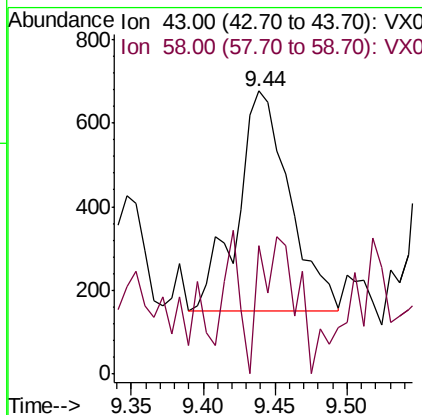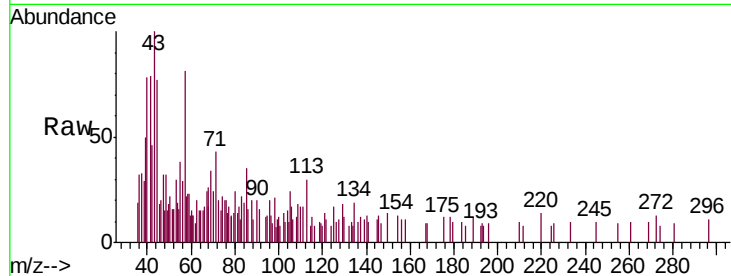

#62
4-Bromofluorobenzene
Concen: 45.996 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX011628.D
Acq: 19 Aug 2019 13:45

Tgt Ion: 95 Resp: 235401
Ion Ratio Lower Upper
95 100
174 99.7 0.0 200.6
176 98.0 0.0 196.6

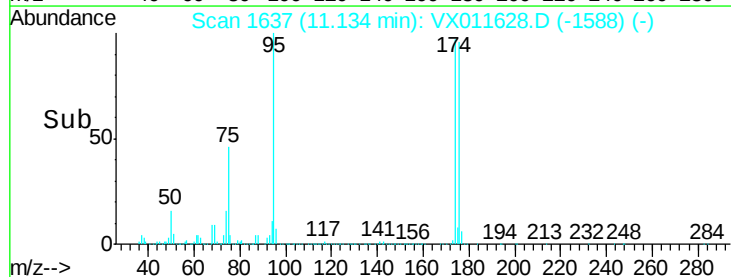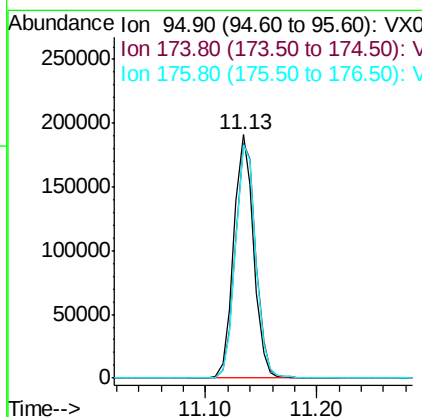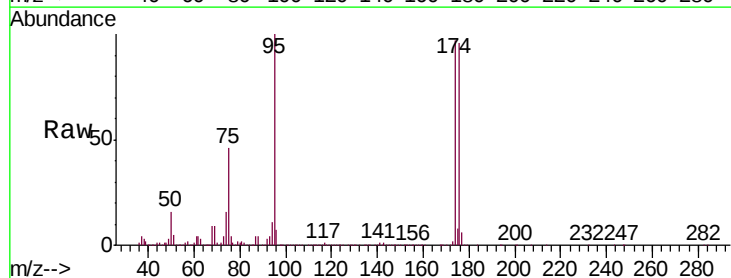

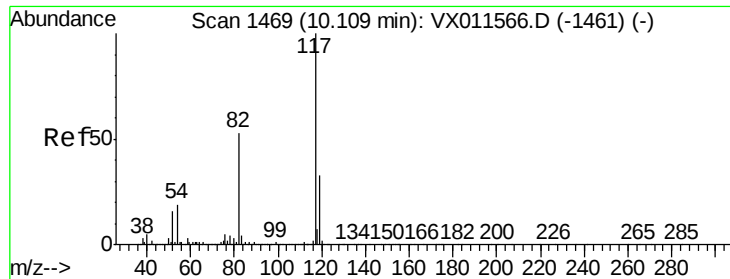

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45

Instrument :

MSVOA_X

ClientSampleId :

PH2-0135


Tgt Ion:117 Resp: 520787

Ion Ratio Lower Upper

117 100

82 52.6 42.0 63.0




119 32.2 26.5 39.7

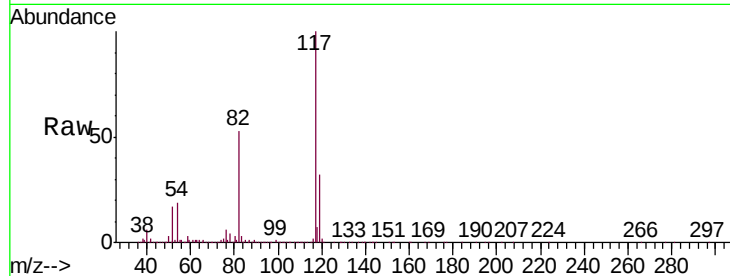

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

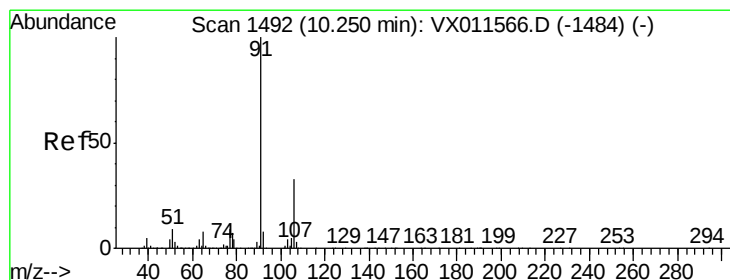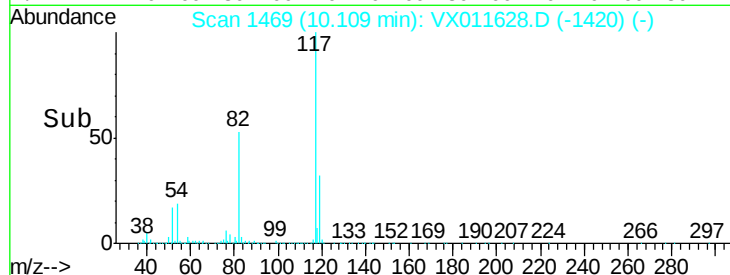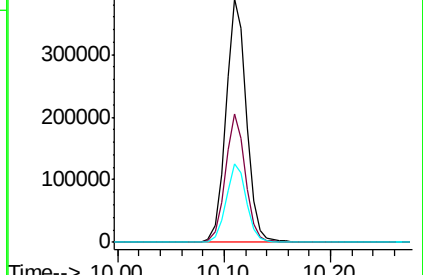

#67

Ethyl Benzene

Concen: 0.941 ug/l

RT: 10.25 min Scan# 1492

Delta R.T. 0.00 min

Lab File: VX011628.D


Acq: 19 Aug 2019 13:45

Tgt Ion: 91 Resp: 17443

Ion Ratio Lower Upper



91 100


106 35.3 26.0 39.0



Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 106.00 (105.70 to 106.70): V

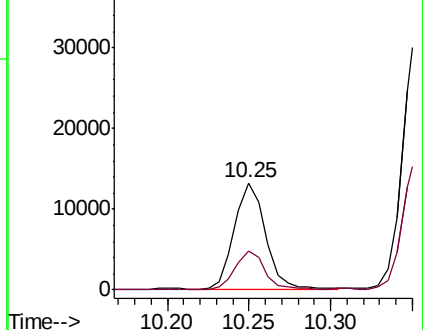

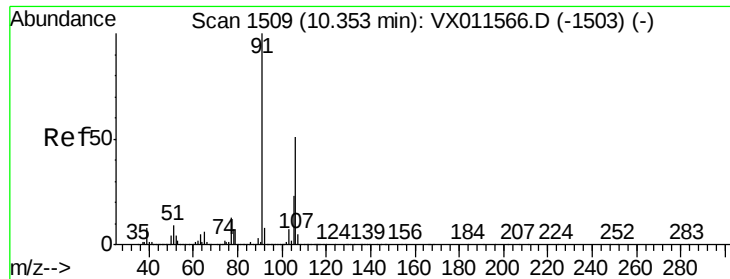

#68

m/p-Xylenes

Concen: 3.660 ug/l

RT: 10.35 min Scan# 1509

Delta R.T. 0.00 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45

Instrument :

MSVOA_X

ClientSampleId :


PH2-0135

Tgt Ion:106 Resp: 26045

Ion Ratio Lower Upper




106 100

91 188.1 156.0 234.0



Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VX0

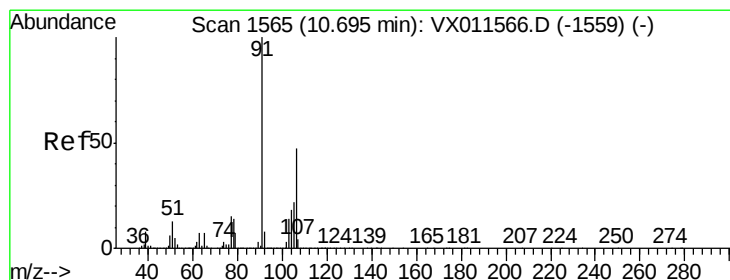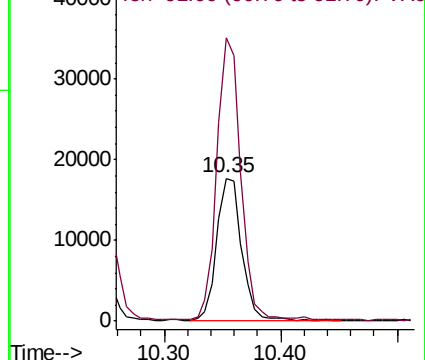

#69

o-Xylene

Concen: 0.378 ug/l

RT: 10.69 min Scan# 1565

Delta R.T. 0.00 min

Lab File: VX011628.D


Acq: 19 Aug 2019 13:45

Tgt Ion:106 Resp: 2635

Ion Ratio Lower Upper



106 100


91 191.7 105.5 316.4



Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VX0



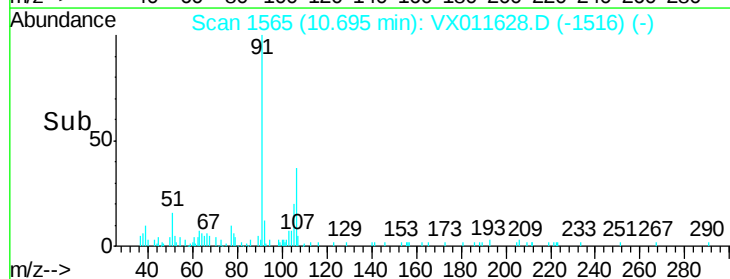
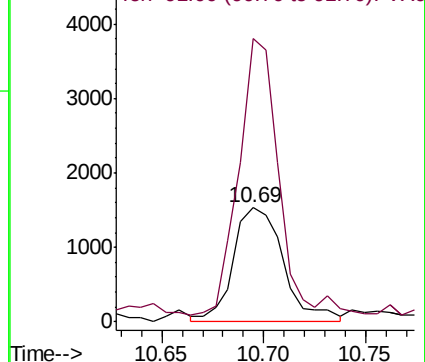


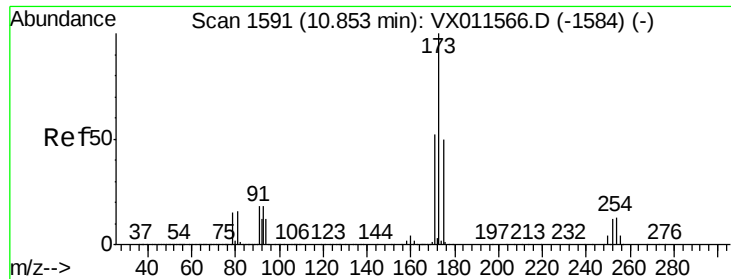

#71
Bromoform
Concen: 3.321 ug/l
RT: 10.66 min Scan# 1559
Delta R.T. -0.19 min
Lab File: VX011628.D
Acq: 19 Aug 2019 13:45




Instrument :
MSVOA_X
ClientSampled :
PH2-0135


Tgt Ion:173 Resp: 129
Ion Ratio Lower Upper
173 100
175 0.0 24.9 74.7#
254 17.8 0.1 0.1#

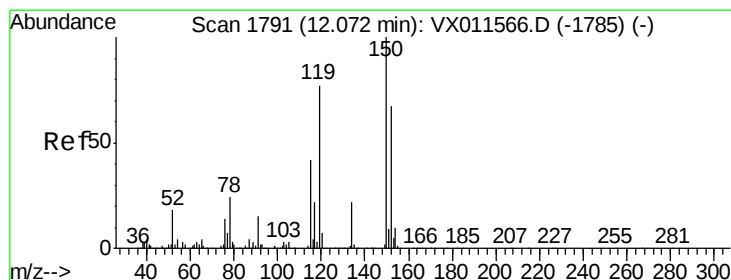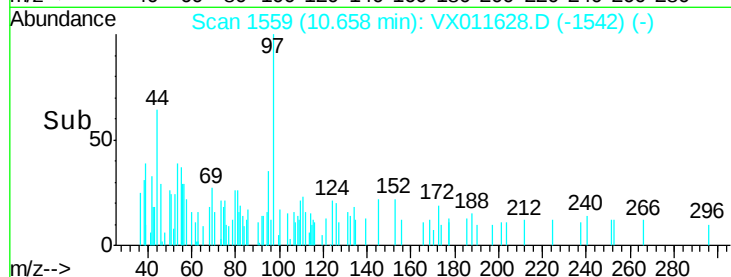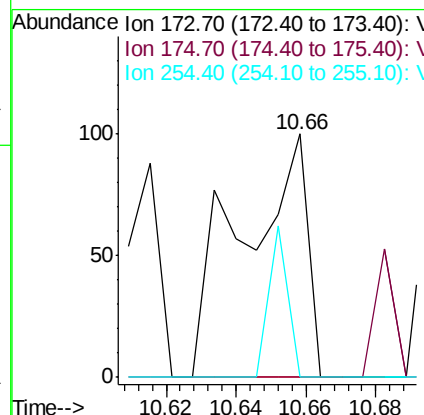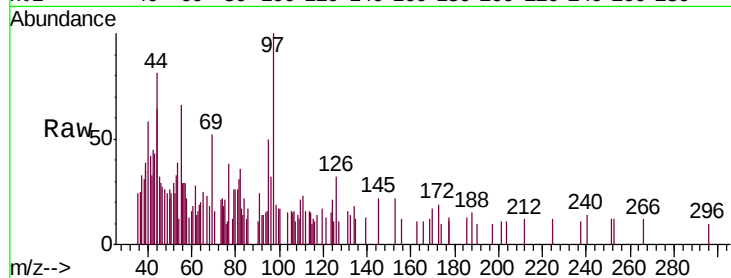

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1791
Delta R.T. 0.00 min
Lab File: VX011628.D
Acq: 19 Aug 2019 13:45

Tgt Ion:152 Resp: 258989
Ion Ratio Lower Upper
152 100
115 52.8 37.3 111.9
150 155.0 0.0 346.2


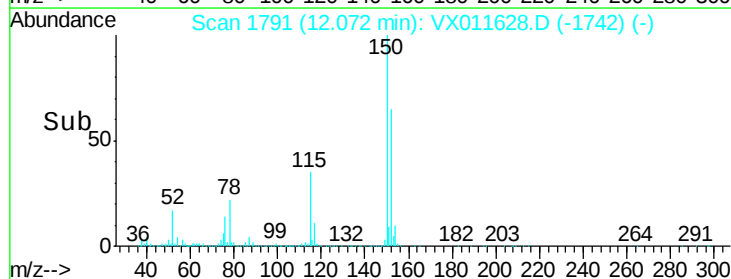
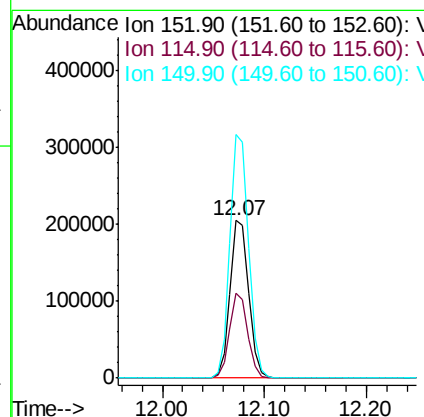
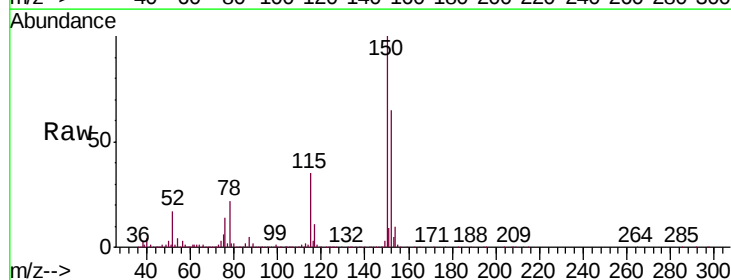


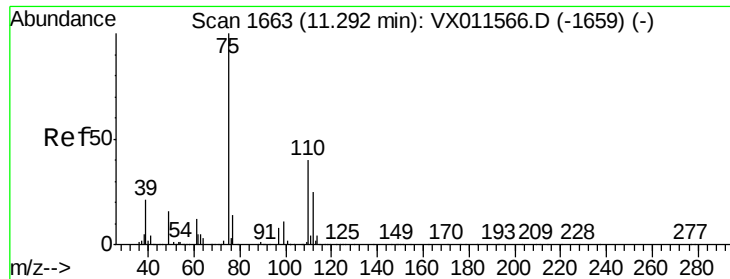

#76
 1,2,3-Trichloropropane
 Concen: 22.040 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. -0.16 min
 Lab File: VX011628.D
 Acq: 19 Aug 2019 13:45




Instrument :
 MSVOA_X
 ClientSampleId :
 PH2-0135


Tgt Ion: 75 Resp: 108239
 Ion Ratio Lower Upper
 75 100
 77 1.0 20.9 62.8#

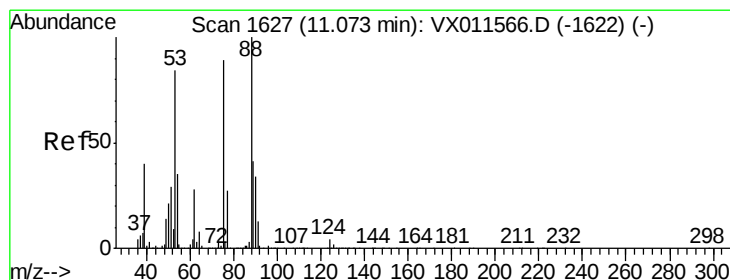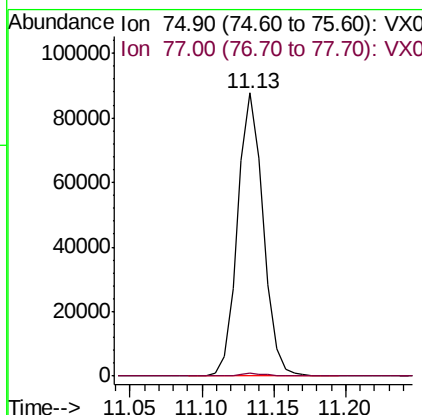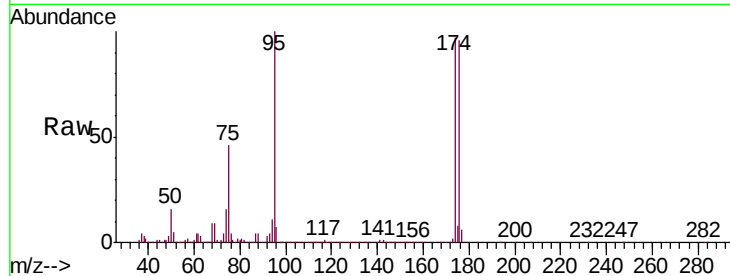

#81
 trans-1,4-Dichloro-2-butene
 Concen: 58.834 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. 0.06 min
 Lab File: VX011628.D
 Acq: 19 Aug 2019 13:45

Tgt Ion: 75 Resp: 108239
 Ion Ratio Lower Upper
 75 100
 53 0.2 77.4 116.0#
 89 0.1 37.3 55.9#

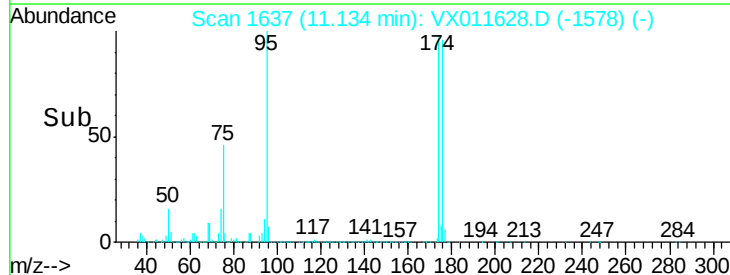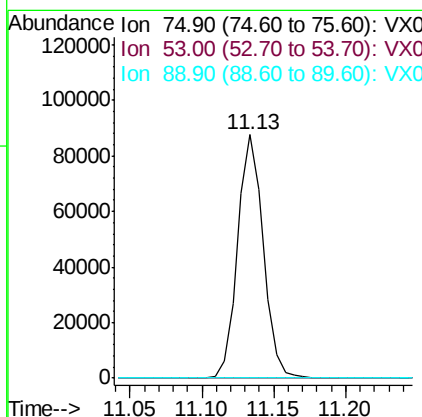



#84

1,2,4-Trimethylbenzene

Concen: 0.443 ug/l

RT: 11.80 min Scan# 1747

Delta R.T. 0.00 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45

Instrument :

MSVOA_X

ClientSampleId :


PH2-0135

Tgt Ion:105 Resp: 6277

Ion Ratio Lower Upper




105 100

120 44.4 23.3 69.9

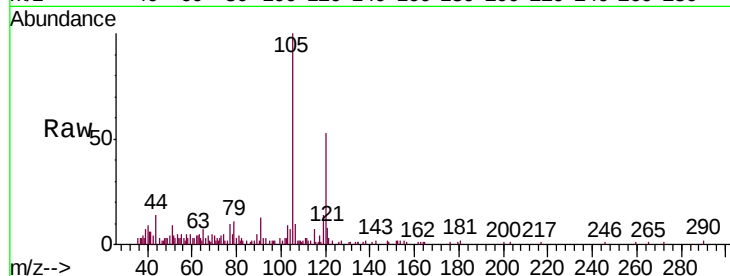

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

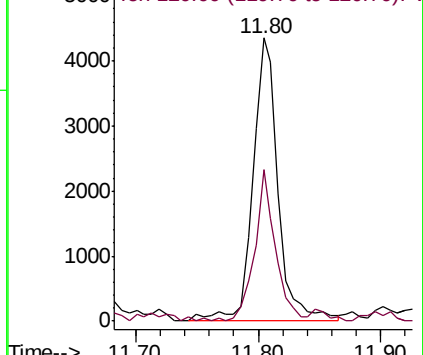

#95

Naphthalene

Concen: 0.202 ug/l

RT: 13.83 min Scan# 2080

Delta R.T. 0.01 min

Lab File: VX011628.D

Acq: 19 Aug 2019 13:45


Tgt Ion:128 Resp: 3668

Ion Ratio Lower Upper

128 100

127 18.9 10.3 15.5#

129 18.4 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

