


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081919\
 Data File : VX011618.D
 Acq On : 19 Aug 2019 09:13
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
 Title : SW846 8260
 Last Update : Fri Aug 16 04:15:26 2019

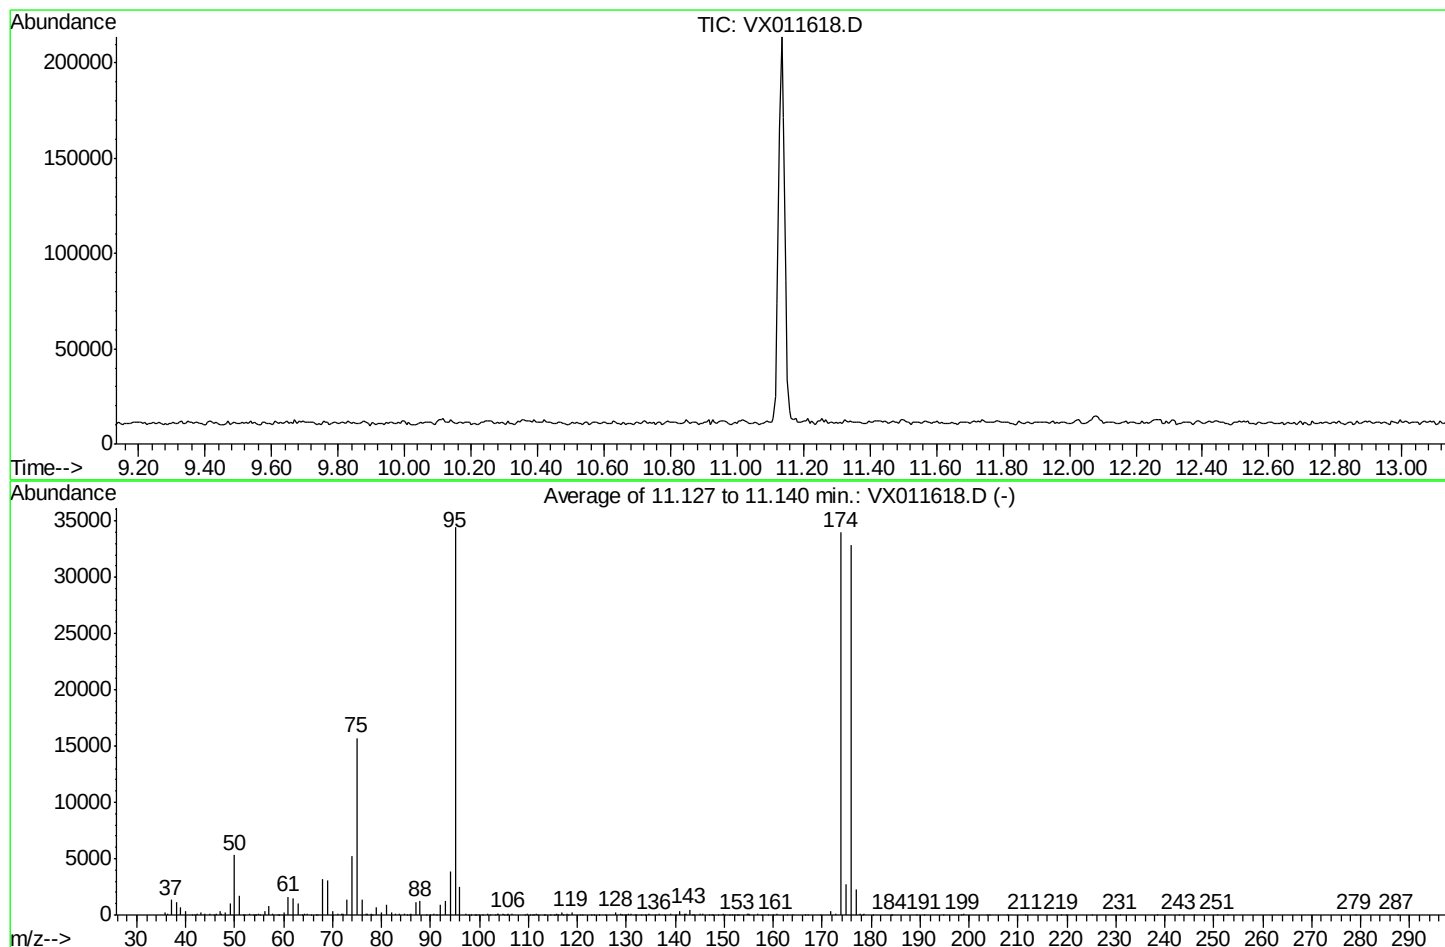

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	5307	PASS
75	95	30	60	45.7	15744	PASS
95	95	100	100	100.0	34426	PASS
96	95	5	9	7.2	2490	PASS
173	174	0.00	2	0.4	136	PASS
174	95	50	100	98.8	34000	PASS
175	174	5	9	8.0	2708	PASS
176	174	95	101	96.5	32808	PASS
177	176	5	9	7.1	2314	PASS