



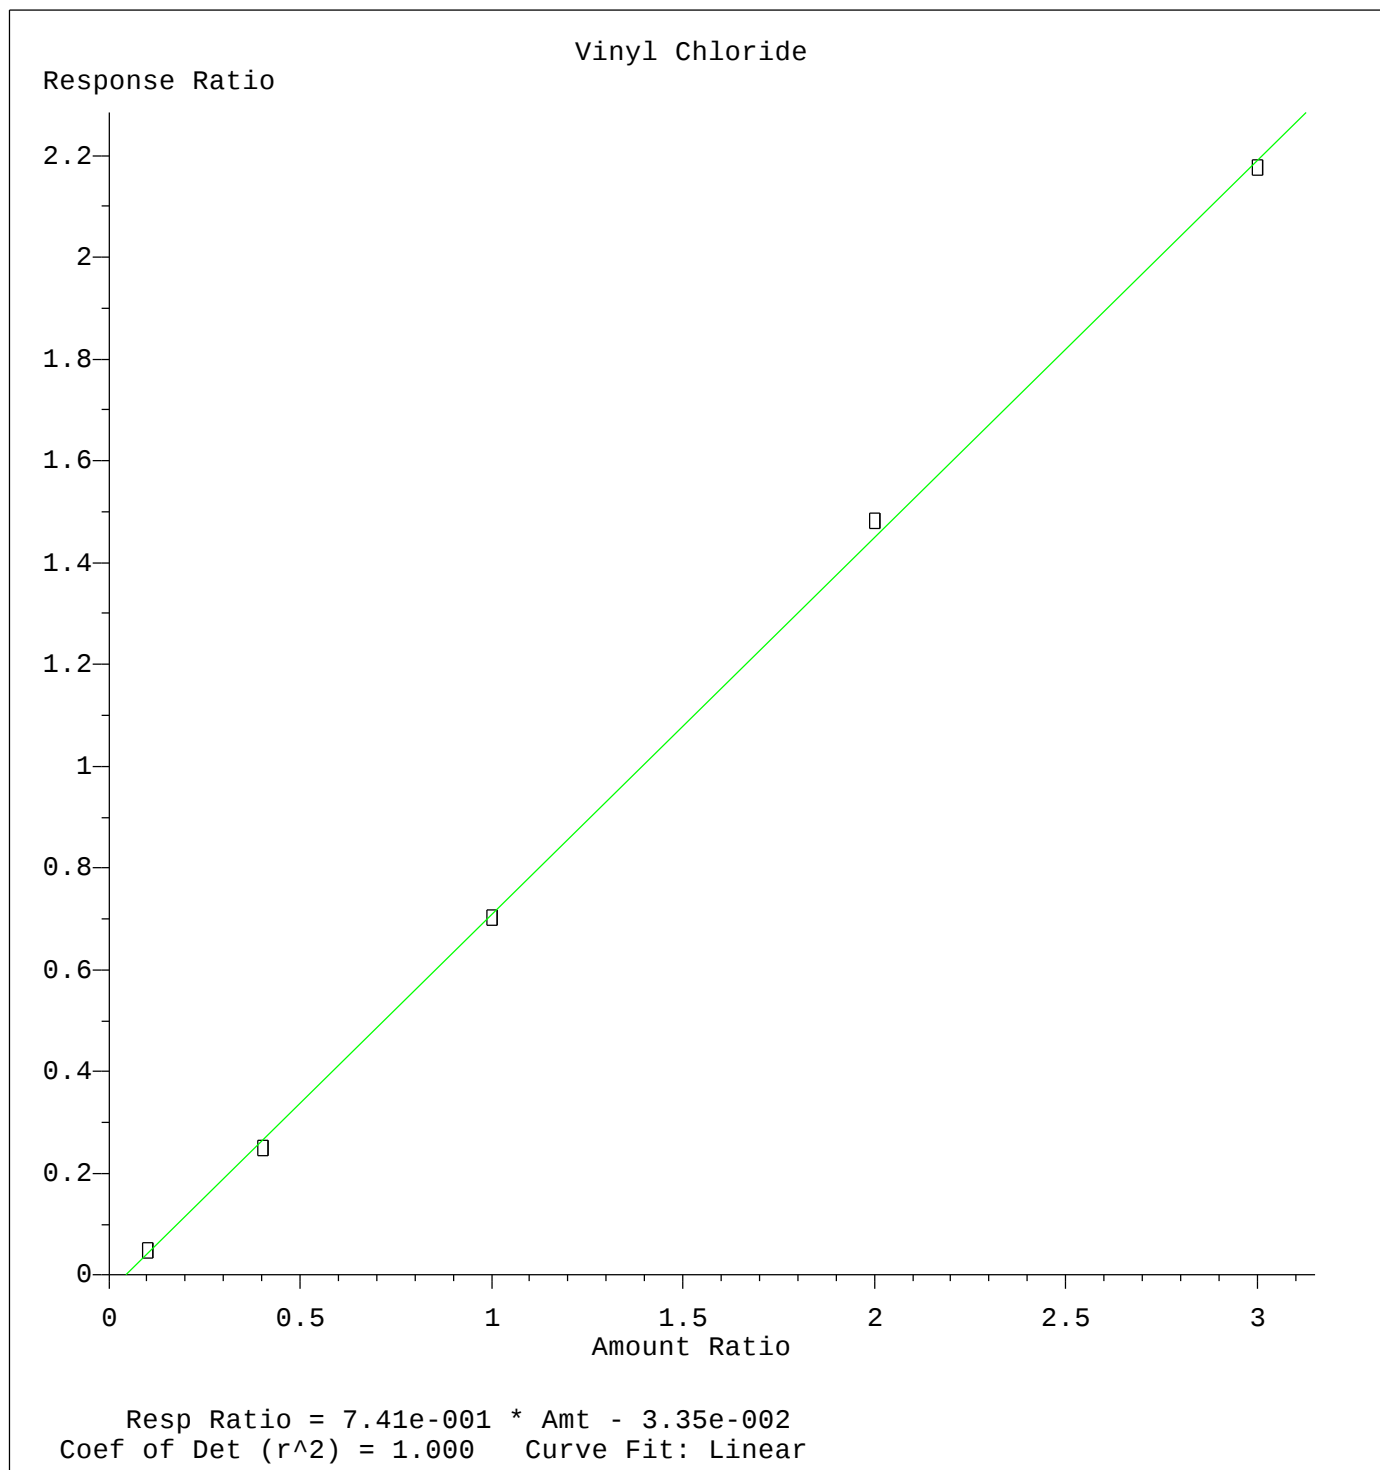

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M
Calibration Table Last Updated: Wed Aug 19 05:36:51 2020

Methylcyclohexane

Response Ratio

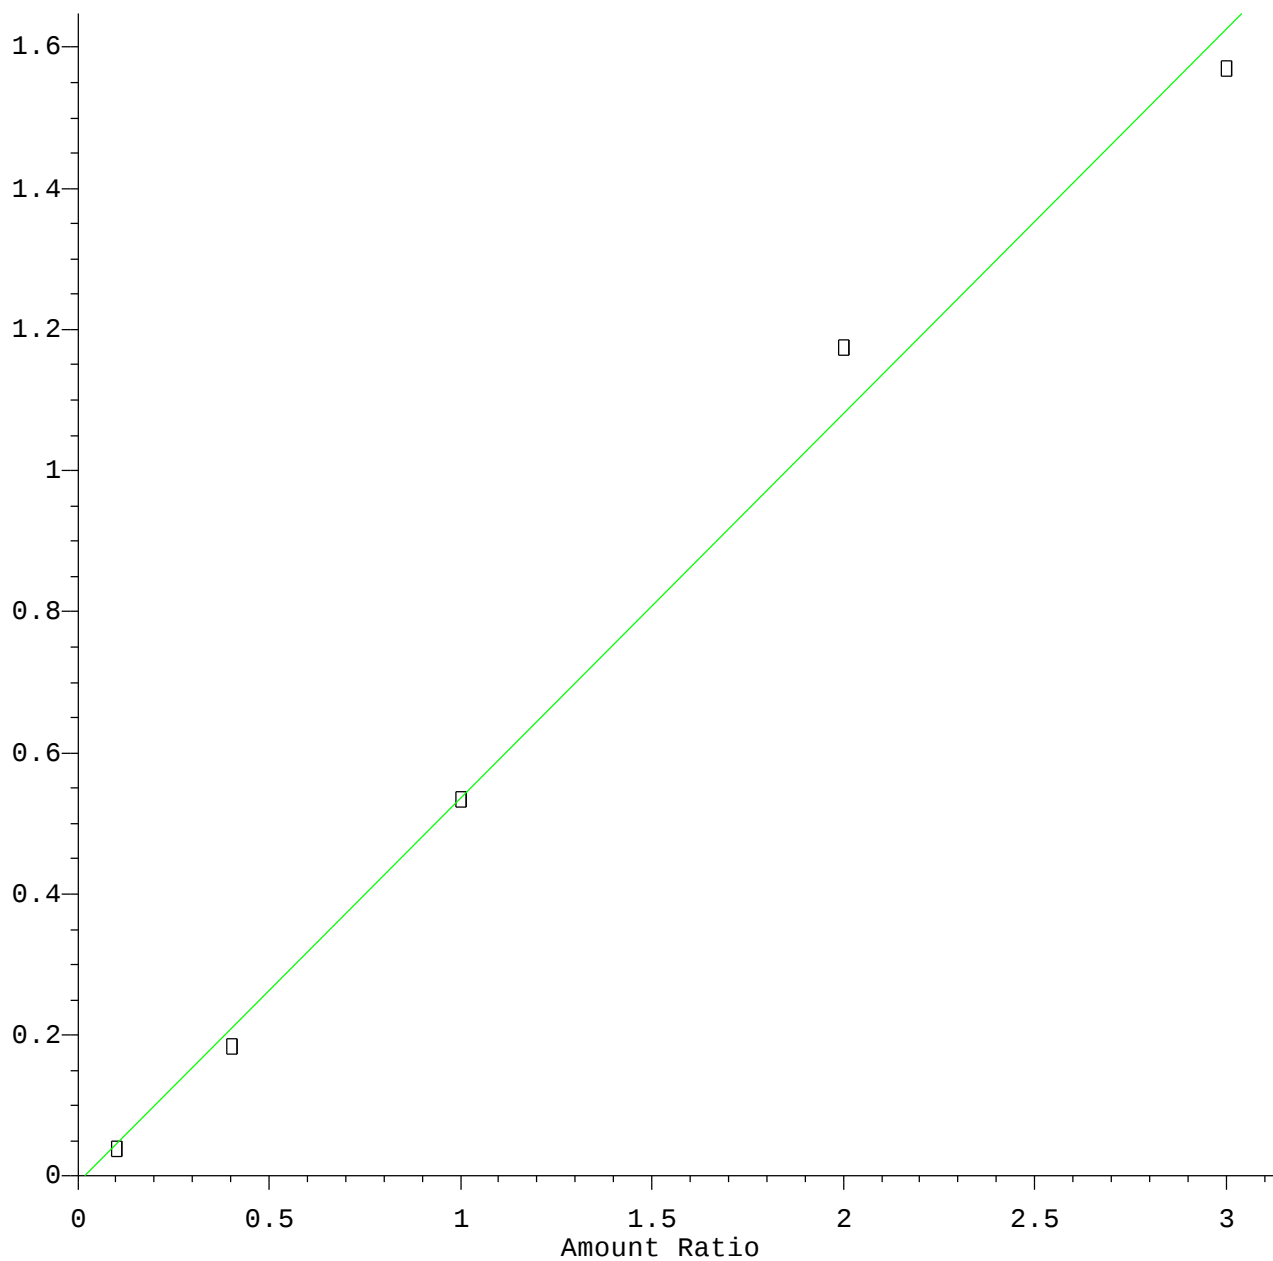


Resp Ratio = $5.45 \times 10^{-1} \times \text{Amt} - 8.86 \times 10^{-3}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M
Calibration Table Last Updated: Wed Aug 19 05:36:51 2020

Dichlorodifluoromethane

Response Ratio

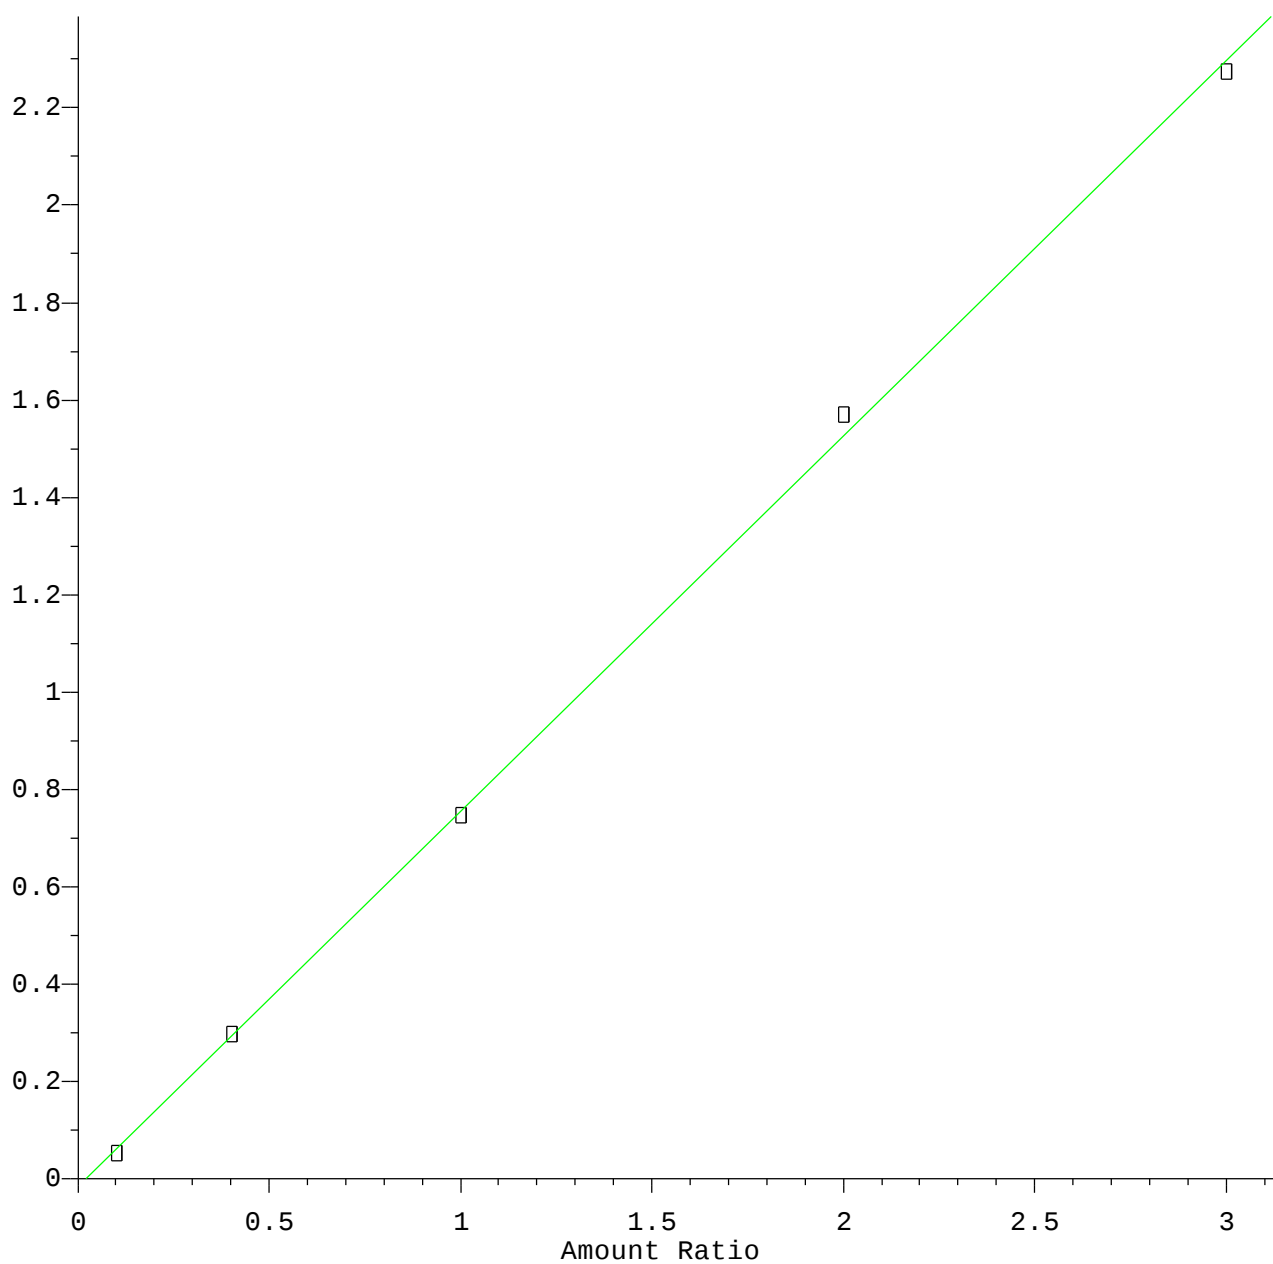

Resp Ratio = $7.71 \times 10^{-1} \times \text{Amt} - 1.52 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M
Calibration Table Last Updated: Wed Aug 19 05:36:51 2020