

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081920\
 Data File : VX017998.D
 Acq On : 19 Aug 2020 21:47
 Operator : JC/SP
 Sample : VX0819WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0819WBL02

Quant Time: Aug 20 05:41:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 19 05:36:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	498765	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	720282	50.00	ug/l	-0.01
63) Chlorobenzene-d5	10.10	117	674647	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	339399	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	324613	44.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.80%	
35) Dibromofluoromethane	5.46	113	257808	48.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.12%	
50) Toluene-d8	8.70	98	946426	49.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.84%	
62) 4-Bromofluorobenzene	11.12	95	319036	45.56	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.12%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081920\
Data File : VX017998.D
Acq On : 19 Aug 2020 21:47
Operator : JC/SP
Sample : VX0819WBL02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0819WBL02

Quant Time: Aug 20 05:41:37 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 19 05:36:51 2020
Response via : Initial Calibration

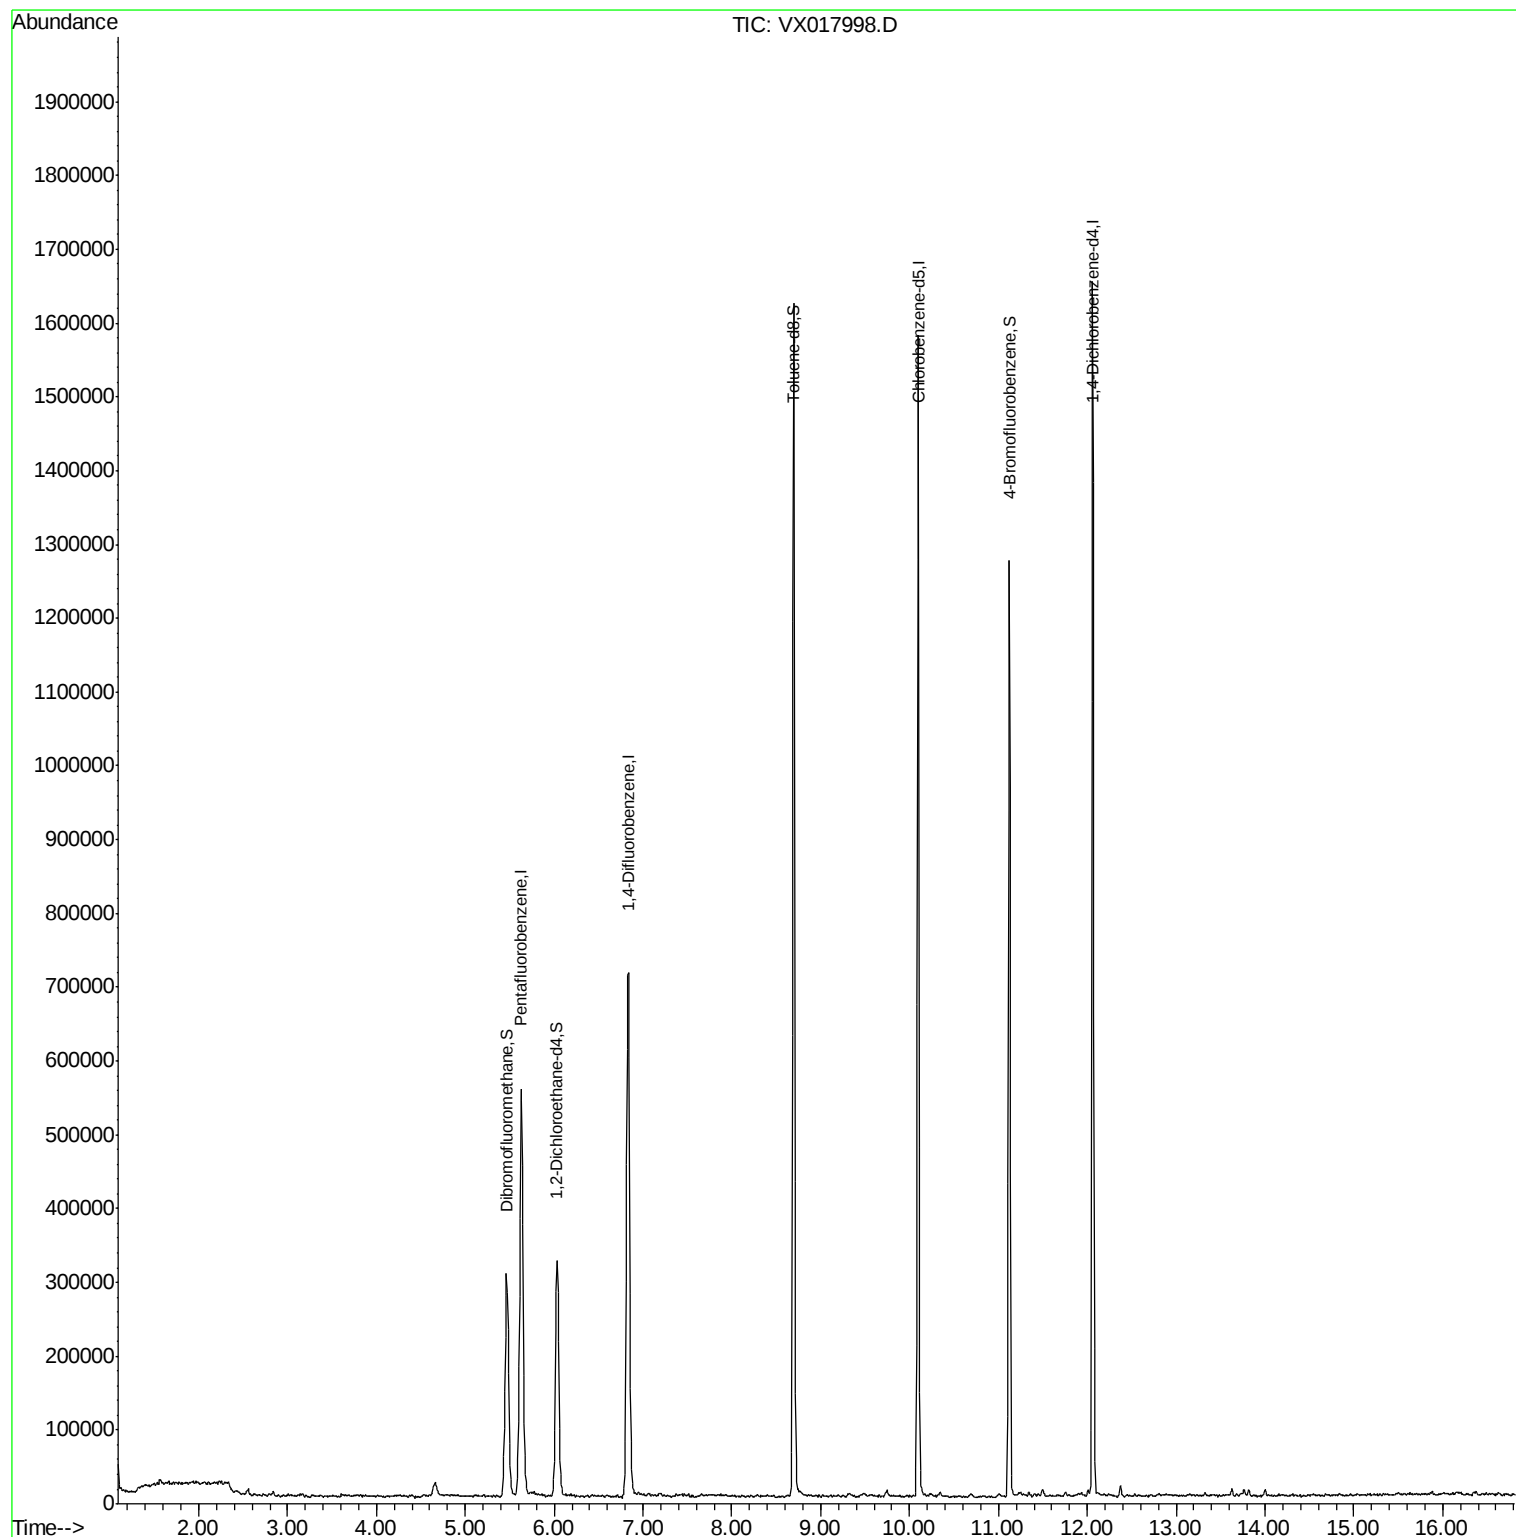

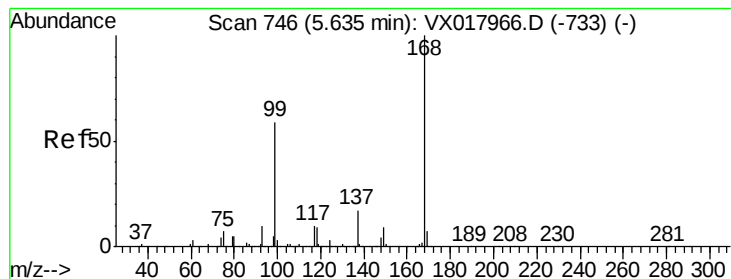

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 746

Delta R.T. 0.00 min

Lab File: VX017998.D

Acq: 19 Aug 2020 21:47

Instrument :

MSVOA_X

ClientSampleId :


VX0819WBL02

Tot Ion:168 Resp: 498765

Ion Ratio Lower Upper

168 100

99 53.8 47.4 71.2

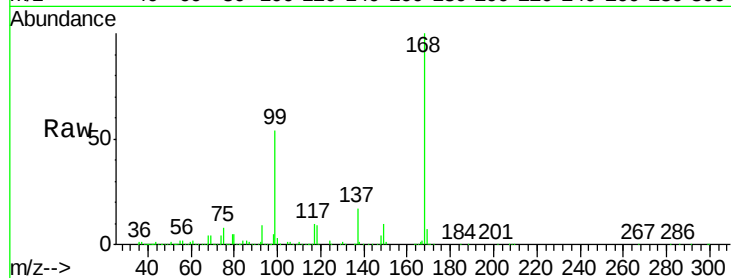

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

200000

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

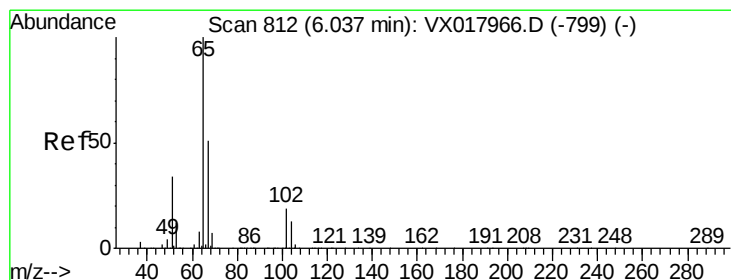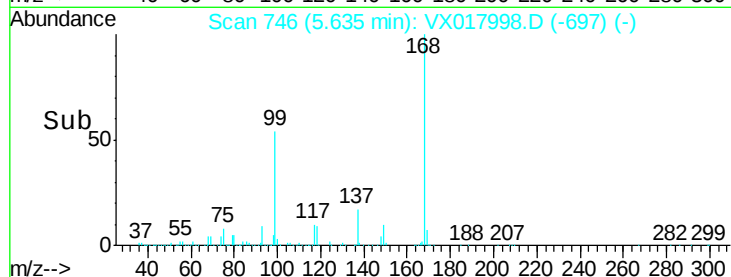

#33

1,2-Dichloroethane-d4

Concen: 44.397 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.01 min

Lab File: VX017998.D


Acq: 19 Aug 2020 21:47

Tgt Ion: 65 Resp: 324613

Ion Ratio Lower Upper

65 100

67 50.9 0.0 103.0

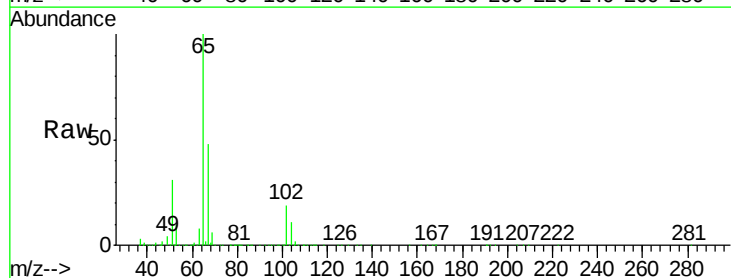

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.03

150000


100000


50000

0

Time-->

5.90 6.00 6.10 6.20

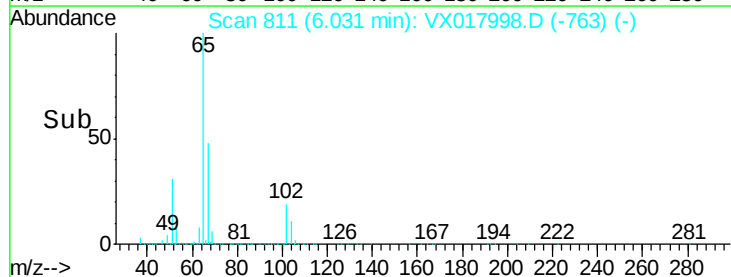

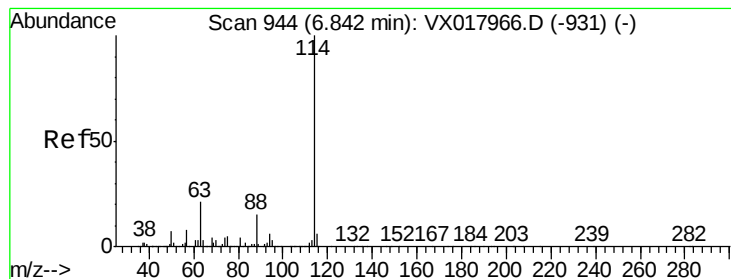

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.01 min

Lab File: VX017998.D

Acq: 19 Aug 2020 21:47

Instrument :

MSVOA_X

ClientSampleId :

VX0819WBL02


Tot Ion:114 Resp: 720282

Ion Ratio Lower Upper

114 100

63 21.0 0.0 42.6




88 16.4 0.0 30.2

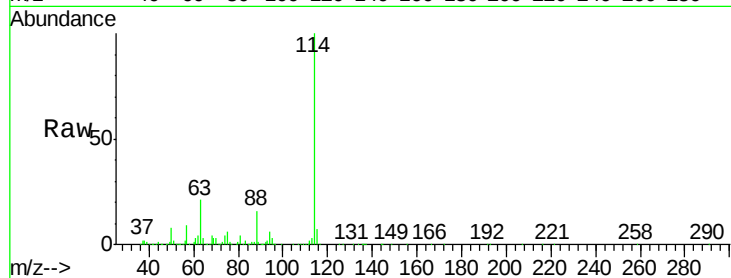

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

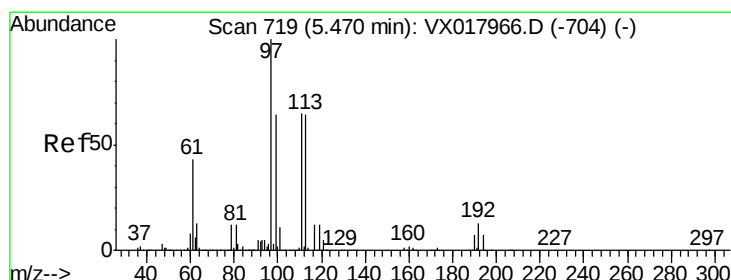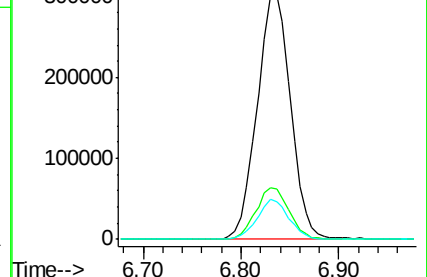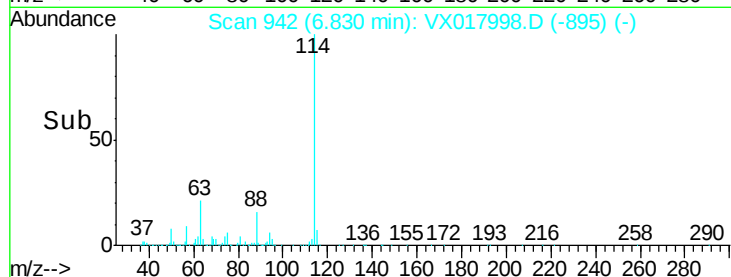

#35

Dibromofluoromethane

Concen: 48.064 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.01 min

Lab File: VX017998.D

Acq: 19 Aug 2020 21:47


Tgt Ion:113 Resp: 257808

Ion Ratio Lower Upper

113 100

111 103.8 83.5 125.3



192 20.6 16.2 24.4

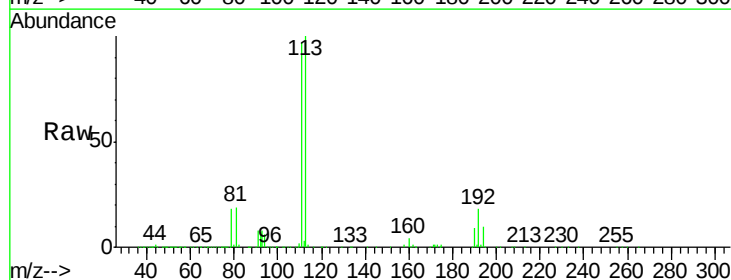


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

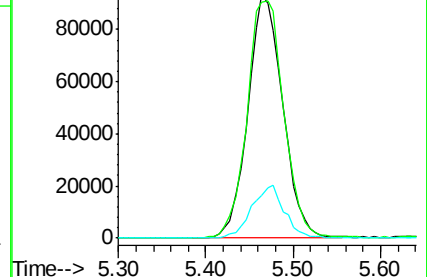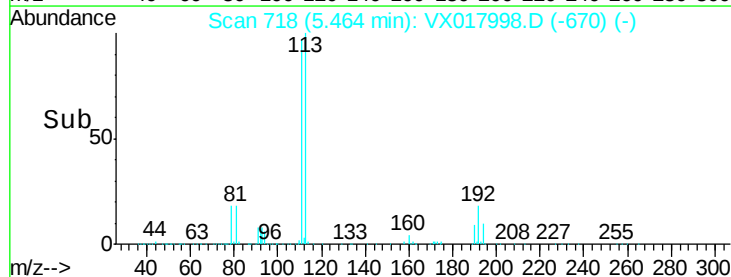

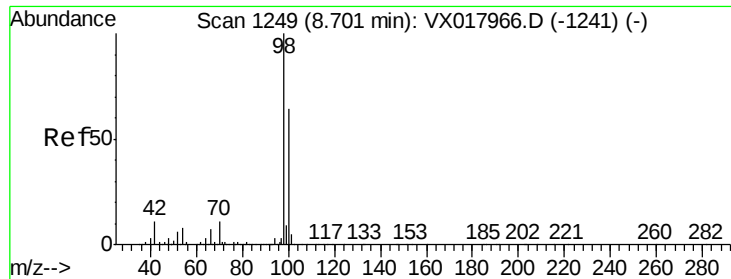

#50

Toluene-d8

Concen: 49.917 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.01 min

Lab File: VX017998.D

Acq: 19 Aug 2020 21:47

Instrument :

MSVOA_X

ClientSampleId :





VX0819WBL02

Tot Ion: 98 Resp: 946426

Ion Ratio Lower Upper

98 100

100 64.0 51.4 77.2

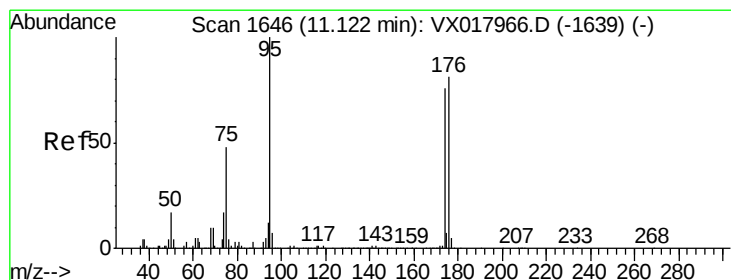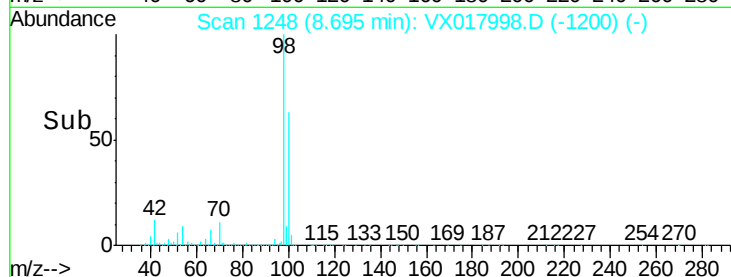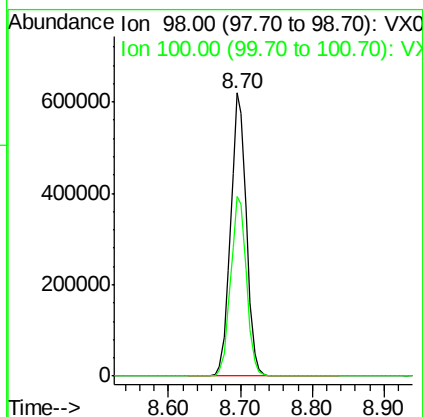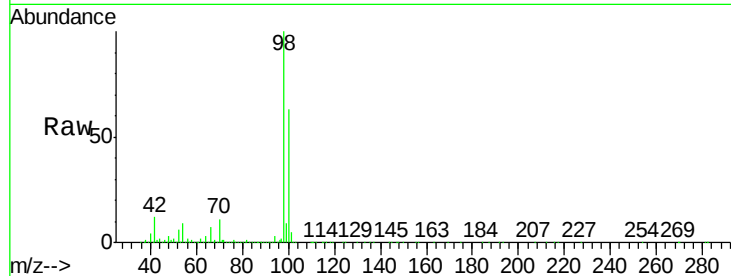

#62

4-Bromofluorobenzene

Concen: 45.559 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.00 min

Lab File: VX017998.D

Acq: 19 Aug 2020 21:47




Tgt Ion: 95 Resp: 319036


Ion Ratio Lower Upper

95 100

174 84.5 0.0 166.0

176 79.7 0.0 161.0


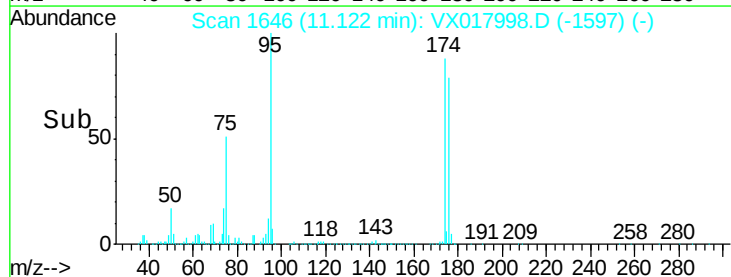
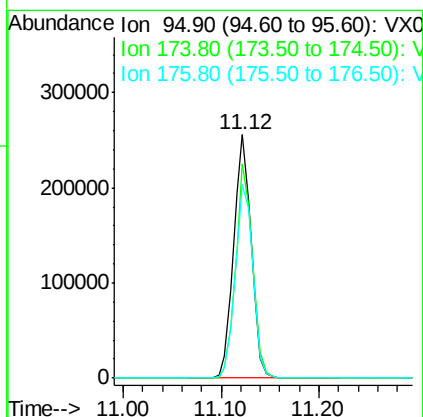
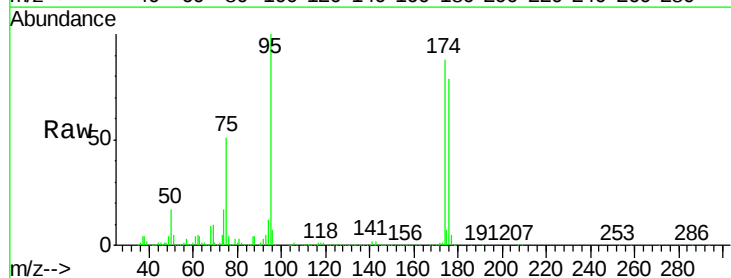


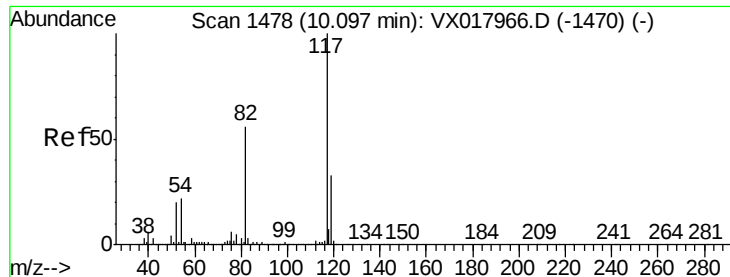

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. 0.00 min
Lab File: VX017998.D
Acq: 19 Aug 2020 21:47

Instrument :
MSVOA_X
ClientSampleId :
VX0819WBL02

Tot Ion:117 Resp: 674647
Ion Ratio Lower Upper
117 100
82 52.8 44.6 66.8
119 31.9 26.2 39.4

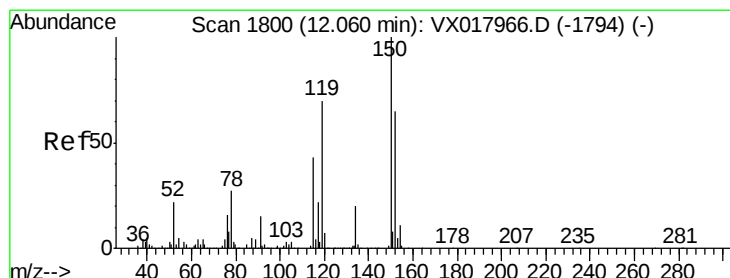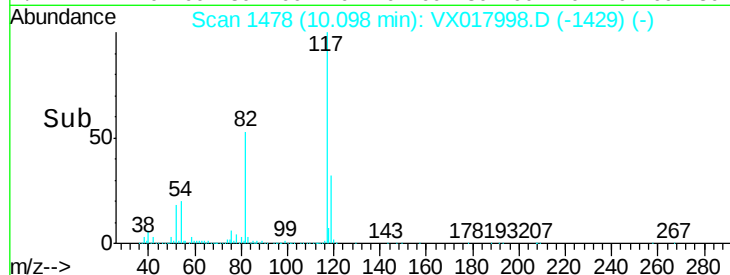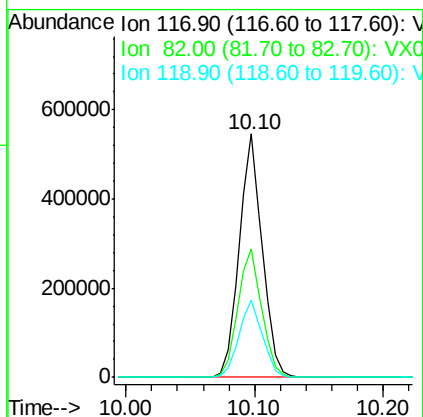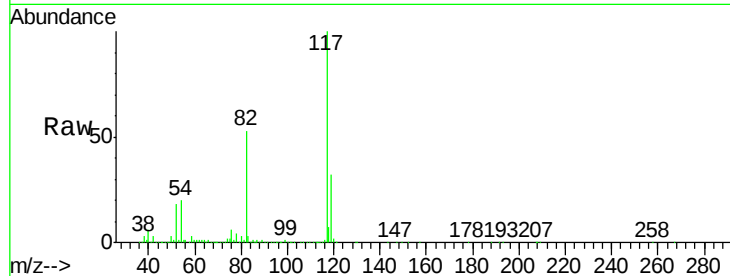

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. 0.00 min
Lab File: VX017998.D
Acq: 19 Aug 2020 21:47

Tgt Ion:152 Resp: 339399
Ion Ratio Lower Upper
152 100
115 57.3 40.6 121.7
150 154.0 0.0 346.4

