

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081920\
 Data File : VX017988.D
 Acq On : 19 Aug 2020 16:27
 Operator : JC/SP
 Sample : L3721-01 10X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 I-OC-6

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.636	74	90	93	rBV8	63307	252145	3.66%	1.099%
2	2.428	215	220	231	rVV	130924	239681	3.48%	1.044%
3	2.538	231	238	257	rVB	4133656	6886968	100.00%	30.010%
4	5.464	707	718	730	rBV	285566	820744	11.92%	3.576%
5	5.629	734	745	756	rBV2	497406	1355260	19.68%	5.905%
6	6.031	800	811	819	rBV	308966	803042	11.66%	3.499%
7	6.111	819	824	835	rVB	45445	116302	1.69%	0.507%
8	6.830	932	942	954	rBV	686443	1675914	24.33%	7.303%
9	8.696	1241	1248	1255	rBV	1473489	2271127	32.98%	9.896%
10	8.769	1255	1260	1271	rVV	33610	75542	1.10%	0.329%
11	8.891	1275	1280	1289	rVB	61222	100144	1.45%	0.436%
12	10.098	1471	1478	1488	rBV	1550769	2074940	30.13%	9.041%
13	10.342	1515	1518	1523	rVB3	43911	72111	1.05%	0.314%
14	11.122	1639	1646	1653	rBV	1302710	1602254	23.27%	6.982%
15	12.061	1794	1800	1808	rBV	1656940	2018629	29.31%	8.796%
16	13.817	2083	2088	2094	rBV	2121069	2460993	35.73%	10.724%
17	13.908	2099	2103	2108	rVB	94744	123364	1.79%	0.538%


Sum of corrected areas: 22949160

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081920\
Data File : VX017988.D
Acq On : 19 Aug 2020 16:27
Operator : JC/SP
Sample : L3721-01 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-OC-6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

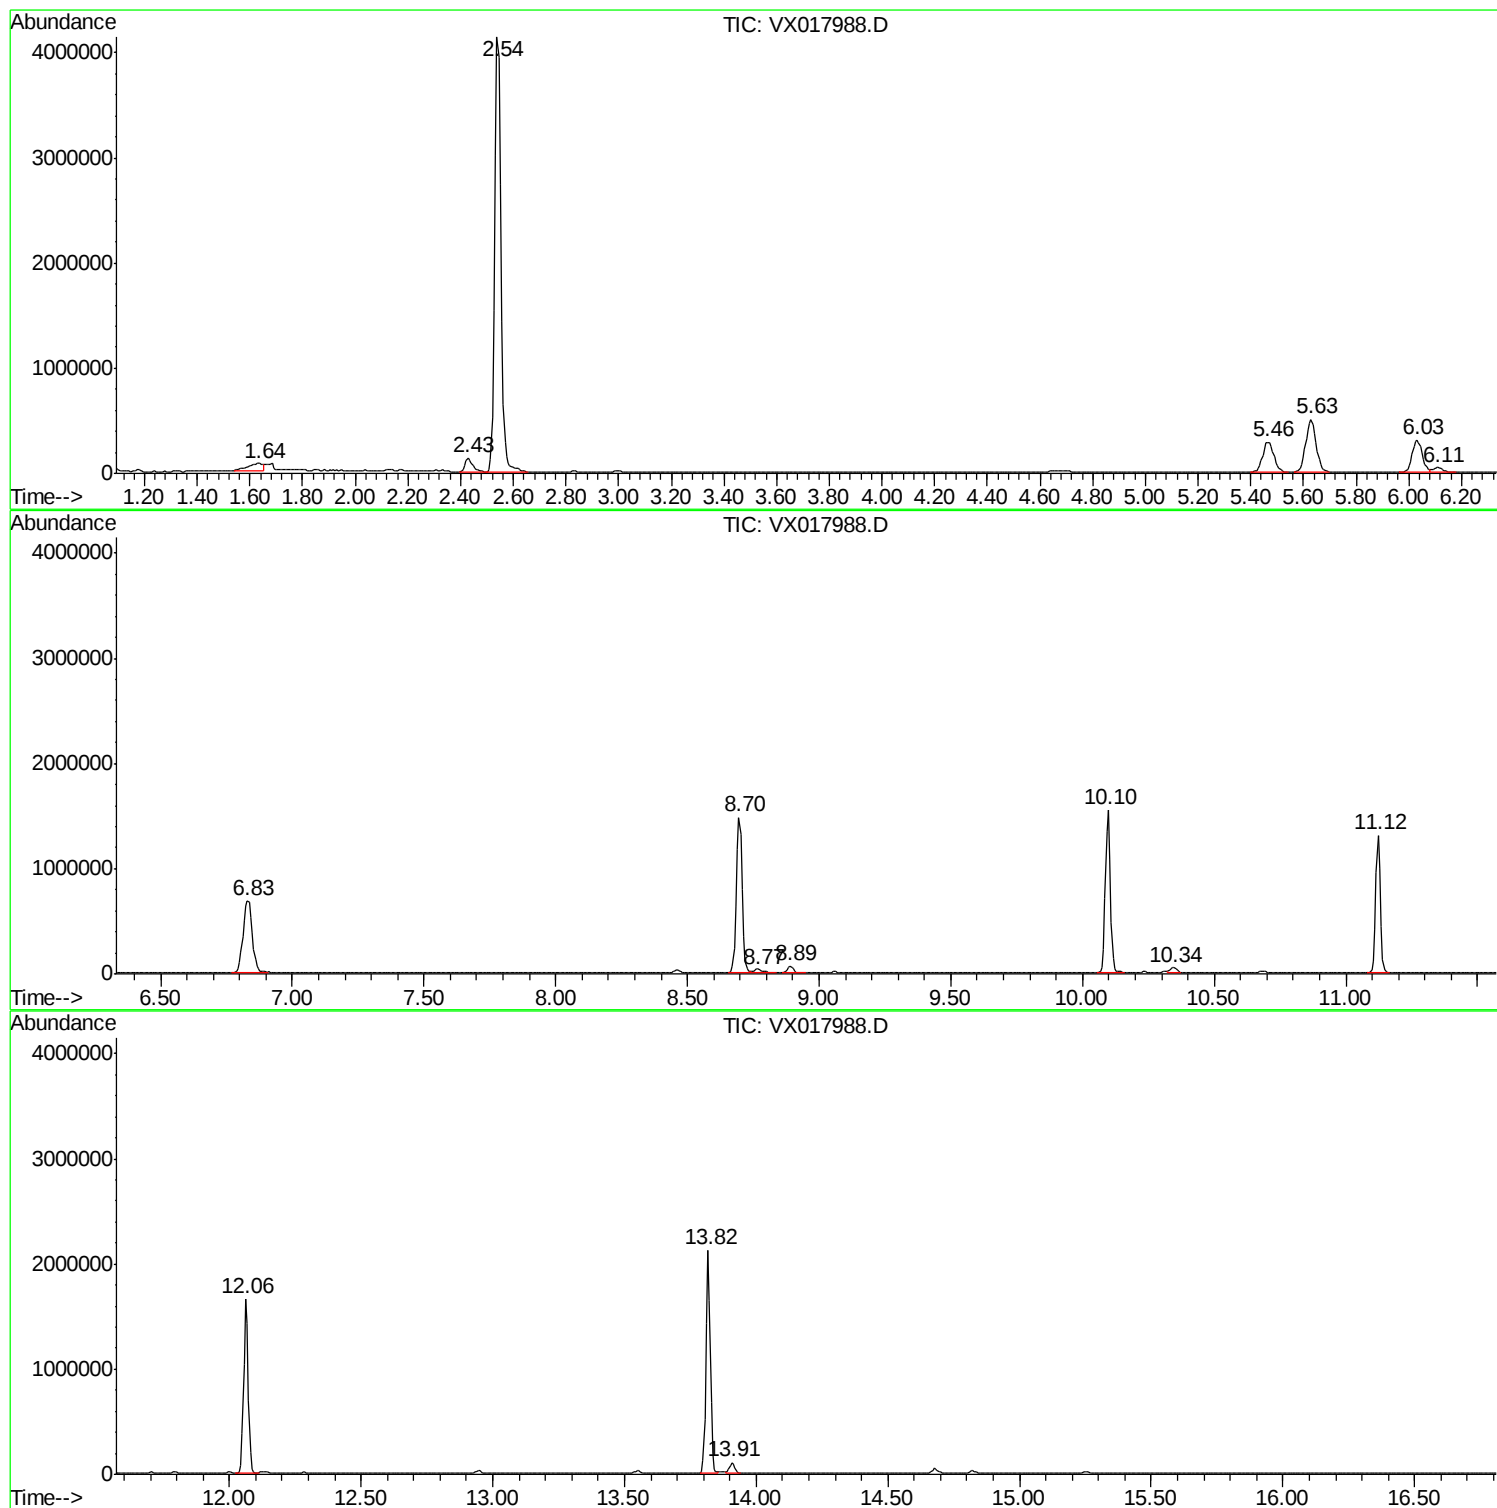

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081920\
Data File : VX017988.D
Acq On : 19 Aug 2020 16:27
Operator : JC/SP
Sample : L3721-01 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
I-OC-6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.64 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.		
1.64	9.30 ug/l	252145	Pentafluorobenzene	5.63		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	4,5-Dichloro-1,3-dioxolan-2-one	156	C3H2Cl2O3	003967-55-3	25	
2	Propanenitrile, 3-chloro-	89	C3H4ClN	000542-76-7	17	
3	2-Chloroethyl methyl sulfoxide	126	C3H7ClOS	005331-57-7	12	
4	Carbonochloridic acid, 4-nitroph...	201	C7H4ClNO4	007693-46-1	10	
5	Propanoic acid, 2-chloro-, ethyl...	136	C5H9ClO2	000535-13-7	10	

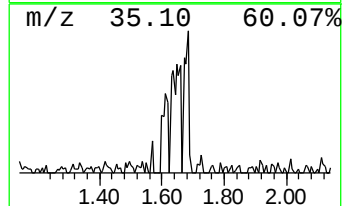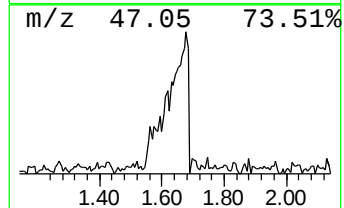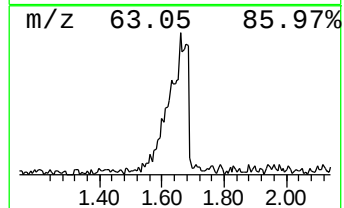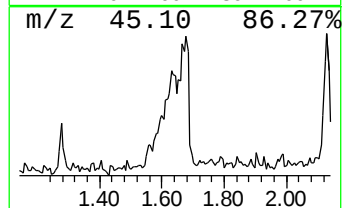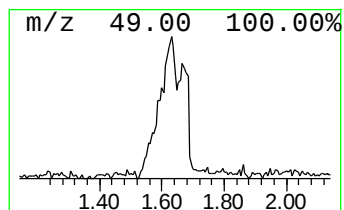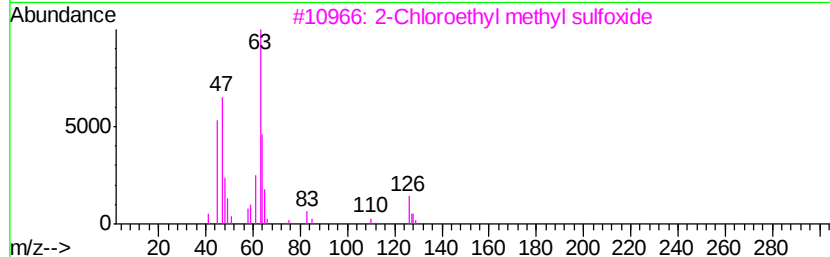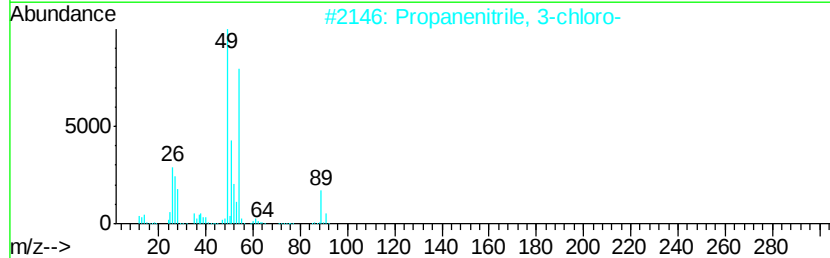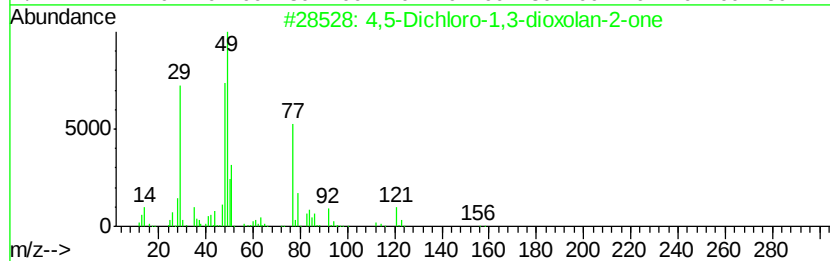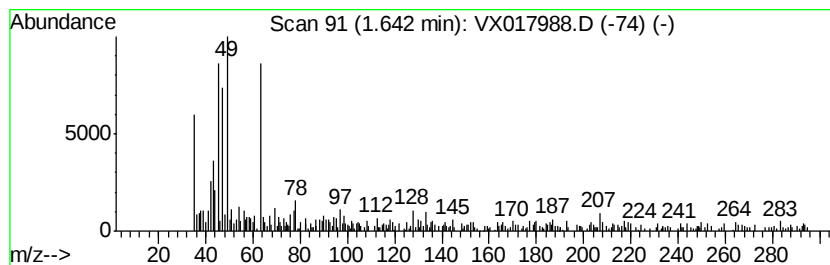

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX081920\
Data File : VX017988.D
Acq On : 19 Aug 2020 16:27
Operator : JC/SP
Sample : L3721-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-OC-6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.64	1.64	9.3	ug/l	252145	1	5.63	1355260	50.0