
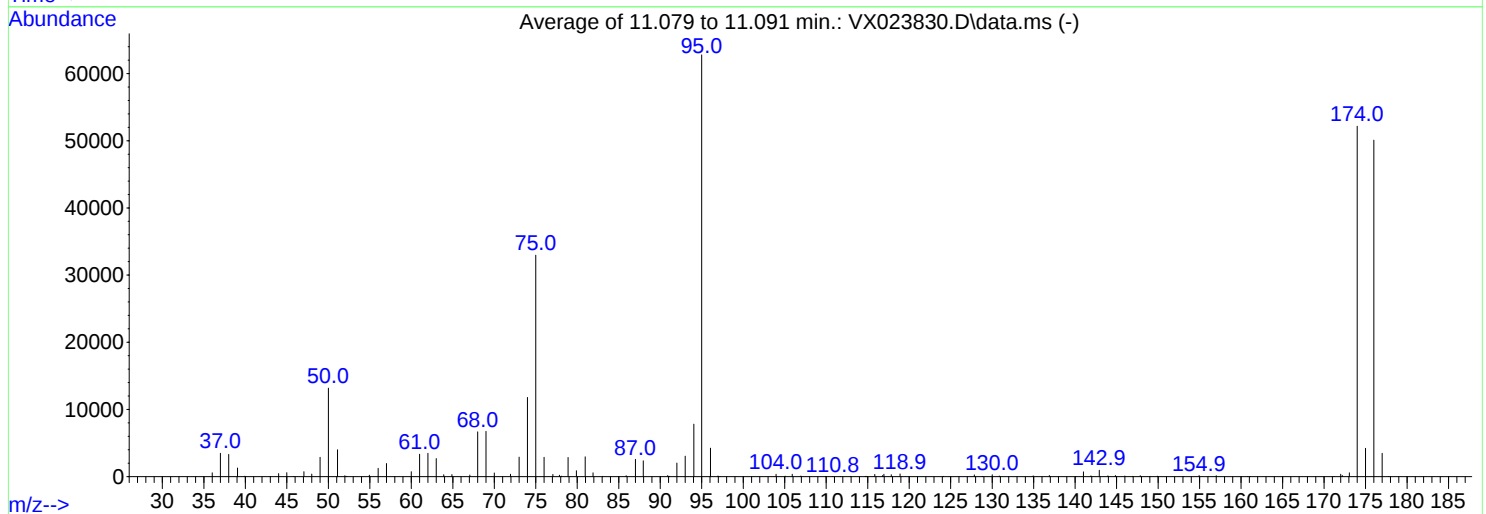


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081921\
 Data File : VX023830.D
 Acq On : 19 Aug 2021 09:04
 Operator : JC/MD
 Sample : BFB604
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB604

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR081921WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Aug 21 04:11:10 2021

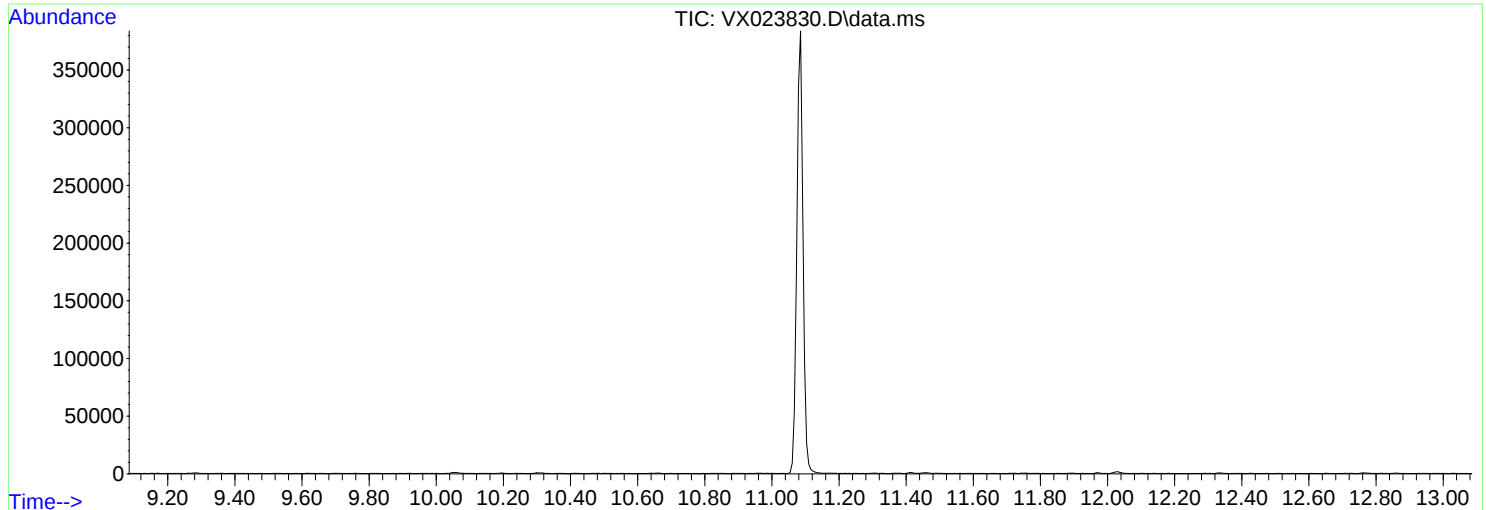

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	13176	PASS
75	95	30	80	52.5	32952	PASS
95	95	100	100	100.0	62787	PASS
96	95	5	9	6.7	4237	PASS
173	174	0.00	2	1.1	582	PASS
174	95	50	120	83.1	52168	PASS
175	174	5	9	8.1	4229	PASS
176	174	95	105	96.0	50083	PASS
177	176	5	10	6.9	3470	PASS

m/z	Abundance
36.00	649.0
37.00	3836.0
38.00	3851.0
39.00	1378.0
39.90	229.0
43.00	60.0
44.00	791.0
45.00	667.0
47.00	883.0
48.00	526.0
49.00	3337.0
50.00	15963.0
51.10	4748.0
52.00	196.0
55.00	256.0
56.00	1412.0
57.00	2166.0
60.00	1007.0
61.00	4280.0
62.00	4401.0
63.00	3136.0
63.90	405.0
64.80	306.0
67.00	286.0
68.00	7729.0
69.00	7665.0
70.00	691.0
71.00	65.0
72.00	401.0
73.00	3171.0
74.00	13619.0
75.00	39624.0
76.00	3420.0
77.10	428.0
77.70	227.0
78.10	195.0
78.90	3423.0
79.90	1068.0
80.90	3457.0
81.80	637.0
83.00	63.0
85.80	170.0
87.00	2950.0
87.90	2672.0
90.90	251.0
92.00	2441.0
93.00	3588.0
94.10	9335.0
95.00	73904.0
96.10	5323.0
97.00	103.0
97.20	100.0
103.90	528.0
105.00	127.0
105.80	429.0
106.90	106.0
109.90	90.0
111.70	63.0
113.00	90.0
114.70	65.0
115.80	405.0
117.00	696.0
117.90	379.0
119.00	433.0
124.10	63.0
127.90	423.0
128.90	68.0
130.00	348.0
130.80	85.0
135.00	134.0
136.90	230.0
140.10	118.0
141.00	802.0
141.90	148.0
142.90	1169.0
143.90	117.0
144.80	229.0
146.00	111.0
146.90	66.0
147.80	194.0
149.00	54.0
149.90	64.0
155.00	311.0
157.00	156.0
160.80	101.0
172.20	478.0
173.00	669.0
174.00	62224.0
175.00	5357.0
176.00	60704.0
177.00	4491.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604

m/z	Abundance
36.10	309.0
37.00	2056.0
38.10	2249.0
39.10	981.0
40.00	198.0
44.00	535.0
45.00	433.0
47.10	411.0
48.00	261.0
49.00	1962.0
50.00	8722.0
51.00	2341.0
52.20	150.0
55.00	145.0
55.90	802.0
56.90	1488.0
60.00	453.0
61.00	2176.0
61.90	2507.0
63.10	1829.0
63.90	173.0
65.00	245.0
67.10	211.0
68.00	4764.0
69.00	4788.0
69.90	406.0
72.00	252.0
73.00	2189.0
74.00	8478.0
75.00	23456.0
76.00	1925.0
77.00	245.0
77.90	211.0
78.90	1831.0
80.00	558.0
80.90	2169.0
82.00	356.0
85.80	84.0
87.00	1844.0
88.00	1447.0
91.10	132.0
92.00	1662.0
93.00	2343.0
94.00	5797.0
95.00	47096.0
96.10	2885.0
97.00	83.0
104.00	218.0
105.00	63.0
105.90	248.0
107.00	51.0
109.90	50.0
114.90	123.0
115.90	279.0
116.90	408.0
117.80	215.0
118.80	288.0
127.90	158.0
130.10	200.0
130.90	57.0
134.80	81.0
136.80	168.0
141.00	695.0
141.90	93.0
142.90	743.0
144.00	95.0
144.80	94.0
145.90	51.0
147.90	98.0
149.90	111.0
155.00	81.0
157.00	132.0
172.00	568.0
173.00	484.0
174.00	45968.0
175.00	3391.0
176.00	43464.0
177.00	2977.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604

m/z	Abundance
40.00	138.0
44.00	221.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604

m/z	Abundance
36.00	760.0
37.00	4534.0
38.00	3857.0
39.00	1477.0
39.90	228.0
44.00	671.0
45.00	671.0
45.80	64.0
47.10	938.0
48.00	393.0
49.00	3323.0
50.00	14844.0
51.10	4894.0
52.00	214.0
54.90	237.0
56.10	1522.0
57.10	2213.0
58.00	81.0
60.00	784.0
61.00	3538.0
62.00	3519.0
63.00	3133.0
63.90	307.0
64.90	371.0
67.00	210.0
68.00	7495.0
69.00	7776.0
70.00	584.0
71.90	394.0
73.00	3364.0
74.00	13302.0
75.00	35776.0
76.00	3271.0
77.00	335.0
77.90	209.0
78.90	3310.0
79.90	1014.0
81.00	3261.0
81.90	740.0
83.10	100.0
86.00	144.0
87.00	2900.0
88.00	2938.0
90.90	246.0
92.00	2006.0
93.00	3206.0
94.00	8348.0
95.00	67360.0
96.00	4503.0
96.90	133.0
104.00	358.0
105.10	63.0
106.00	383.0
107.00	106.0
110.80	73.0
112.90	89.0
114.70	76.0
115.90	323.0
116.80	518.0
117.90	245.0
118.90	528.0
124.10	56.0
127.80	200.0
128.80	64.0
129.90	292.0
130.90	147.0
135.00	125.0
137.00	100.0
141.00	658.0
141.90	123.0
142.90	985.0
143.90	160.0
144.90	171.0
146.00	132.0
146.90	69.0
147.90	148.0
149.90	66.0
153.10	58.0
154.90	134.0
157.00	177.0
161.10	111.0
171.20	98.0
172.00	504.0
173.10	594.0
174.00	48312.0
175.00	3939.0
176.00	46080.0
177.00	2942.0
177.80	103.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604