

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030698.D
 Acq On : 19 Aug 2022 12:05
 Operator : JC/MD
 Sample : N4267-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ZG7

Quant Time: Aug 20 02:13:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 20 02:12:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	299151	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	269231	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	125528	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	93019	48.420	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.840%
7) Chloroethane-d5	1.666	69	72508	53.540	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.080%
11) 1,1-Dichloroethene-d2	2.307	63	142800	39.296	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.600%
21) 2-Butanone-d5	4.459	46	177749	99.859	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.860%
24) Chloroform-d	5.062	84	203636	51.493	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.980%
26) 1,2-Dichloroethane-d4	5.958	65	128792	47.963	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.920%
32) Benzene-d6	5.977	84	422442	54.777	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.560%
36) 1,2-Dichloropropane-d6	7.312	67	139035	55.567	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	111.140%
41) Toluene-d8	8.653	98	378649	52.088	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.180%
43) trans-1,3-Dichloroprop...	8.952	79	59162	47.529	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.060%
47) 2-Hexanone-d5	9.385	63	133596	104.750	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.750%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	186553	56.755	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	113.520%
66) 1,2-Dichlorobenzene-d4	12.323	152	137841	56.614	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.220%
Target Compounds						
					Qvalue	
13) Acetone	2.386	43	3027	2.320	ug/L	92
22) 2-Butanone	4.574	43	10971	5.331	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030698.D
Acq On : 19 Aug 2022 12:05
Operator : JC/MD
Sample : N4267-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZG7

Quant Time: Aug 20 02:13:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 20 02:12:38 2022
Response via : Initial Calibration




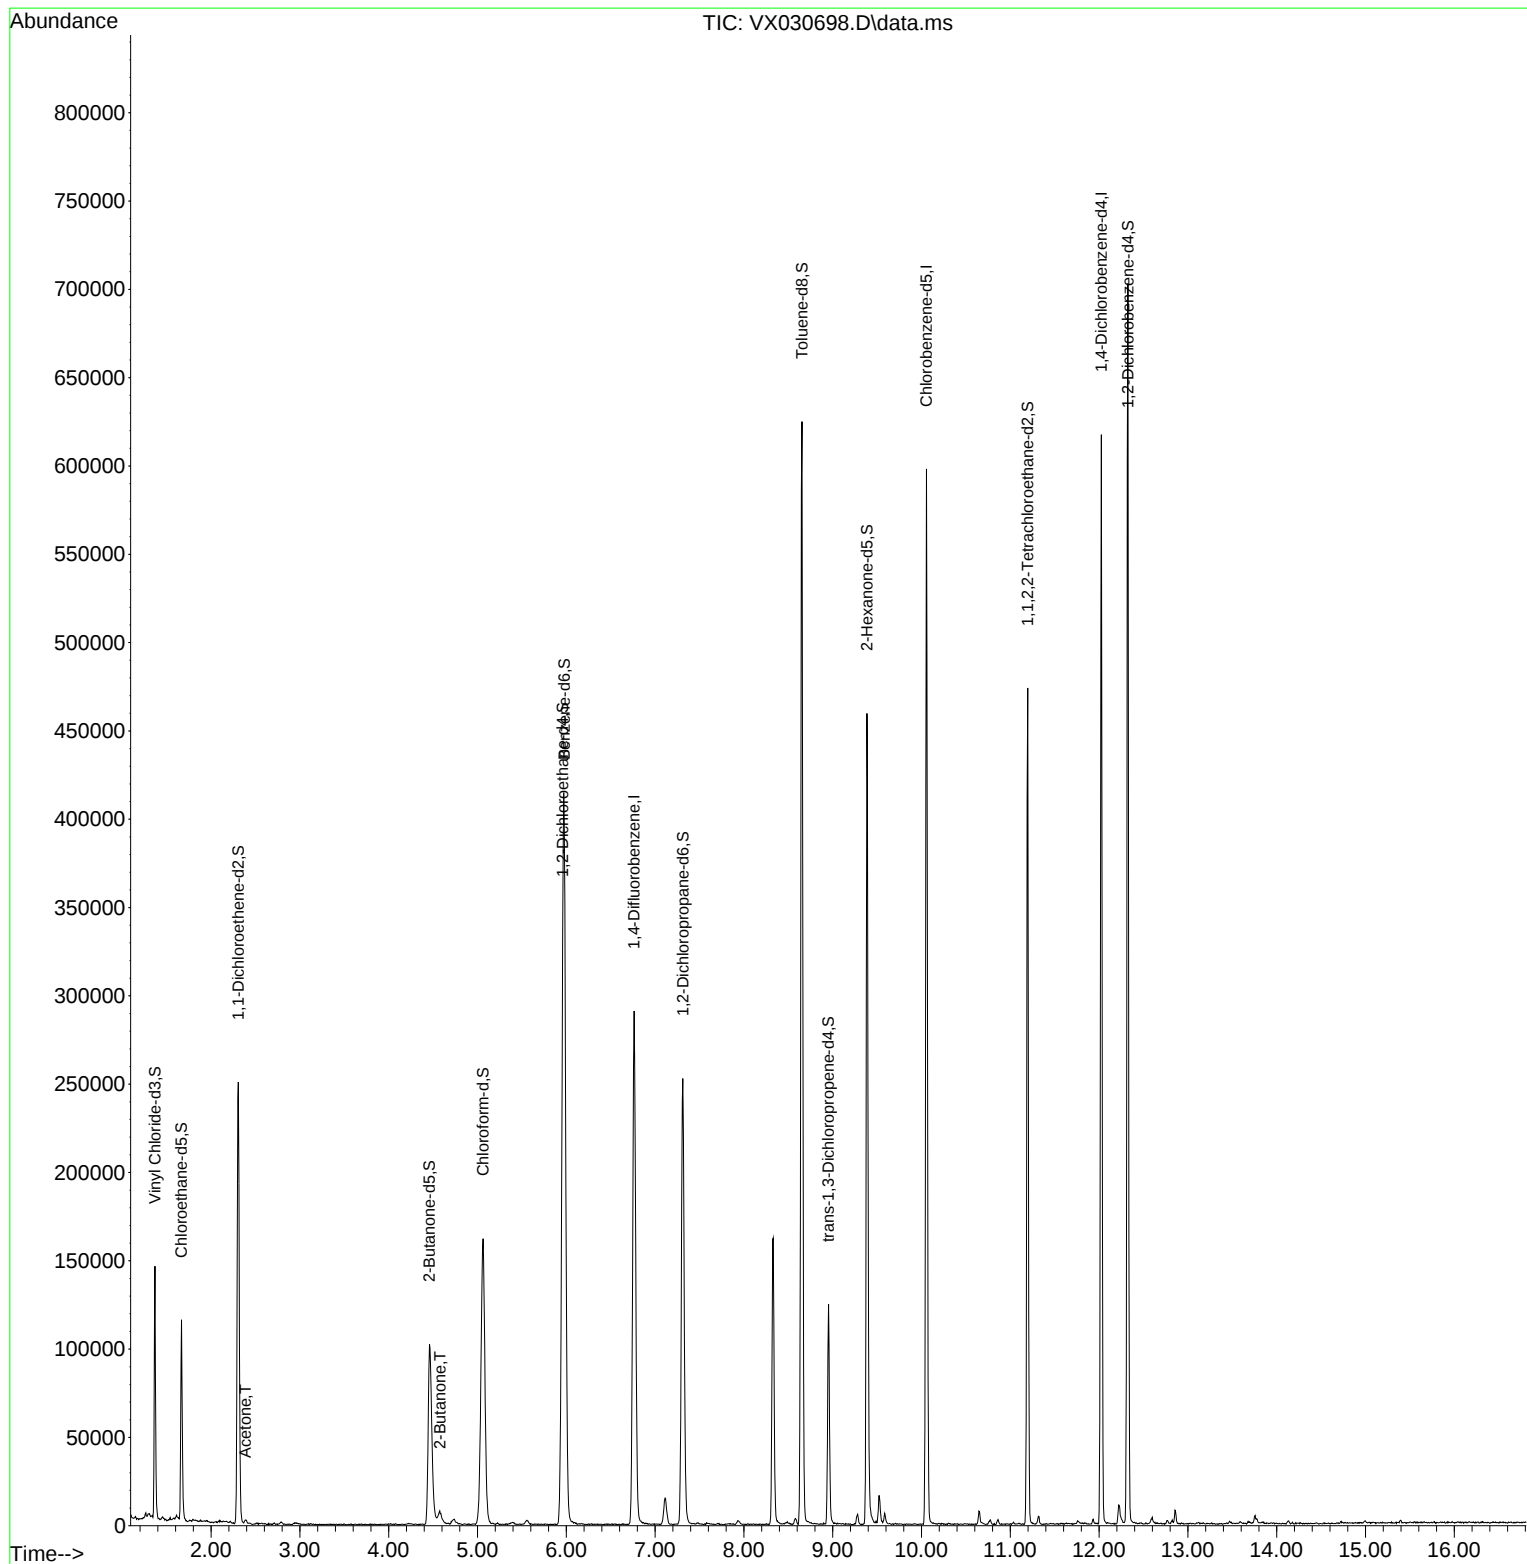


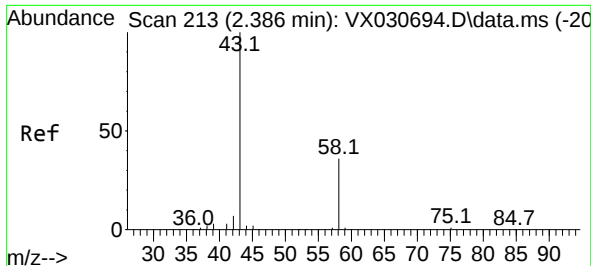

#13
Acetone
Concen: 2.320 ug/L
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX030698.D
Acq: 19 Aug 2022 12:05

Instrument :
MSVOA_X
ClientSampleId :
C0ZG7

Tgt Ion: 43 Resp: 3027
Ion Ratio Lower Upper
43 100
58 24.8 0.0 57.8

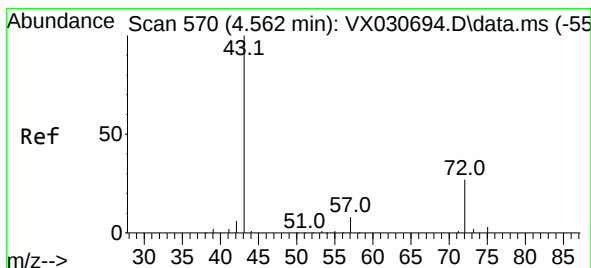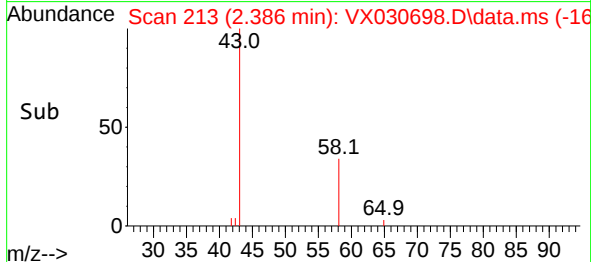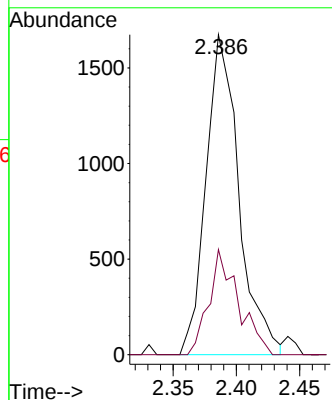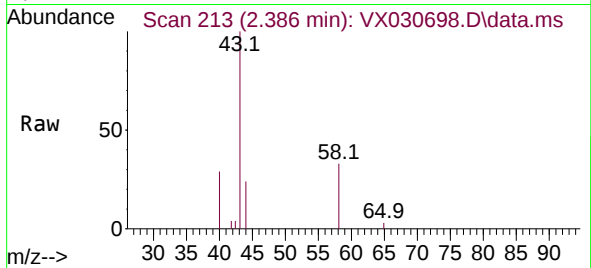

#22
2-Butanone
Concen: 5.331 ug/L
RT: 4.574 min Scan# 572
Delta R.T. 0.012 min
Lab File: VX030698.D
Acq: 19 Aug 2022 12:05

Tgt Ion: 43 Resp: 10971
Ion Ratio Lower Upper
43 100
72 31.0 11.7 35.1

