

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030695.D
 Acq On : 19 Aug 2022 10:42
 Operator : JC/MD
 Sample : VX0819WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK692

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030695.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rVB	152634	165017	13.16%	1.711%
2	1.666	91	95	105	rVB	115906	147191	11.74%	1.526%
3	2.307	194	200	210	rVB	278527	421912	33.64%	4.374%
4	2.508	230	233	238	rBV2	1475	2493	0.20%	0.026%
5	2.642	253	255	258	rBV2	429	368	0.03%	0.004%
6	2.788	273	279	287	rBV	14540	26985	2.15%	0.280%
7	2.947	297	305	312	rBV2	4810	10896	0.87%	0.113%
8	3.239	352	353	357	rBV2	436	512	0.04%	0.005%
9	3.361	371	373	374	rBV2	324	302	0.02%	0.003%
10	3.422	382	383	386	rBV2	453	345	0.03%	0.004%
11	3.562	403	406	411	rVB2	406	628	0.05%	0.007%
12	3.666	421	423	424	rBV	572	387	0.03%	0.004%
13	3.879	457	458	462	rVB	361	402	0.03%	0.004%
14	3.916	462	464	465	rBV	435	306	0.02%	0.003%
15	3.971	471	473	476	rBV2	292	353	0.03%	0.004%
16	4.166	502	505	507	rBV2	439	455	0.04%	0.005%
17	4.221	513	514	518	rVB2	392	404	0.03%	0.004%
18	4.276	521	523	526	rBV2	372	306	0.02%	0.003%
19	4.355	532	536	539	rVB	490	694	0.06%	0.007%
20	4.392	539	542	543	rBV2	417	440	0.04%	0.005%
21	4.459	545	553	564	rBV	107009	307238	24.50%	3.185%
22	4.843	612	616	618	rBV	388	624	0.05%	0.006%
23	4.873	618	621	624	rVB3	442	606	0.05%	0.006%
24	4.983	636	639	640	rBV2	421	495	0.04%	0.005%
25	5.062	640	652	671	rBV	164242	517076	41.23%	5.360%
26	5.282	687	688	691	rVB	352	314	0.03%	0.003%
27	5.330	691	696	699	rBV	494	685	0.05%	0.007%
28	5.373	699	703	704	rBV3	1914	2163	0.17%	0.022%
29	5.550	726	732	743	rVV2	4088	11294	0.90%	0.117%
30	5.647	746	748	750	rBV2	419	355	0.03%	0.004%
31	5.666	750	751	755	rBV3	502	463	0.04%	0.005%
32	5.757	765	766	770	rBV	591	568	0.05%	0.006%
33	5.971	788	801	818	rBV2	427858	1254241	100.00%	13.002%
34	6.227	840	843	844	rBV3	403	425	0.03%	0.004%
35	6.440	876	878	879	rBV	358	309	0.02%	0.003%
36	6.659	912	914	918	rBV	380	447	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030695.D
 Acq On : 19 Aug 2022 10:42
 Operator : JC/MD
 Sample : VX0819WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK692

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.763	922	931	944	rBV2	303770	732157	58.37%	7.590%
38	6.885	949	951	953	rVB	618	374	0.03%	0.004%
39	7.111	978	988	1001	rBV3	13811	32153	2.56%	0.333%
40	7.202	1001	1003	1008	rVB	743	940	0.07%	0.010%
41	7.312	1011	1021	1037	rBV	264147	578241	46.10%	5.994%
42	7.452	1042	1044	1045	rVB2	723	399	0.03%	0.004%
43	7.476	1045	1048	1053	rBV3	949	1580	0.13%	0.016%
44	7.635	1070	1074	1076	rBV2	451	673	0.05%	0.007%
45	7.879	1111	1114	1115	rBV2	333	330	0.03%	0.003%
46	7.903	1116	1118	1119	rBV	375	303	0.02%	0.003%
47	7.940	1119	1124	1127	rVB4	1326	2566	0.20%	0.027%
48	8.116	1151	1153	1156	rBV2	529	462	0.04%	0.005%
49	8.232	1169	1172	1175	rBV2	268	376	0.03%	0.004%
50	8.324	1181	1187	1198	rBV	173676	290490	23.16%	3.011%
51	8.482	1208	1213	1217	rVB4	1469	2061	0.16%	0.021%
52	8.562	1224	1226	1229	rBV2	441	478	0.04%	0.005%
53	8.647	1234	1240	1250	rBV	632148	1007542	80.33%	10.445%
54	8.818	1266	1268	1271	rVB3	561	674	0.05%	0.007%
55	8.915	1281	1284	1285	rBV	484	432	0.03%	0.004%
56	8.952	1285	1290	1300	rVV	124421	186829	14.90%	1.937%
57	9.080	1309	1311	1312	rVB2	625	337	0.03%	0.003%
58	9.104	1313	1315	1318	rVB2	513	416	0.03%	0.004%
59	9.244	1335	1338	1340	rBV2	376	481	0.04%	0.005%
60	9.275	1340	1343	1349	rVB4	1878	2679	0.21%	0.028%
61	9.317	1349	1350	1353	rBV2	357	389	0.03%	0.004%
62	9.385	1356	1361	1374	rVV	496376	692219	55.19%	7.176%
63	9.702	1410	1413	1419	rVB4	2207	2967	0.24%	0.031%
64	9.750	1419	1421	1424	rBV2	552	417	0.03%	0.004%
65	10.055	1465	1471	1485	rVV	612027	839232	66.91%	8.700%
66	10.195	1491	1494	1499	rBV3	1698	2234	0.18%	0.023%
67	10.238	1499	1501	1503	rVB2	599	419	0.03%	0.004%
68	10.305	1508	1512	1515	rVV2	1361	1509	0.12%	0.016%
69	10.494	1542	1543	1545	rBV2	358	357	0.03%	0.004%
70	10.512	1545	1546	1548	rVB	513	336	0.03%	0.003%
71	10.586	1557	1558	1561	rVB2	483	304	0.02%	0.003%
72	10.653	1565	1569	1574	rVB3	1502	2779	0.22%	0.029%
73	10.823	1593	1597	1599	rBV2	454	653	0.05%	0.007%
74	10.964	1618	1620	1625	rVB3	1154	1482	0.12%	0.015%
75	11.012	1625	1628	1632	rVB	545	423	0.03%	0.004%
76	11.049	1632	1634	1637	rBV2	333	414	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030695.D
 Acq On : 19 Aug 2022 10:42
 Operator : JC/MD
 Sample : VX0819WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK692

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.079	1637	1639	1643	rBV2	569	712	0.06%	0.007%
78	11.195	1652	1658	1672	rVB	500958	639242	50.97%	6.627%
79	11.305	1674	1676	1677	rBV	450	348	0.03%	0.004%
80	11.372	1685	1687	1689	rBV2	567	301	0.02%	0.003%
81	11.457	1697	1701	1703	rVB3	1159	1357	0.11%	0.014%
82	11.506	1707	1709	1711	rVB2	591	466	0.04%	0.005%
83	11.756	1747	1750	1753	rBV2	1231	1693	0.13%	0.018%
84	11.848	1764	1765	1768	rBV	325	360	0.03%	0.004%
85	11.976	1780	1786	1788	rVB2	1952	2413	0.19%	0.025%
86	12.024	1788	1794	1804	rBV	658080	815908	65.05%	8.458%
87	12.128	1809	1811	1812	rBV	554	444	0.04%	0.005%
88	12.177	1817	1819	1821	rBV2	402	478	0.04%	0.005%
89	12.244	1829	1830	1832	rVB2	737	476	0.04%	0.005%
90	12.323	1837	1843	1849	rBV	709479	896462	71.47%	9.293%
91	12.853	1928	1930	1933	rBV2	699	597	0.05%	0.006%
92	13.116	1970	1973	1976	rBV2	2840	3164	0.25%	0.033%
93	13.195	1983	1986	1989	rBV2	398	601	0.05%	0.006%
94	13.585	2047	2050	2054	rBV5	1979	2895	0.23%	0.030%
95	13.676	2063	2065	2067	rBV	386	339	0.03%	0.004%
96	13.780	2079	2082	2087	rVB3	2449	3498	0.28%	0.036%
97	13.963	2108	2112	2117	rVB3	2204	3101	0.25%	0.032%
98	14.134	2136	2140	2146	rVB2	2230	3484	0.28%	0.036%
99	14.207	2150	2152	2153	rBV	584	400	0.03%	0.004%
100	14.408	2183	2185	2188	rBV3	465	656	0.05%	0.007%




Sum of corrected areas: 9646201

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030695.D
Acq On : 19 Aug 2022 10:42
Operator : JC/MD
Sample : VX0819WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK692

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

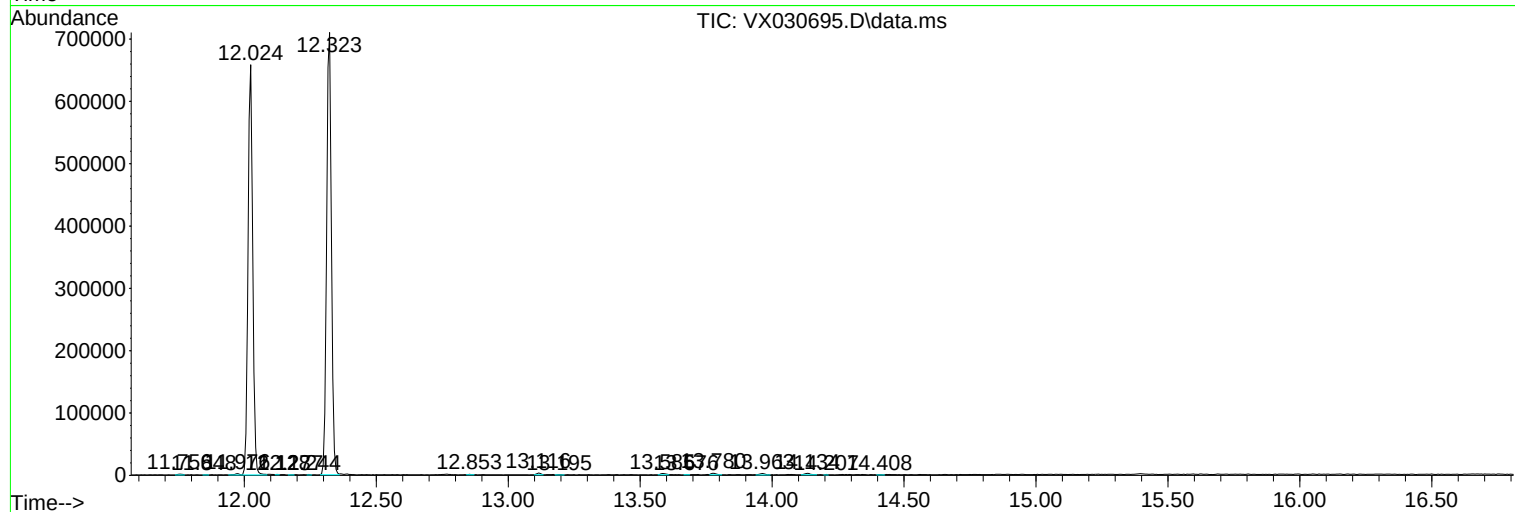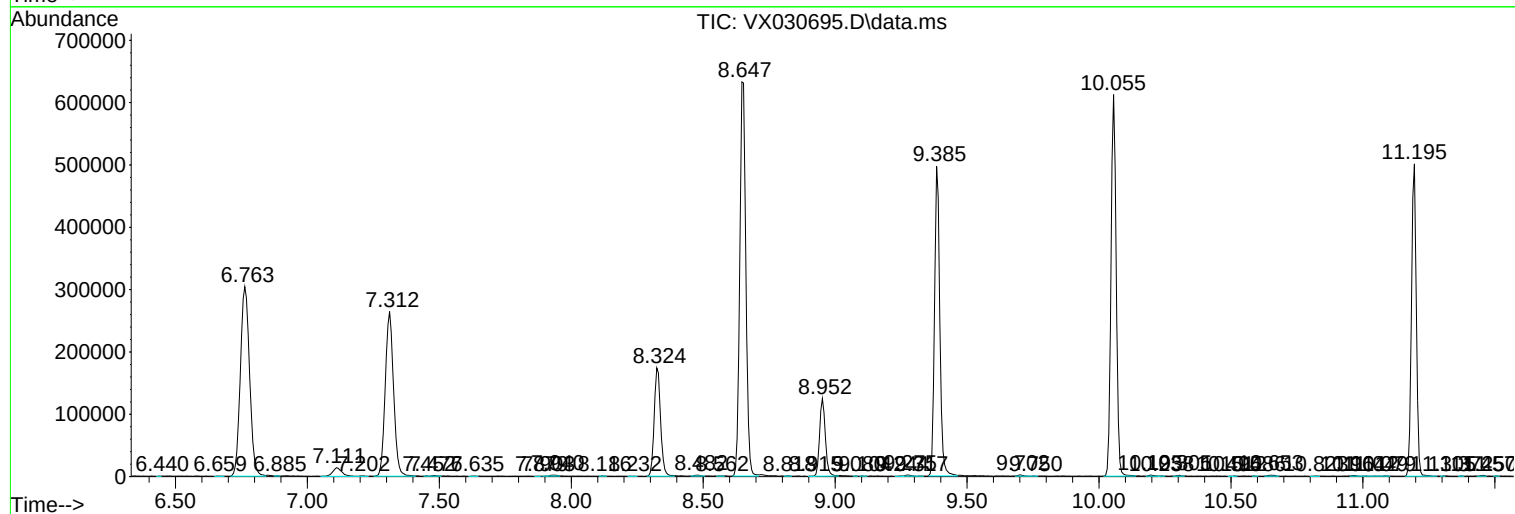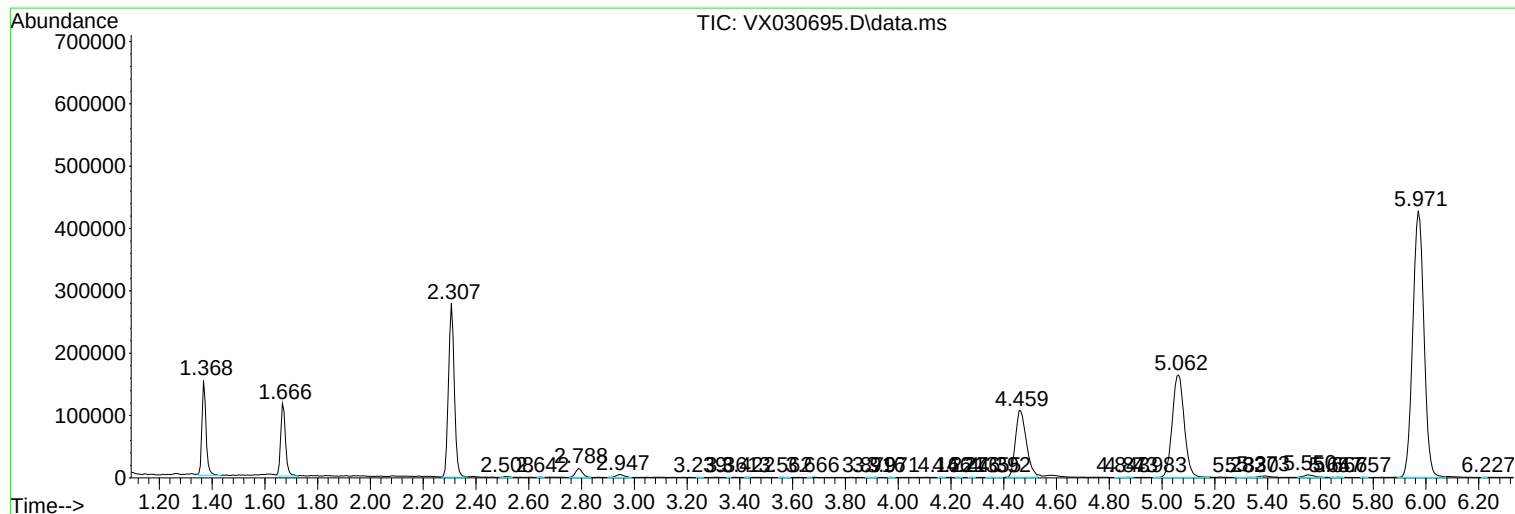

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030695.D
Acq On : 19 Aug 2022 10:42
Operator : JC/MD
Sample : VX0819WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK692

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030695.D
Acq On : 19 Aug 2022 10:42
Operator : JC/MD
Sample : VX0819WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK692

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc