

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030696.D
 Acq On : 19 Aug 2022 11:09
 Operator : JC/MD
 Sample : VX0819MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK693

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	137876	142745	11.92%	1.558%
2	1.666	91	95	103	rVB	112553	136197	11.37%	1.486%
3	2.307	194	200	210	rVB	264536	397787	33.22%	4.342%
4	2.441	221	222	225	rBV2	535	353	0.03%	0.004%
5	2.502	230	232	233	rBV	707	470	0.04%	0.005%
6	2.605	247	249	253	rBV2	387	476	0.04%	0.005%
7	2.636	253	254	255	rBV	580	289	0.02%	0.003%
8	2.788	271	279	287	rBV	13665	25999	2.17%	0.284%
9	2.843	287	288	291	rVB	641	388	0.03%	0.004%
10	2.867	291	292	296	rBV2	643	717	0.06%	0.008%
11	2.941	298	304	313	rVV2	6550	14425	1.20%	0.157%
12	3.087	324	328	331	rBV2	738	1052	0.09%	0.011%
13	3.270	356	358	360	rVB2	427	422	0.04%	0.005%
14	3.300	360	363	366	rVB	312	427	0.04%	0.005%
15	3.325	366	367	370	rBV2	270	240	0.02%	0.003%
16	3.361	370	373	374	rBV2	325	346	0.03%	0.004%
17	3.581	406	409	410	rBV	244	234	0.02%	0.003%
18	3.818	446	448	450	rBV	441	396	0.03%	0.004%
19	3.886	455	459	460	rBV2	861	802	0.07%	0.009%
20	4.056	485	487	489	rBV2	354	460	0.04%	0.005%
21	4.105	492	495	498	rVB2	351	612	0.05%	0.007%
22	4.129	498	499	500	rBV	594	229	0.02%	0.002%
23	4.337	531	533	534	rVB	388	251	0.02%	0.003%
24	4.465	541	554	568	rBV	104316	306678	25.61%	3.347%
25	4.891	621	624	627	rBV	319	372	0.03%	0.004%
26	4.958	634	635	637	rBV	308	241	0.02%	0.003%
27	5.062	639	652	671	rBV	156021	487961	40.75%	5.326%
28	5.227	674	679	681	rVB3	604	855	0.07%	0.009%
29	5.336	693	697	698	rVB3	330	320	0.03%	0.003%
30	5.361	700	701	702	rBV	645	398	0.03%	0.004%
31	5.471	718	719	722	rBV2	301	320	0.03%	0.003%
32	5.556	725	733	740	rBV3	2743	6855	0.57%	0.075%
33	5.653	748	749	751	rBV	515	415	0.03%	0.005%
34	5.812	773	775	776	rBV2	423	313	0.03%	0.003%
35	5.897	787	789	790	rBV2	485	464	0.04%	0.005%
36	5.971	790	801	817	rVV2	407641	1197482	100.00%	13.069%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030696.D
 Acq On : 19 Aug 2022 11:09
 Operator : JC/MD
 Sample : VX0819MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK693

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.190	835	837	840	rVB3	533	518	0.04%	0.006%
38	6.227	840	843	845	rBV2	303	326	0.03%	0.004%
39	6.324	855	859	861	rBV	516	401	0.03%	0.004%
40	6.342	861	862	868	rVV3	475	521	0.04%	0.006%
41	6.409	872	873	876	rBV	386	296	0.02%	0.003%
42	6.525	891	892	894	rBV	434	247	0.02%	0.003%
43	6.556	894	897	898	rBV2	530	636	0.05%	0.007%
44	6.763	918	931	947	rBV	279961	675073	56.37%	7.368%
45	6.940	959	960	966	rVB3	655	658	0.05%	0.007%
46	6.989	966	968	972	rBV2	420	480	0.04%	0.005%
47	7.117	980	989	998	rVB4	14001	32166	2.69%	0.351%
48	7.190	998	1001	1002	rBV	499	383	0.03%	0.004%
49	7.208	1002	1004	1005	rBV	493	415	0.03%	0.005%
50	7.312	1013	1021	1036	rVB	254571	558008	46.60%	6.090%
51	7.464	1044	1046	1048	rBV	560	654	0.05%	0.007%
52	7.556	1058	1061	1063	rBV2	421	644	0.05%	0.007%
53	7.598	1066	1068	1069	rBV	478	310	0.03%	0.003%
54	7.787	1097	1099	1103	rBV2	275	270	0.02%	0.003%
55	7.940	1117	1124	1131	rVB4	2162	4956	0.41%	0.054%
56	8.019	1134	1137	1139	rBV2	373	405	0.03%	0.004%
57	8.251	1173	1175	1176	rBV	489	369	0.03%	0.004%
58	8.324	1181	1187	1197	rBV	162570	276324	23.08%	3.016%
59	8.476	1209	1212	1218	rVB4	1688	3275	0.27%	0.036%
60	8.653	1234	1241	1250	rBV	625488	971469	81.13%	10.603%
61	8.891	1277	1280	1283	rBV2	579	799	0.07%	0.009%
62	8.952	1285	1290	1300	rVV	125903	183161	15.30%	1.999%
63	9.141	1318	1321	1323	rBV3	352	405	0.03%	0.004%
64	9.275	1339	1343	1349	rVB4	2109	3204	0.27%	0.035%
65	9.385	1356	1361	1374	rBV	484319	677182	56.55%	7.391%
66	9.622	1399	1400	1404	rVB2	754	519	0.04%	0.006%
67	9.708	1409	1414	1419	rVB3	2857	4224	0.35%	0.046%
68	9.823	1431	1433	1435	rVB	448	244	0.02%	0.003%
69	9.952	1453	1454	1456	rBV	367	253	0.02%	0.003%
70	10.055	1465	1471	1485	rBV	599570	787132	65.73%	8.591%
71	10.195	1491	1494	1497	rBV3	823	1259	0.11%	0.014%
72	10.305	1510	1512	1517	rVB3	980	904	0.08%	0.010%
73	10.378	1522	1524	1526	rBV	295	267	0.02%	0.003%
74	10.512	1545	1546	1547	rBV	479	299	0.02%	0.003%
75	10.640	1565	1567	1568	rBV2	410	354	0.03%	0.004%
76	10.884	1605	1607	1613	rVB2	442	638	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030696.D
 Acq On : 19 Aug 2022 11:09
 Operator : JC/MD
 Sample : VX0819MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK693

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.049	1632	1634	1635	rBV	389	319	0.03%	0.003%
78	11.116	1644	1645	1649	rVB	405	322	0.03%	0.004%
79	11.195	1652	1658	1668	rVV	470702	605433	50.56%	6.608%
80	11.390	1688	1690	1695	rBV2	377	512	0.04%	0.006%
81	11.427	1695	1696	1697	rVV	439	270	0.02%	0.003%
82	11.457	1699	1701	1704	rVV2	1286	1307	0.11%	0.014%
83	11.512	1708	1710	1713	rVB2	544	525	0.04%	0.006%
84	11.659	1732	1734	1735	rBV2	414	251	0.02%	0.003%
85	11.756	1748	1750	1752	rBV	601	421	0.04%	0.005%
86	11.976	1784	1786	1789	rVV	1095	542	0.05%	0.006%
87	12.024	1789	1794	1804	rVV	615339	751175	62.73%	8.198%
88	12.323	1837	1843	1854	rBV	701409	872563	72.87%	9.523%
89	12.762	1913	1915	1919	rVB3	1381	1733	0.14%	0.019%
90	12.969	1947	1949	1950	rBV	403	257	0.02%	0.003%
91	13.024	1956	1958	1959	rVB	511	246	0.02%	0.003%
92	13.140	1976	1977	1981	rBV2	571	590	0.05%	0.006%
93	13.353	2010	2012	2014	rBV	398	384	0.03%	0.004%
94	13.433	2023	2025	2027	rBV2	440	264	0.02%	0.003%
95	13.597	2047	2052	2056	rVV4	693	1412	0.12%	0.015%
96	14.128	2135	2139	2147	rVB4	2048	2965	0.25%	0.032%
97	14.408	2183	2185	2186	rBV2	645	482	0.04%	0.005%
98	14.640	2221	2223	2224	rVB	899	480	0.04%	0.005%
99	14.658	2224	2226	2227	rBV	626	515	0.04%	0.006%
100	15.383	2344	2345	2351	rVB3	1331	1823	0.15%	0.020%




Sum of corrected areas: 9162430

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030696.D
Acq On : 19 Aug 2022 11:09
Operator : JC/MD
Sample : VX0819MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK693

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

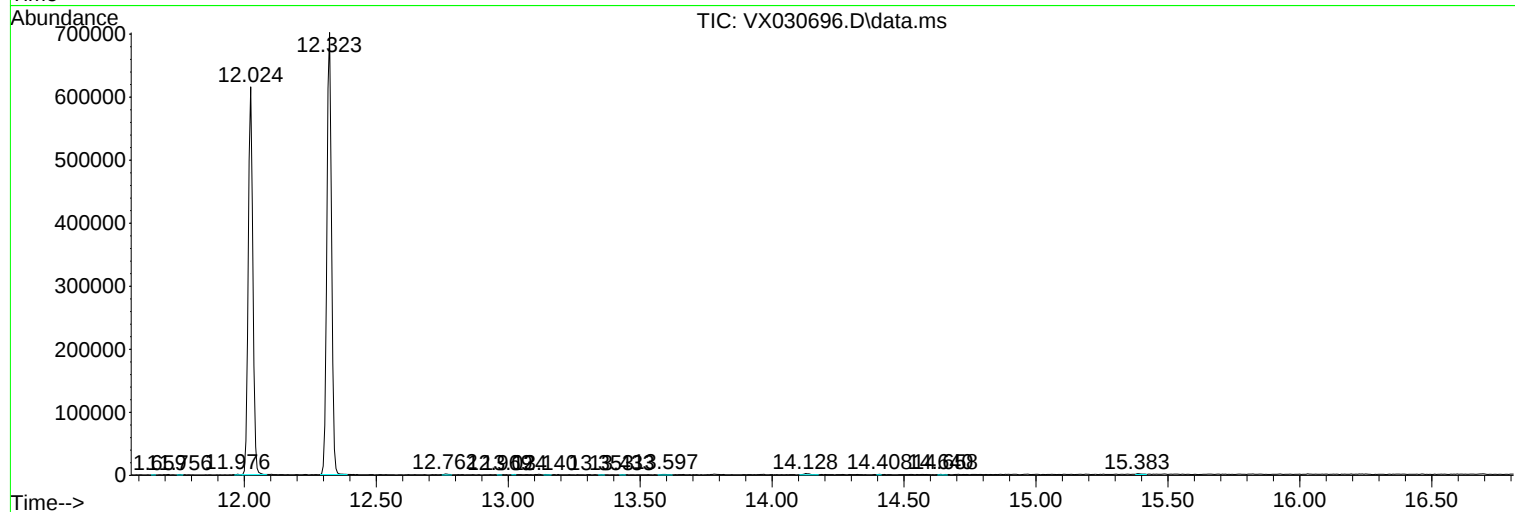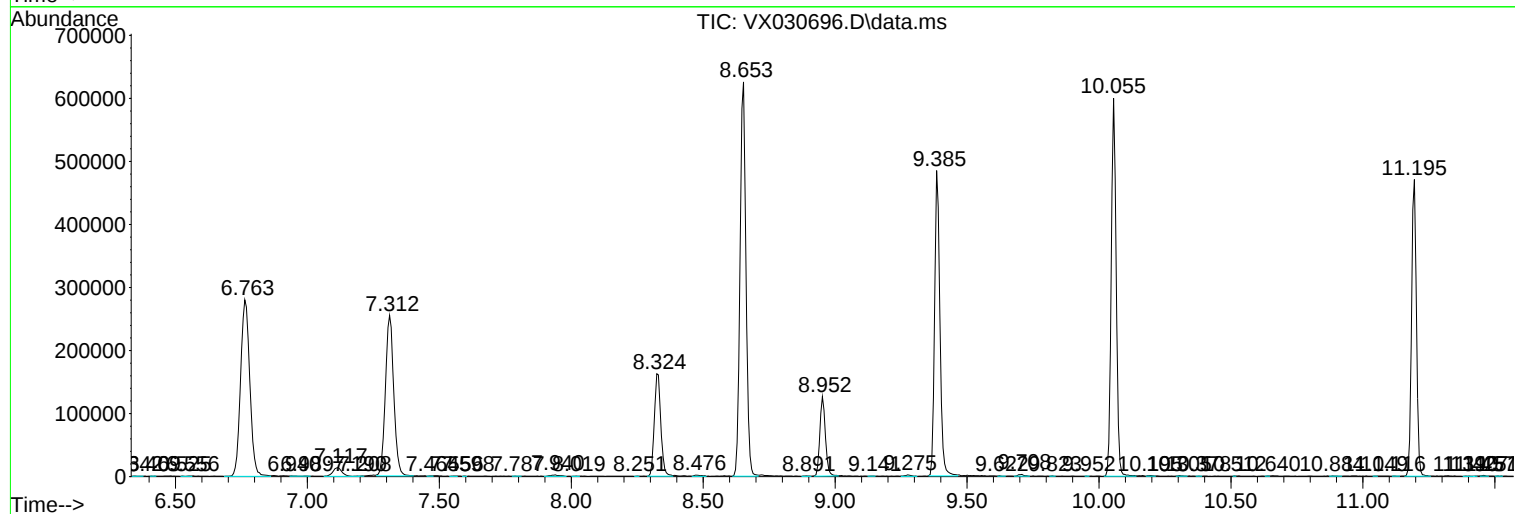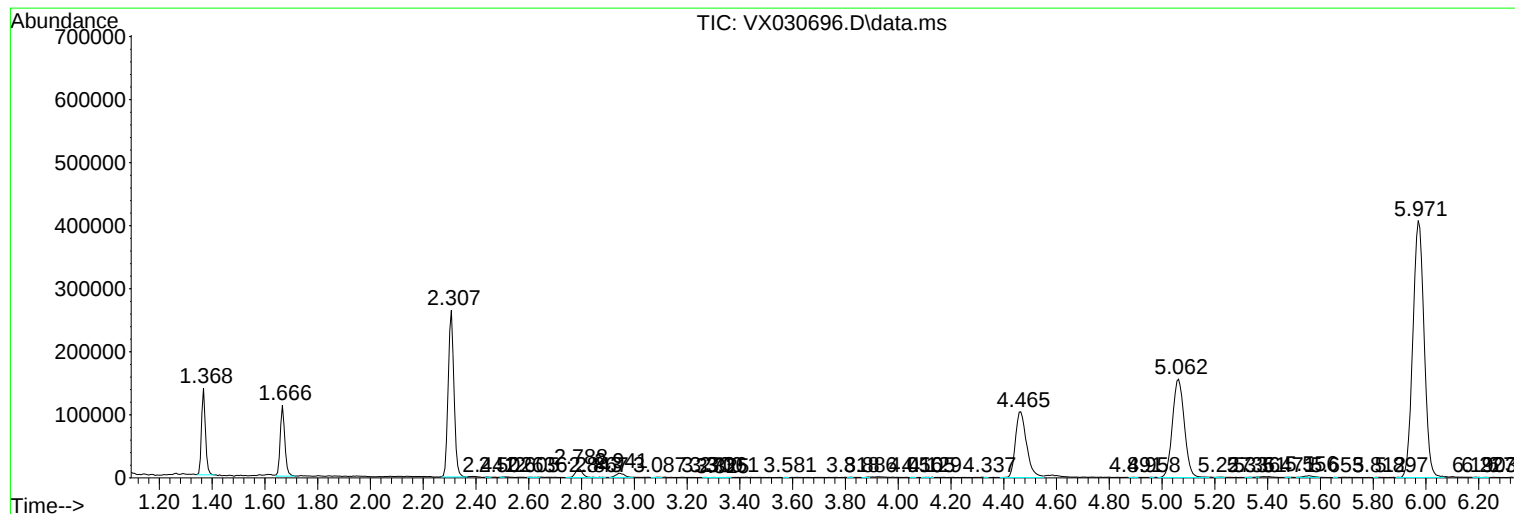

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030696.D
Acq On : 19 Aug 2022 11:09
Operator : JC/MD
Sample : VX0819MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK693

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030696.D
Acq On : 19 Aug 2022 11:09
Operator : JC/MD
Sample : VX0819MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK693

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc