

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030697.D
 Acq On : 19 Aug 2022 11:35
 Operator : JC/MD
 Sample : N4221-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	54	rVB	168970	173055	13.65%	1.685%
2	1.666	91	95	107	rVB	124545	149733	11.81%	1.458%
3	2.306	194	200	211	rVB	291188	453207	35.74%	4.414%
4	2.507	229	233	238	rBV4	923	1586	0.13%	0.015%
5	2.672	257	260	263	rBV3	654	728	0.06%	0.007%
6	2.751	271	273	275	rBV2	308	312	0.02%	0.003%
7	2.794	275	280	290	rVB4	4070	7599	0.60%	0.074%
8	2.879	290	294	296	rBV2	512	725	0.06%	0.007%
9	2.946	299	305	311	rVV	5519	10061	0.79%	0.098%
10	3.087	325	328	329	rBV3	609	672	0.05%	0.007%
11	3.324	365	367	370	rBV2	454	370	0.03%	0.004%
12	3.519	397	399	402	rVB2	499	360	0.03%	0.004%
13	3.562	402	406	407	rBV	460	360	0.03%	0.004%
14	3.599	407	412	413	rBV2	899	1116	0.09%	0.011%
15	3.672	421	424	426	rVB2	461	347	0.03%	0.003%
16	3.782	441	442	445	rBV2	403	388	0.03%	0.004%
17	3.885	457	459	461	rBV2	526	371	0.03%	0.004%
18	4.214	511	513	517	rVB2	510	596	0.05%	0.006%
19	4.263	519	521	524	rBV2	344	491	0.04%	0.005%
20	4.318	528	530	535	rBV2	380	555	0.04%	0.005%
21	4.464	545	554	570	rBV2	115914	390620	30.81%	3.804%
22	4.763	601	603	606	rVB2	344	330	0.03%	0.003%
23	4.891	622	624	625	rVV2	479	354	0.03%	0.003%
24	5.062	640	652	670	rVB2	163827	509949	40.22%	4.967%
25	5.232	677	680	684	rVB	592	779	0.06%	0.008%
26	5.385	700	705	715	rVB7	3313	8341	0.66%	0.081%
27	5.556	727	733	734	rBV3	2874	4555	0.36%	0.044%
28	5.745	761	764	765	rBV	415	347	0.03%	0.003%
29	5.793	769	772	774	rVB2	389	385	0.03%	0.004%
30	5.818	774	776	780	rBV2	443	594	0.05%	0.006%
31	5.860	780	783	784	rBV	290	362	0.03%	0.004%
32	5.970	789	801	822	rBV2	430726	1267931	100.00%	12.349%
33	6.232	842	844	848	rBV3	429	449	0.04%	0.004%
34	6.287	851	853	856	rVB	563	330	0.03%	0.003%
35	6.373	865	867	868	rBV2	659	444	0.04%	0.004%
36	6.763	922	931	945	rBV	322654	759621	59.91%	7.398%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030697.D
 Acq On : 19 Aug 2022 11:35
 Operator : JC/MD
 Sample : N4221-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.013	970	972	975	rVB2	529	469	0.04%	0.005%
38	7.128	979	991	1000	rBV3	43811	107220	8.46%	1.044%
39	7.311	1012	1021	1032	rBV	265110	572135	45.12%	5.572%
40	7.537	1056	1058	1059	rVB2	611	401	0.03%	0.004%
41	7.604	1068	1069	1071	rBV	491	299	0.02%	0.003%
42	7.787	1096	1099	1101	rVB2	309	325	0.03%	0.003%
43	7.842	1104	1108	1110	rVB2	436	526	0.04%	0.005%
44	7.927	1118	1122	1130	rBV4	1822	3889	0.31%	0.038%
45	8.043	1139	1141	1144	rBV2	368	425	0.03%	0.004%
46	8.244	1170	1174	1175	rBV2	395	542	0.04%	0.005%
47	8.329	1181	1188	1199	rBV	168864	286187	22.57%	2.787%
48	8.476	1209	1212	1215	rBV5	1528	2010	0.16%	0.020%
49	8.531	1219	1221	1224	rVB2	559	510	0.04%	0.005%
50	8.653	1234	1241	1253	rBV	646401	1015503	80.09%	9.890%
51	8.951	1284	1290	1298	rBV	124799	185534	14.63%	1.807%
52	9.079	1309	1311	1312	rVB2	654	339	0.03%	0.003%
53	9.104	1312	1315	1318	rVB2	401	472	0.04%	0.005%
54	9.274	1336	1343	1351	rBV	278699	400298	31.57%	3.899%
55	9.384	1356	1361	1373	rBV	456318	668570	52.73%	6.511%
56	9.604	1395	1397	1399	rVB2	727	635	0.05%	0.006%
57	9.622	1399	1400	1402	rBV2	451	380	0.03%	0.004%
58	9.671	1407	1408	1410	rBV	473	374	0.03%	0.004%
59	9.805	1428	1430	1432	rVV2	560	437	0.03%	0.004%
60	9.902	1443	1446	1451	rBV2	566	900	0.07%	0.009%
61	10.000	1459	1462	1463	rBV2	443	349	0.03%	0.003%
62	10.055	1465	1471	1480	rBV	659894	890944	70.27%	8.677%
63	10.201	1490	1495	1499	rVB3	629	1271	0.10%	0.012%
64	10.232	1499	1500	1501	rBV	663	359	0.03%	0.003%
65	10.299	1508	1511	1514	rBV3	723	756	0.06%	0.007%
66	10.372	1521	1523	1526	rVB2	332	329	0.03%	0.003%
67	10.634	1563	1566	1567	rBV	371	364	0.03%	0.004%
68	10.658	1567	1570	1571	rVV3	489	488	0.04%	0.005%
69	10.677	1571	1573	1575	rVV2	478	354	0.03%	0.003%
70	10.695	1575	1576	1578	rVB2	519	355	0.03%	0.003%
71	10.786	1589	1591	1594	rVB2	326	345	0.03%	0.003%
72	10.963	1618	1620	1622	rVB2	383	322	0.03%	0.003%
73	11.091	1638	1641	1644	rBV3	527	729	0.06%	0.007%
74	11.134	1646	1648	1652	rBV	317	329	0.03%	0.003%
75	11.195	1652	1658	1668	rBV	483829	629154	49.62%	6.128%
76	11.317	1676	1678	1682	rVB3	993	1156	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030697.D
 Acq On : 19 Aug 2022 11:35
 Operator : JC/MD
 Sample : N4221-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.433	1694	1697	1698	rBV	389	325	0.03%	0.003%
78	11.603	1721	1725	1727	rBV2	273	404	0.03%	0.004%
79	11.634	1728	1730	1731	rVV	572	366	0.03%	0.004%
80	11.652	1731	1733	1739	rVB	369	505	0.04%	0.005%
81	11.750	1748	1749	1754	rVB2	916	860	0.07%	0.008%
82	11.829	1761	1762	1765	rBV	496	468	0.04%	0.005%
83	12.024	1789	1794	1803	rBV	681188	838830	66.16%	8.170%
84	12.109	1806	1808	1809	rBV2	577	480	0.04%	0.005%
85	12.323	1837	1843	1851	rBV	704628	886739	69.94%	8.636%
86	12.560	1878	1882	1883	rBV	565	737	0.06%	0.007%
87	12.737	1910	1911	1912	rVV	700	365	0.03%	0.004%
88	12.762	1912	1915	1921	rVB3	1156	1803	0.14%	0.018%
89	13.060	1963	1964	1967	rVB	573	373	0.03%	0.004%
90	13.383	2016	2017	2020	rBV2	277	313	0.02%	0.003%
91	13.627	2055	2057	2059	rBV	363	472	0.04%	0.005%
92	13.780	2079	2082	2086	rBV4	810	1358	0.11%	0.013%
93	13.822	2086	2089	2092	rBV2	665	965	0.08%	0.009%
94	14.133	2137	2140	2144	rVB	2882	3184	0.25%	0.031%
95	14.517	2202	2203	2204	rBV	938	392	0.03%	0.004%
96	14.889	2262	2264	2266	rBV	577	434	0.03%	0.004%
97	14.920	2266	2269	2271	rBV	1302	1125	0.09%	0.011%
98	15.743	2402	2404	2407	rBV3	781	734	0.06%	0.007%
99	16.200	2477	2479	2481	rBV2	1110	930	0.07%	0.009%
100	16.352	2502	2504	2508	rVB3	1263	1385	0.11%	0.013%




Sum of corrected areas: 10267554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030697.D
Acq On : 19 Aug 2022 11:35
Operator : JC/MD
Sample : N4221-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

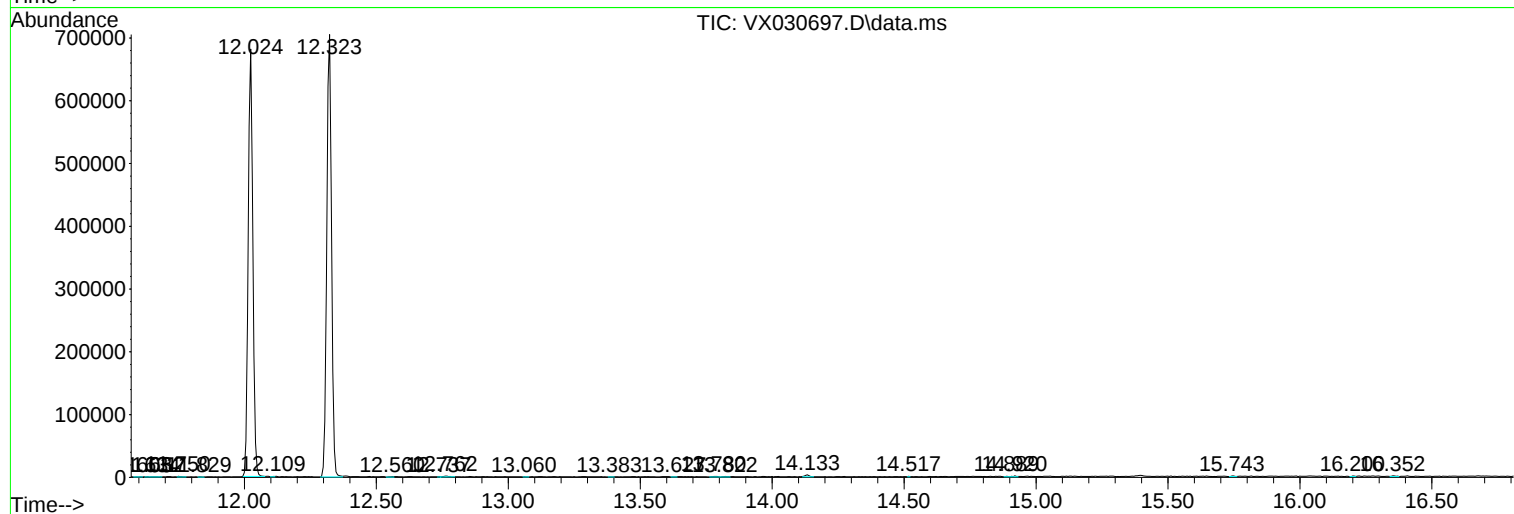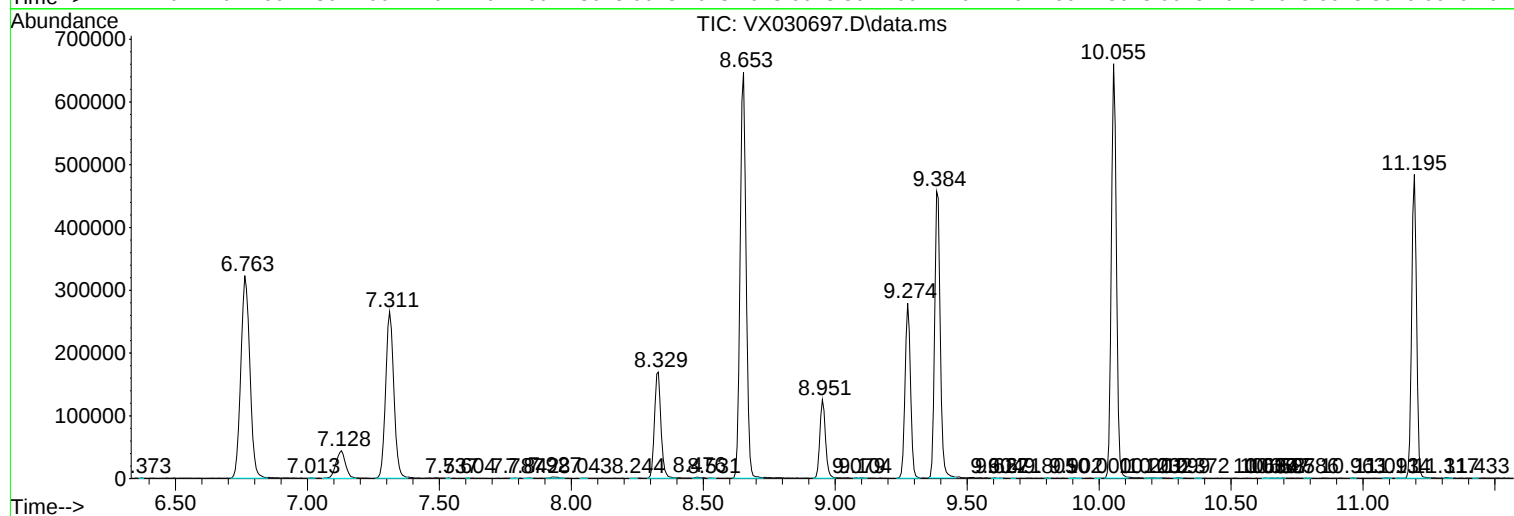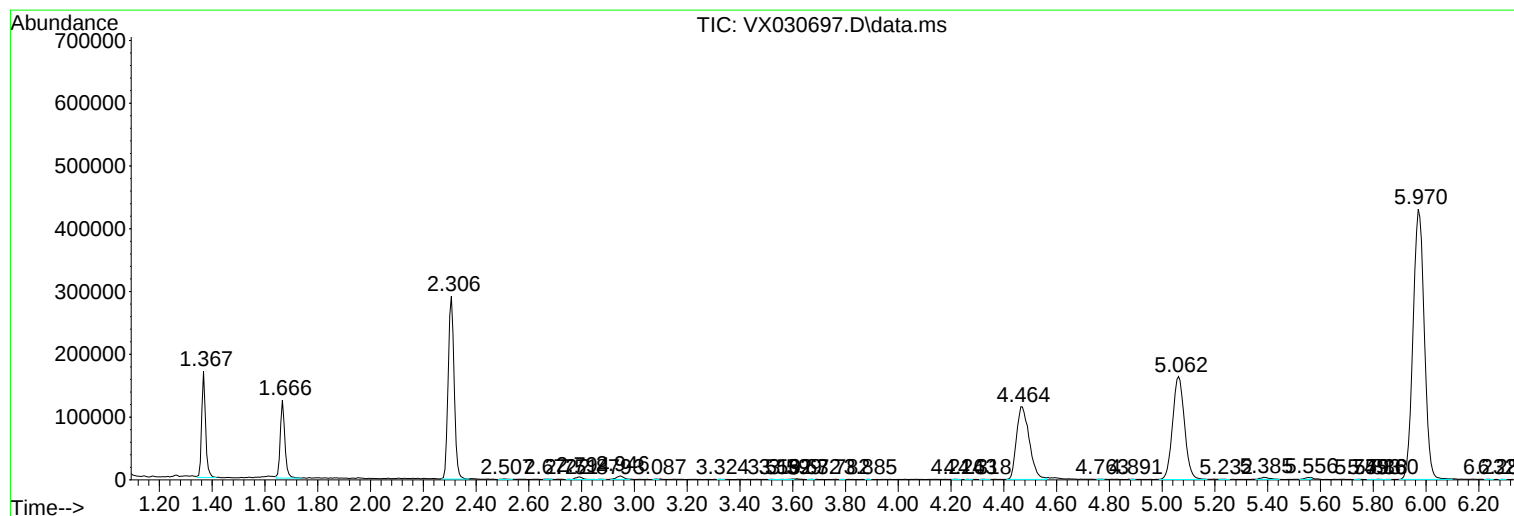

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030697.D
Acq On : 19 Aug 2022 11:35
Operator : JC/MD
Sample : N4221-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030697.D
Acq On : 19 Aug 2022 11:35
Operator : JC/MD
Sample : N4221-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc