

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030698.D
 Acq On : 19 Aug 2022 12:05
 Operator : JC/MD
 Sample : N4267-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ZG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rVB	142879	147611	12.21%	1.597%
2	1.666	91	95	106	rVB	114249	140112	11.59%	1.516%
3	2.307	193	200	210	rBV	250119	400562	33.13%	4.334%
4	2.386	210	213	219	rVB2	1949	3368	0.28%	0.036%
5	2.508	232	233	235	rBV	576	449	0.04%	0.005%
6	2.666	257	259	261	rVV	413	377	0.03%	0.004%
7	2.709	263	266	269	rVV3	970	1066	0.09%	0.012%
8	2.788	275	279	284	rVB4	1405	2423	0.20%	0.026%
9	2.928	299	302	303	rBV2	696	650	0.05%	0.007%
10	3.081	324	327	328	rBV2	337	398	0.03%	0.004%
11	3.117	331	333	337	rVV2	608	785	0.06%	0.008%
12	3.178	341	343	345	rBV2	396	365	0.03%	0.004%
13	3.453	386	388	389	rBV2	391	365	0.03%	0.004%
14	3.495	392	395	399	rVB	593	680	0.06%	0.007%
15	3.575	406	408	410	rVB	570	400	0.03%	0.004%
16	3.697	424	428	429	rVB2	371	413	0.03%	0.004%
17	3.959	469	471	476	rVV2	326	587	0.05%	0.006%
18	3.995	476	477	480	rVV2	436	423	0.03%	0.005%
19	4.020	480	481	484	rVV2	575	460	0.04%	0.005%
20	4.075	488	490	494	rBV2	710	824	0.07%	0.009%
21	4.300	524	527	532	rVB2	391	559	0.05%	0.006%
22	4.459	545	553	566	rBV	101758	290698	24.04%	3.145%
23	4.739	592	599	606	rVV4	2802	7750	0.64%	0.084%
24	4.794	606	608	614	rVB3	694	1013	0.08%	0.011%
25	4.855	614	618	622	rBV4	498	767	0.06%	0.008%
26	4.952	630	634	638	rBV2	296	620	0.05%	0.007%
27	5.062	638	652	667	rBV	161838	503520	41.65%	5.448%
28	5.227	675	679	682	rBV2	998	1521	0.13%	0.016%
29	5.349	697	699	700	rBV2	393	374	0.03%	0.004%
30	5.373	700	703	704	rBV2	813	843	0.07%	0.009%
31	5.556	727	733	739	rVB5	2317	5426	0.45%	0.059%
32	5.757	765	766	770	rBV2	389	432	0.04%	0.005%
33	5.873	782	785	786	rBV	425	446	0.04%	0.005%
34	5.971	788	801	816	rBV2	414464	1209060	100.00%	13.082%
35	6.513	888	890	893	rVB2	481	407	0.03%	0.004%
36	6.635	907	910	911	rBV	456	373	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030698.D
 Acq On : 19 Aug 2022 12:05
 Operator : JC/MD
 Sample : N4267-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ZG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.763	921	931	947	rBV	290670	682967	56.49%	7.390%
38	6.897	951	953	955	rVV2	530	398	0.03%	0.004%
39	7.111	980	988	998	rBV4	14970	35176	2.91%	0.381%
40	7.312	1011	1021	1038	rBV	252382	550483	45.53%	5.956%
41	7.482	1045	1049	1051	rVB3	726	900	0.07%	0.010%
42	7.580	1063	1065	1068	rBV2	1129	1443	0.12%	0.016%
43	7.708	1081	1086	1089	rVB4	739	1192	0.10%	0.013%
44	7.934	1118	1123	1131	rVB6	2097	4797	0.40%	0.052%
45	8.043	1138	1141	1144	rBV2	446	521	0.04%	0.006%
46	8.330	1180	1188	1202	rBV	162415	277604	22.96%	3.004%
47	8.488	1209	1214	1216	rBV4	1280	1762	0.15%	0.019%
48	8.580	1224	1229	1234	rBV6	3368	5999	0.50%	0.065%
49	8.653	1234	1241	1251	rBV	624367	974455	80.60%	10.544%
50	8.897	1280	1281	1284	rBV2	748	504	0.04%	0.005%
51	8.952	1284	1290	1300	rVV	124389	179125	14.82%	1.938%
52	9.055	1305	1307	1309	rBV	594	471	0.04%	0.005%
53	9.196	1328	1330	1332	rVB2	444	380	0.03%	0.004%
54	9.244	1335	1338	1339	rBV2	612	512	0.04%	0.006%
55	9.281	1339	1344	1351	rVB4	5693	8795	0.73%	0.095%
56	9.385	1356	1361	1376	rVV	458963	651207	53.86%	7.046%
57	9.488	1376	1378	1379	rVV	1587	1087	0.09%	0.012%
58	9.525	1379	1384	1390	rVV2	15947	26248	2.17%	0.284%
59	9.586	1390	1394	1400	rVB	5883	8218	0.68%	0.089%
60	9.830	1432	1434	1436	rBV2	338	368	0.03%	0.004%
61	10.055	1465	1471	1482	rBV	597595	781628	64.65%	8.457%
62	10.195	1491	1494	1496	rBV3	524	542	0.04%	0.006%
63	10.305	1510	1512	1514	rBV	690	737	0.06%	0.008%
64	10.445	1530	1535	1538	rBV2	348	565	0.05%	0.006%
65	10.647	1563	1568	1580	rVV2	7524	12321	1.02%	0.133%
66	10.775	1584	1589	1595	rVB4	2754	4795	0.40%	0.052%
67	10.860	1598	1603	1608	rBV4	2857	4074	0.34%	0.044%
68	11.000	1624	1626	1628	rVB2	489	366	0.03%	0.004%
69	11.037	1628	1632	1635	rBV4	1341	1803	0.15%	0.020%
70	11.140	1646	1649	1651	rVB2	486	434	0.04%	0.005%
71	11.195	1652	1658	1671	rVV	473561	593569	49.09%	6.422%
72	11.317	1674	1678	1683	rVV3	4546	6536	0.54%	0.071%
73	11.372	1686	1687	1690	rBV	317	357	0.03%	0.004%
74	11.579	1718	1721	1726	rVB3	597	867	0.07%	0.009%
75	11.634	1726	1730	1731	rBV3	725	810	0.07%	0.009%
76	11.726	1741	1745	1746	rBV2	572	680	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030698.D
 Acq On : 19 Aug 2022 12:05
 Operator : JC/MD
 Sample : N4267-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ZG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.756	1748	1750	1755	rVV3	1646	2344	0.19%	0.025%
78	11.933	1776	1779	1782	rBV2	2755	3031	0.25%	0.033%
79	12.024	1789	1794	1804	rBV	616467	762708	63.08%	8.253%
80	12.219	1822	1826	1836	rVV	10752	21518	1.78%	0.233%
81	12.323	1837	1843	1853	rVB	701719	864311	71.49%	9.352%
82	12.457	1863	1865	1867	rBV2	490	447	0.04%	0.005%
83	12.524	1875	1876	1879	rVB2	637	482	0.04%	0.005%
84	12.597	1883	1888	1892	rVV5	3656	5975	0.49%	0.065%
85	12.646	1894	1896	1899	rBV2	526	513	0.04%	0.006%
86	12.732	1906	1910	1911	rVB2	457	481	0.04%	0.005%
87	12.768	1913	1916	1919	rVV4	2042	2718	0.22%	0.029%
88	12.823	1922	1925	1927	rVV2	2133	2323	0.19%	0.025%
89	12.853	1927	1930	1935	rVB3	7513	9572	0.79%	0.104%
90	12.927	1940	1942	1944	rBV2	676	643	0.05%	0.007%
91	13.170	1981	1982	1986	rVB2	716	495	0.04%	0.005%
92	13.353	2011	2012	2014	rBV	471	392	0.03%	0.004%
93	13.469	2028	2031	2033	rBV3	1356	1501	0.12%	0.016%
94	13.676	2063	2065	2066	rBV2	1142	673	0.06%	0.007%
95	13.756	2074	2078	2080	rBV3	4162	5247	0.43%	0.057%
96	14.134	2135	2140	2143	rBV3	1773	3052	0.25%	0.033%
97	14.176	2145	2147	2150	rVB	1056	879	0.07%	0.010%
98	14.304	2166	2168	2169	rBV	554	400	0.03%	0.004%
99	14.524	2202	2204	2206	rBV	522	486	0.04%	0.005%
100	14.725	2234	2237	2238	rBV2	1141	1015	0.08%	0.011%


Sum of corrected areas: 9242029

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030698.D
Acq On : 19 Aug 2022 12:05
Operator : JC/MD
Sample : N4267-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

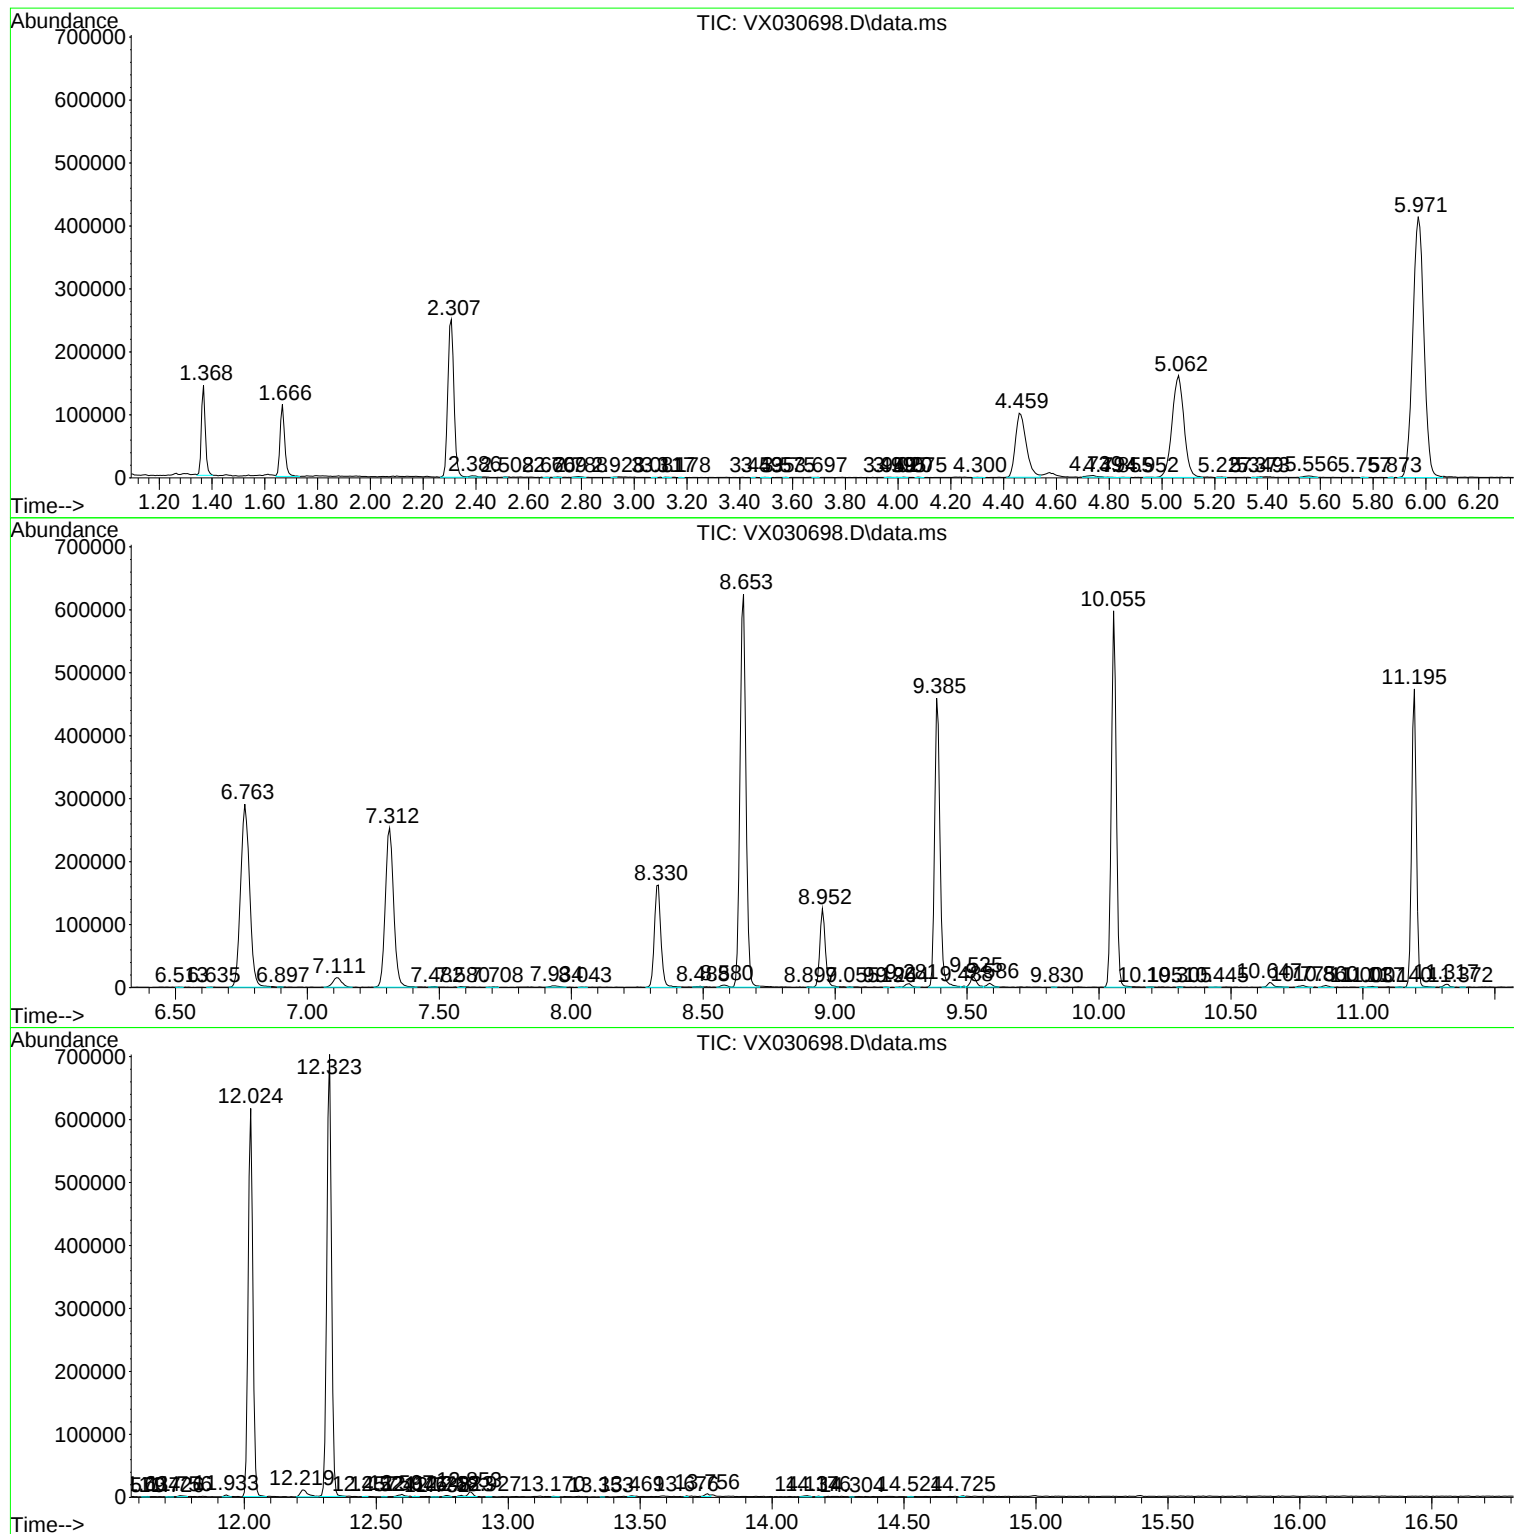

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030698.D
Acq On : 19 Aug 2022 12:05
Operator : JC/MD
Sample : N4267-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030698.D
Acq On : 19 Aug 2022 12:05
Operator : JC/MD
Sample : N4267-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc