

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030699.D
 Acq On : 19 Aug 2022 12:29
 Operator : JC/MD
 Sample : N4231-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	12	rVB	5734	4371	0.32%	0.035%
2	1.368	42	46	55	rVB2	192189	203828	14.84%	1.627%
3	1.666	91	95	105	rVB	116296	145998	10.63%	1.165%
4	2.313	194	201	219	rVB3	464209	871737	63.49%	6.958%
5	2.788	272	279	286	rBV3	4446	9080	0.66%	0.072%
6	2.867	290	292	297	rVB2	495	641	0.05%	0.005%
7	2.947	297	305	313	rBV	11808	27634	2.01%	0.221%
8	3.093	326	329	335	rVV5	1387	2668	0.19%	0.021%
9	3.239	352	353	355	rVB2	654	321	0.02%	0.003%
10	3.373	373	375	378	rVV	430	437	0.03%	0.003%
11	3.398	378	379	381	rVB	565	336	0.02%	0.003%
12	3.495	391	395	396	rBV2	392	462	0.03%	0.004%
13	3.538	401	402	405	rVV2	316	331	0.02%	0.003%
14	3.617	405	415	425	rVB	7075	17893	1.30%	0.143%
15	3.690	425	427	431	rBV2	371	626	0.05%	0.005%
16	3.727	431	433	437	rVB2	508	691	0.05%	0.006%
17	3.782	439	442	443	rVV2	490	520	0.04%	0.004%
18	3.977	471	474	476	rBV2	387	515	0.04%	0.004%
19	4.068	487	489	492	rVB	454	417	0.03%	0.003%
20	4.270	520	522	525	rBV2	321	371	0.03%	0.003%
21	4.306	525	528	530	rVB2	396	395	0.03%	0.003%
22	4.361	534	537	539	rBV2	623	608	0.04%	0.005%
23	4.404	539	544	545	rBV	344	517	0.04%	0.004%
24	4.483	545	557	569	rBV2	153025	564627	41.12%	4.507%
25	4.812	609	611	615	rBV2	343	429	0.03%	0.003%
26	5.062	639	652	672	rBV	160083	497615	36.24%	3.972%
27	5.227	677	679	680	rVB2	624	370	0.03%	0.003%
28	5.385	695	705	717	rVV5	12909	40944	2.98%	0.327%
29	5.544	726	731	733	rBV2	2773	3729	0.27%	0.030%
30	5.641	745	747	750	rVB2	687	483	0.04%	0.004%
31	5.708	756	758	760	rVB2	495	302	0.02%	0.002%
32	5.794	769	772	774	rBV2	397	486	0.04%	0.004%
33	5.855	781	782	784	rVB	586	318	0.02%	0.003%
34	5.873	784	785	787	rBV	568	331	0.02%	0.003%
35	5.977	789	802	818	rBV2	414067	1221833	88.99%	9.753%
36	6.190	836	837	841	rVB3	400	363	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030699.D
 Acq On : 19 Aug 2022 12:29
 Operator : JC/MD
 Sample : N4231-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.263	847	849	851	rBV	267	345	0.03%	0.003%
38	6.379	866	868	871	rVB	750	543	0.04%	0.004%
39	6.544	894	895	900	rVB3	480	708	0.05%	0.006%
40	6.653	911	913	915	rVB2	523	470	0.03%	0.004%
41	6.769	921	932	950	rBV	289641	706287	51.44%	5.637%
42	7.037	974	976	978	rBV	420	303	0.02%	0.002%
43	7.129	981	991	1005	rBV	547297	1201160	87.48%	9.588%
44	7.312	1013	1021	1032	rBV	249427	551157	40.14%	4.399%
45	7.470	1045	1047	1049	rVV3	551	542	0.04%	0.004%
46	7.549	1058	1060	1061	rVB	454	298	0.02%	0.002%
47	7.690	1077	1083	1094	rBV4	2199	5698	0.41%	0.045%
48	7.866	1108	1112	1113	rBV2	405	415	0.03%	0.003%
49	7.934	1118	1123	1128	rBV5	1798	3606	0.26%	0.029%
50	8.013	1134	1136	1137	rBV	413	418	0.03%	0.003%
51	8.086	1146	1148	1150	rBV2	390	346	0.03%	0.003%
52	8.330	1181	1188	1200	rBV	165538	273690	19.93%	2.185%
53	8.488	1208	1214	1218	rBV3	1670	2663	0.19%	0.021%
54	8.519	1218	1219	1222	rBV3	532	341	0.02%	0.003%
55	8.653	1234	1241	1253	rBV	635394	974194	70.95%	7.776%
56	8.952	1285	1290	1298	rBV	123007	176929	12.89%	1.412%
57	9.153	1321	1323	1327	rBV2	622	779	0.06%	0.006%
58	9.275	1336	1343	1356	rVV	958821	1373055	100.00%	10.960%
59	9.384	1356	1361	1379	rVB	454853	662931	48.28%	5.291%
60	9.744	1417	1420	1423	rVB2	1015	910	0.07%	0.007%
61	9.817	1429	1432	1434	rBV2	405	468	0.03%	0.004%
62	9.964	1454	1456	1457	rVB2	420	304	0.02%	0.002%
63	10.055	1466	1471	1480	rBV	624285	813306	59.23%	6.492%
64	10.238	1499	1501	1504	rVB2	676	634	0.05%	0.005%
65	10.275	1504	1507	1510	rVB2	587	582	0.04%	0.005%
66	10.299	1510	1511	1512	rBV	851	419	0.03%	0.003%
67	10.317	1512	1514	1516	rVB	589	380	0.03%	0.003%
68	10.378	1521	1524	1529	rVB3	1403	1613	0.12%	0.013%
69	10.494	1541	1543	1546	rVB	638	506	0.04%	0.004%
70	10.555	1550	1553	1556	rBV2	376	510	0.04%	0.004%
71	10.720	1578	1580	1582	rVB2	486	365	0.03%	0.003%
72	10.750	1582	1585	1589	rBV2	515	963	0.07%	0.008%
73	10.878	1603	1606	1609	rBV2	480	460	0.03%	0.004%
74	11.012	1627	1628	1630	rBV	427	330	0.02%	0.003%
75	11.091	1636	1641	1644	rBV4	1093	1924	0.14%	0.015%
76	11.195	1652	1658	1666	rBV	473941	598175	43.57%	4.775%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030699.D
 Acq On : 19 Aug 2022 12:29
 Operator : JC/MD
 Sample : N4231-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.415	1692	1694	1695	rBV	481	355	0.03%	0.003%
78	11.671	1733	1736	1737	rBV	429	364	0.03%	0.003%
79	11.750	1748	1749	1751	rBV	591	460	0.03%	0.004%
80	11.799	1755	1757	1759	rVB2	733	572	0.04%	0.005%
81	11.975	1783	1786	1789	rBV2	438	584	0.04%	0.005%
82	12.024	1789	1794	1803	rBV	612411	737616	53.72%	5.888%
83	12.232	1824	1828	1832	rBV4	1993	3480	0.25%	0.028%
84	12.323	1837	1843	1854	rVV	630969	791649	57.66%	6.319%
85	12.463	1865	1866	1869	rVB3	563	376	0.03%	0.003%
86	12.597	1886	1888	1891	rBV2	457	471	0.03%	0.004%
87	12.768	1913	1916	1920	rVB3	957	1400	0.10%	0.011%
88	13.164	1979	1981	1983	rBV	358	298	0.02%	0.002%
89	13.347	2009	2011	2013	rBV2	653	563	0.04%	0.004%
90	13.573	2045	2048	2050	rBV2	431	437	0.03%	0.003%
91	13.591	2050	2051	2054	rVB2	568	394	0.03%	0.003%
92	13.774	2079	2081	2082	rBV2	510	489	0.04%	0.004%
93	13.993	2115	2117	2118	rBV	494	299	0.02%	0.002%
94	14.134	2135	2140	2143	rBV2	2425	3306	0.24%	0.026%
95	14.402	2181	2184	2186	rBV3	719	906	0.07%	0.007%
96	14.597	2214	2216	2218	rBV2	480	447	0.03%	0.004%
97	14.719	2234	2236	2238	rBV3	631	635	0.05%	0.005%
98	15.237	2320	2321	2323	rBV2	714	626	0.05%	0.005%
99	16.243	2483	2486	2489	rBV3	833	841	0.06%	0.007%
100	16.310	2495	2497	2501	rBV3	759	867	0.06%	0.007%




Sum of corrected areas: 12528389

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030699.D
Acq On : 19 Aug 2022 12:29
Operator : JC/MD
Sample : N4231-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

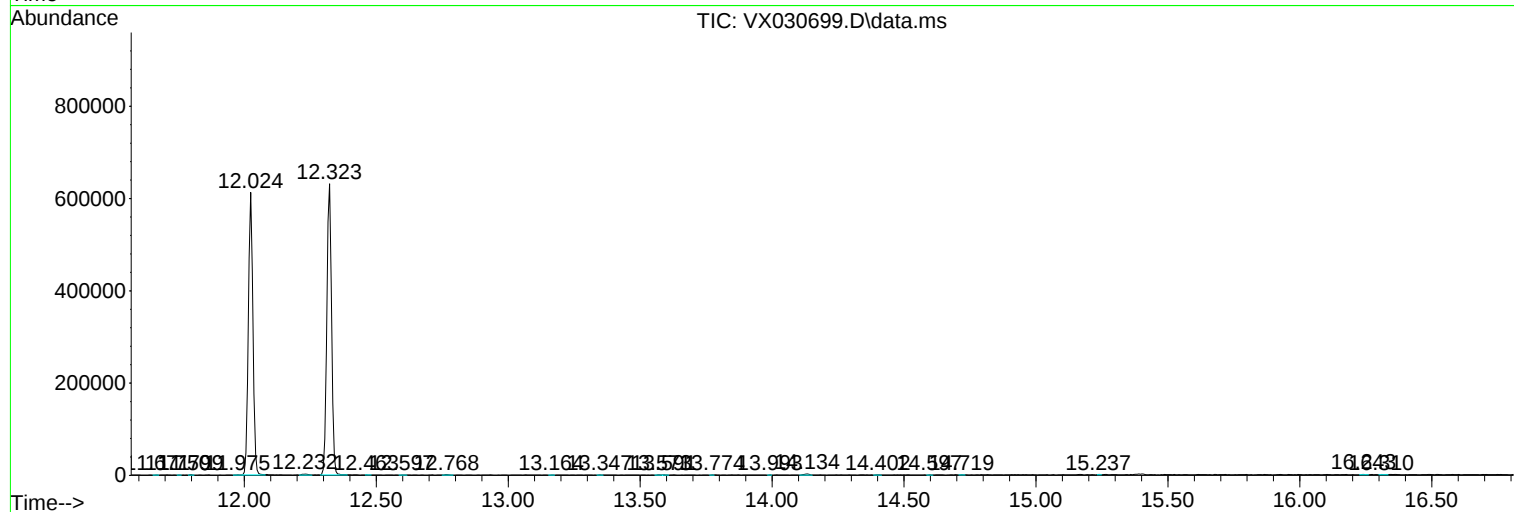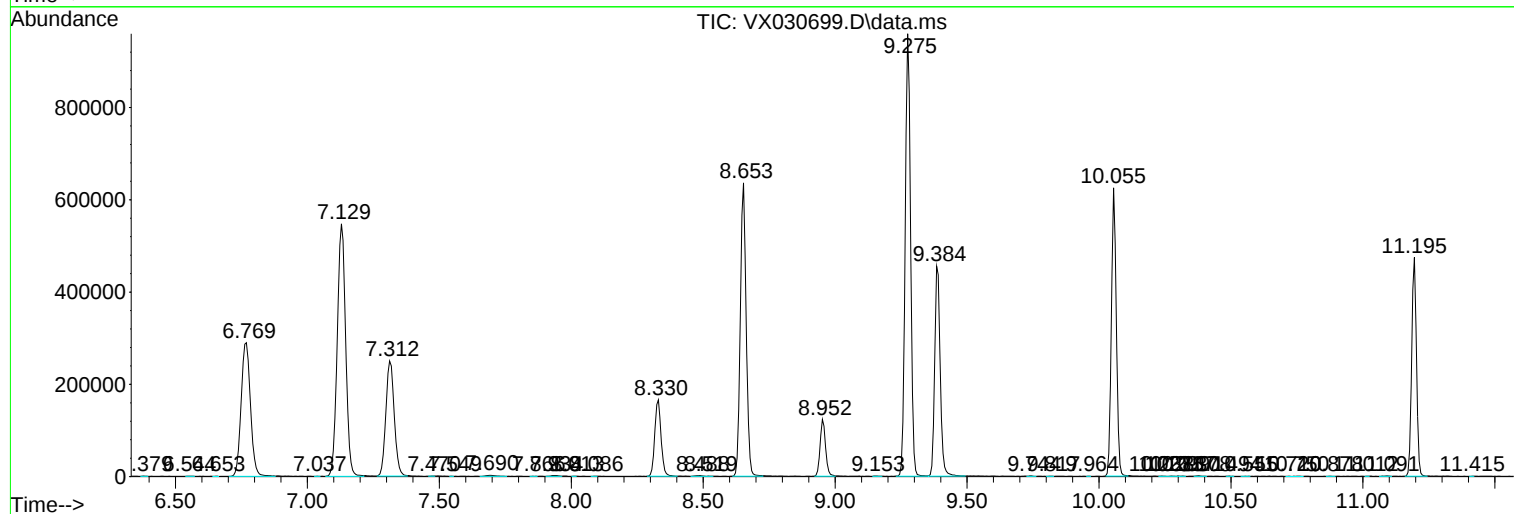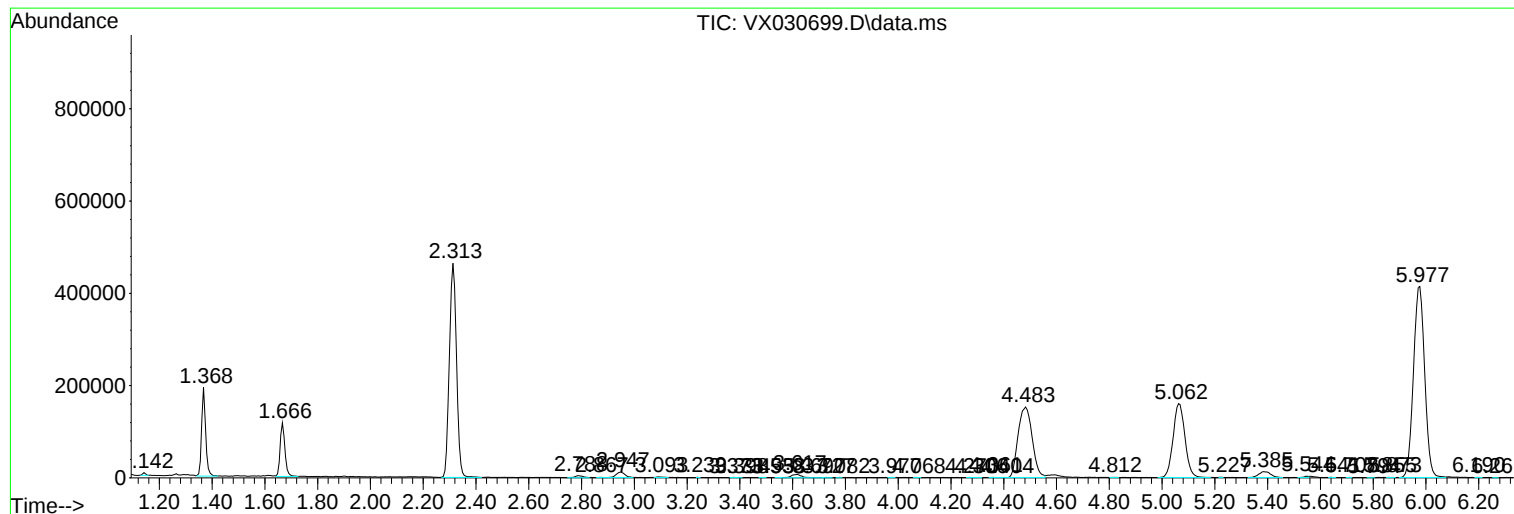

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030699.D
Acq On : 19 Aug 2022 12:29
Operator : JC/MD
Sample : N4231-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030699.D
Acq On : 19 Aug 2022 12:29
Operator : JC/MD
Sample : N4231-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc