

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030700.D
 Acq On : 19 Aug 2022 12:52
 Operator : JC/MD
 Sample : N4231-07DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	13	rVB2	8247	8332	0.66%	0.072%
2	1.367	42	46	53	rVB2	231973	256594	20.34%	2.211%
3	1.666	91	95	106	rVB	125514	152941	12.12%	1.318%
4	2.032	153	155	157	rBV2	1269	919	0.07%	0.008%
5	2.312	194	201	213	rBV3	476074	891693	70.68%	7.682%
6	2.654	252	257	259	rBV3	661	1076	0.09%	0.009%
7	2.678	259	261	263	rVV3	382	266	0.02%	0.002%
8	2.794	274	280	286	rBV3	4221	7950	0.63%	0.068%
9	2.946	297	305	318	rVB	11351	27610	2.19%	0.238%
10	3.038	318	320	322	rBV2	284	289	0.02%	0.002%
11	3.056	322	323	325	rBV	430	403	0.03%	0.003%
12	3.093	326	329	336	rVB4	1660	3031	0.24%	0.026%
13	3.227	350	351	353	rBV	320	260	0.02%	0.002%
14	3.263	356	357	359	rBV	565	400	0.03%	0.003%
15	3.337	366	369	371	rBV2	445	461	0.04%	0.004%
16	3.379	374	376	379	rBV2	289	264	0.02%	0.002%
17	3.428	382	384	387	rVV2	323	300	0.02%	0.003%
18	3.550	401	404	405	rBV	305	243	0.02%	0.002%
19	3.611	405	414	423	rBV2	9980	23705	1.88%	0.204%
20	3.678	423	425	426	rVB	498	241	0.02%	0.002%
21	3.922	463	465	470	rVB2	538	675	0.05%	0.006%
22	3.977	470	474	475	rBV2	519	691	0.05%	0.006%
23	3.995	475	477	481	rBV2	510	628	0.05%	0.005%
24	4.483	545	557	569	rBV2	179360	658437	52.19%	5.673%
25	4.916	627	628	631	rVB2	402	302	0.02%	0.003%
26	5.062	640	652	671	rBV2	163184	508634	40.32%	4.382%
27	5.214	674	677	678	rBV	528	400	0.03%	0.003%
28	5.562	726	734	744	rVB4	2963	7775	0.62%	0.067%
29	5.635	744	746	749	rBV	564	519	0.04%	0.004%
30	5.659	749	750	752	rVB2	478	257	0.02%	0.002%
31	5.678	752	753	755	rBV2	378	343	0.03%	0.003%
32	5.726	759	761	764	rBV	364	300	0.02%	0.003%
33	5.976	789	802	816	rBV2	430595	1261524	100.00%	10.868%
34	6.263	847	849	850	rBV	633	378	0.03%	0.003%
35	6.306	854	856	859	rBV	398	285	0.02%	0.002%
36	6.385	863	869	870	rBV4	994	1648	0.13%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030700.D
 Acq On : 19 Aug 2022 12:52
 Operator : JC/MD
 Sample : N4231-07DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.543	893	895	896	rVV	506	274	0.02%	0.002%
38	6.769	921	932	947	rBV	306825	738252	58.52%	6.360%
39	7.025	972	974	975	rBV	472	286	0.02%	0.002%
40	7.129	981	991	1005	rBV	387343	850090	67.39%	7.324%
41	7.312	1011	1021	1033	rBV	265953	576393	45.69%	4.966%
42	7.683	1077	1082	1089	rVV3	4576	10296	0.82%	0.089%
43	7.763	1093	1095	1097	rBV2	348	341	0.03%	0.003%
44	7.787	1097	1099	1103	rVB2	534	474	0.04%	0.004%
45	7.933	1119	1123	1130	rBV4	2561	4428	0.35%	0.038%
46	7.988	1130	1132	1134	rBV2	281	257	0.02%	0.002%
47	8.007	1134	1135	1140	rVB	427	375	0.03%	0.003%
48	8.128	1154	1155	1156	rBV	441	236	0.02%	0.002%
49	8.220	1169	1170	1171	rBV	462	286	0.02%	0.002%
50	8.330	1181	1188	1199	rVV	171159	282528	22.40%	2.434%
51	8.482	1209	1213	1220	rVB5	1817	2821	0.22%	0.024%
52	8.653	1234	1241	1251	rBV	663715	1016757	80.60%	8.759%
53	8.848	1269	1273	1280	rVB6	916	2177	0.17%	0.019%
54	8.951	1285	1290	1299	rBV	125159	184205	14.60%	1.587%
55	9.067	1307	1309	1311	rVB2	445	251	0.02%	0.002%
56	9.275	1333	1343	1352	rBV	175436	257441	20.41%	2.218%
57	9.390	1356	1362	1375	rBV	467625	690593	54.74%	5.950%
58	9.579	1391	1393	1394	rBV2	425	324	0.03%	0.003%
59	9.622	1399	1400	1405	rVB2	648	476	0.04%	0.004%
60	9.988	1459	1460	1463	rVB2	398	335	0.03%	0.003%
61	10.055	1465	1471	1479	rBV	639155	859824	68.16%	7.407%
62	10.281	1504	1508	1509	rVB2	392	408	0.03%	0.004%
63	10.311	1509	1513	1514	rBV	617	823	0.07%	0.007%
64	10.378	1518	1524	1528	rVV3	1929	2692	0.21%	0.023%
65	10.451	1534	1536	1538	rBV2	566	626	0.05%	0.005%
66	10.512	1545	1546	1550	rVB2	454	480	0.04%	0.004%
67	10.591	1557	1559	1562	rBV2	473	585	0.05%	0.005%
68	10.659	1569	1570	1573	rBV	813	662	0.05%	0.006%
69	10.811	1593	1595	1598	rBV2	241	316	0.03%	0.003%
70	10.866	1602	1604	1609	rVB2	482	550	0.04%	0.005%
71	10.969	1618	1621	1625	rVB2	599	979	0.08%	0.008%
72	11.000	1625	1626	1627	rBV	504	258	0.02%	0.002%
73	11.195	1652	1658	1665	rBV	482459	620132	49.16%	5.343%
74	11.427	1694	1696	1697	rBV	498	441	0.03%	0.004%
75	11.475	1702	1704	1707	rBV2	397	603	0.05%	0.005%
76	11.683	1736	1738	1740	rBV2	311	344	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030700.D
 Acq On : 19 Aug 2022 12:52
 Operator : JC/MD
 Sample : N4231-07DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.707	1740	1742	1746	rVB2	386	454	0.04%	0.004%
78	11.786	1752	1755	1757	rBV	270	276	0.02%	0.002%
79	12.024	1789	1794	1803	rBV	665967	797572	63.22%	6.871%
80	12.231	1823	1828	1829	rBV2	879	1190	0.09%	0.010%
81	12.323	1837	1843	1853	rBV	704909	866309	68.67%	7.463%
82	12.518	1873	1875	1877	rBV2	327	294	0.02%	0.003%
83	12.768	1914	1916	1921	rVB3	723	688	0.05%	0.006%
84	12.945	1943	1945	1947	rVB2	495	408	0.03%	0.004%
85	12.969	1947	1949	1951	rBV	355	299	0.02%	0.003%
86	13.006	1953	1955	1956	rBV	438	332	0.03%	0.003%
87	13.024	1956	1958	1960	rBV	540	413	0.03%	0.004%
88	13.176	1981	1983	1985	rVB	442	338	0.03%	0.003%
89	13.286	1998	2001	2005	rBV2	594	964	0.08%	0.008%
90	13.676	2063	2065	2067	rBV	451	406	0.03%	0.003%
91	14.066	2128	2129	2131	rVB2	421	261	0.02%	0.002%
92	14.133	2136	2140	2144	rVB	2198	3073	0.24%	0.026%
93	14.213	2151	2153	2154	rBV	487	331	0.03%	0.003%
94	14.377	2178	2180	2182	rBV	449	329	0.03%	0.003%
95	14.774	2243	2245	2248	rBV2	776	590	0.05%	0.005%
96	14.889	2260	2264	2268	rBV3	764	1475	0.12%	0.013%
97	14.944	2272	2273	2275	rVV	622	395	0.03%	0.003%
98	15.267	2325	2326	2329	rBV3	739	582	0.05%	0.005%
99	15.359	2339	2341	2342	rBV2	1033	701	0.06%	0.006%
100	15.542	2369	2371	2373	rBV2	653	439	0.03%	0.004%




Sum of corrected areas: 11607512

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030700.D
Acq On : 19 Aug 2022 12:52
Operator : JC/MD
Sample : N4231-07DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

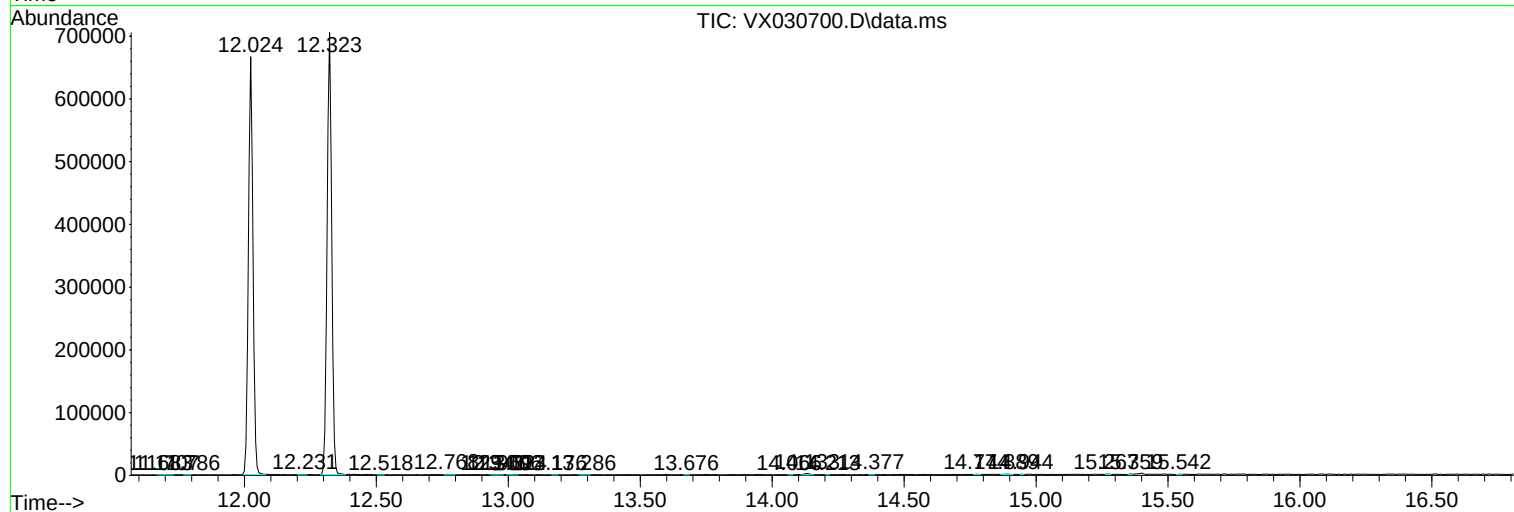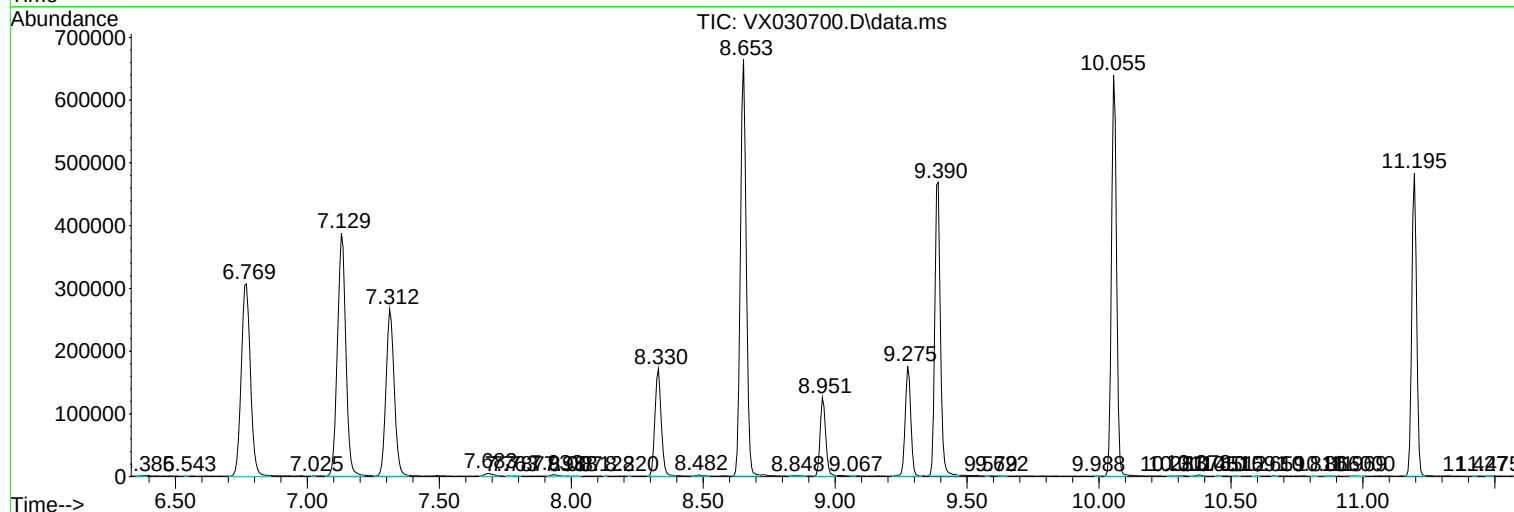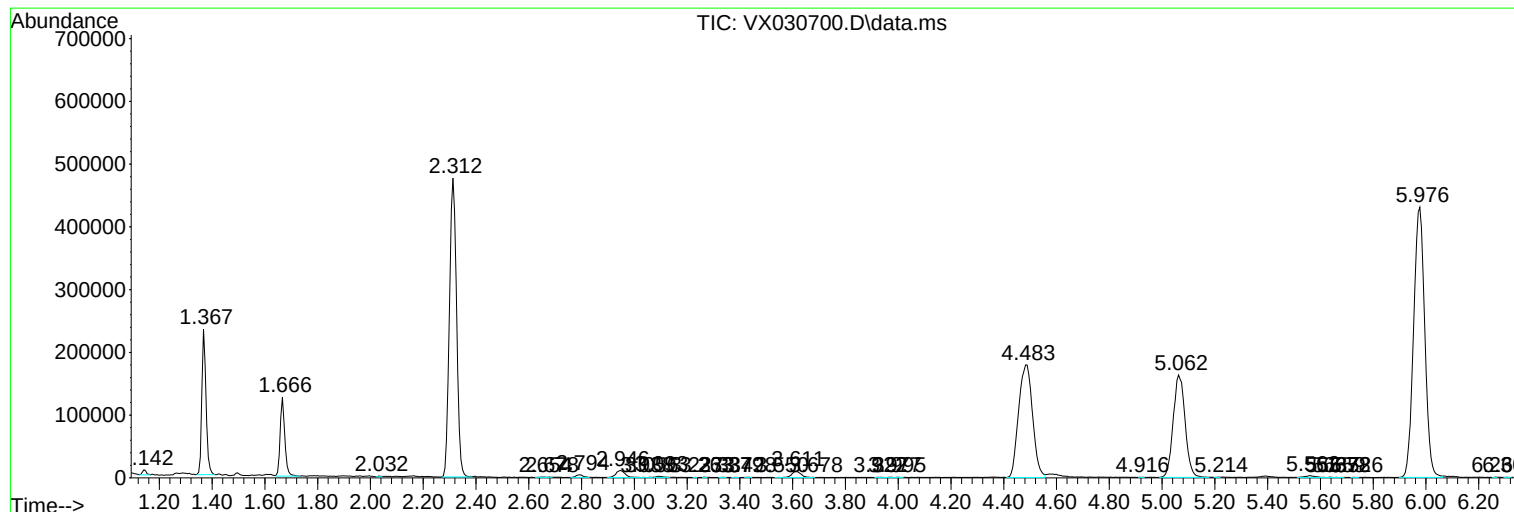

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030700.D
Acq On : 19 Aug 2022 12:52
Operator : JC/MD
Sample : N4231-07DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030700.D
Acq On : 19 Aug 2022 12:52
Operator : JC/MD
Sample : N4231-07DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc