

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030702.D
 Acq On : 19 Aug 2022 14:53
 Operator : JC/MD
 Sample : N4231-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	55	rVB	140895	149736	12.79%	1.657%
2	1.666	90	95	106	rVB	109318	139314	11.90%	1.541%
3	2.306	194	200	208	rVB	253067	386152	33.00%	4.272%
4	2.428	218	220	221	rBV	628	381	0.03%	0.004%
5	2.501	230	232	235	rBV2	564	495	0.04%	0.005%
6	2.788	274	279	284	rVB2	4013	7026	0.60%	0.078%
7	2.940	301	304	313	rVB3	911	2248	0.19%	0.025%
8	3.013	313	316	318	rBV2	492	487	0.04%	0.005%
9	3.056	321	323	324	rBV	505	401	0.03%	0.004%
10	3.306	362	364	365	rVV2	483	296	0.03%	0.003%
11	3.324	365	367	369	rVB	450	400	0.03%	0.004%
12	3.544	402	403	406	rBV	403	312	0.03%	0.003%
13	3.684	423	426	429	rVB2	390	500	0.04%	0.006%
14	3.739	433	435	438	rVB2	312	325	0.03%	0.004%
15	3.782	438	442	443	rBV	243	310	0.03%	0.003%
16	3.794	443	444	448	rVB2	492	440	0.04%	0.005%
17	4.001	475	478	479	rVB2	438	384	0.03%	0.004%
18	4.160	501	504	508	rBV2	341	433	0.04%	0.005%
19	4.263	519	521	523	rBV	446	310	0.03%	0.003%
20	4.306	527	528	531	rVB2	365	304	0.03%	0.003%
21	4.336	531	533	536	rBV2	409	399	0.03%	0.004%
22	4.464	544	554	570	rBV	103903	301965	25.80%	3.341%
23	5.062	640	652	670	rVB	157722	473039	40.42%	5.234%
24	5.220	675	678	680	rBV2	302	368	0.03%	0.004%
25	5.263	683	685	688	rVB2	561	516	0.04%	0.006%
26	5.294	688	690	693	rBV2	427	593	0.05%	0.007%
27	5.324	693	695	698	rVB2	346	318	0.03%	0.004%
28	5.391	701	706	709	rBV3	1248	2436	0.21%	0.027%
29	5.525	726	728	729	rBV	619	471	0.04%	0.005%
30	5.550	729	732	733	rBV2	1019	1008	0.09%	0.011%
31	5.653	747	749	752	rVB2	328	337	0.03%	0.004%
32	5.970	789	801	818	rVV2	402684	1170308	100.00%	12.949%
33	6.214	839	841	844	rVB	495	385	0.03%	0.004%
34	6.293	852	854	857	rBV2	470	548	0.05%	0.006%
35	6.348	862	863	869	rBV3	700	1152	0.10%	0.013%
36	6.763	921	931	943	rBV	294741	690831	59.03%	7.644%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030702.D
 Acq On : 19 Aug 2022 14:53
 Operator : JC/MD
 Sample : N4231-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

37	7.019	970	973	975	rVB3	344	372	0.03%	0.004%
38	7.110	982	988	998	rVB3	13281	29577	2.53%	0.327%
39	7.311	1011	1021	1033	rBV	245710	542986	46.40%	6.008%
40	7.476	1045	1048	1049	rBV2	1046	887	0.08%	0.010%
41	7.750	1092	1093	1096	rBV2	359	305	0.03%	0.003%
42	7.836	1104	1107	1108	rBV2	379	364	0.03%	0.004%
43	7.939	1118	1124	1132	rVB4	1863	4422	0.38%	0.049%
44	8.183	1162	1164	1168	rBV2	488	754	0.06%	0.008%
45	8.256	1171	1176	1181	rBV4	2769	4749	0.41%	0.053%
46	8.323	1181	1187	1199	rBV	154973	265532	22.69%	2.938%
47	8.409	1199	1201	1203	rVB	483	387	0.03%	0.004%
48	8.482	1208	1213	1218	rBV2	1559	2869	0.25%	0.032%
49	8.519	1218	1219	1221	rVB	591	303	0.03%	0.003%
50	8.573	1226	1228	1229	rBV2	412	321	0.03%	0.004%
51	8.653	1232	1241	1250	rBV	605495	941065	80.41%	10.412%
52	8.951	1285	1290	1301	rBV	117770	173701	14.84%	1.922%
53	9.153	1321	1323	1324	rBV	535	316	0.03%	0.003%
54	9.220	1331	1334	1335	rVB2	542	467	0.04%	0.005%
55	9.275	1340	1343	1348	rVB4	1732	2422	0.21%	0.027%
56	9.384	1356	1361	1374	rBV	459395	657990	56.22%	7.280%
57	9.701	1410	1413	1419	rVB3	977	1555	0.13%	0.017%
58	9.799	1425	1429	1432	rVB2	515	668	0.06%	0.007%
59	9.829	1432	1434	1435	rBV	464	337	0.03%	0.004%
60	10.006	1461	1463	1465	rVB	376	300	0.03%	0.003%
61	10.055	1465	1471	1480	rBV	597948	812672	69.44%	8.992%
62	10.311	1507	1513	1518	rBV3	765	1470	0.13%	0.016%
63	10.384	1522	1525	1528	rBV2	303	343	0.03%	0.004%
64	10.494	1541	1543	1546	rVV2	361	343	0.03%	0.004%
65	10.628	1564	1565	1568	rBV	673	694	0.06%	0.008%
66	10.707	1575	1578	1580	rBV2	322	438	0.04%	0.005%
67	10.786	1589	1591	1592	rBV	560	329	0.03%	0.004%
68	11.085	1638	1640	1642	rBV	366	355	0.03%	0.004%
69	11.195	1652	1658	1667	rBV	469828	599318	51.21%	6.631%
70	11.317	1675	1678	1680	rBV2	470	609	0.05%	0.007%
71	11.402	1689	1692	1694	rBV2	332	412	0.04%	0.005%
72	11.451	1698	1700	1702	rBV2	497	541	0.05%	0.006%
73	11.750	1748	1749	1751	rBV2	686	674	0.06%	0.007%
74	11.939	1779	1780	1781	rBV	578	295	0.03%	0.003%
75	12.024	1789	1794	1807	rVV	635632	782747	66.88%	8.660%
76	12.140	1811	1813	1818	rVB2	402	543	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030702.D
 Acq On : 19 Aug 2022 14:53
 Operator : JC/MD
 Sample : N4231-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1850	rBV	678652	853659	72.94%	9.445%
78	12.426	1858	1860	1861	rVB2	661	366	0.03%	0.004%
79	12.445	1861	1863	1864	rBV	420	333	0.03%	0.004%
80	12.579	1884	1885	1889	rBV2	560	479	0.04%	0.005%
81	12.701	1903	1905	1908	rVB2	792	615	0.05%	0.007%
82	12.762	1912	1915	1919	rVV3	1492	2011	0.17%	0.022%
83	12.817	1922	1924	1929	rBV2	421	760	0.06%	0.008%
84	13.012	1954	1956	1958	rBV2	401	338	0.03%	0.004%
85	13.067	1963	1965	1966	rBV2	440	363	0.03%	0.004%
86	13.152	1977	1979	1981	rVB2	358	332	0.03%	0.004%
87	13.176	1981	1983	1984	rBV2	372	317	0.03%	0.004%
88	13.457	2027	2029	2031	rBV	462	502	0.04%	0.006%
89	13.499	2034	2036	2038	rBV	484	519	0.04%	0.006%
90	13.713	2069	2071	2075	rBV2	361	447	0.04%	0.005%
91	13.749	2075	2077	2079	rVB	523	367	0.03%	0.004%
92	14.127	2135	2139	2144	rBV	2681	3094	0.26%	0.034%
93	14.219	2152	2154	2157	rBV3	468	518	0.04%	0.006%
94	14.274	2162	2163	2165	rBV	581	509	0.04%	0.006%
95	14.341	2173	2174	2176	rBV2	683	646	0.06%	0.007%
96	14.414	2185	2186	2187	rBV	557	311	0.03%	0.003%
97	15.127	2302	2303	2305	rBV	723	543	0.05%	0.006%
98	15.450	2354	2356	2358	rBV	844	544	0.05%	0.006%
99	15.511	2365	2366	2369	rBV2	809	717	0.06%	0.008%
100	16.444	2518	2519	2521	rVB	840	484	0.04%	0.005%


Sum of corrected areas: 9038134

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030702.D
Acq On : 19 Aug 2022 14:53
Operator : JC/MD
Sample : N4231-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

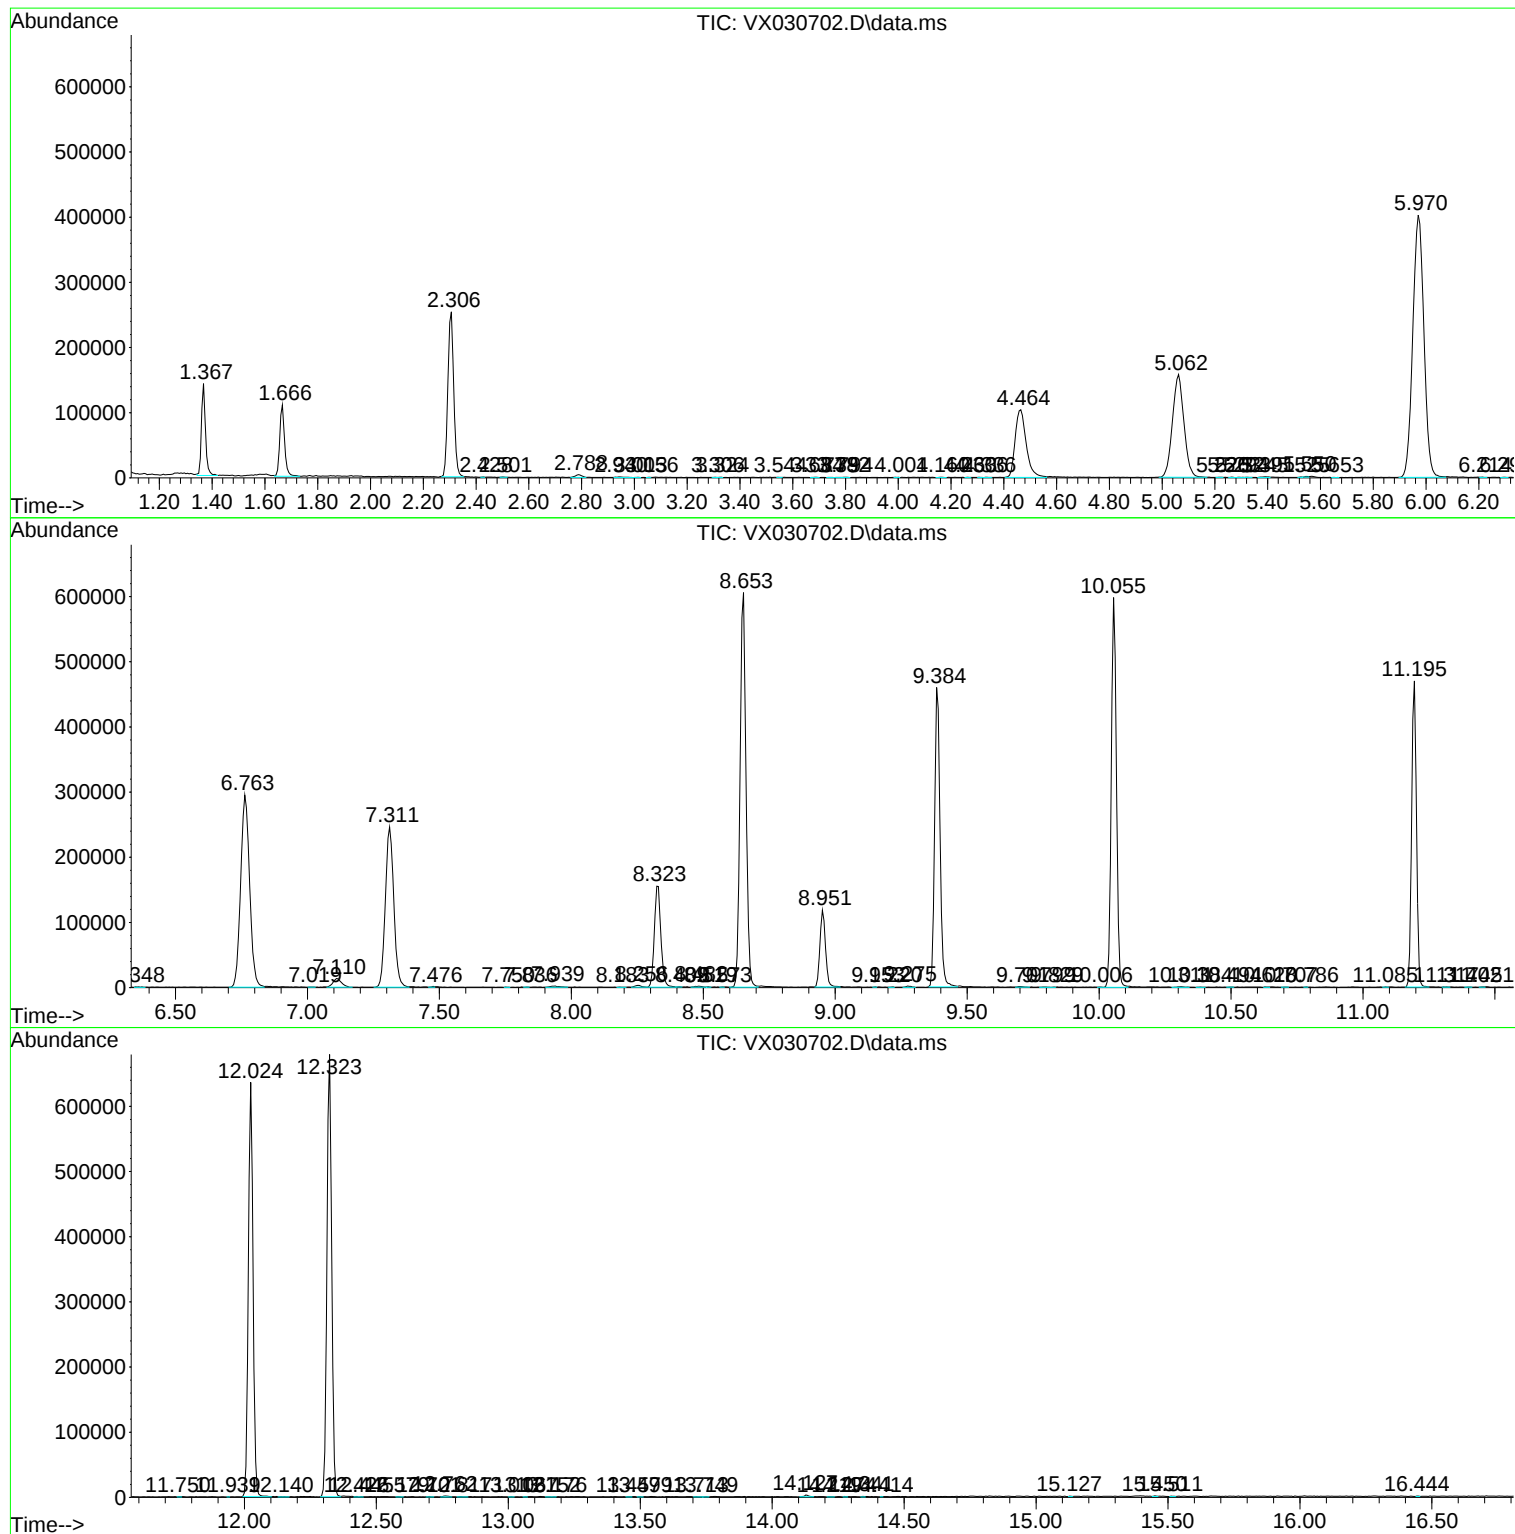

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030702.D
Acq On : 19 Aug 2022 14:53
Operator : JC/MD
Sample : N4231-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030702.D
Acq On : 19 Aug 2022 14:53
Operator : JC/MD
Sample : N4231-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc