

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030704.D
 Acq On : 19 Aug 2022 15:49
 Operator : JC/MD
 Sample : N4221-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	128265	136614	12.04%	1.563%
2	1.666	90	95	104	rVB	101040	127111	11.20%	1.454%
3	2.307	193	200	208	rVB	229631	355036	31.28%	4.062%
4	2.502	230	232	238	rVB3	450	663	0.06%	0.008%
5	2.630	250	253	255	rBV3	536	517	0.05%	0.006%
6	2.654	255	257	261	rBV2	643	679	0.06%	0.008%
7	2.788	274	279	286	rVB	4694	8109	0.71%	0.093%
8	2.855	286	290	292	rBV2	328	489	0.04%	0.006%
9	2.904	295	298	299	rBV	341	341	0.03%	0.004%
10	2.947	299	305	311	rVV	3454	6909	0.61%	0.079%
11	3.111	330	332	335	rVB2	558	535	0.05%	0.006%
12	3.239	348	353	355	rVB2	450	565	0.05%	0.006%
13	3.367	372	374	375	rBV2	362	314	0.03%	0.004%
14	3.410	379	381	383	rBV2	312	353	0.03%	0.004%
15	3.447	385	387	388	rBV	586	407	0.04%	0.005%
16	3.569	404	407	408	rBV2	506	458	0.04%	0.005%
17	3.770	439	440	443	rVB	548	317	0.03%	0.004%
18	3.800	443	445	448	rBV3	320	399	0.04%	0.005%
19	3.879	456	458	460	rBV2	316	310	0.03%	0.004%
20	3.965	468	472	473	rVB2	407	383	0.03%	0.004%
21	3.977	473	474	477	rVB2	543	440	0.04%	0.005%
22	4.075	488	490	493	rBV2	441	523	0.05%	0.006%
23	4.465	544	554	568	rBV	112026	316566	27.89%	3.621%
24	4.672	586	588	590	rVB	730	578	0.05%	0.007%
25	4.709	590	594	596	rBV3	622	854	0.08%	0.010%
26	4.806	607	610	611	rBV	451	458	0.04%	0.005%
27	4.958	633	635	638	rVB2	482	485	0.04%	0.006%
28	5.062	638	652	669	rBV2	155312	469090	41.33%	5.366%
29	5.300	687	691	692	rBV	255	391	0.03%	0.004%
30	5.397	699	707	714	rVV5	2076	5202	0.46%	0.060%
31	5.477	716	720	721	rBV2	312	371	0.03%	0.004%
32	5.525	726	728	729	rBV	945	721	0.06%	0.008%
33	5.562	729	734	743	rVB4	2727	6176	0.54%	0.071%
34	5.660	748	750	753	rVB2	339	425	0.04%	0.005%
35	5.684	753	754	757	rBV2	332	407	0.04%	0.005%
36	5.879	784	786	789	rBV	281	349	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030704.D
 Acq On : 19 Aug 2022 15:49
 Operator : JC/MD
 Sample : N4221-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	5.977	789	802	822	rVV2	385502	1135075	100.00%	12.985%
38	6.233	843	844	847	rBV2	345	432	0.04%	0.005%
39	6.635	906	910	912	rBV2	421	523	0.05%	0.006%
40	6.769	922	932	946	rBV	264387	635761	56.01%	7.273%
41	6.879	949	950	956	rVB3	974	955	0.08%	0.011%
42	7.019	971	973	975	rBV2	490	458	0.04%	0.005%
43	7.117	981	989	998	rBV5	12866	31592	2.78%	0.361%
44	7.312	1012	1021	1035	rBV	241680	534657	47.10%	6.116%
45	7.489	1045	1050	1051	rBV3	630	1017	0.09%	0.012%
46	7.604	1068	1069	1074	rVB2	422	401	0.04%	0.005%
47	7.818	1101	1104	1105	rBV	683	441	0.04%	0.005%
48	7.940	1118	1124	1126	rBV3	2297	3886	0.34%	0.044%
49	8.141	1155	1157	1162	rVB2	467	484	0.04%	0.006%
50	8.251	1171	1175	1181	rBV3	2705	5216	0.46%	0.060%
51	8.330	1181	1188	1201	rVV	159330	262455	23.12%	3.002%
52	8.421	1201	1203	1205	rVB3	850	540	0.05%	0.006%
53	8.482	1211	1213	1215	rVB2	1117	631	0.06%	0.007%
54	8.531	1220	1221	1225	rVB3	551	662	0.06%	0.008%
55	8.586	1227	1230	1232	rBV	709	673	0.06%	0.008%
56	8.653	1234	1241	1252	rBV	567391	887703	78.21%	10.155%
57	8.952	1284	1290	1301	rBV	116859	171472	15.11%	1.962%
58	9.275	1339	1343	1348	rVB4	7501	11852	1.04%	0.136%
59	9.391	1356	1362	1374	rBV	479853	690037	60.79%	7.894%
60	9.714	1409	1415	1419	rVB4	1614	2528	0.22%	0.029%
61	9.756	1419	1422	1424	rBV2	335	385	0.03%	0.004%
62	9.854	1436	1438	1443	rVB2	704	973	0.09%	0.011%
63	9.909	1443	1447	1448	rBV	486	725	0.06%	0.008%
64	9.988	1459	1460	1462	rBV	567	424	0.04%	0.005%
65	10.055	1465	1471	1479	rBV	544613	740119	65.20%	8.467%
66	10.165	1487	1489	1493	rVB	547	410	0.04%	0.005%
67	10.232	1499	1500	1506	rVB2	891	943	0.08%	0.011%
68	10.305	1509	1512	1514	rVV3	713	869	0.08%	0.010%
69	10.348	1518	1519	1520	rBV	641	335	0.03%	0.004%
70	10.433	1530	1533	1534	rBV2	552	463	0.04%	0.005%
71	10.512	1545	1546	1548	rVB	543	308	0.03%	0.004%
72	10.659	1569	1570	1572	rVB2	764	356	0.03%	0.004%
73	11.085	1638	1640	1643	rVB3	602	613	0.05%	0.007%
74	11.195	1652	1658	1670	rBV	506773	623928	54.97%	7.138%
75	11.281	1670	1672	1674	rVV2	600	559	0.05%	0.006%
76	11.305	1674	1676	1682	rVB4	895	1319	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030704.D
 Acq On : 19 Aug 2022 15:49
 Operator : JC/MD
 Sample : N4221-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.348	1682	1683	1685	rBV2	551	322	0.03%	0.004%
78	11.433	1695	1697	1698	rBV	441	310	0.03%	0.004%
79	11.451	1698	1700	1703	rVB2	722	646	0.06%	0.007%
80	11.579	1720	1721	1724	rBV	339	381	0.03%	0.004%
81	11.640	1729	1731	1734	rVB	522	446	0.04%	0.005%
82	11.701	1739	1741	1744	rBV2	357	386	0.03%	0.004%
83	11.793	1755	1756	1759	rVB	476	316	0.03%	0.004%
84	11.878	1769	1770	1773	rBV2	462	351	0.03%	0.004%
85	12.024	1789	1794	1801	rBV	593073	712828	62.80%	8.155%
86	12.213	1821	1825	1827	rBV3	533	965	0.09%	0.011%
87	12.323	1837	1843	1850	rBV	661553	819480	72.20%	9.375%
88	12.524	1874	1876	1877	rBV	573	409	0.04%	0.005%
89	12.689	1901	1903	1905	rBV	564	483	0.04%	0.006%
90	12.860	1929	1931	1933	rBV2	562	511	0.05%	0.006%
91	13.036	1958	1960	1961	rVB	580	336	0.03%	0.004%
92	13.512	2036	2038	2039	rVB	654	373	0.03%	0.004%
93	13.567	2045	2047	2048	rBV	513	346	0.03%	0.004%
94	13.719	2071	2072	2074	rVB2	538	315	0.03%	0.004%
95	13.951	2108	2110	2111	rBV2	613	445	0.04%	0.005%
96	14.000	2116	2118	2122	rVB	750	675	0.06%	0.008%
97	14.140	2134	2141	2146	rBV3	2020	4120	0.36%	0.047%
98	14.298	2166	2167	2169	rBV	519	332	0.03%	0.004%
99	14.378	2178	2180	2181	rVB	634	317	0.03%	0.004%
100	16.231	2482	2484	2486	rBV	903	660	0.06%	0.008%


Sum of corrected areas: 8741478

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030704.D
Acq On : 19 Aug 2022 15:49
Operator : JC/MD
Sample : N4221-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

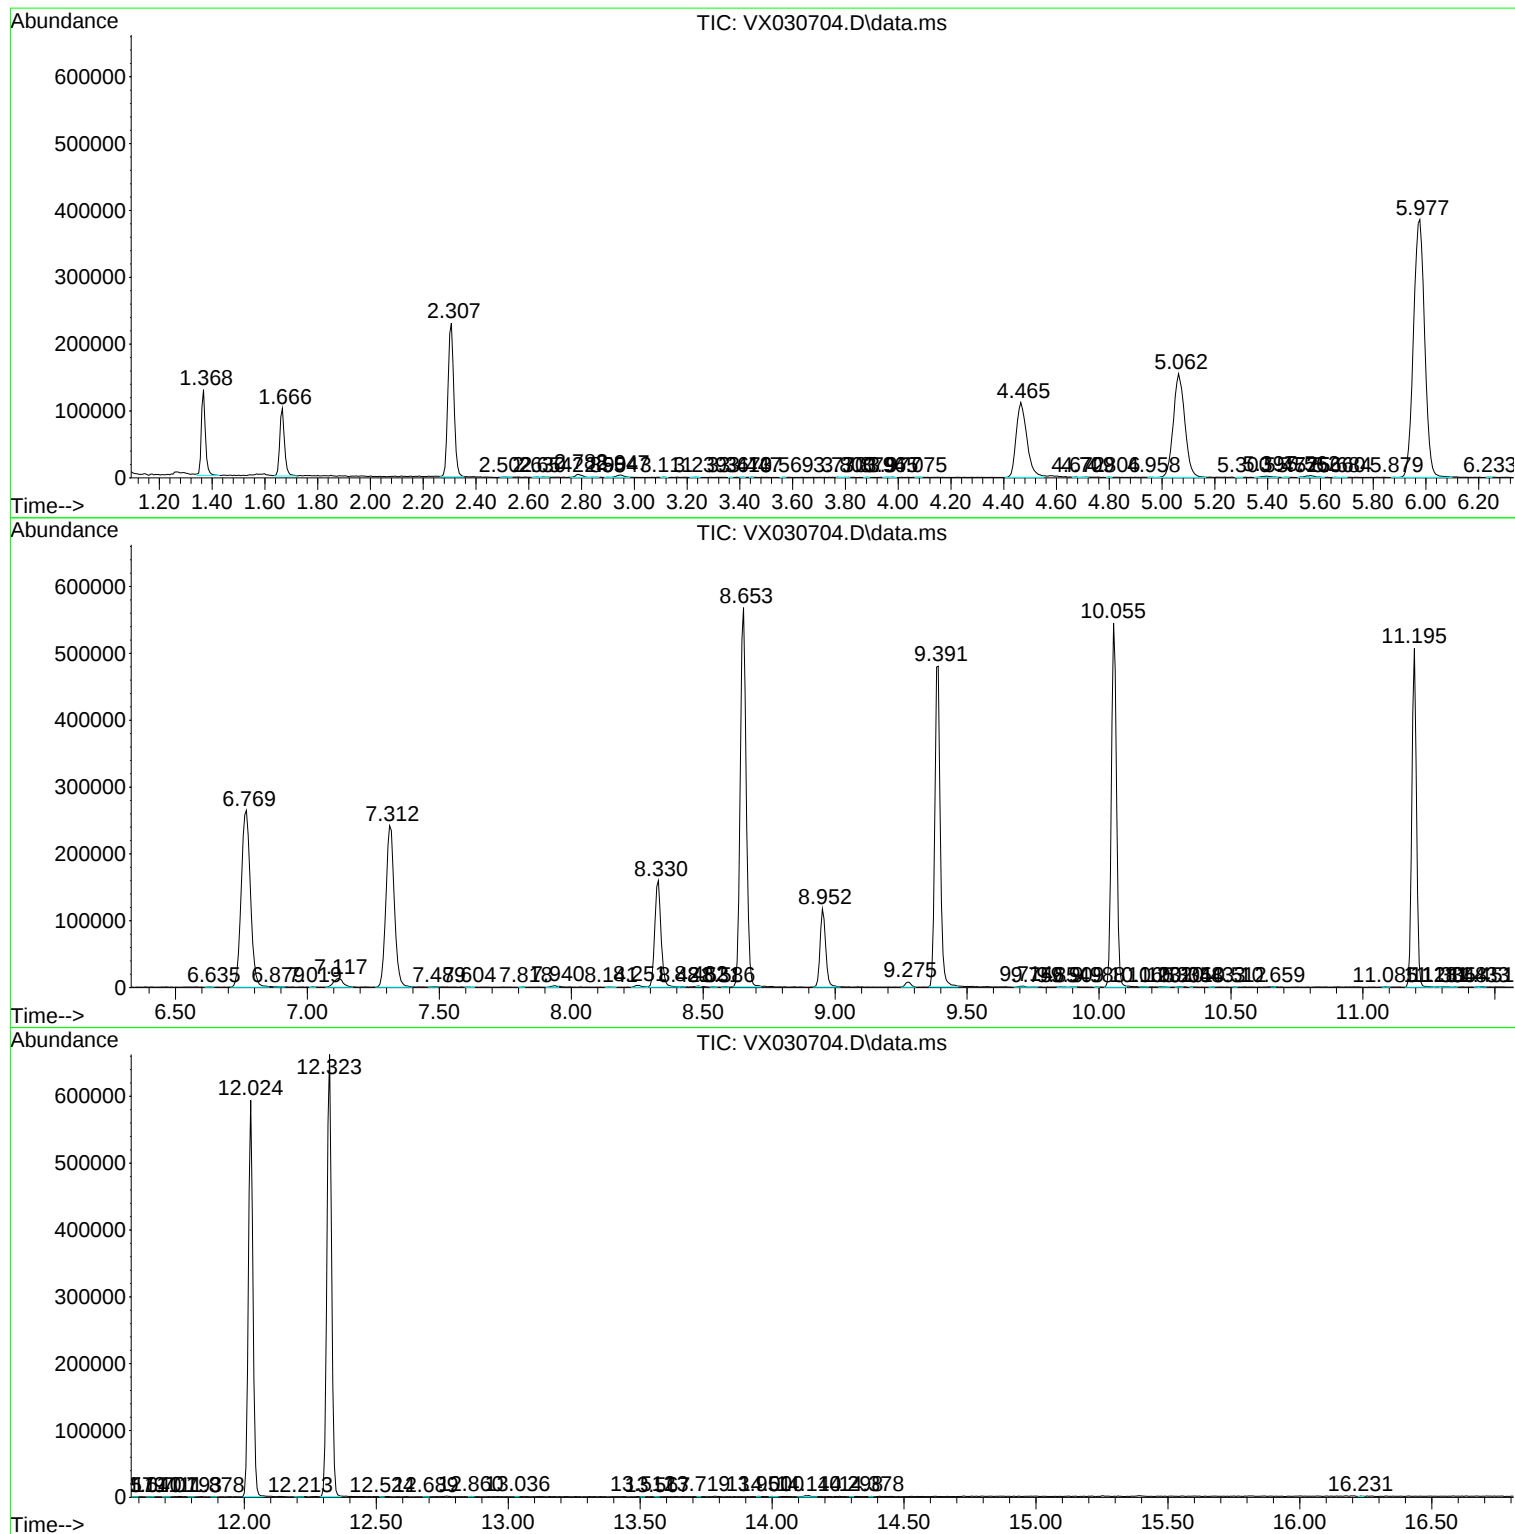

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030704.D
Acq On : 19 Aug 2022 15:49
Operator : JC/MD
Sample : N4221-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
Data File : VX030704.D
Acq On : 19 Aug 2022 15:49
Operator : JC/MD
Sample : N4221-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc