
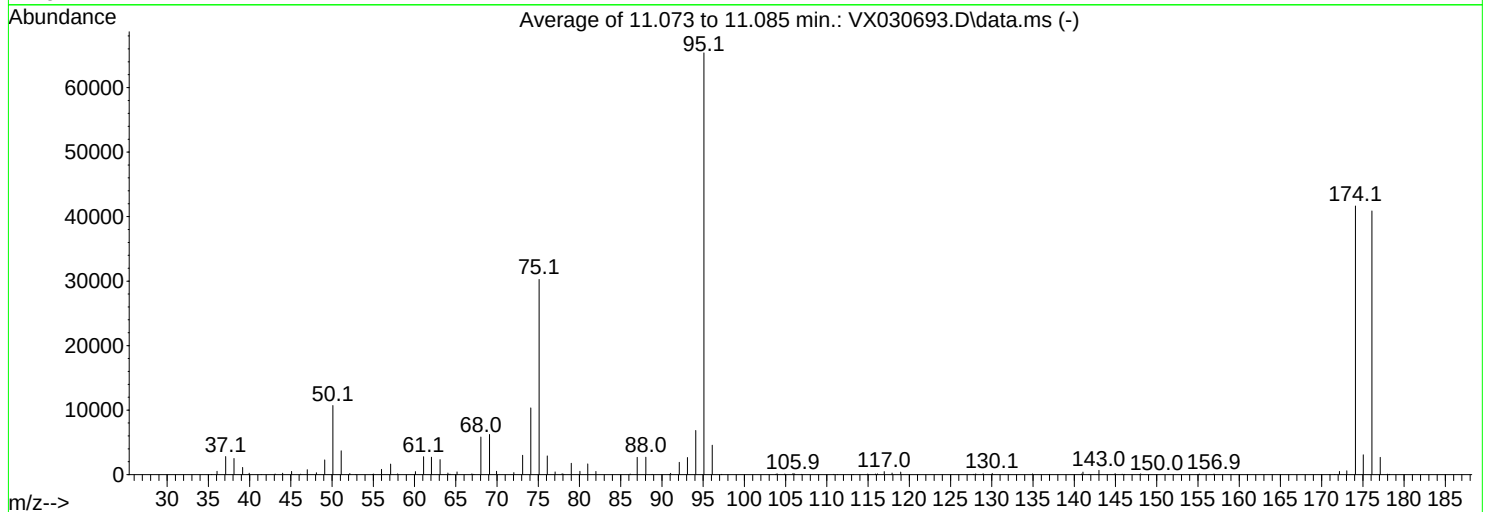


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081922\
 Data File : VX030693.D
 Acq On : 19 Aug 2022 09:39
 Operator : JC/MD
 Sample : BFB683
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB683

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Sat Aug 20 02:12:38 2022

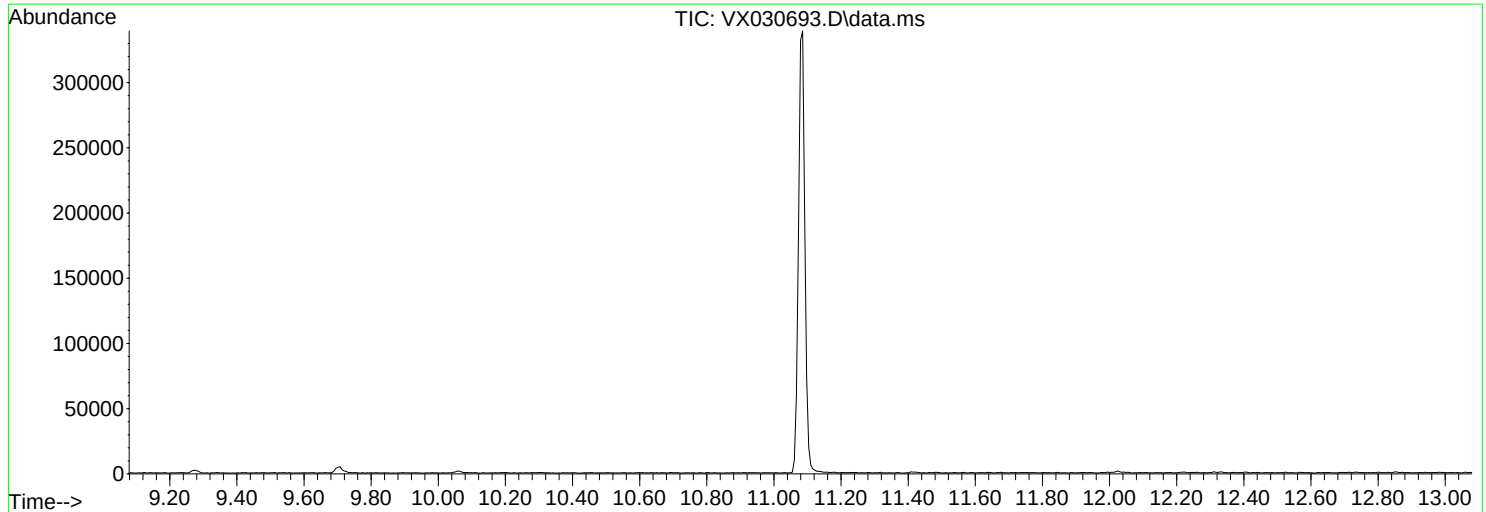

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	10711	PASS
75	95	30	80	46.3	30272	PASS
95	95	100	100	100.0	65387	PASS
96	95	5	9	7.0	4563	PASS
173	174	0.00	2	1.4	584	PASS
174	95	50	120	63.7	41659	PASS
175	174	5	9	7.4	3073	PASS
176	174	95	101	98.1	40872	PASS
177	176	5	9	6.5	2677	PASS

m/z	Abundance
39.90	305.0
44.00	385.0
55.90	97.0

Instrument :
MSVOA_X
ClientSampleId :
BFB683

m/z	Abundance
36.00	440.0
37.10	2204.0
38.10	1568.0
39.20	742.0
40.00	649.0
43.10	115.0
44.00	540.0
45.00	497.0
47.00	735.0
48.00	221.0
49.10	1672.0
50.10	8391.0
51.10	2546.0
52.10	217.0
54.90	188.0
56.00	568.0
57.10	1093.0
58.00	97.0
60.10	455.0
61.10	1975.0
62.10	1952.0
63.10	1603.0
64.30	218.0
65.10	303.0
66.90	119.0
68.10	4001.0
69.10	4485.0
69.90	398.0
72.10	227.0
73.10	2020.0
74.10	7221.0
75.10	20984.0
76.10	2099.0
77.10	304.0
77.90	164.0
79.00	1084.0
80.10	326.0
81.00	1176.0
82.00	268.0
86.20	84.0
87.00	1981.0
88.10	1553.0
90.90	159.0
92.10	1142.0
93.10	1728.0
94.10	4100.0
95.10	42416.0
96.10	2951.0
97.30	82.0
103.80	181.0
104.90	77.0
105.90	284.0
106.90	53.0
115.00	62.0
116.10	117.0
117.00	381.0
118.00	158.0
119.00	339.0
128.10	126.0
128.90	63.0
130.10	74.0
135.10	64.0
140.90	300.0
143.00	472.0
145.00	116.0
145.80	112.0
147.90	74.0
155.20	83.0
157.00	61.0
171.60	110.0
172.20	258.0
173.10	252.0
174.10	22976.0
175.10	1650.0
176.10	22896.0
177.10	1691.0
178.00	77.0

Instrument :
MSVOA_X
ClientSampleId :
BFB683

m/z	Abundance
35.40	57.0
36.00	748.0
37.10	3735.0
38.10	3356.0
39.10	1402.0
40.00	488.0
41.40	98.0
43.10	62.0
44.10	733.0
45.10	505.0
46.20	137.0
47.00	731.0
48.10	373.0
49.10	2284.0
50.10	12765.0
51.10	4820.0
52.20	89.0
55.10	175.0
56.10	1181.0
57.10	2102.0
57.90	141.0
60.20	462.0
61.10	3740.0
62.10	3699.0
63.10	2723.0
64.00	338.0
65.20	621.0
67.00	277.0
68.00	6843.0
69.10	7400.0
70.00	565.0
72.10	439.0
73.10	3609.0
74.10	12702.0
75.10	34792.0
76.10	3681.0
77.10	498.0
77.90	270.0
79.00	2193.0
80.00	663.0
81.00	2021.0
81.90	664.0
86.20	59.0
87.00	2906.0
88.00	3202.0
88.80	123.0
91.10	199.0
92.10	2419.0
93.10	3138.0
94.10	7649.0
95.10	77944.0
96.10	5519.0
104.00	247.0
104.90	101.0
106.10	367.0
106.90	55.0
110.90	70.0
111.30	79.0
114.90	136.0
116.20	292.0
116.90	488.0
117.80	300.0
118.90	547.0
127.80	177.0
128.90	162.0
130.10	277.0
134.90	157.0
141.10	653.0
141.80	61.0
142.90	757.0
144.90	213.0
145.80	82.0
148.10	166.0
155.10	223.0
157.00	150.0
172.10	570.0
173.00	735.0
174.10	46688.0
175.00	3810.0
176.10	44320.0
177.10	2959.0
178.20	122.0

Instrument :
MSVOA_X
ClientSampleId :
BFB683

m/z	Abundance
36.10	415.0
37.10	2469.0
38.10	2632.0
39.10	1182.0
40.00	441.0
43.10	110.0
44.10	533.0
45.20	489.0
46.20	79.0
47.00	824.0
48.20	288.0
49.10	2927.0
50.10	10977.0
51.10	3741.0
52.10	203.0
52.90	63.0
55.00	143.0
56.00	1018.0
57.10	1707.0
57.90	141.0
60.00	544.0
61.10	2641.0
62.00	2465.0
63.10	2651.0
64.10	409.0
65.10	379.0
67.20	182.0
68.10	6664.0
69.10	6783.0
70.00	577.0
71.90	328.0
73.10	3363.0
74.10	11131.0
75.10	35040.0
76.10	2938.0
77.00	463.0
78.10	220.0
79.00	2036.0
80.00	611.0
81.00	1798.0
82.10	556.0
86.10	193.0
87.00	3127.0
88.10	3354.0
91.00	393.0
92.10	2173.0
93.10	3102.0
94.10	8788.0
95.10	75800.0
96.10	5219.0
97.20	54.0
103.90	209.0
104.90	124.0
105.90	293.0
107.00	79.0
110.80	55.0
113.20	63.0
114.90	69.0
115.90	320.0
116.90	560.0
118.00	281.0
119.00	287.0
128.00	285.0
129.00	208.0
130.00	282.0
134.90	162.0
137.00	164.0
141.00	573.0
141.80	61.0
143.10	755.0
145.00	213.0
146.10	141.0
148.00	215.0
150.00	57.0
156.90	113.0
159.00	83.0
161.00	101.0
171.00	81.0
172.10	680.0
173.00	764.0
174.10	55312.0
175.10	3758.0
176.10	55400.0
177.10	3381.0
178.00	122.0

Instrument :
MSVOA_X
ClientSampleId :
BFB683