

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081925\
 Data File : VX047401.D
 Acq On : 19 Aug 2025 10:05
 Operator : JC/MD
 Sample : VX0819MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0819MBL01

Quant Time: Aug 20 01:24:05 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	182788	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.763	114	363576	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	362613	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	179617	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	147768	57.763	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 115.520%			
35) Dibromofluoromethane	5.397	113	127737	54.134	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 108.260%			
50) Toluene-d8	8.647	98	448031	53.122	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 106.240%			
62) 4-Bromofluorobenzene	11.079	95	184176	59.177	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 118.360%			
Target Compounds						Qvalue
3) Chloromethane	1.306	50	557	0.266	ug/l #	65
5) Bromomethane	1.642	94	761	0.716	ug/l #	68
6) Chloroethane	1.776	64	334	0.207	ug/l	95
10) Methyl Iodide	2.483	142	4111	1.063	ug/l #	77
11) Tert butyl alcohol	2.959	59	160	0.719	ug/l #	72
13) Acrolein	2.251	56	325	0.692	ug/l #	1
15) Acrylonitrile	3.093	53	802	0.746	ug/l #	79
16) Acetone	2.392	43	1714	1.783	ug/l	89
17) Carbon Disulfide	2.526	76	7250	1.044	ug/l	98
21) trans-1,2-Dichloroethene	3.105	96	648	0.265	ug/l	89
29) Tetrahydrofuran	5.074	42	216	0.265	ug/l #	45
38) Carbon Tetrachloride	5.562	117	19923	4.895	ug/l #	14
49) 1,4-Dioxane	7.708	88	66	2.354	ug/l #	1
51) 4-Methyl-2-Pentanone	8.579	43	1399	0.438	ug/l #	66
58) 2-Chloroethyl Vinyl ether	8.281	63	280	8.502	ug/l #	46
64) Tetrachloroethene	9.281	164	526	0.201	ug/l #	77
68) m/p-Xylenes	10.305	106	1579	0.286	ug/l	90
76) 1,2,3-Trichloropropane	11.079	75	94378	28.648	ug/l #	38
78) n-propylbenzene	11.311	91	3447	0.205	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.079	75	94378	112.805	ug/l #	7
85) sec-Butylbenzene	11.890	105	4291	0.300	ug/l	93
86) p-Isopropyltoluene	12.006	119	4237	0.350	ug/l	91
87) 1,3-Dichlorobenzene	11.969	146	1916	0.292	ug/l	90
88) 1,4-Dichlorobenzene	11.969	146	1916	0.284	ug/l	90
89) n-Butylbenzene	12.335	91	6042	0.537	ug/l	91
90) Hexachloroethane	12.542	117	575	0.271	ug/l	87
91) 1,2-Dichlorobenzene	12.341	146	1358	0.218	ug/l	97
93) 1,2,4-Trichlorobenzene	13.591	180	3359	0.805	ug/l	97
94) Hexachlorobutadiene	13.719	225	4858	3.271	ug/l	99
95) Naphthalene	13.774	128	6687	0.561	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	3176	0.808	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081925\
Data File : VX047401.D
Acq On : 19 Aug 2025 10:05
Operator : JC/MD
Sample : VX0819MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01

Quant Time: Aug 20 01:24:05 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration




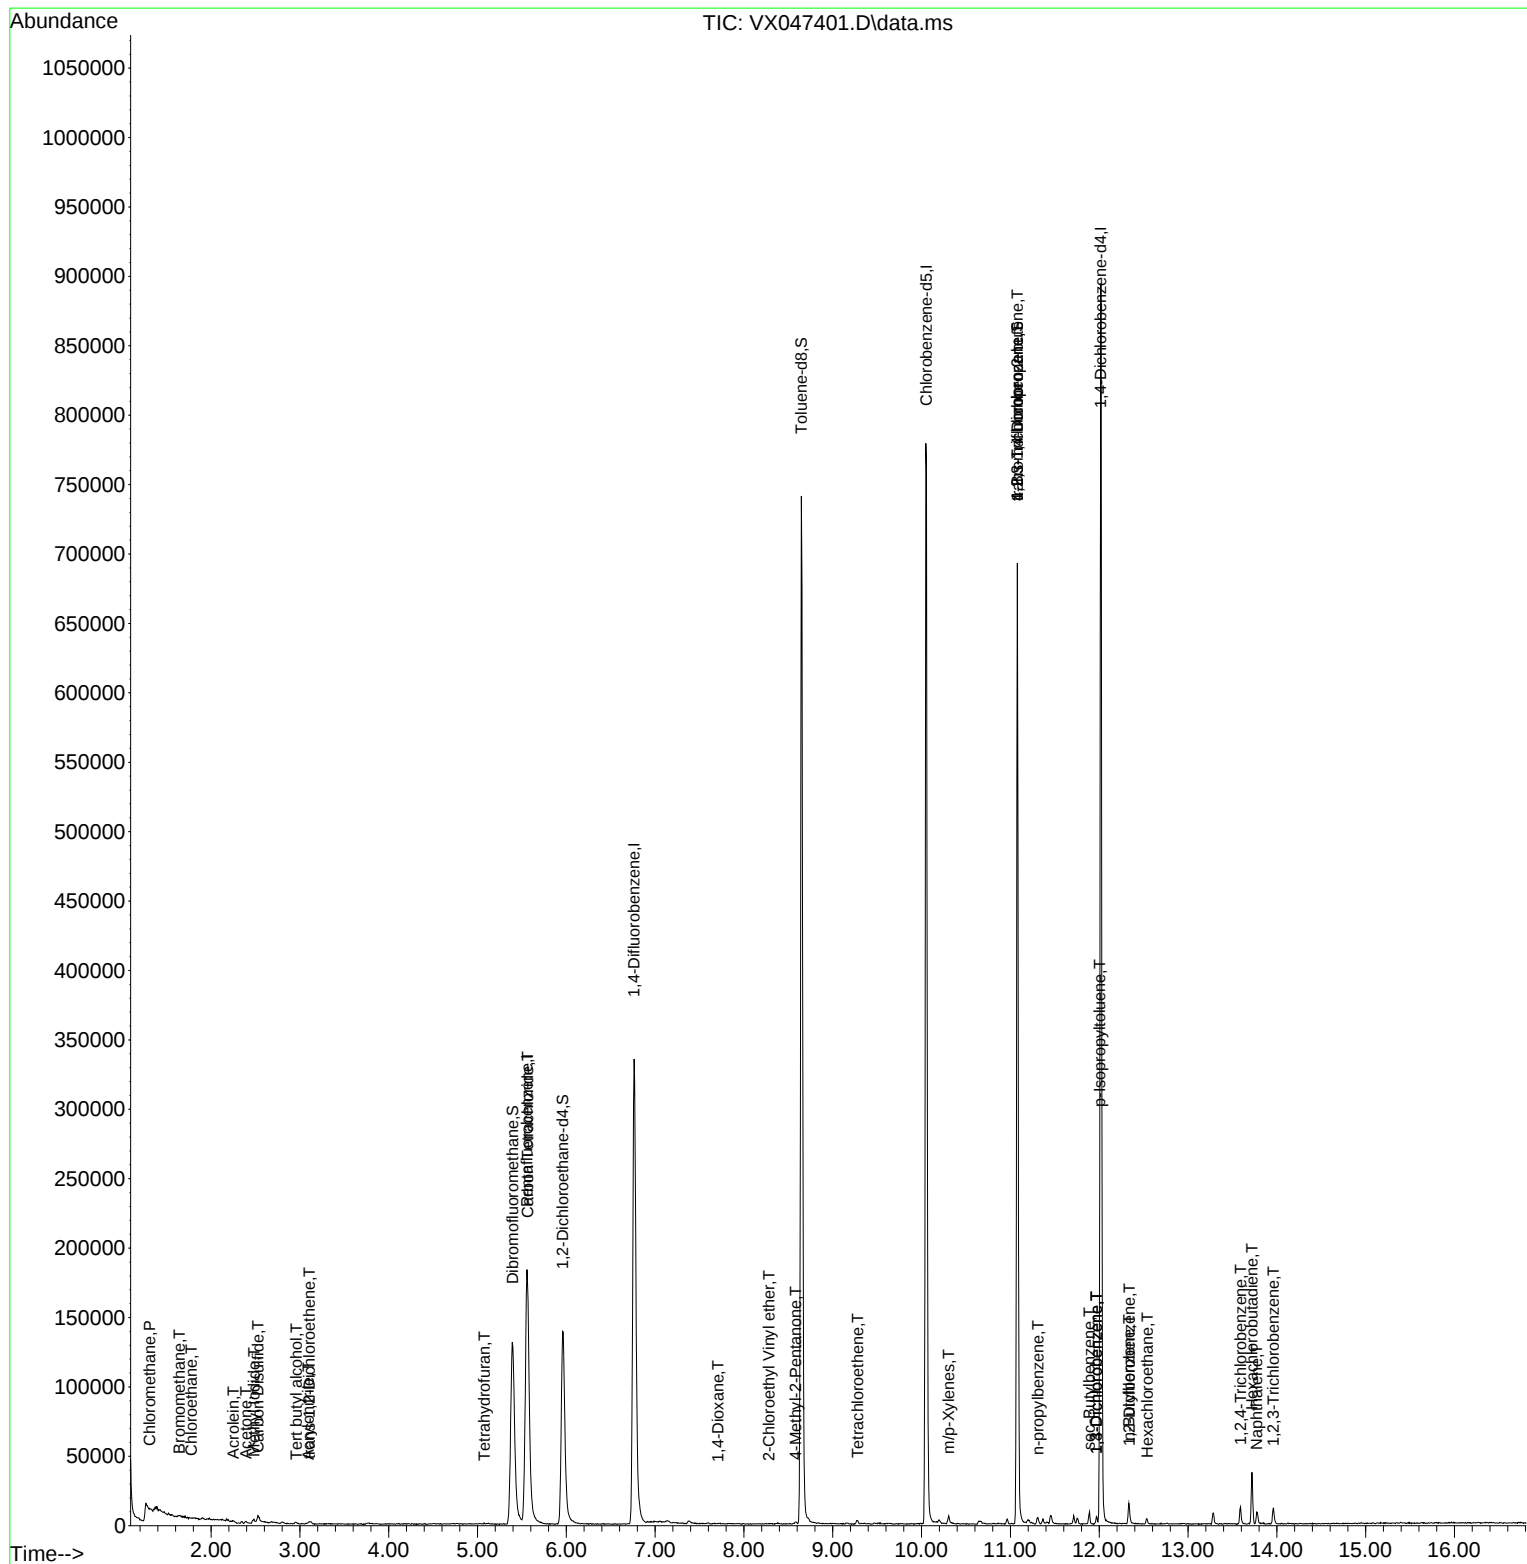




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.012 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion:168 Resp: 182788
Ion Ratio Lower Upper
168 100
99 66.8 47.9 71.9

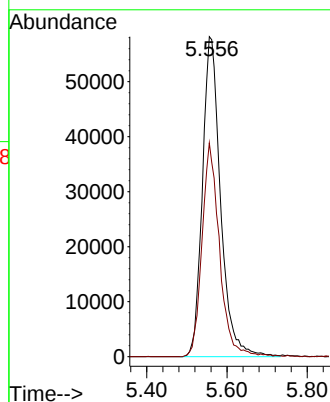

#3
Chloromethane
Concen: 0.266 ug/l
RT: 1.306 min Scan# 36
Delta R.T. -0.006 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion: 50 Resp: 557
Ion Ratio Lower Upper
50 100
52 13.9 27.0 40.4#


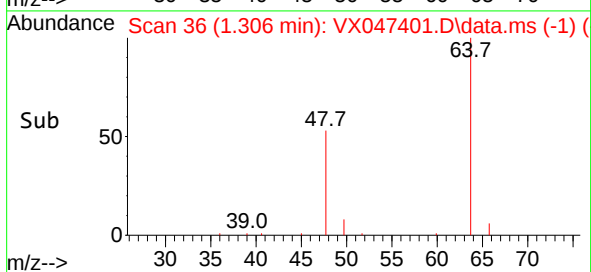
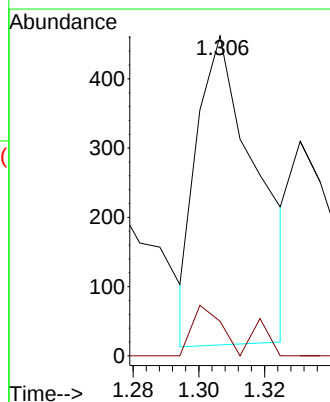
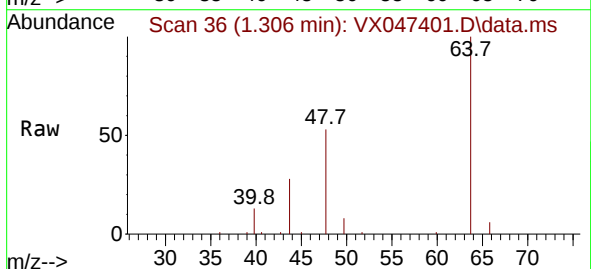


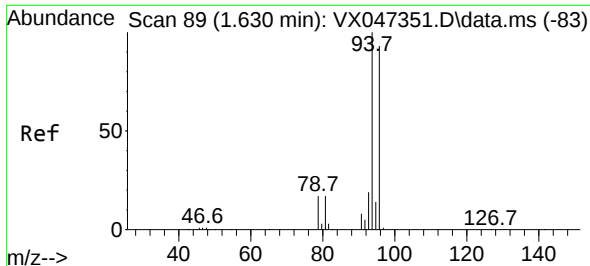

#5
Bromomethane
Concen: 0.716 ug/l
RT: 1.642 min Scan# 91
Delta R.T. 0.012 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion: 94 Resp: 761
Ion Ratio Lower Upper
94 100
96 62.8 74.7 112.1#

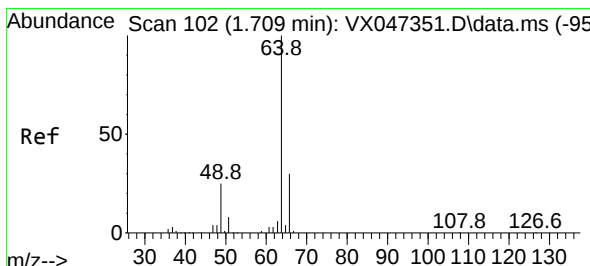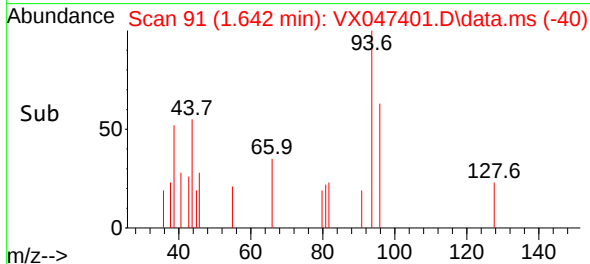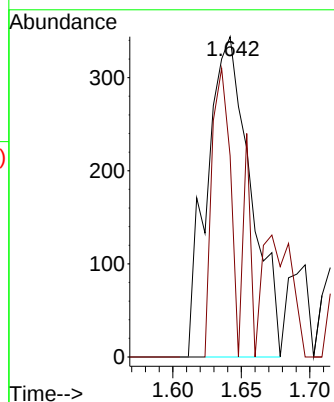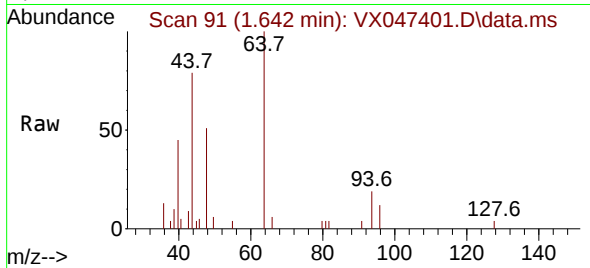

#6
Chloroethane
Concen: 0.207 ug/l
RT: 1.776 min Scan# 113
Delta R.T. 0.067 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion: 64 Resp: 334
Ion Ratio Lower Upper
64 100
66 27.9 24.4 36.6


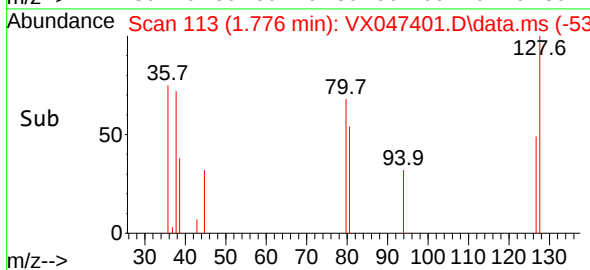
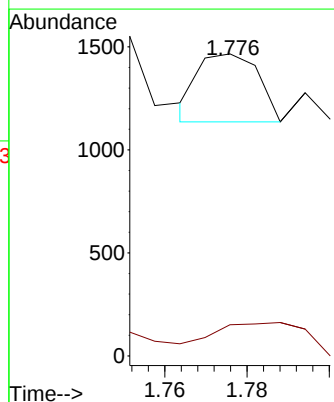
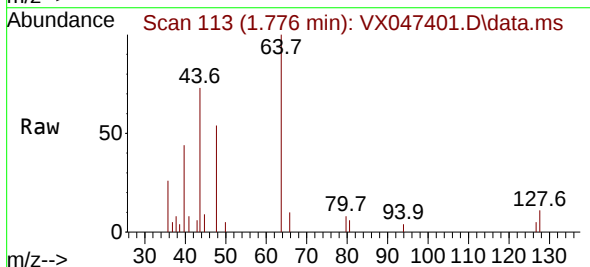


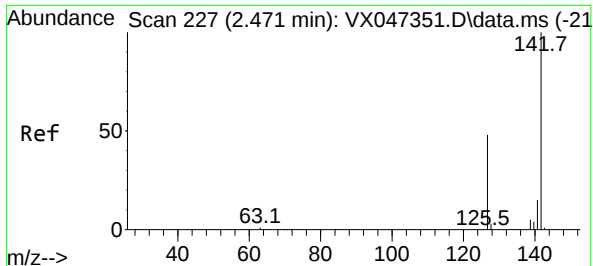

#10
Methyl Iodide
Concen: 1.063 ug/l
RT: 2.483 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion:142 Resp: 4111
Ion Ratio Lower Upper
142 100
127 64.0 36.1 54.1#
141 13.0 11.1 16.7

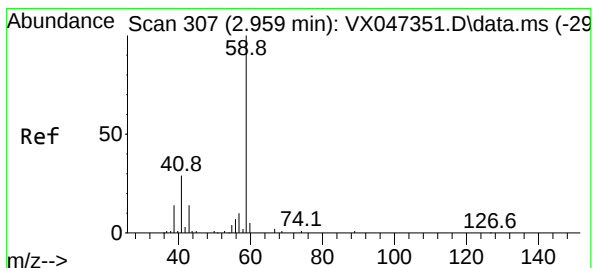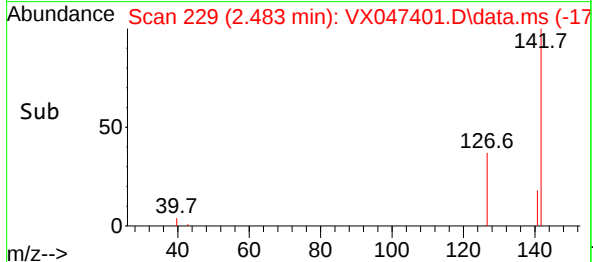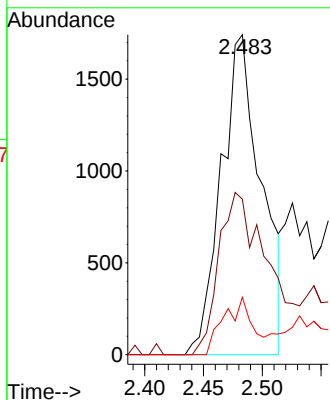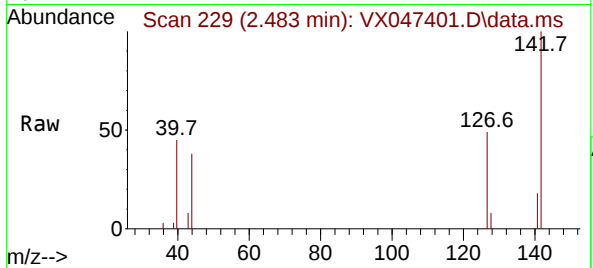

#11
Tert butyl alcohol
Concen: 0.719 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion: 59 Resp: 160
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


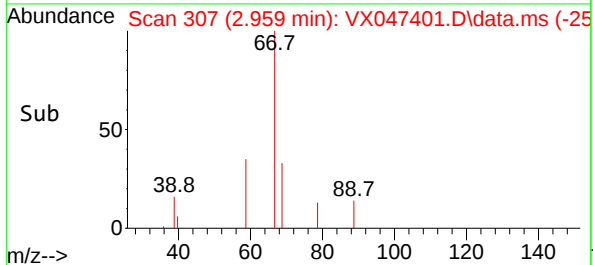
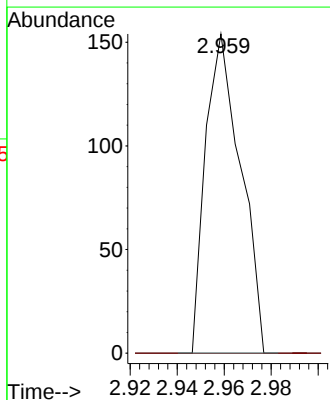
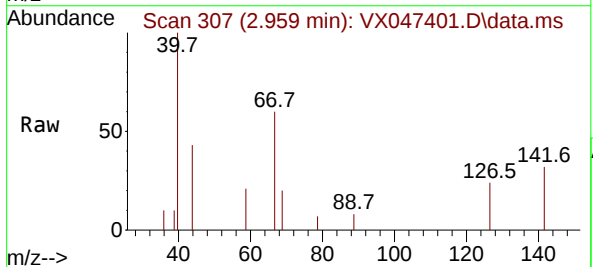




#13
Acrolein
Concen: 0.692 ug/l
RT: 2.251 min Scan# 191
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion: 56 Resp: 325
Ion Ratio Lower Upper
56 100
55 151.4 55.5 83.3#

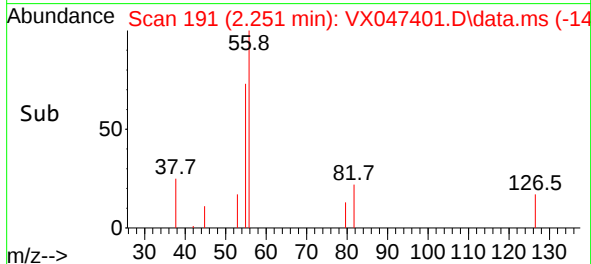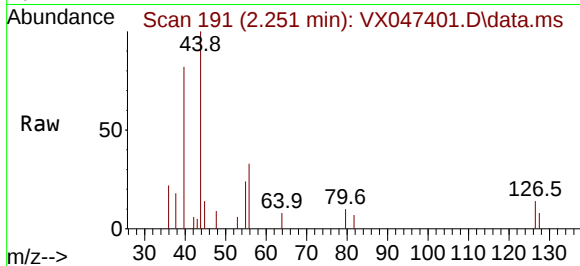

#15
Acrylonitrile
Concen: 0.746 ug/l
RT: 3.093 min Scan# 329
Delta R.T. 0.012 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion: 53 Resp: 802
Ion Ratio Lower Upper
53 100
52 93.3 65.8 98.6
51 11.8 28.2 42.2#


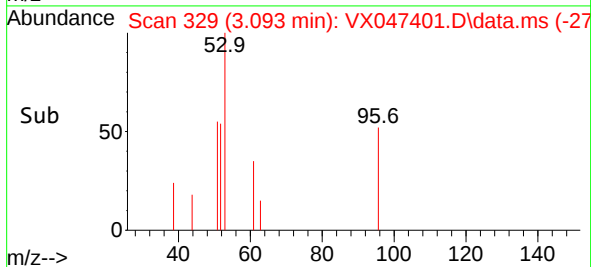

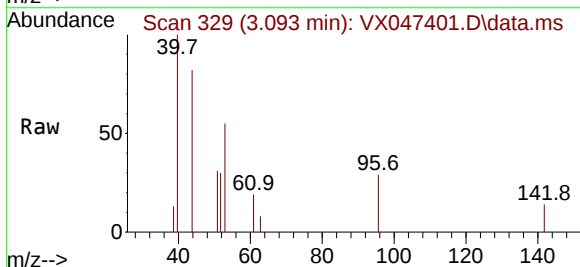




#16
Acetone
Concen: 1.783 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion: 43 Resp: 1714
Ion Ratio Lower Upper
43 100
58 24.9 24.8 37.2

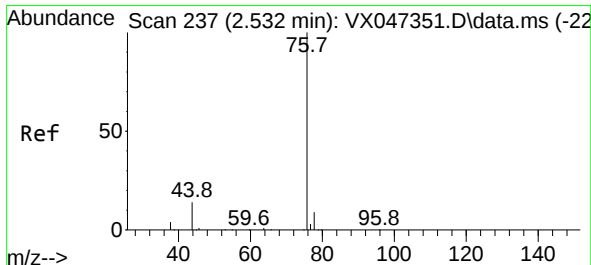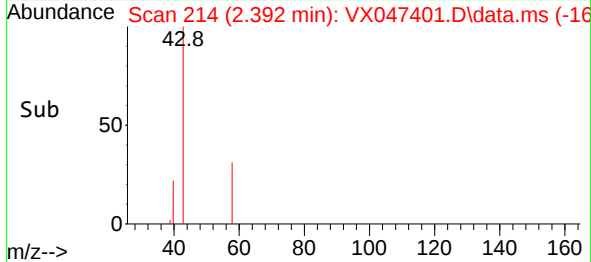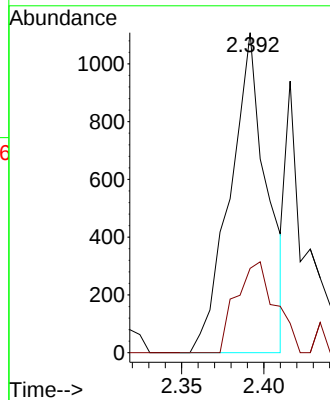

#17
Carbon Disulfide
Concen: 1.044 ug/l
RT: 2.526 min Scan# 236
Delta R.T. -0.006 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion: 76 Resp: 7250
Ion Ratio Lower Upper
76 100
78 9.7 7.2 10.8


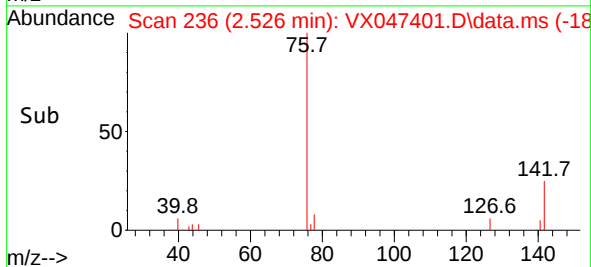
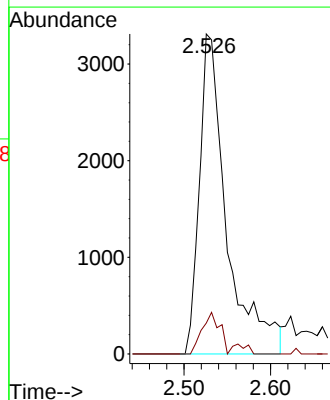
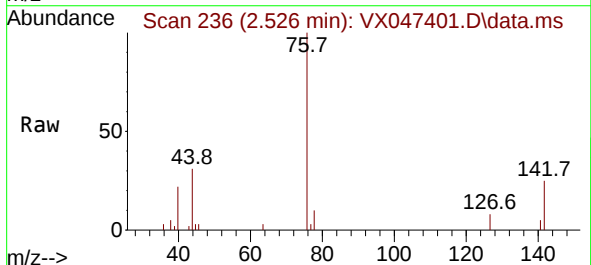




#21
trans-1,2-Dichloroethene
Concen: 0.265 ug/l
RT: 3.105 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion: 96 Resp: 648
Ion Ratio Lower Upper
96 100
61 122.3 112.6 169.0
98 64.4 50.9 76.3

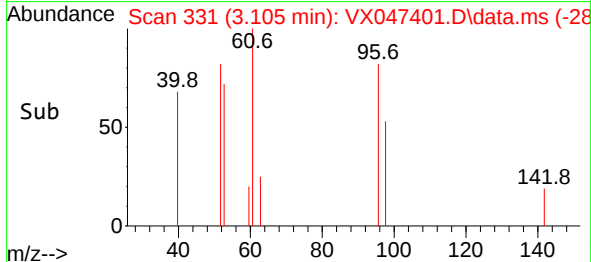

#29
Tetrahydrofuran
Concen: 0.265 ug/l
RT: 5.074 min Scan# 654
Delta R.T. 0.049 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion: 42 Resp: 216
Ion Ratio Lower Upper
42 100
72 0.0 34.6 51.8#
71 14.8 32.6 49.0#

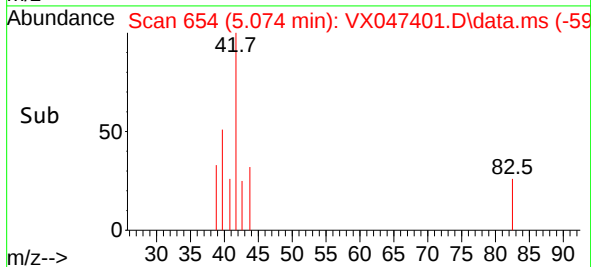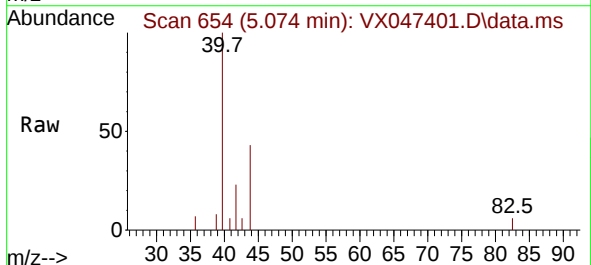



#33

1,2-Dichloroethane-d4

Concen: 57.763 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX047401.D

Acq: 19 Aug 2025 10:05

Instrument :

MSVOA_X

ClientSampleId :





VX0819MBL01

Tgt Ion: 65 Resp: 147768

Ion Ratio Lower Upper

65 100

67 51.9 0.0 106.0

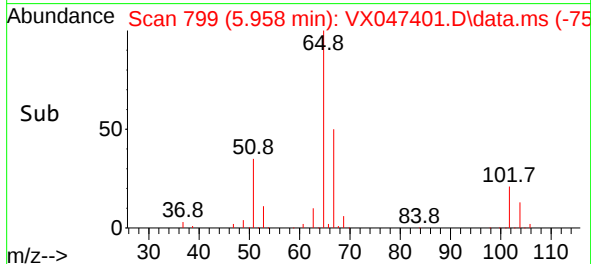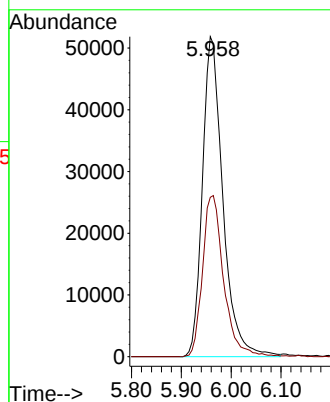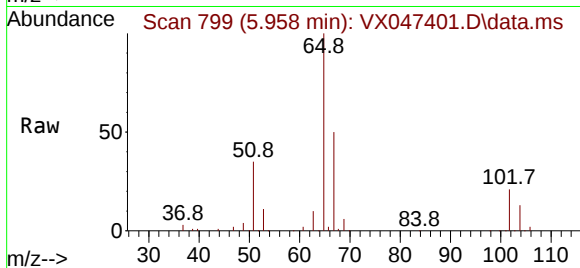

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX047401.D

Acq: 19 Aug 2025 10:05




Tgt Ion: 114 Resp: 363576


Ion Ratio Lower Upper

114 100

63 22.2 0.0 42.4

88 15.7 0.0 33.0


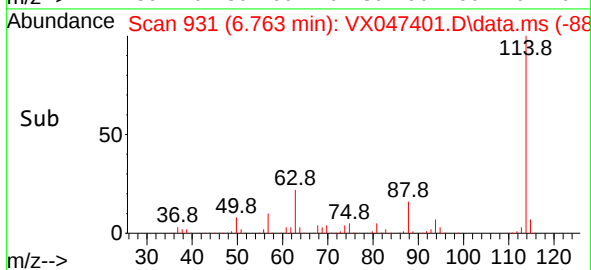
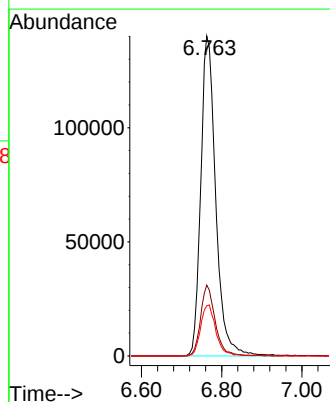
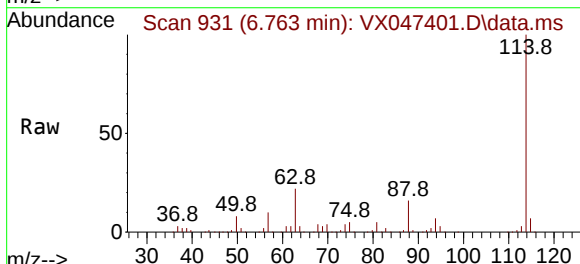




#35
Dibromofluoromethane
Concen: 54.134 ug/l
RT: 5.397 min Scan# 707
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion:113 Resp: 127737
Ion Ratio Lower Upper
113 100
111 102.6 81.4 122.2
192 17.8 14.1 21.1

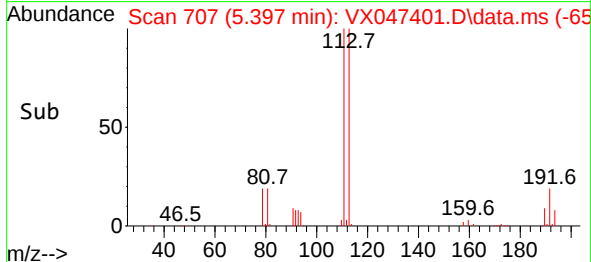

#38
Carbon Tetrachloride
Concen: 4.895 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion:117 Resp: 19923
Ion Ratio Lower Upper
117 100
119 3.7 78.5 117.7#
121 0.0 24.7 37.1#

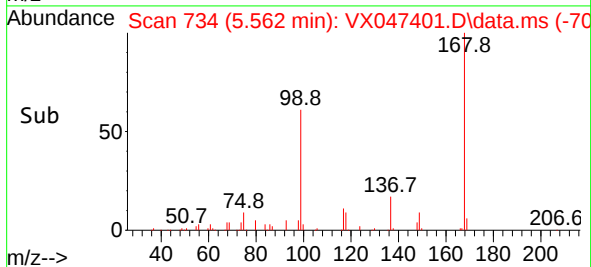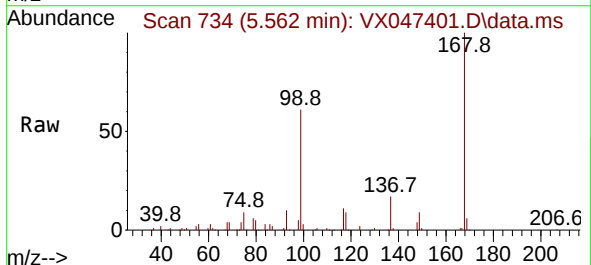

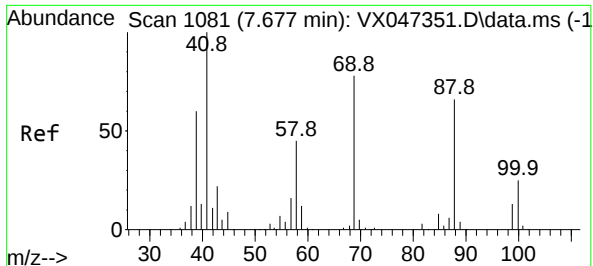

#49

1,4-Dioxane

Concen: 2.354 ug/l

RT: 7.708 min Scan# 1

Delta R.T. 0.030 min

Lab File: VX047401.D

Acq: 19 Aug 2025 10:05

Instrument :

MSVOA_X

ClientSampleId :

VX0819MBL01





Tgt Ion: 88 Resp: 66

Ion Ratio Lower Upper

88 100

43 293.9 32.4 48.6#

58 0.0 56.9 85.3#

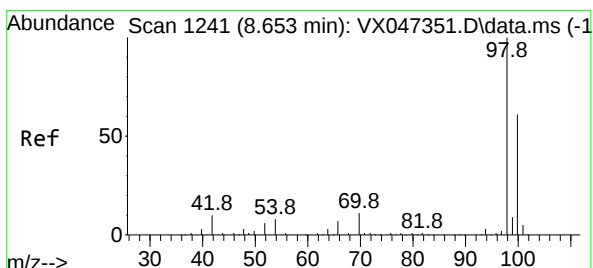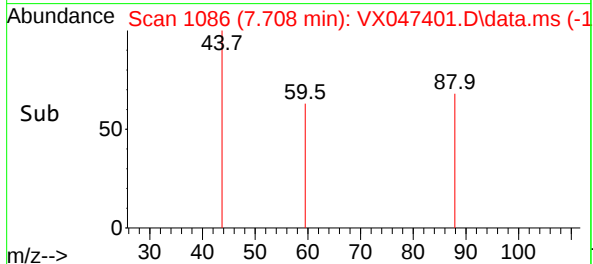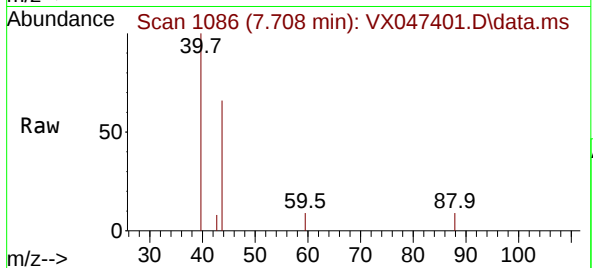

#50

Toluene-d8

Concen: 53.122 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX047401.D




Acq: 19 Aug 2025 10:05


Tgt Ion: 98 Resp: 448031

Ion Ratio Lower Upper

98 100

100 66.4 53.9 80.9

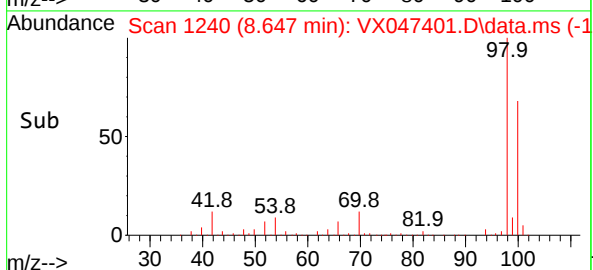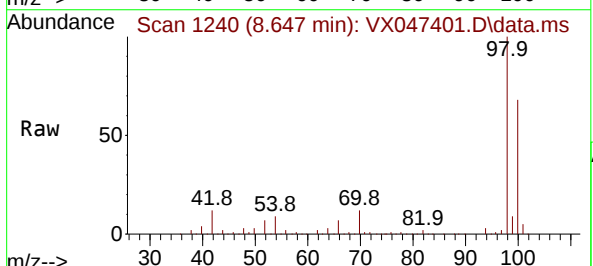

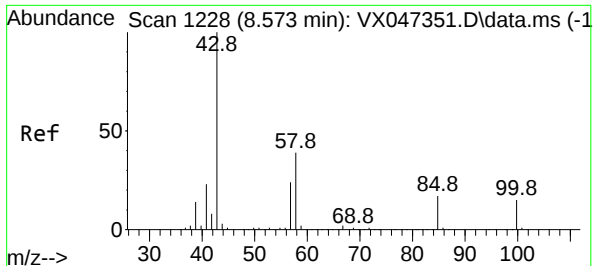

#51

4-Methyl-2-Pentanone

Concen: 0.438 ug/l

RT: 8.579 min Scan# 1180

Delta R.T. 0.006 min

Lab File: VX047401.D

Acq: 19 Aug 2025 10:05

Instrument :

MSVOA_X

ClientSampleId :





VX0819MBL01

Tgt Ion: 43 Resp: 1399

Ion Ratio Lower Upper

43 100

58 18.2 31.2 46.8#

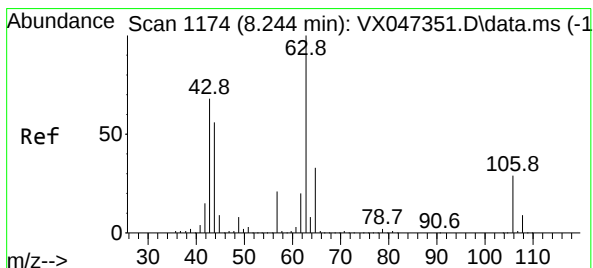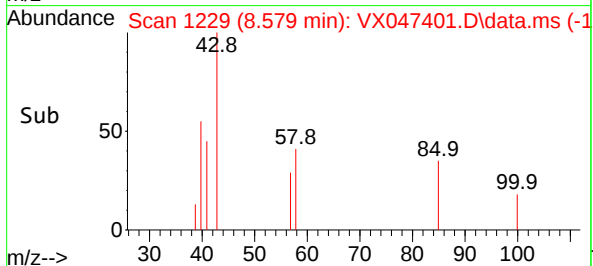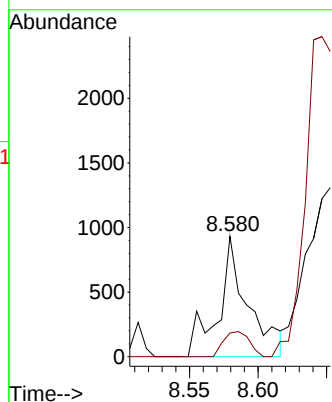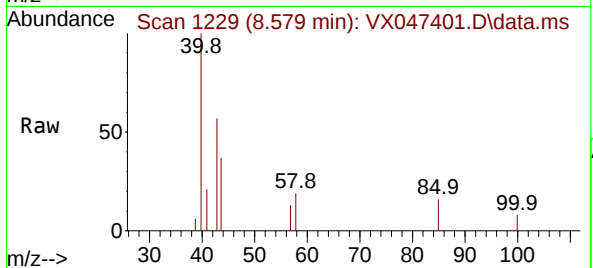

#58

2-Chloroethyl Vinyl ether

Concen: 8.502 ug/l

RT: 8.281 min Scan# 1180

Delta R.T. 0.037 min

Lab File: VX047401.D




Acq: 19 Aug 2025 10:05


Tgt Ion: 63 Resp: 280

Ion Ratio Lower Upper

63 100

106 0.0 22.8 34.2#


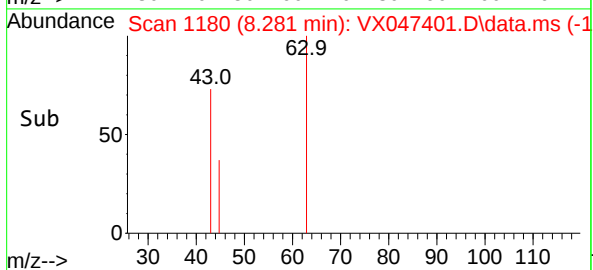
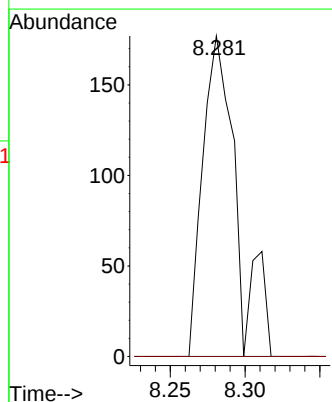
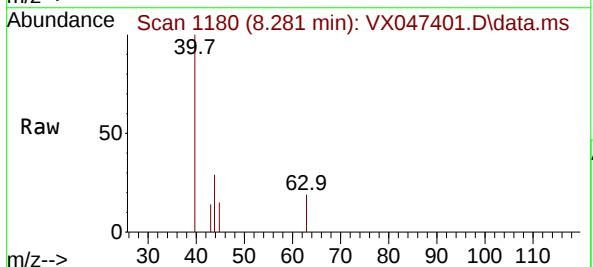




#62
4-Bromofluorobenzene
Concen: 59.177 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion: 95 Resp: 184176
Ion Ratio Lower Upper
95 100
174 73.8 0.0 148.0
176 69.9 0.0 145.4

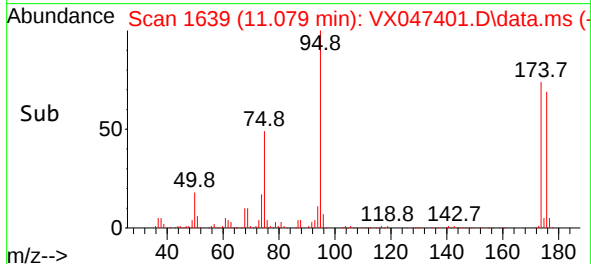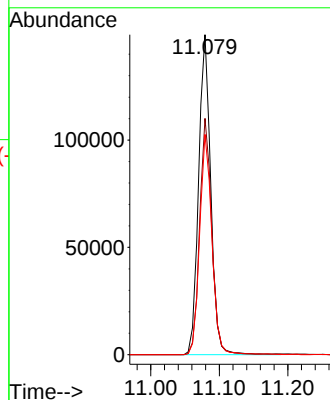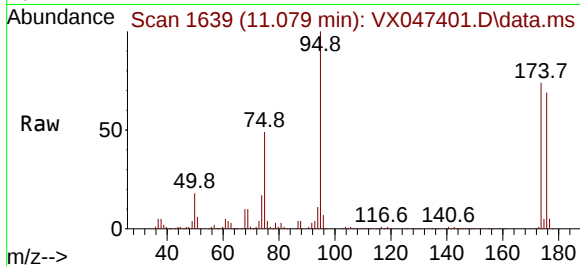

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05


Tgt Ion: 117 Resp: 362613
Ion Ratio Lower Upper
117 100
82 53.6 45.0 67.4
119 31.4 25.8 38.8

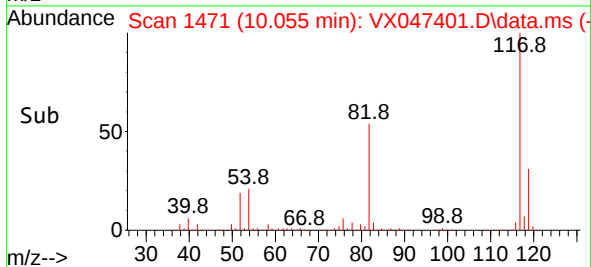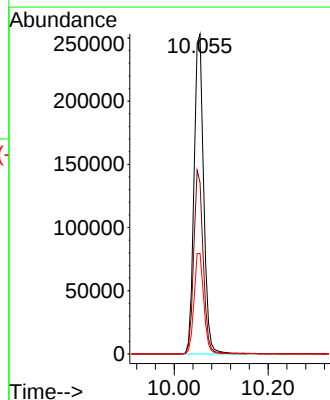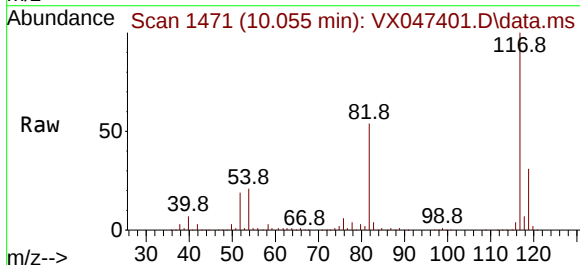






#64
Tetrachloroethene
Concen: 0.201 ug/l
RT: 9.281 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05


Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01

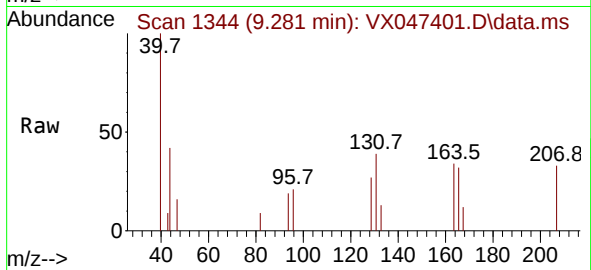



Tgt Ion:164 Resp: 526
Ion Ratio Lower Upper
164 100
166 95.2 100.3 150.5#
129 78.7 77.7 116.5
131 115.9 74.8 112.2#

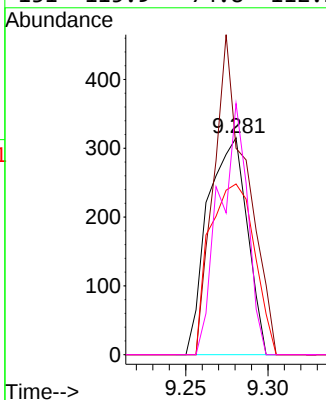


#68
m/p-Xylenes
Concen: 0.286 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

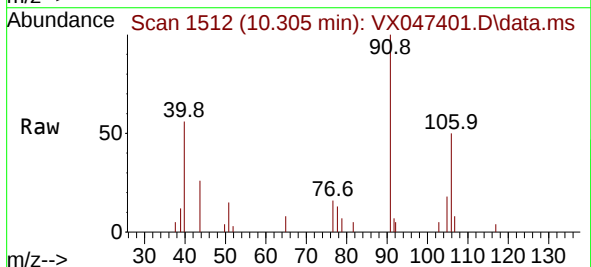

Tgt Ion:106 Resp: 1579
Ion Ratio Lower Upper
106 100
91 221.3 164.7 247.1



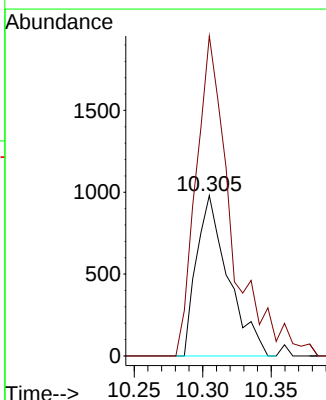





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion:152 Resp: 179617
Ion Ratio Lower Upper
152 100
115 62.2 44.6 133.8
150 154.1 0.0 349.8

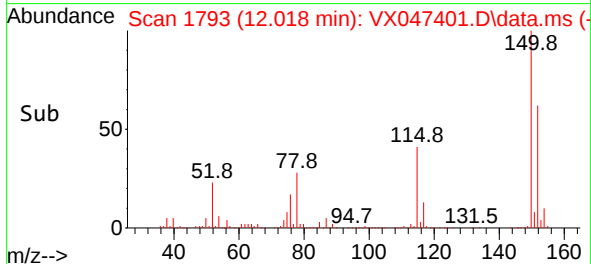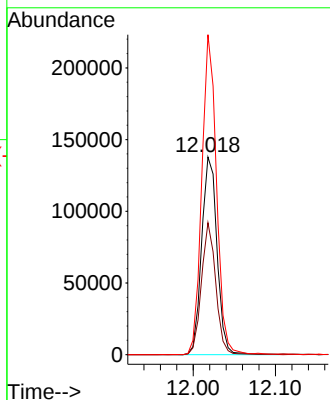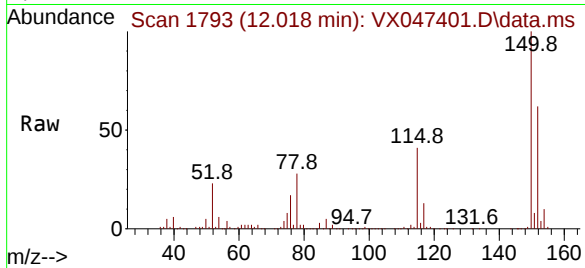

#76
1,2,3-Trichloropropane
Concen: 28.648 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion: 75 Resp: 94378
Ion Ratio Lower Upper
75 100
77 0.9 19.4 58.2#



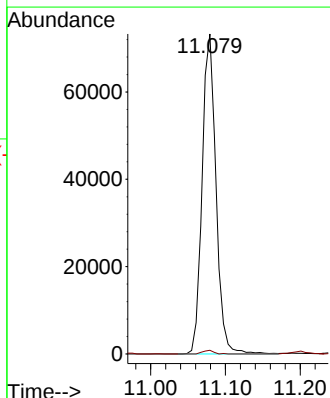
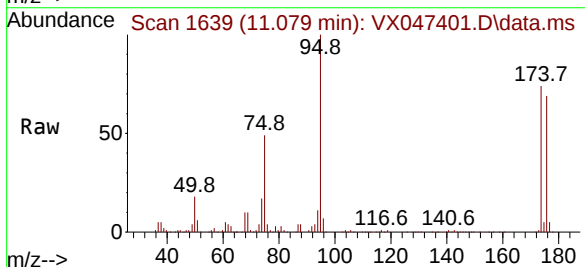


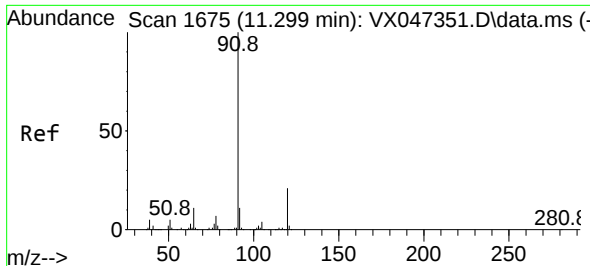

#78
n-propylbenzene
Concen: 0.205 ug/l
RT: 11.311 min Scan# 1675
Delta R.T. 0.012 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion: 91 Resp: 3447
Ion Ratio Lower Upper
91 100
120 24.7 11.0 33.0

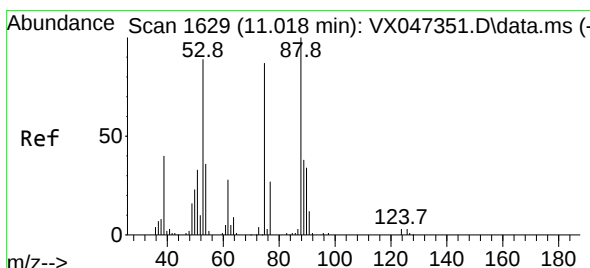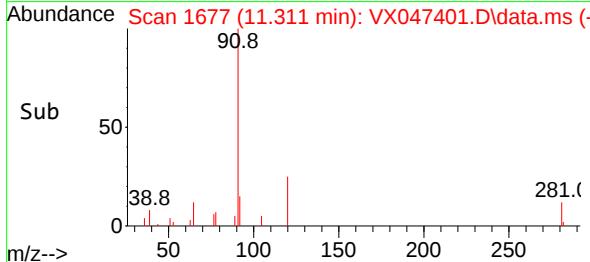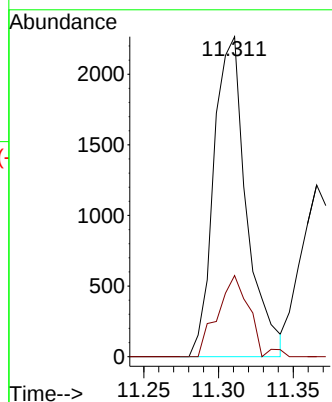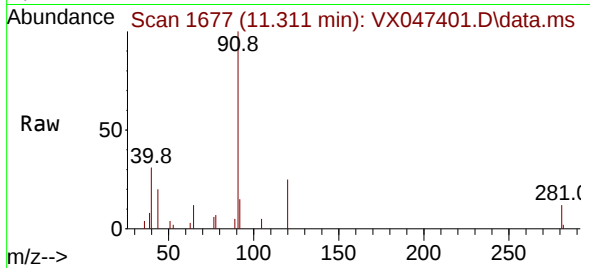

#81
trans-1,4-Dichloro-2-butene
Concen: 112.805 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion: 75 Resp: 94378
Ion Ratio Lower Upper
75 100
53 0.0 85.2 127.8#
89 0.0 36.7 55.1#


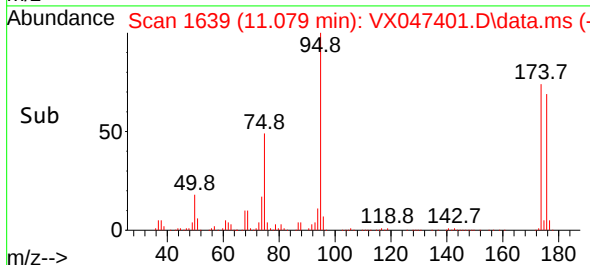

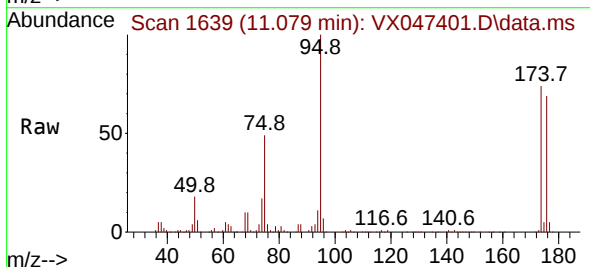




#85
 sec-Butylbenzene
 Concen: 0.300 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. -0.000 min
 Lab File: VX047401.D
 Acq: 19 Aug 2025 10:05




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0819MBL01


Tgt Ion:105 Resp: 4291
 Ion Ratio Lower Upper
 105 100
 134 23.1 9.8 29.5

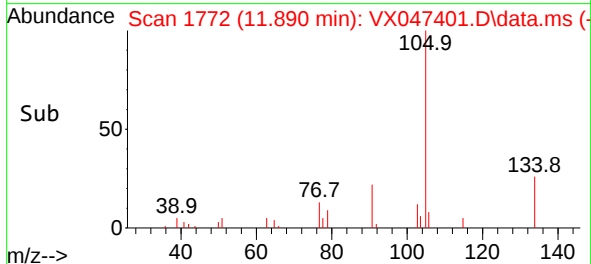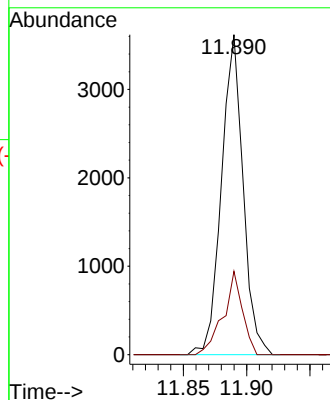

#86
 p-Isopropyltoluene
 Concen: 0.350 ug/l
 RT: 12.006 min Scan# 1791
 Delta R.T. -0.000 min
 Lab File: VX047401.D
 Acq: 19 Aug 2025 10:05

Tgt Ion:119 Resp: 4237
 Ion Ratio Lower Upper
 119 100
 134 21.2 12.8 38.4
 91 29.3 12.4 37.4



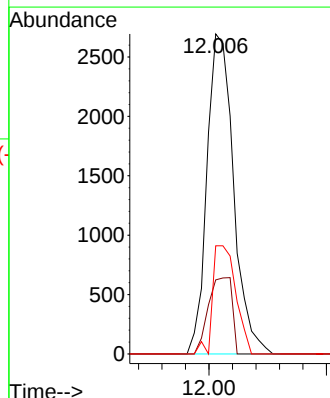
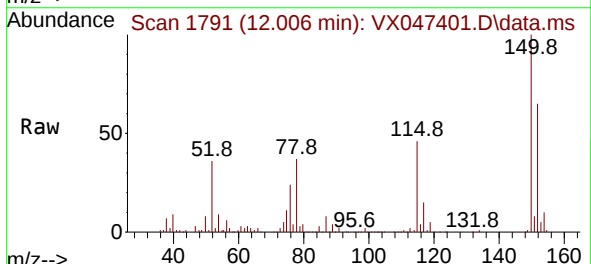




#87
1,3-Dichlorobenzene
Concen: 0.292 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion:146 Resp: 1916
Ion Ratio Lower Upper
146 100
111 44.8 20.6 61.8
148 54.0 31.9 95.5

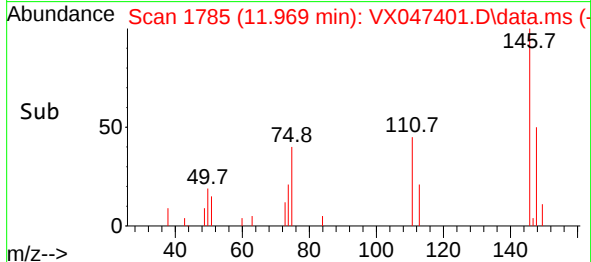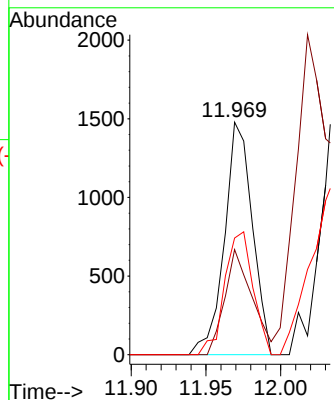

#88
1,4-Dichlorobenzene
Concen: 0.284 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.067 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05

Tgt Ion:146 Resp: 1916
Ion Ratio Lower Upper
146 100
111 44.8 20.4 61.2
148 54.0 31.7 95.1

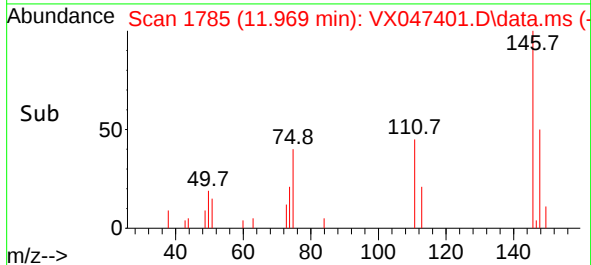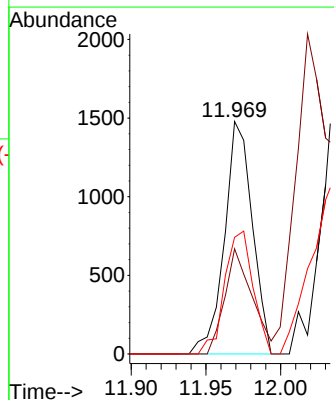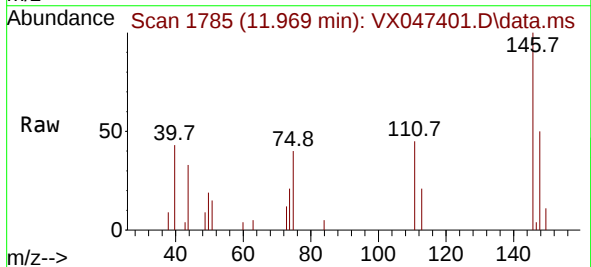



#89

n-Butylbenzene

Concen: 0.537 ug/l

RT: 12.335 min Scan# 1844

Delta R.T. 0.006 min

Lab File: VX047401.D

Acq: 19 Aug 2025 10:05

Instrument :

MSVOA_X

ClientSampleId :

VX0819MBL01





Tgt Ion: 91 Resp: 6042

Ion Ratio Lower Upper

91 100

92 47.6 27.2 81.5

134 21.8 12.6 37.8

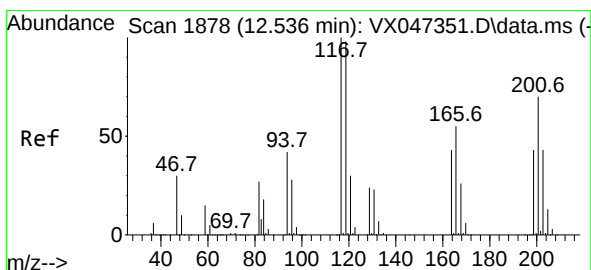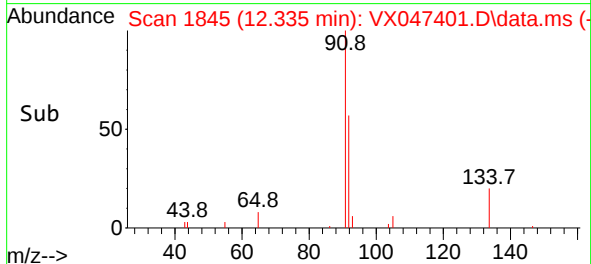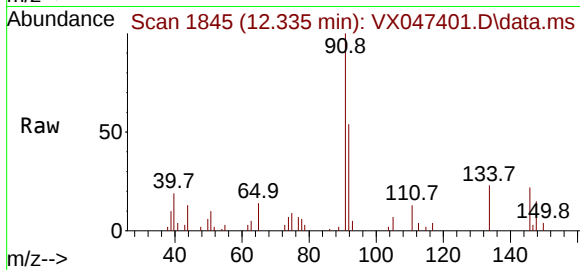

#90

Hexachloroethane

Concen: 0.271 ug/l

RT: 12.542 min Scan# 1879

Delta R.T. 0.006 min

Lab File: VX047401.D




Acq: 19 Aug 2025 10:05


Tgt Ion: 117 Resp: 575

Ion Ratio Lower Upper

117 100

201 80.9 35.1 105.3


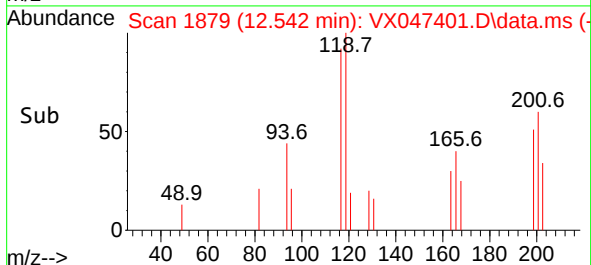

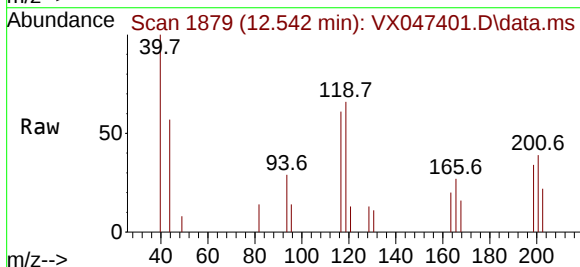




#91
 1,2-Dichlorobenzene
 Concen: 0.218 ug/l
 RT: 12.341 min Scan# 1846
 Delta R.T. 0.006 min
 Lab File: VX047401.D
 Acq: 19 Aug 2025 10:05




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0819MBL01


Tgt Ion:	146	Resp:	1358
Ion	Ratio	Lower	Upper
146	100		
111	48.8	22.1	66.1
148	63.7	31.9	95.5

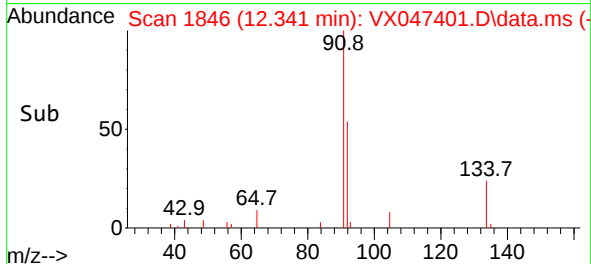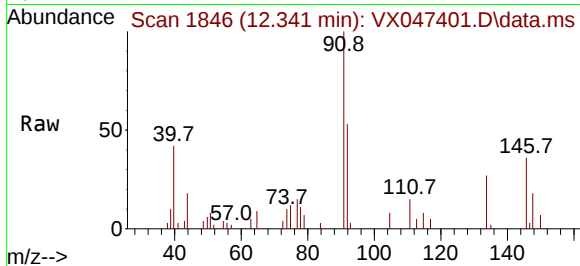

#93
 1,2,4-Trichlorobenzene
 Concen: 0.805 ug/l
 RT: 13.591 min Scan# 2051
 Delta R.T. 0.006 min
 Lab File: VX047401.D
 Acq: 19 Aug 2025 10:05

Tgt Ion:	180	Resp:	3359
Ion	Ratio	Lower	Upper
180	100		
182	92.9	48.1	144.4
145	33.7	16.2	48.5


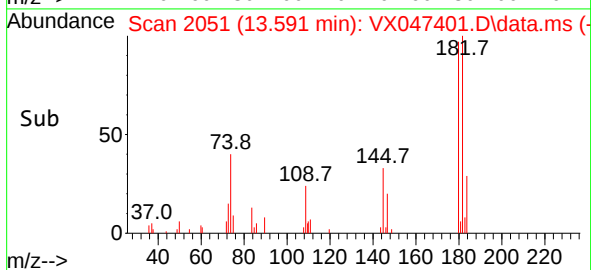

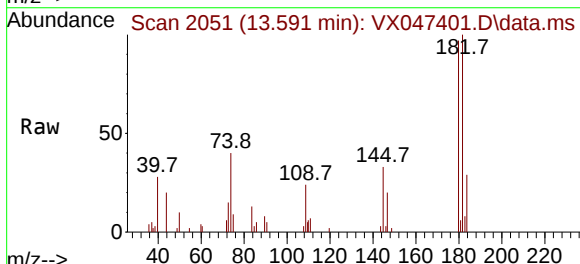




#94
Hexachlorobutadiene
Concen: 3.271 ug/l
RT: 13.719 min Scan# 2072
Delta R.T. -0.006 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05




Instrument :
MSVOA_X
ClientSampleId :
VX0819MBL01


Tgt Ion:225 Resp: 4858
Ion Ratio Lower Upper
225 100
223 65.3 32.2 96.6
227 62.5 31.6 95.0

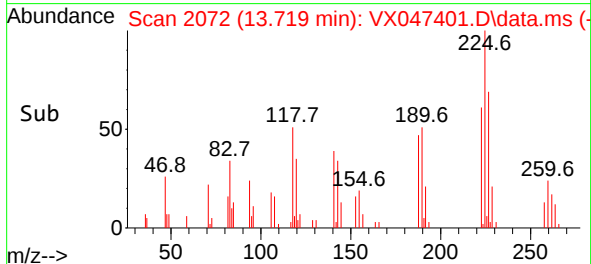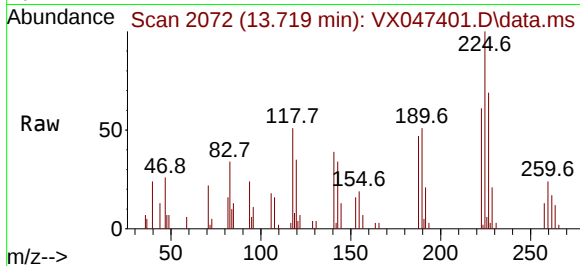

#95
Naphthalene
Concen: 0.561 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX047401.D
Acq: 19 Aug 2025 10:05


Tgt Ion:128 Resp: 6687
Ion Ratio Lower Upper
128 100
127 11.9 10.1 15.1
129 10.9 8.7 13.1

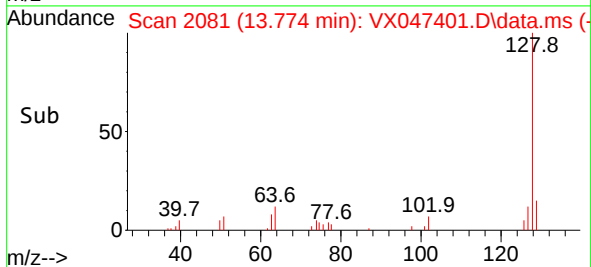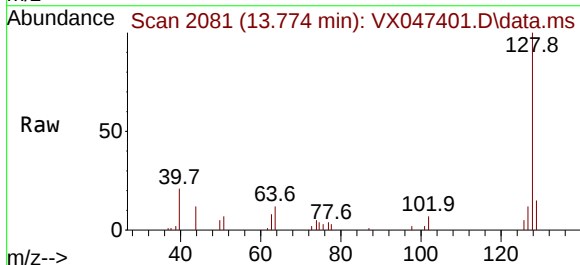



#96
 1,2,3-Trichlorobenzene
 Concen: 0.808 ug/l
 RT: 13.963 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX047401.D
 Acq: 19 Aug 2025 10:05

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0819MBL01

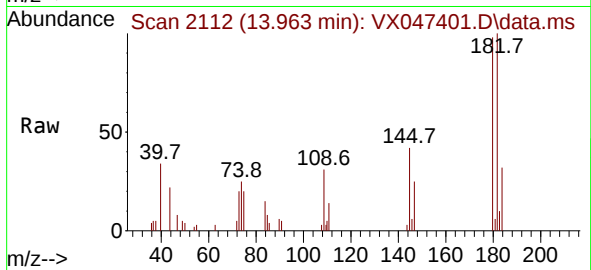

Tgt Ion:180 Resp: 3176

Ion	Ratio	Lower	Upper
180	100		
182	101.5	48.0	144.2
145	34.6	17.4	52.2

