

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081925\
 Data File : VX047417.D
 Acq On : 19 Aug 2025 16:57
 Operator : JC/MD
 Sample : Q2869-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB02-081325

Quant Time: Aug 20 01:29:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	205773	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	414097	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	417583	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	212656	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	164219	57.023	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	114.040%
35) Dibromofluoromethane	5.397	113	137119	51.021	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.040%
50) Toluene-d8	8.653	98	483216	50.304	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.600%
62) 4-Bromofluorobenzene	11.079	95	199041	56.150	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	112.300%
Target Compounds						
16) Acetone	2.398	43	8905	8.226	ug/l	Qvalue # 84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081925\
Data File : VX047417.D
Acq On : 19 Aug 2025 16:57
Operator : JC/MD
Sample : Q2869-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB02-081325

Quant Time: Aug 20 01:29:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration




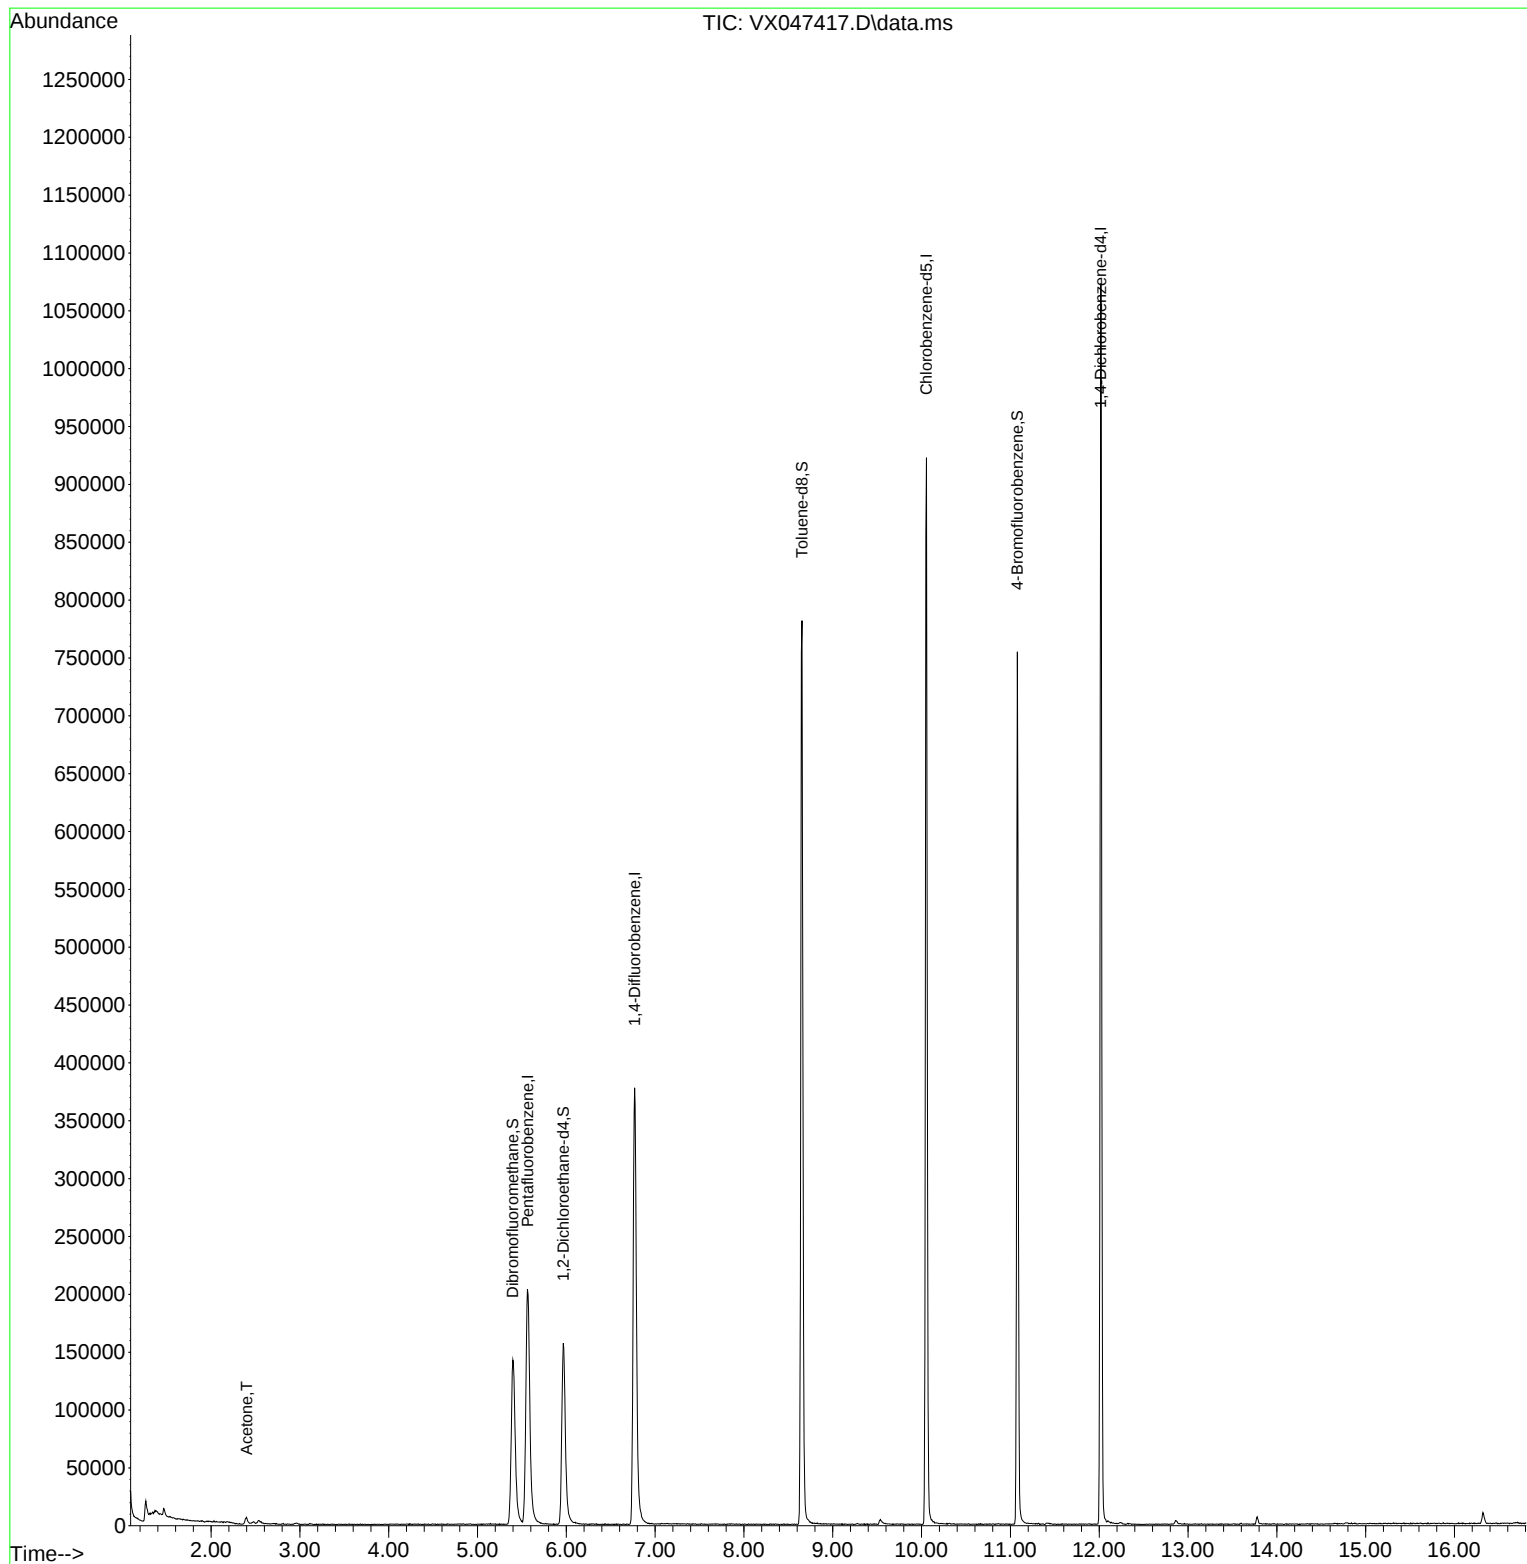




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX047417.D
Acq: 19 Aug 2025 16:57




Instrument :
MSVOA_X
ClientSampleId :
EB02-081325


Tgt Ion:168 Resp: 205773
Ion Ratio Lower Upper
168 100
99 63.7 47.9 71.9

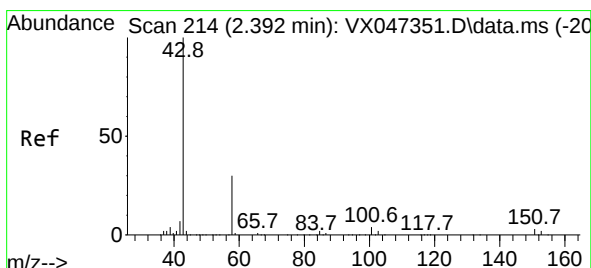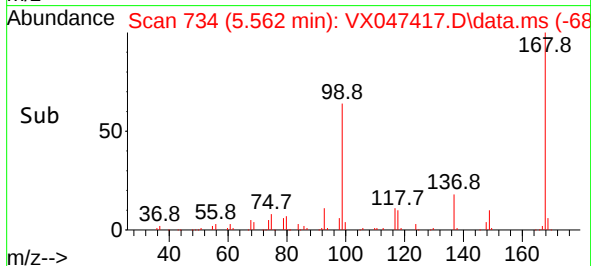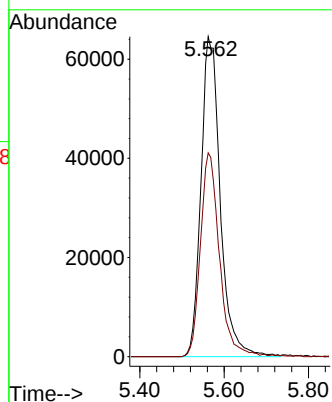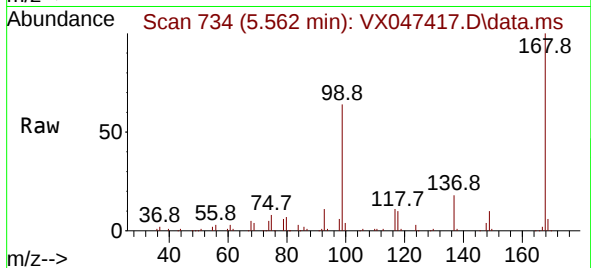

#16
Acetone
Concen: 8.226 ug/l
RT: 2.398 min Scan# 215
Delta R.T. 0.006 min
Lab File: VX047417.D
Acq: 19 Aug 2025 16:57

Tgt Ion: 43 Resp: 8905
Ion Ratio Lower Upper
43 100
58 40.0 24.8 37.2#

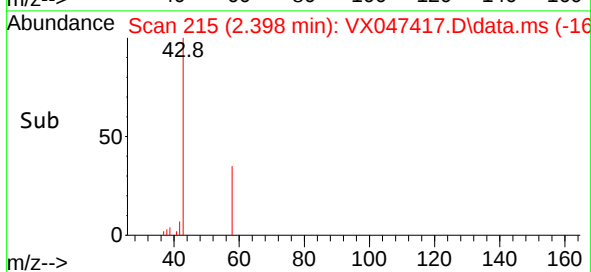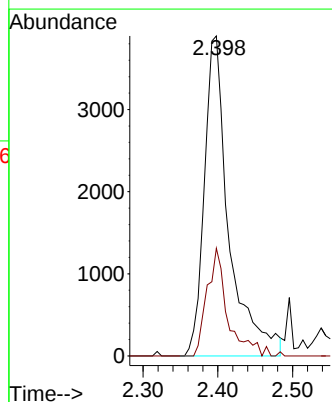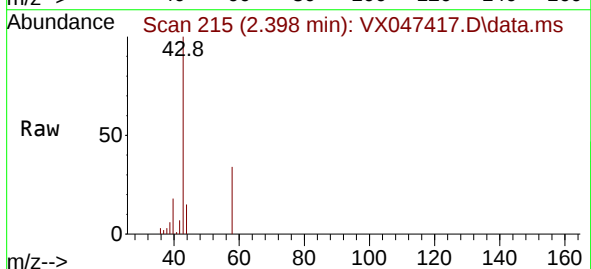

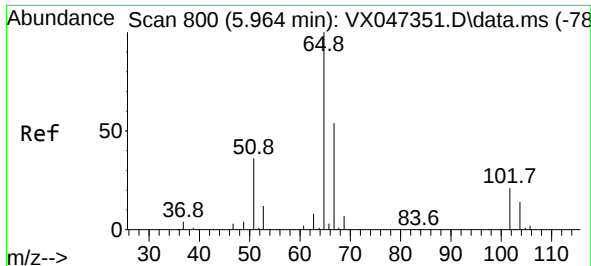

#33

1,2-Dichloroethane-d4

Concen: 57.023 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX047417.D

Acq: 19 Aug 2025 16:57

Instrument :

MSVOA_X

ClientSampleId :





EB02-081325

Tgt Ion: 65 Resp: 164219

Ion Ratio Lower Upper

65 100

67 51.8 0.0 106.0

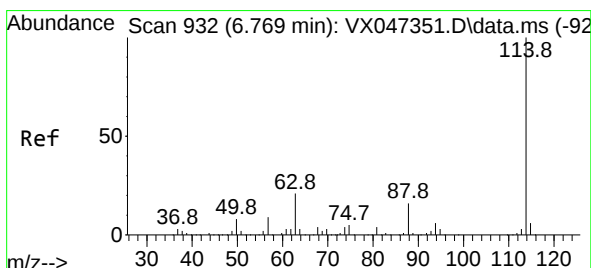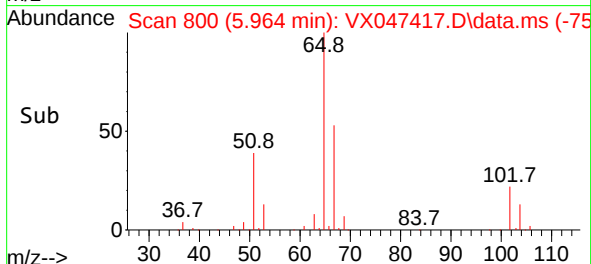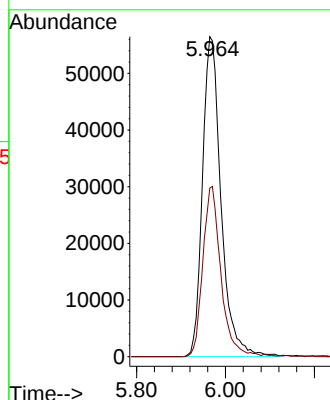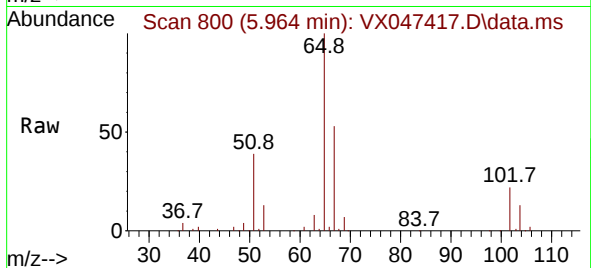

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX047417.D

Acq: 19 Aug 2025 16:57




Tgt Ion: 114 Resp: 414097


Ion Ratio Lower Upper

114 100

63 24.8 0.0 42.4


88 15.9 0.0 33.0

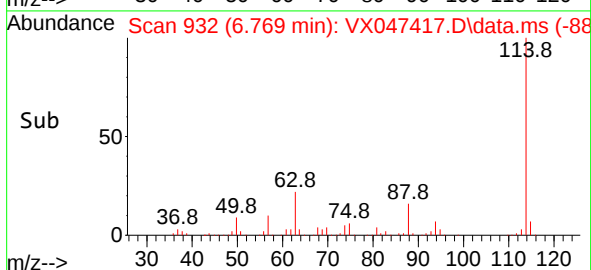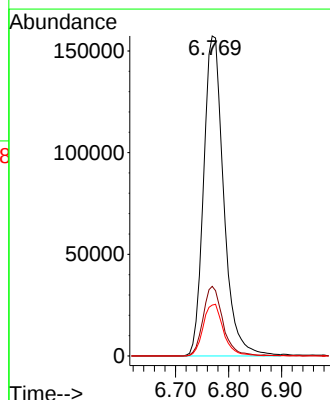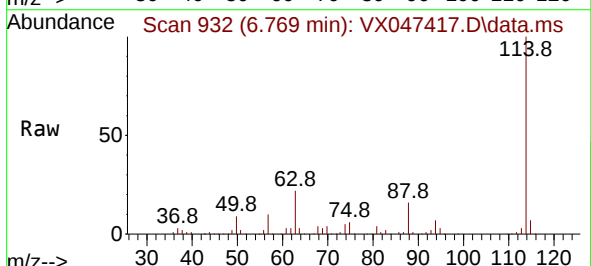



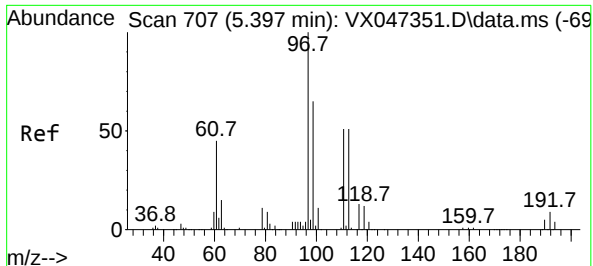


#35
Dibromofluoromethane
Concen: 51.021 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX047417.D
Acq: 19 Aug 2025 16:57

Instrument :
MSVOA_X
ClientSampleId :
EB02-081325



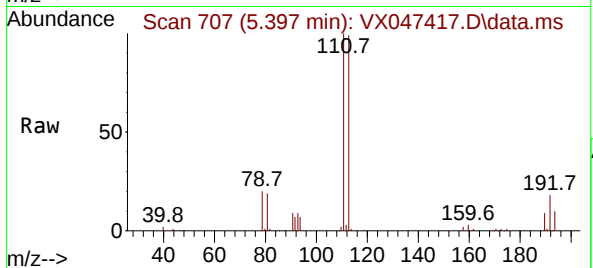



Tgt Ion:113 Resp: 137119
Ion Ratio Lower Upper
113 100
111 102.6 81.4 122.2
192 17.8 14.1 21.1

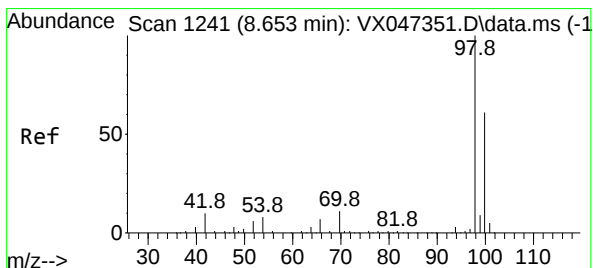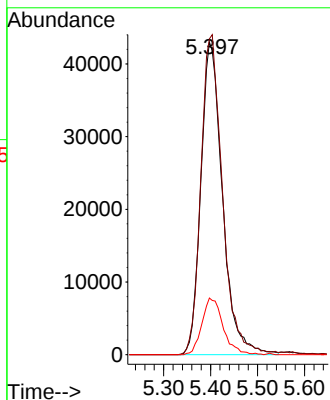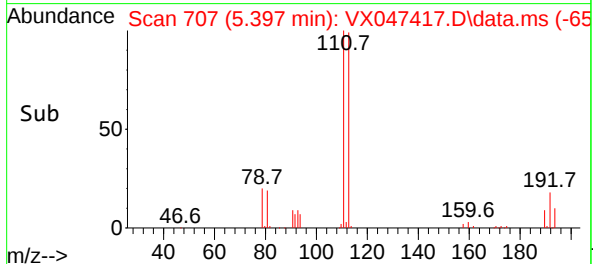

#50
Toluene-d8
Concen: 50.304 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX047417.D
Acq: 19 Aug 2025 16:57

Tgt Ion: 98 Resp: 483216
Ion Ratio Lower Upper
98 100
100 66.8 53.9 80.9


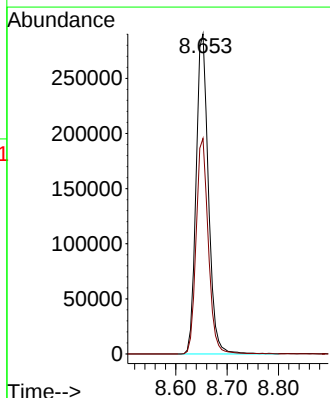
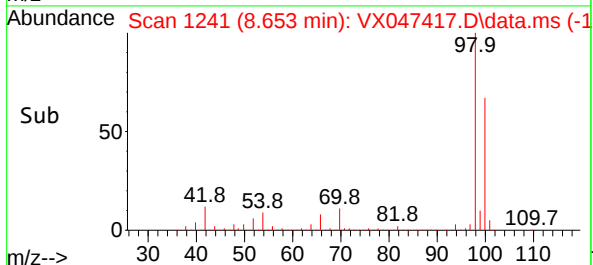
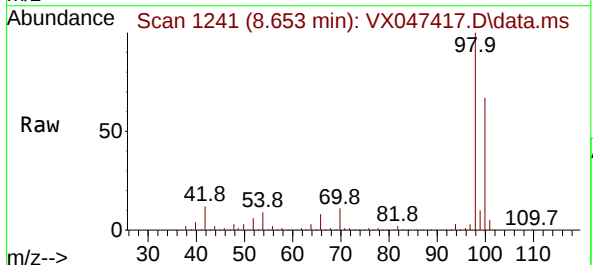


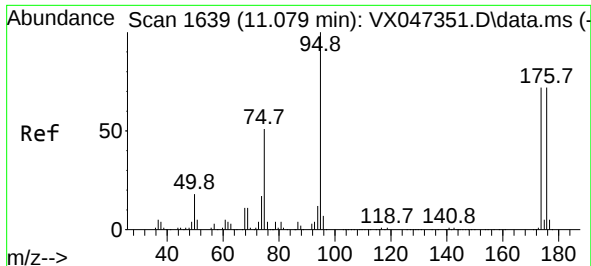

#62
4-Bromofluorobenzene
Concen: 56.150 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047417.D
Acq: 19 Aug 2025 16:57




Instrument :
MSVOA_X
ClientSampleId :
EB02-081325


Tgt Ion: 95 Resp: 199041
Ion Ratio Lower Upper
95 100
174 74.0 0.0 148.0
176 70.7 0.0 145.4

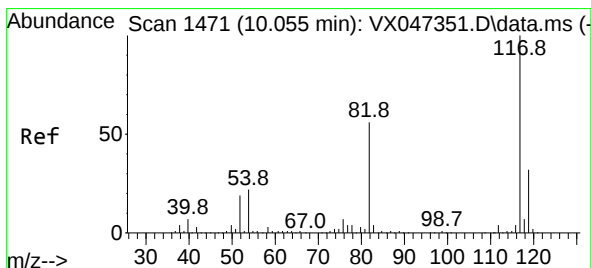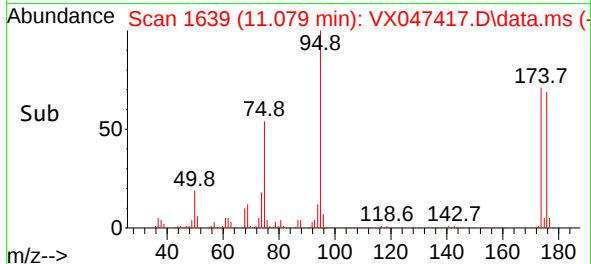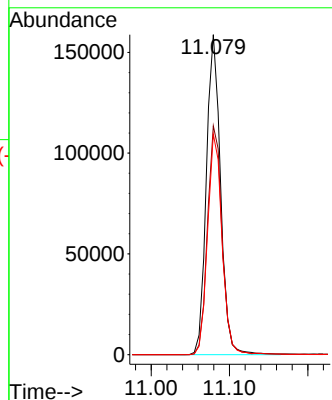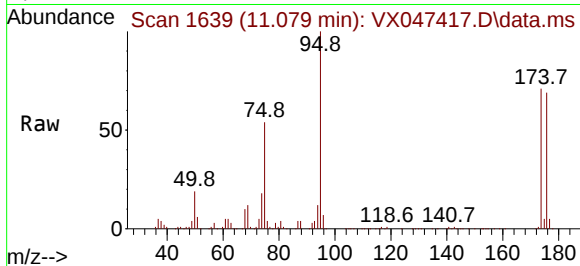

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX047417.D
Acq: 19 Aug 2025 16:57


Tgt Ion: 117 Resp: 417583
Ion Ratio Lower Upper
117 100
82 56.5 45.0 67.4
119 32.2 25.8 38.8

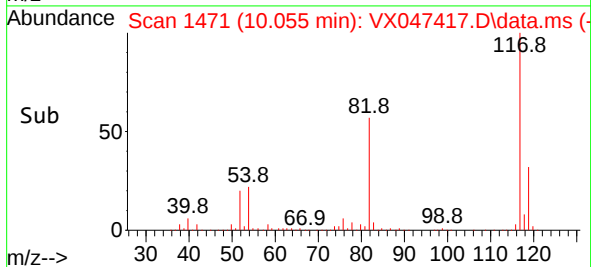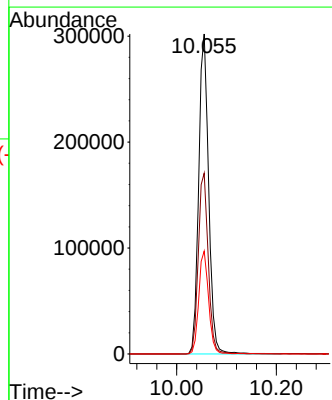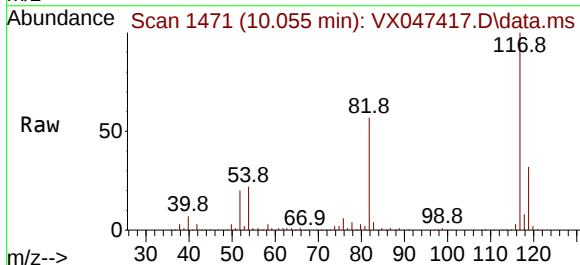

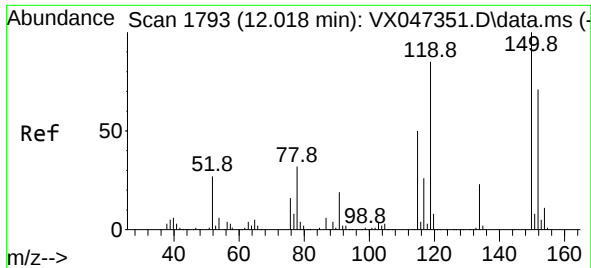

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX047417.D
 Acq: 19 Aug 2025 16:57

Instrument :
 MSVOA_X
 ClientSampleId :
 EB02-081325

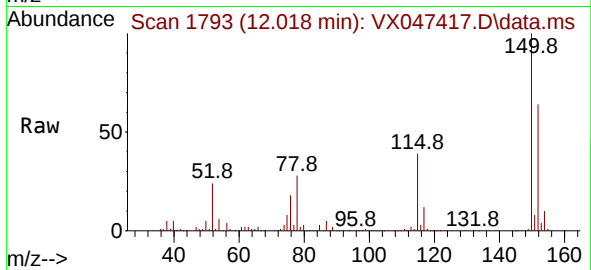

Tgt Ion:152 Resp: 212656
 Ion Ratio Lower Upper
 152 100
 115 61.8 44.6 133.8
 150 158.1 0.0 349.8

