

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081925\
 Data File : VX047418.D
 Acq On : 19 Aug 2025 17:18
 Operator : JC/MD
 Sample : Q2869-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB01-081325

Quant Time: Aug 20 01:30:04 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	204851	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	415100	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	420679	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	219893	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	167900	58.564	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 117.120%#	
35) Dibromofluoromethane	5.397	113	134098	49.776	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 99.560%	
50) Toluene-d8	8.653	98	464326	48.221	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 96.440%	
62) 4-Bromofluorobenzene	11.079	95	198402	55.835	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 111.660%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081925\
Data File : VX047418.D
Acq On : 19 Aug 2025 17:18
Operator : JC/MD
Sample : Q2869-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB01-081325


Quant Time: Aug 20 01:30:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration

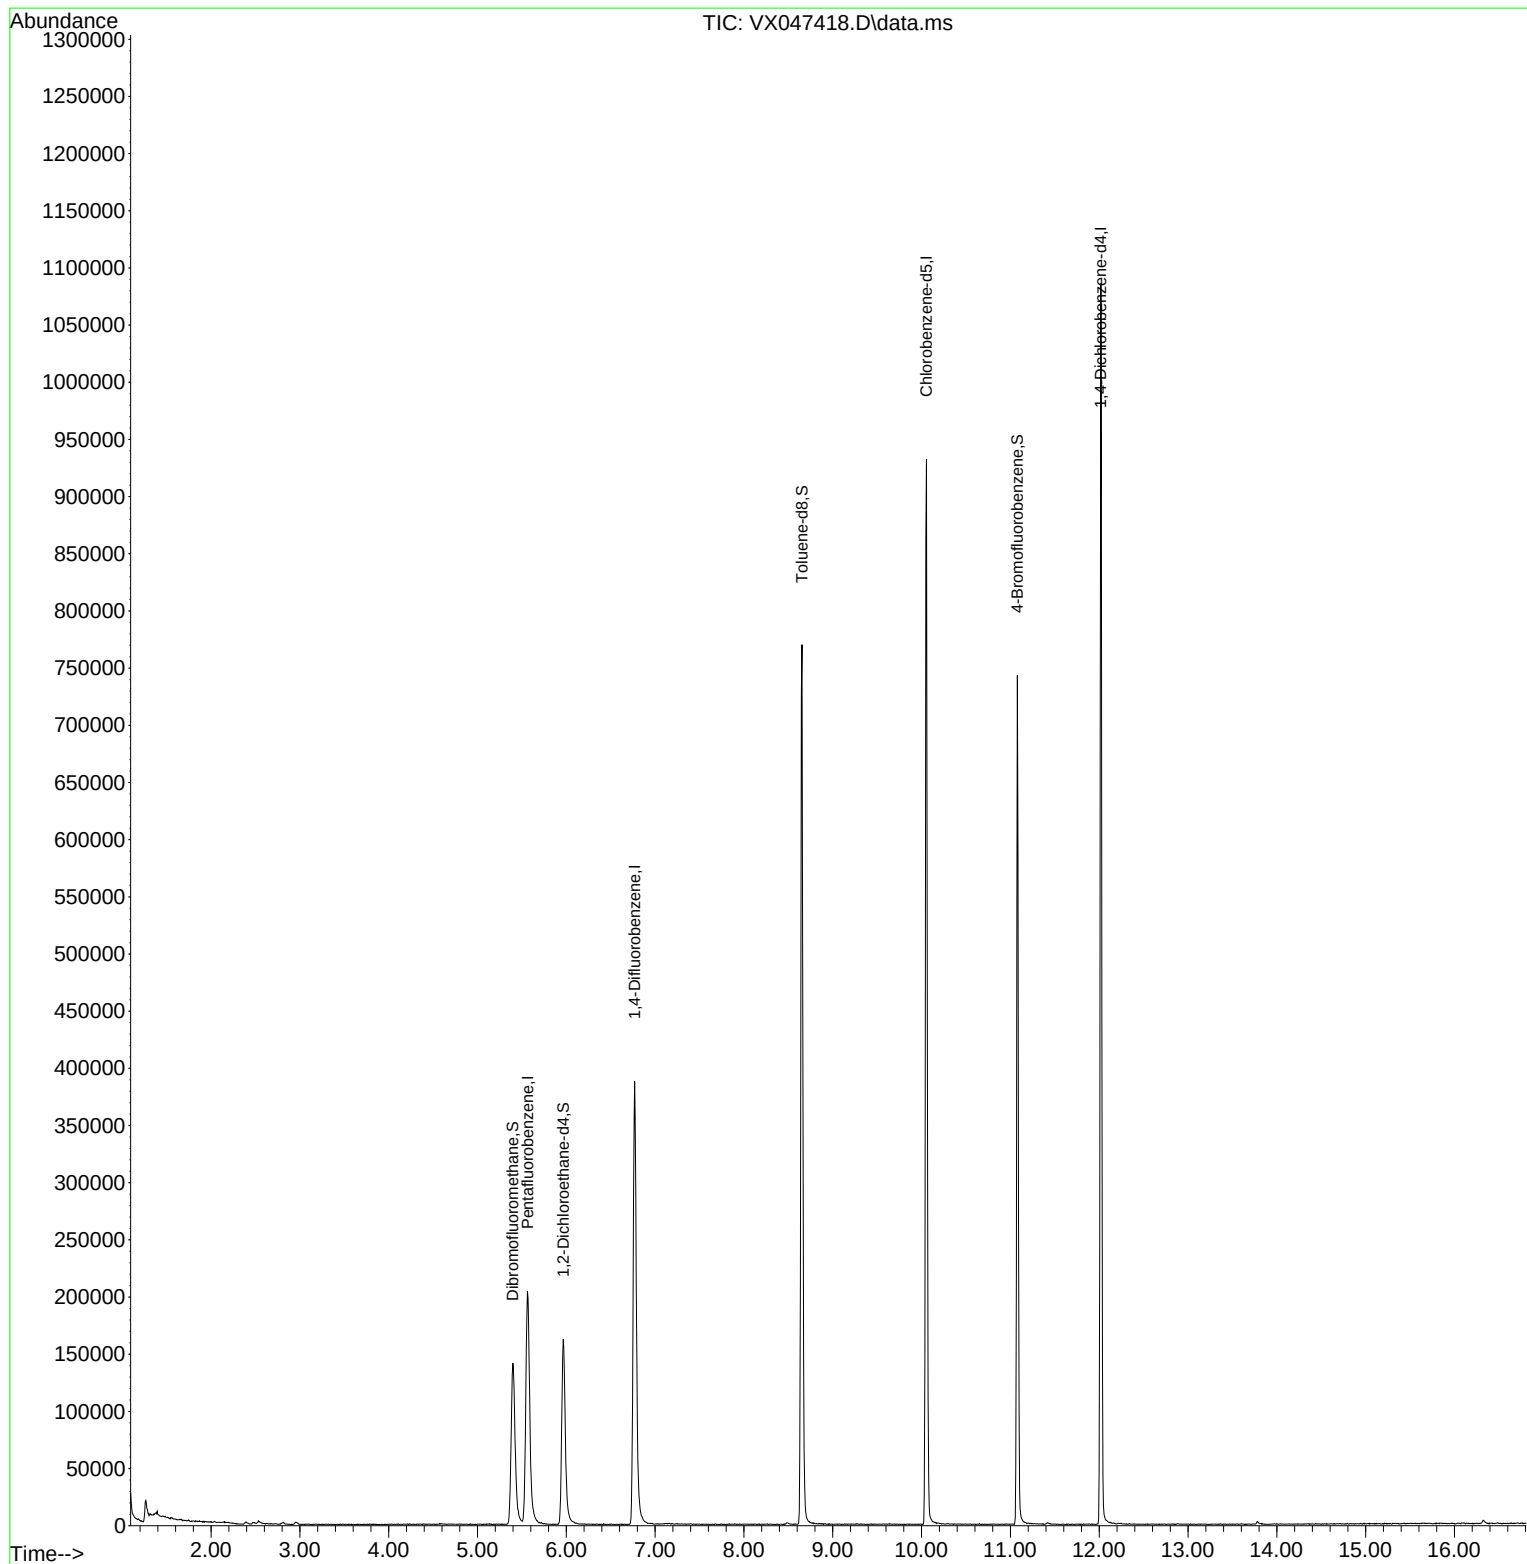



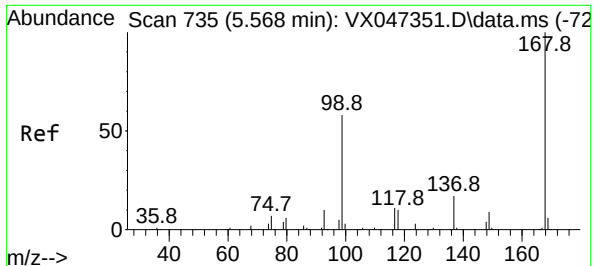


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX047418.D
Acq: 19 Aug 2025 17:18

Instrument :
MSVOA_X
ClientSampleId :
TB01-081325



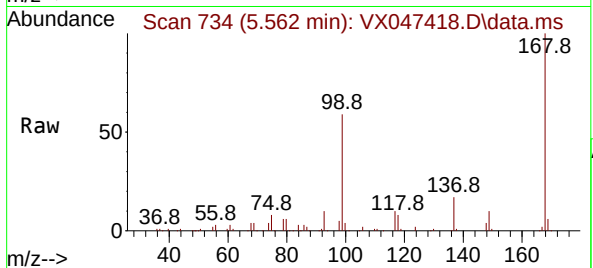



Tgt Ion:168 Resp: 204851
Ion Ratio Lower Upper
168 100
99 59.3 47.9 71.9

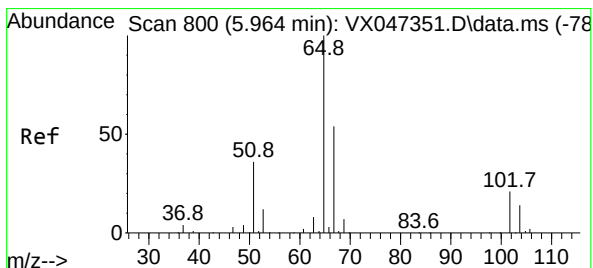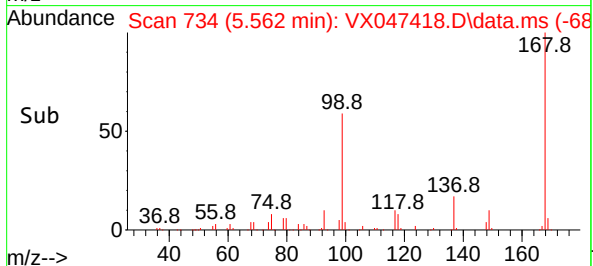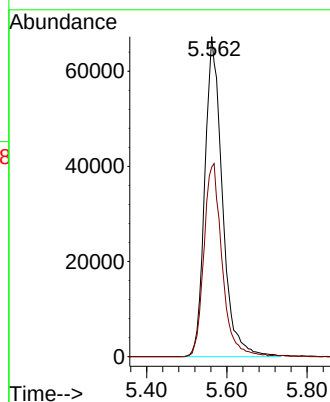

#33
1,2-Dichloroethane-d4
Concen: 58.564 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX047418.D
Acq: 19 Aug 2025 17:18

Tgt Ion: 65 Resp: 167900
Ion Ratio Lower Upper
65 100
67 52.9 0.0 106.0


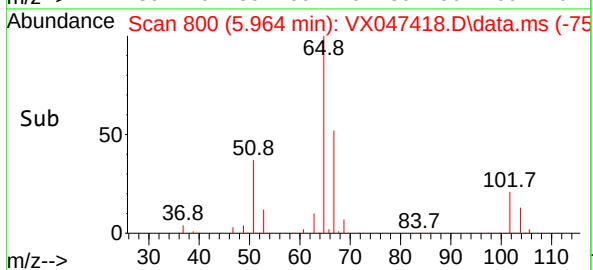
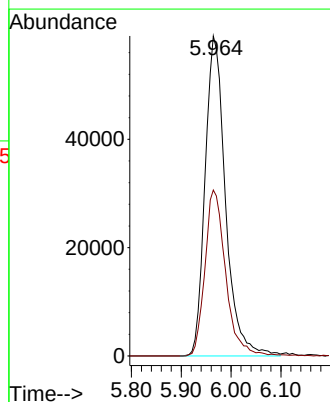
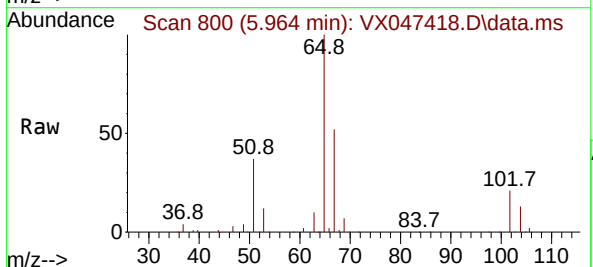


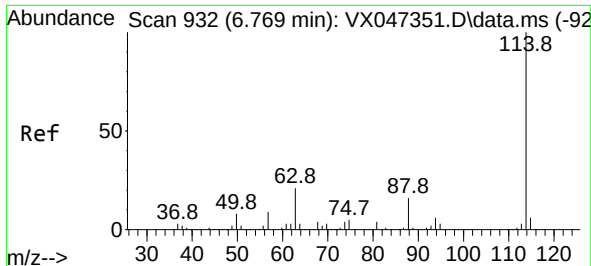

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX047418.D
Acq: 19 Aug 2025 17:18




Instrument :
MSVOA_X
ClientSampleId :
TB01-081325


Tgt Ion:114 Resp: 415100
Ion Ratio Lower Upper
114 100
63 21.8 0.0 42.4
88 16.2 0.0 33.0

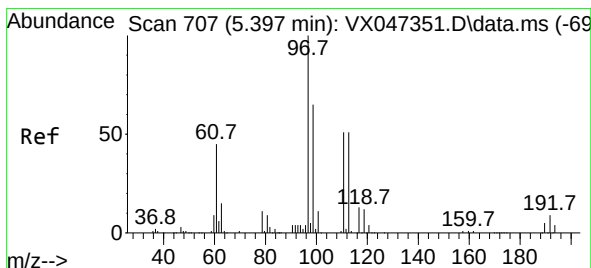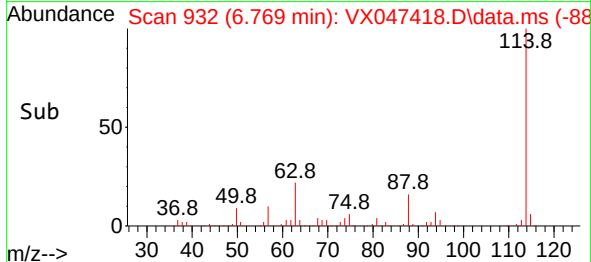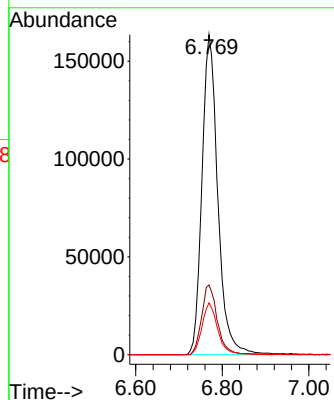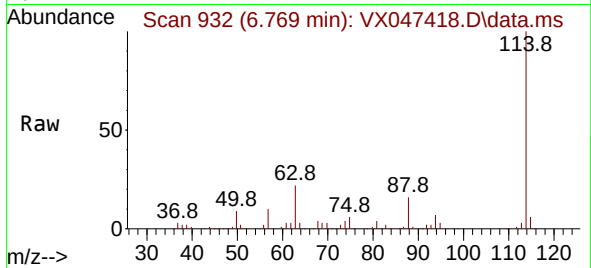

#35
Dibromofluoromethane
Concen: 49.776 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX047418.D
Acq: 19 Aug 2025 17:18

Tgt Ion:113 Resp: 134098
Ion Ratio Lower Upper
113 100
111 103.8 81.4 122.2
192 18.8 14.1 21.1


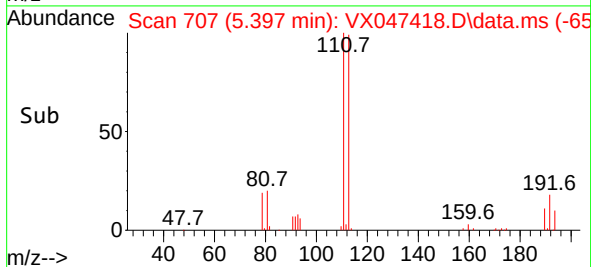
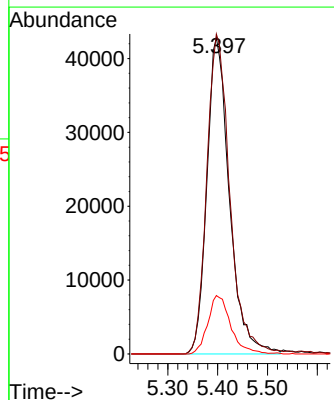
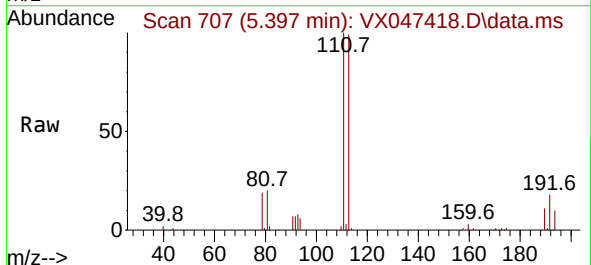


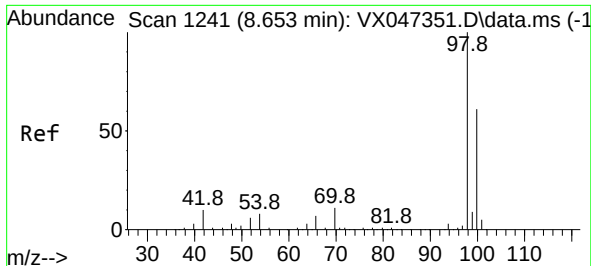

#50
Toluene-d8
Concen: 48.221 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX047418.D
Acq: 19 Aug 2025 17:18




Instrument :
MSVOA_X
ClientSampleId :
TB01-081325


Tgt Ion: 98 Resp: 464326
Ion Ratio Lower Upper
98 100
100 66.9 53.9 80.9

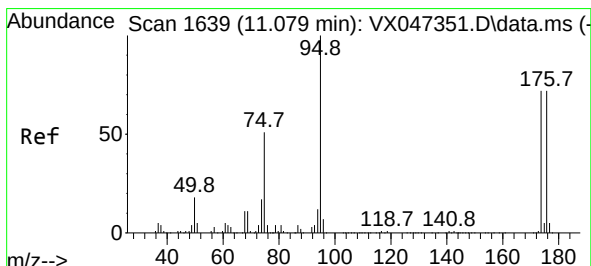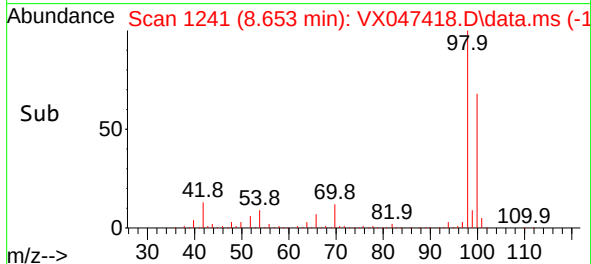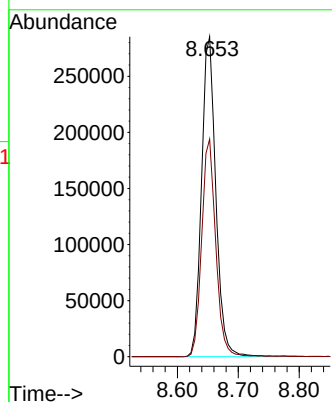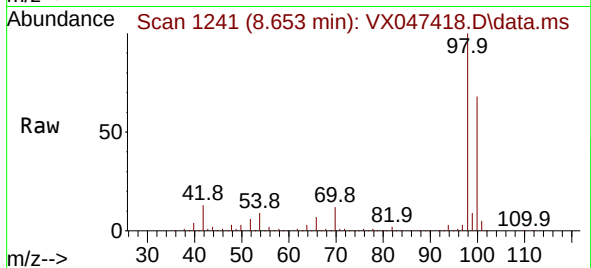

#62
4-Bromofluorobenzene
Concen: 55.835 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047418.D
Acq: 19 Aug 2025 17:18

Tgt Ion: 95 Resp: 198402
Ion Ratio Lower Upper
95 100
174 74.5 0.0 148.0
176 71.3 0.0 145.4

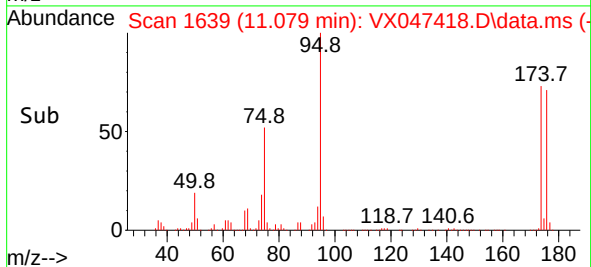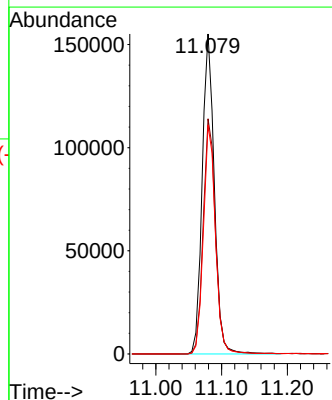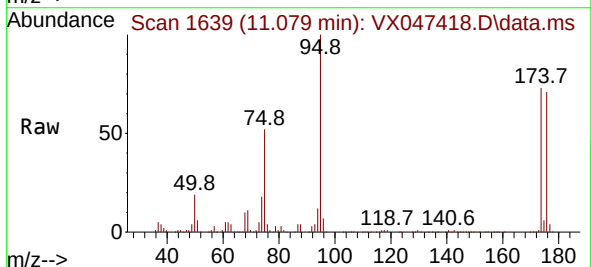

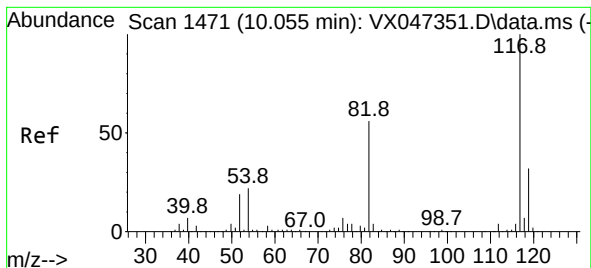

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX047418.D

Acq: 19 Aug 2025 17:18

Instrument :

MSVOA_X

ClientSampleId :

TB01-081325





Tgt Ion:117 Resp: 420679

Ion Ratio Lower Upper

117 100

82 55.7 45.0 67.4

119 31.8 25.8 38.8

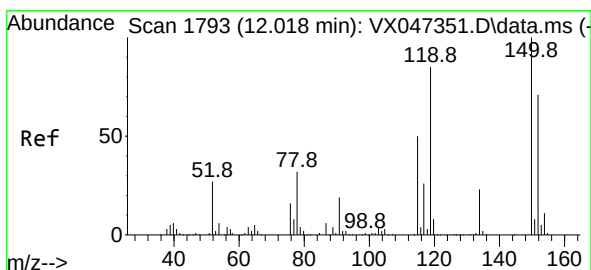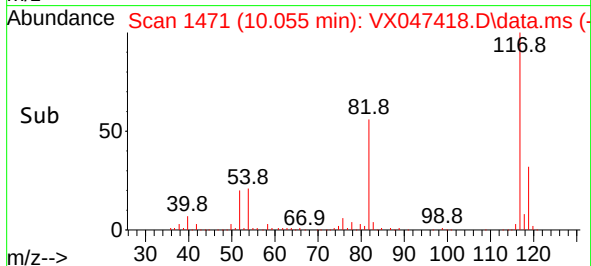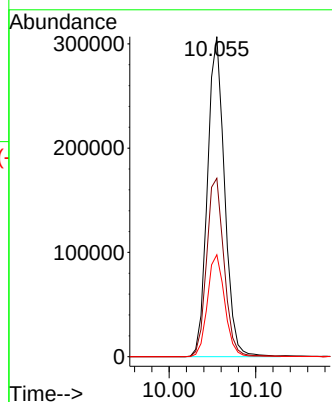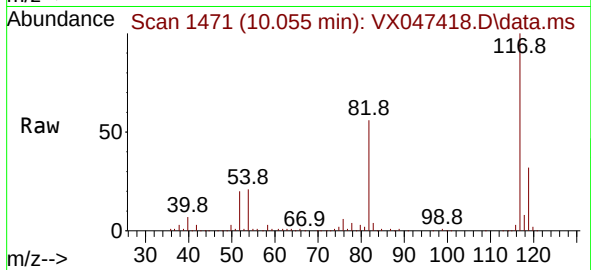

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX047418.D

Acq: 19 Aug 2025 17:18

Tgt Ion:152 Resp: 219893

Ion Ratio Lower Upper

152 100

115 61.5 44.6 133.8

150 155.1 0.0 349.8

