

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX082018\  
 Data File : VX004148.D  
 Acq On : 20 Aug 2018 13:09  
 Operator : JC/MD  
 Sample : J4541-01  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 KY037MW097-180815

Quant Time: Aug 21 01:01:36 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X081418W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Aug 14 13:27:25 2018  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 5.67  | 168  | 277917   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 6.86  | 114  | 423722   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.12 | 117  | 406254   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.08 | 152  | 213816   | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|-------|---------|----------|
| 33) 1,2-Dichloroethane-d4   | 6.07  | 65   | 210774   | 53.83 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 107.66% |          |
| 35) Dibromofluoromethane    | 5.51  | 113  | 182099   | 57.42 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 114.84% |          |
| 50) Toluene-d8              | 8.72  | 98   | 629256   | 48.94 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 97.88%  |          |
| 62) 4-Bromofluorobenzene    | 11.14 | 95   | 201305   | 43.17 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 86.34%  |          |


| Target Compounds               | R.T.  | QIon | Response | Conc      | Units  | Qvalue |
|--------------------------------|-------|------|----------|-----------|--------|--------|
| 3) Chloromethane               | 1.32  | 50   | 2676     | 0.81      | ug/l   | 93     |
| 4) Vinyl Chloride              | 1.40  | 62   | 5892     | 1.64      | ug/l   | 98     |
| 5) Bromomethane                | 1.65  | 94   | 722      | 0.22      | ug/l # | 73     |
| 6) Chloroethane                | 1.71  | 64   | 210      | Below Cal | #      | 42     |
| 10) Methyl Iodide              | 2.53  | 142  | 680      | 5.19      | ug/l # | 80     |
| 11) Tert butyl alcohol         | 3.03  | 59   | 908      | 1.15      | ug/l # | 73     |
| 12) 1,1-Dichloroethene         | 2.38  | 96   | 839      | 0.29      | ug/l   | 94     |
| 13) Acrolein                   | 2.29  | 56   | 167      | 11.25     | ug/l # | 15     |
| 16) Acetone                    | 2.44  | 43   | 1104     | 0.54      | ug/l   | 92     |
| 20) Methylene Chloride         | 2.87  | 84   | 234      | Below Cal | #      | 70     |
| 21) trans-1,2-Dichloroethene   | 3.17  | 96   | 3136     | 0.94      | ug/l # | 86     |
| 27) cis-1,2-Dichloroethene     | 4.60  | 96   | 82295    | 22.04     | ug/l   | 87     |
| 29) Tetrahydrofuran            | 5.15  | 42   | 855      | 0.51      | ug/l # | 78     |
| 31) Cyclohexane                | 5.66  | 56   | 5248     | 0.97      | ug/l # | 1      |
| 36) 1,1-Dichloropropene        | 5.66  | 75   | 19054    | 3.95      | ug/l # | 49     |
| 38) Carbon Tetrachloride       | 5.67  | 117  | 24142    | 5.15      | ug/l # | 17     |
| 44) Trichloroethene            | 7.21  | 130  | 982      | 0.25      | ug/l   | 85     |
| 60) Dibromochloromethane       | 9.34  | 129  | 1794     | 0.49      | ug/l # | 11     |
| 64) Tetrachloroethene          | 9.34  | 164  | 2028     | 0.53      | ug/l # | 92     |
| 76) 1,2,3-Trichloropropane     | 11.14 | 75   | 101937   | 23.77     | ug/l # | 36     |
| 81) trans-1,4-Dichloro-2-buten | 11.14 | 75   | 101937   | 73.59     | ug/l # | 9      |
| 95) Naphthalene                | 13.83 | 128  | 507      | 1.18      | ug/l # | 75     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX082018\  
Data File : VX004148.D  
Acq On : 20 Aug 2018 13:09  
Operator : JC/MD  
Sample : J4541-01  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY037MW097-180815

Quant Time: Aug 21 01:01:36 2018  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X081418W.M  
Quant Title : SW846 8260  
QLast Update : Tue Aug 14 13:27:25 2018  
Response via : Initial Calibration

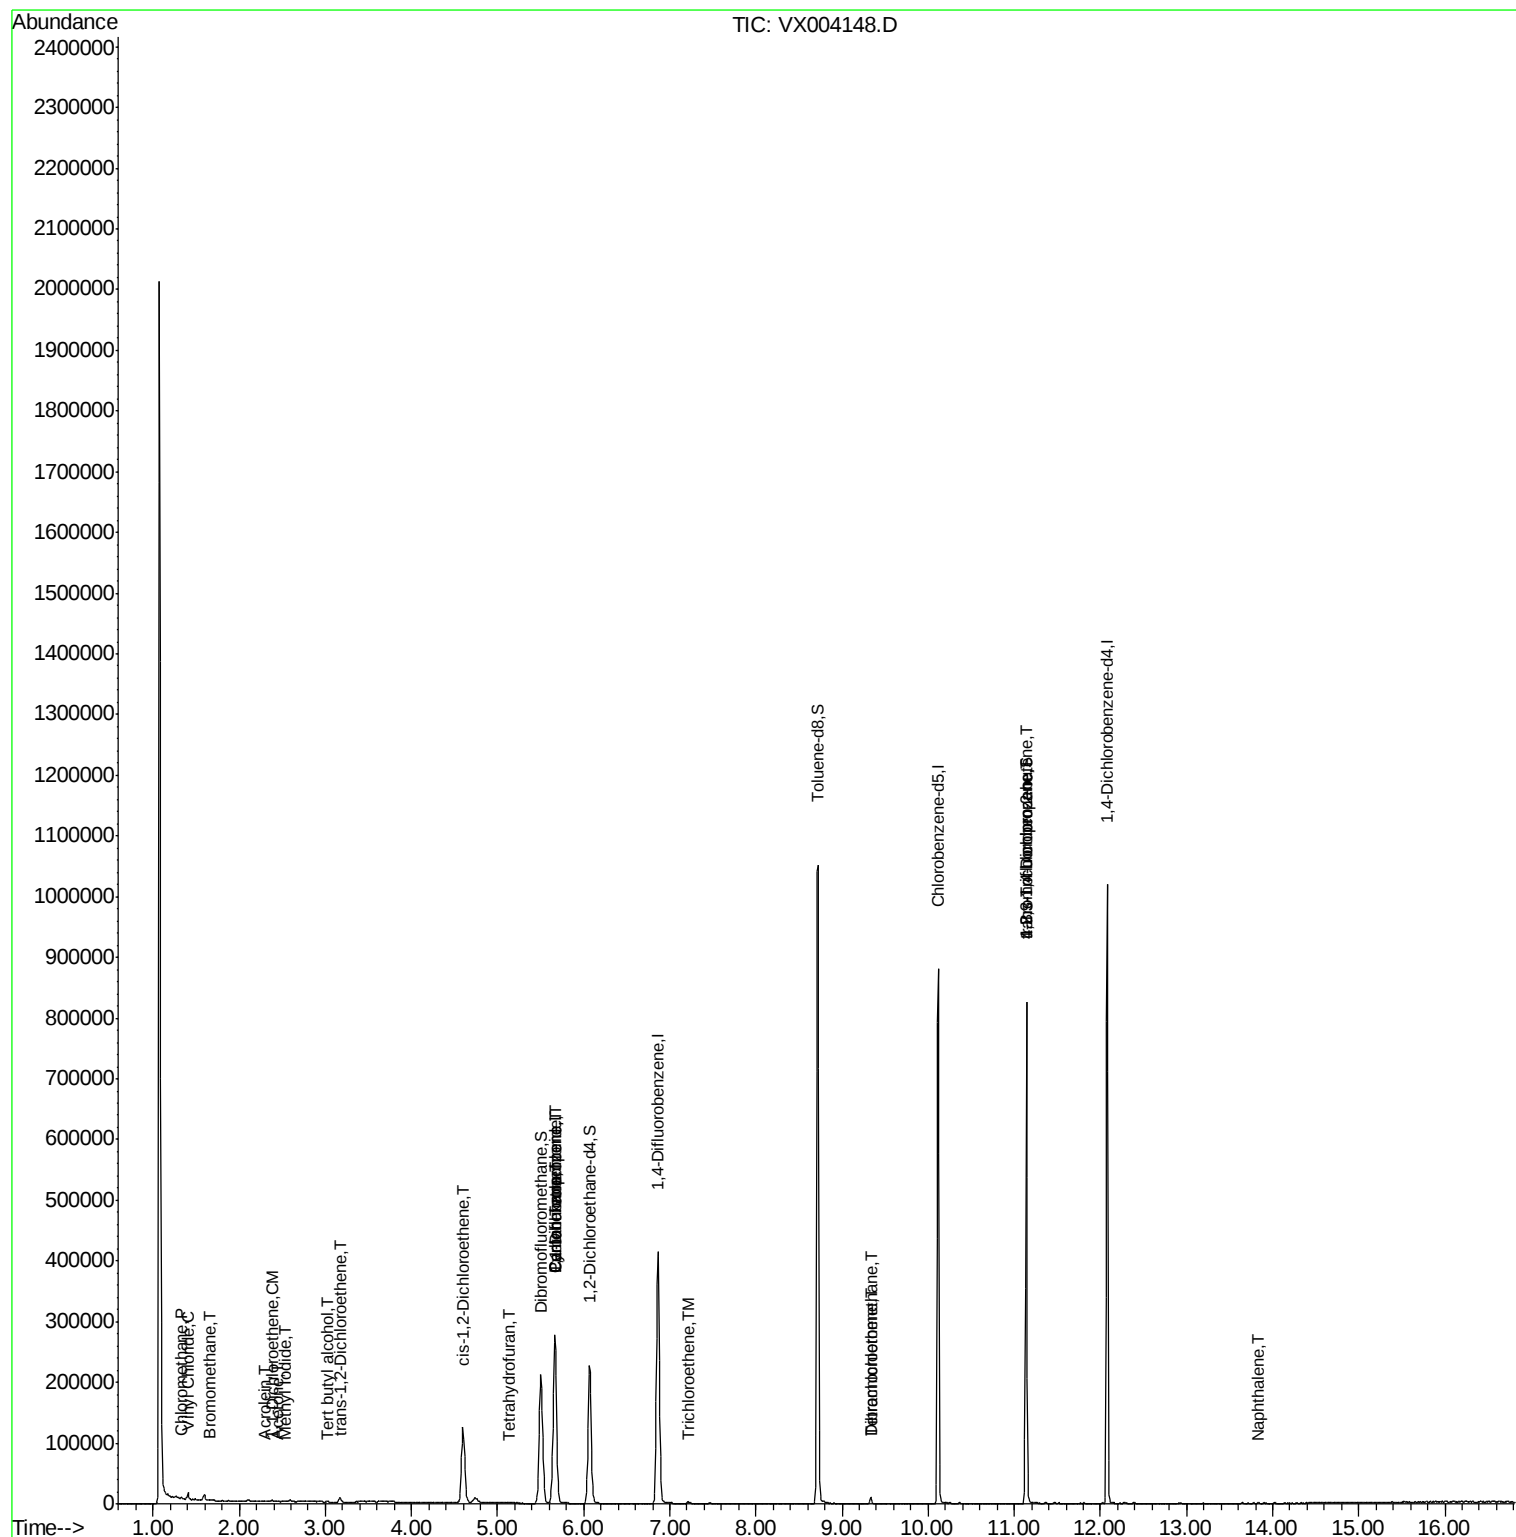



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. 0.00 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :


KY037MW097-180815

Tot Ion:168 Resp: 277917

Ion Ratio Lower Upper




168 100

99 50.0 40.1 60.1

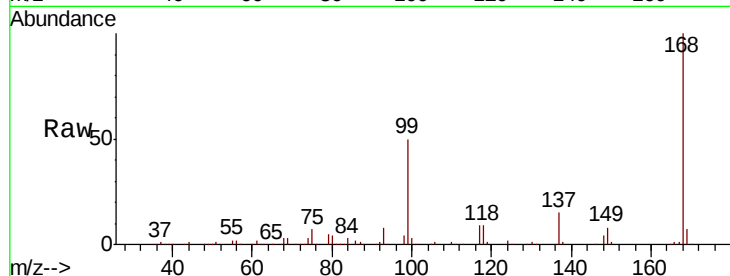

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

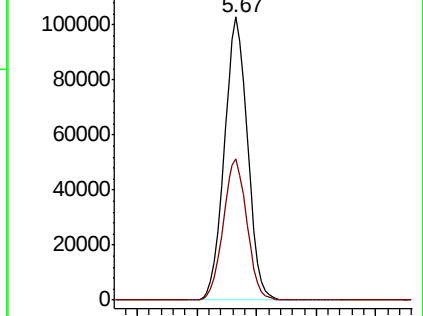

#3

Chloromethane

Concen: 0.81 ug/l

RT: 1.32 min Scan# 121

Delta R.T. 0.00 min

Lab File: VX004148.D


Acq: 20 Aug 2018 13:09

Tgt Ion: 50 Resp: 2676

Ion Ratio Lower Upper



50 100


52 29.2 26.6 39.8



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

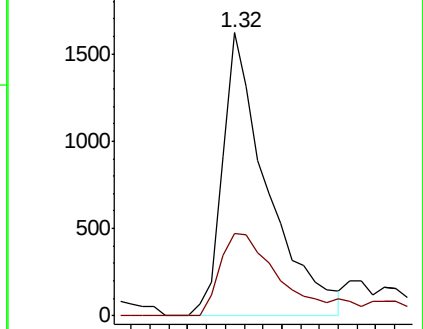



#4

Vinyl Chloride

Concen: 1.64 ug/l

RT: 1.40 min Scan# 134

Delta R.T. -0.00 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :


KY037MW097-180815

Tot Ion: 62 Resp: 5892

Ion Ratio Lower Upper




62 100

64 31.4 26.0 39.0

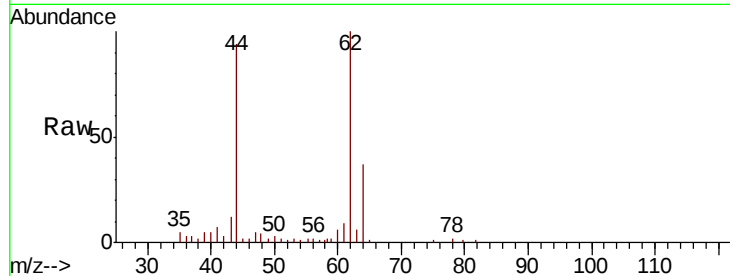

Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 63.90 (63.60 to 64.60): VX0

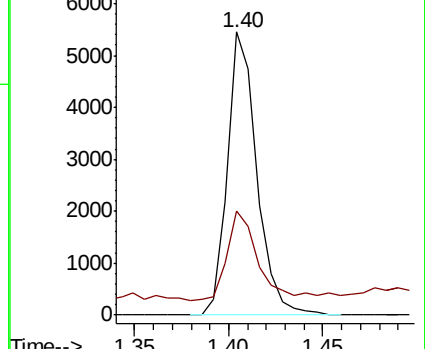

#5

Bromomethane

Concen: 0.22 ug/l

RT: 1.65 min Scan# 174

Delta R.T. 0.01 min

Lab File: VX004148.D


Acq: 20 Aug 2018 13:09

Tgt Ion: 94 Resp: 722

Ion Ratio Lower Upper



94 100


96 67.7 75.2 112.8#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

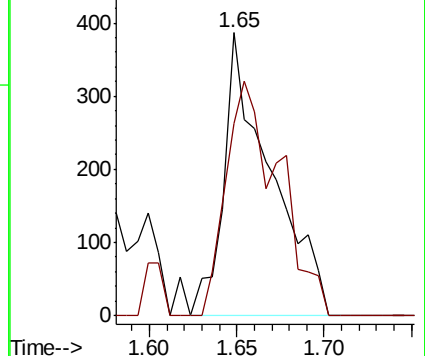

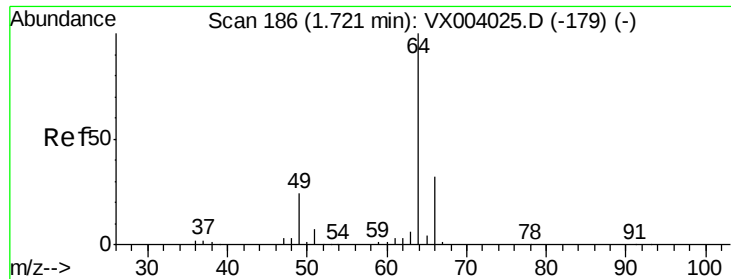

#6

Chloroethane

Concen: Below Cal

RT: 1.71 min Scan# 184

Delta R.T. -0.01 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :


KY037MW097-180815

Tot Ion: 64 Resp: 210

Ion Ratio Lower Upper

64 100

66 0.0 26.5 39.7#

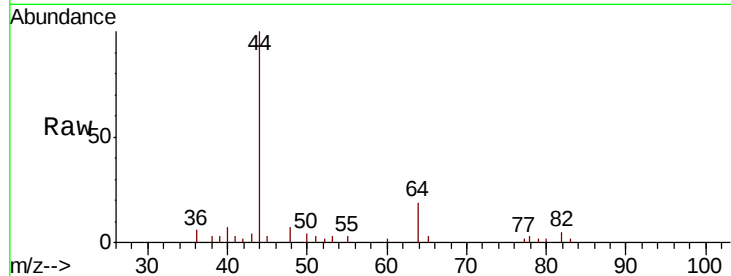

Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

1.71



600

400

200

0

Time-->



#10

Methyl Iodide

Concen: 5.19 ug/l

RT: 2.53 min Scan# 318

Delta R.T. 0.01 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09


Tgt Ion:142 Resp: 680

Ion Ratio Lower Upper

142 100

127 28.4 33.1 49.7#

141 6.6 11.1 16.7#



Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

400


300


200

100

0

Time-->









#11  
Tert butvl alcohol  
Concen: 1.15 ug/l  
RT: 3.03 min Scan# 401  
Delta R.T. -0.02 min  
Lab File: VX004148.D  
Acq: 20 Aug 2018 13:09




Instrument :  
MSVOA\_X  
ClientSampleId :  
KY037MW097-180815


Tot Ion: 59 Resp: 908  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.1 12.1#

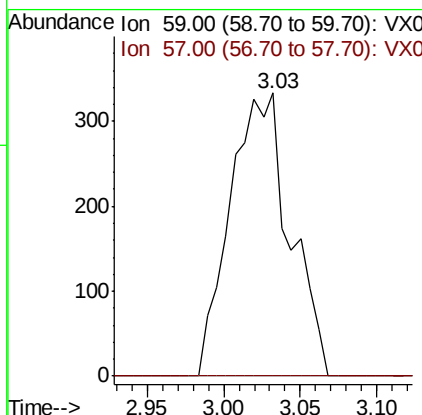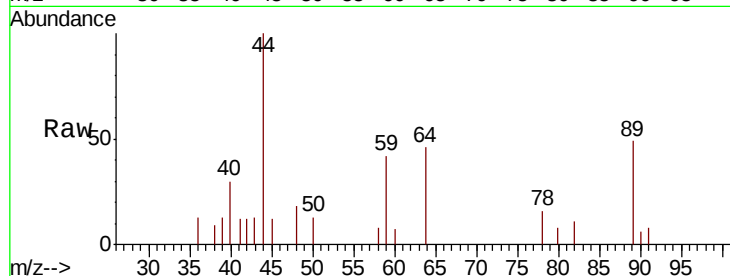

#12  
1,1-Dichloroethene  
Concen: 0.29 ug/l  
RT: 2.38 min Scan# 294  
Delta R.T. 0.01 min  
Lab File: VX004148.D  
Acq: 20 Aug 2018 13:09

Tgt Ion: 96 Resp: 839  
Ion Ratio Lower Upper  
96 100  
61 169.6 131.3 196.9  
98 73.8 51.8 77.6

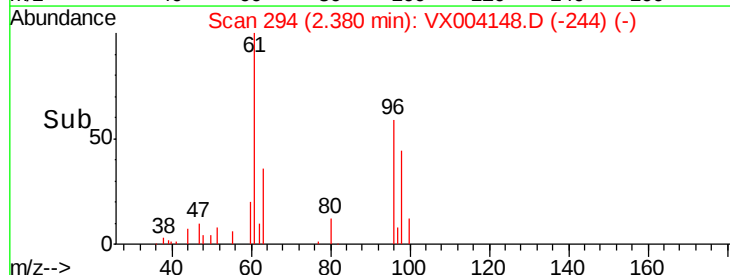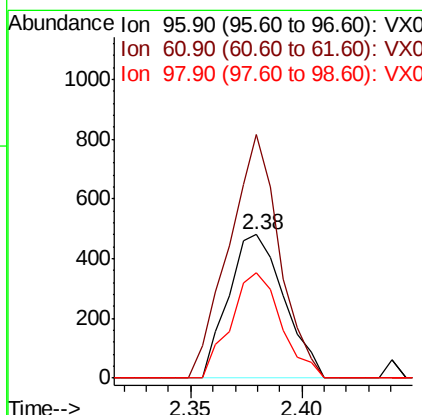



#13

Acrolein

Concen: 11.25 ug/l

RT: 2.29 min Scan# 279

Delta R.T. 0.00 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :


KY037MW097-180815

Tot Ion: 56 Resp: 167

Ion Ratio Lower Upper




56 100

55 0.0 56.1 84.1#

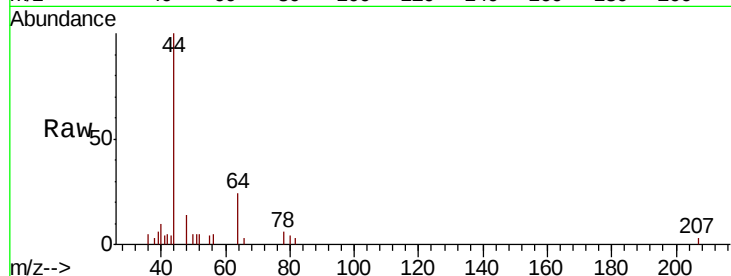

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

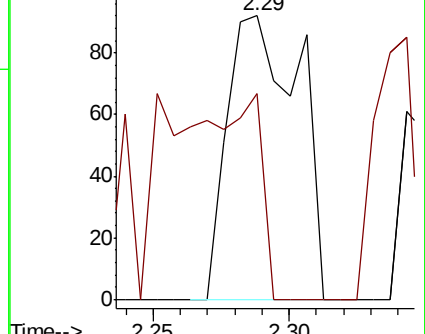

#16

Acetone

Concen: 0.54 ug/l

RT: 2.44 min Scan# 304

Delta R.T. -0.00 min

Lab File: VX004148.D


Acq: 20 Aug 2018 13:09

Tgt Ion: 43 Resp: 1104

Ion Ratio Lower Upper



43 100


58 28.3 26.4 39.6



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




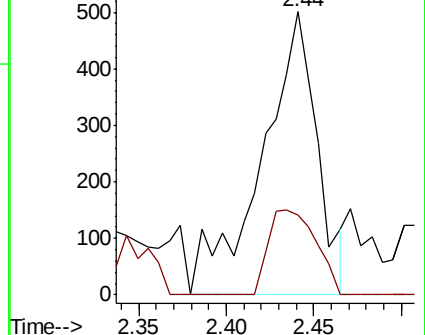


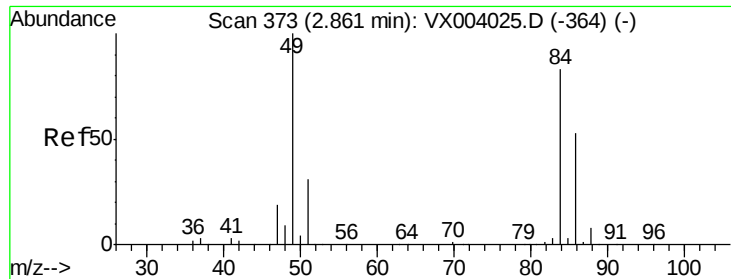

#20  
Methvlene Chloride  
Concen: Below Cal  
RT: 2.87 min Scan# 374  
Delta R.T. 0.01 min  
Lab File: VX004148.D  
Acq: 20 Aug 2018 13:09




Instrument :  
MSVOA\_X  
ClientSampleId :  
KY037MW097-180815


Tot Ion: 84 Resp: 234  
Ion Ratio Lower Upper  
84 100  
49 147.7 98.9 148.3  
51 80.8 29.9 44.9#  
86 45.4 51.0 76.6#

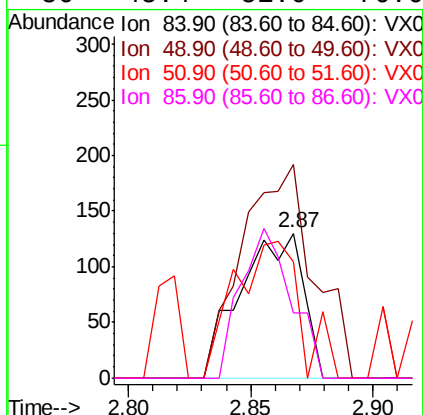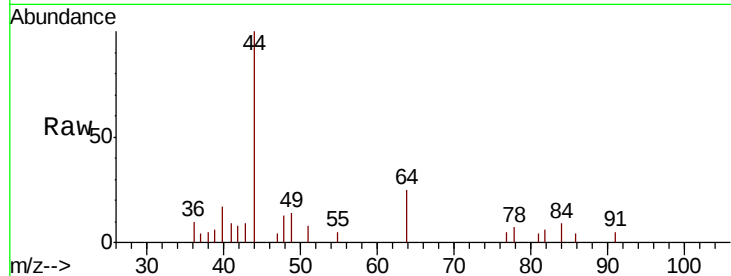

#21  
trans-1,2-Dichloroethene  
Concen: 0.94 ug/l  
RT: 3.17 min Scan# 423  
Delta R.T. 0.00 min  
Lab File: VX004148.D  
Acq: 20 Aug 2018 13:09

Tgt Ion: 96 Resp: 3136  
Ion Ratio Lower Upper  
96 100  
61 125.4 111.8 167.6  
98 49.1 51.8 77.6#

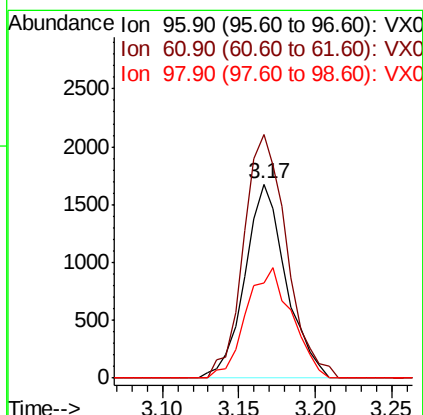

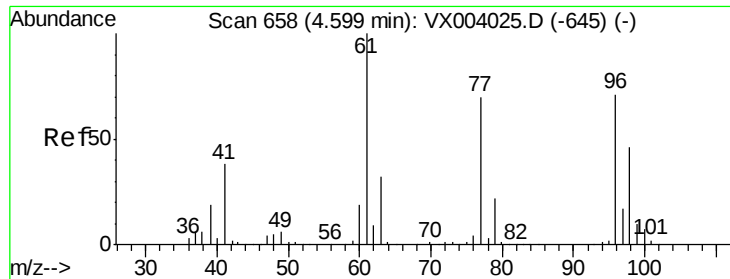

#27

cis-1,2-Dichloroethene

Concen: 22.04 ug/l

RT: 4.60 min Scan# 658

Delta R.T. -0.00 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :

KY037MW097-180815


Tot Ion: 96 Resp: 82295

Ion Ratio Lower Upper




96 100

61 124.9 0.0 293.0

98 63.2 0.0 131.8



Abundance Ion 95.90 (95.60 to 96.60): VX0  
Ion 60.90 (60.60 to 61.60): VX0  
Ion 97.90 (97.60 to 98.60): VX0

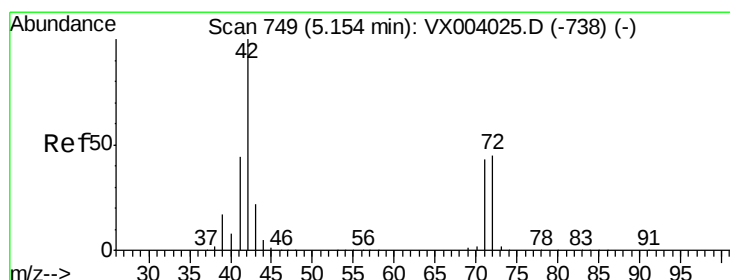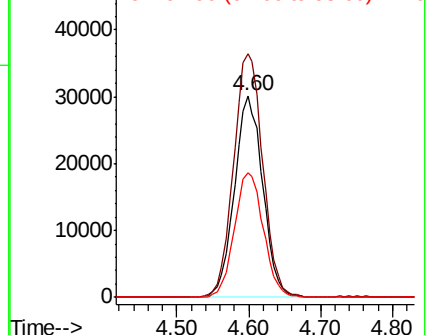

#29

Tetrahydrofuran

Concen: 0.51 ug/l

RT: 5.15 min Scan# 748

Delta R.T. -0.01 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09


Tgt Ion: 42 Resp: 855

Ion Ratio Lower Upper



42 100


72 26.4 37.7 56.5#

71 36.1 35.0 52.6



Abundance Ion 42.00 (41.70 to 42.70): VX0  
Ion 72.00 (71.70 to 72.70): VX0  
Ion 71.00 (70.70 to 71.70): VX0

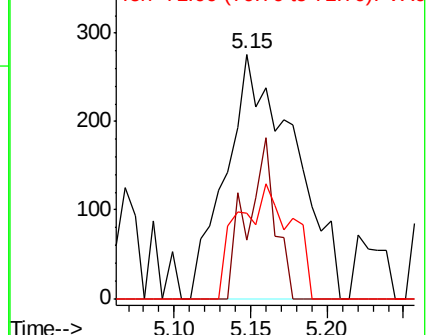


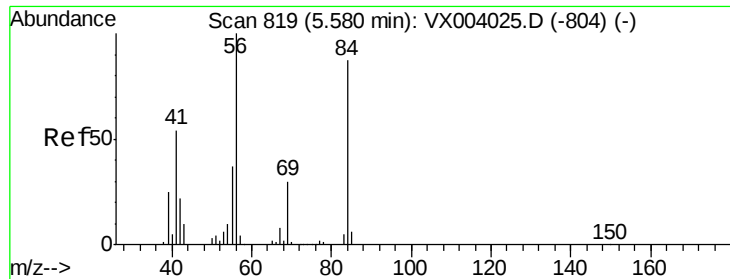




#31  
Cyclohexane  
Concen: 0.97 ug/l  
RT: 5.66 min Scan# 832  
Delta R.T. 0.08 min  
Lab File: VX004148.D  
Acq: 20 Aug 2018 13:09

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY037MW097-180815

Tot Ion: 56 Resp: 5248  
Ion Ratio Lower Upper  
56 100  
69 181.8 24.9 37.3#  
84 146.9 71.7 107.5#

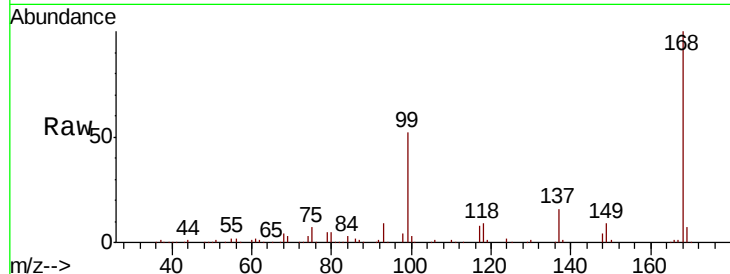


Abundance Ion 56.00 (55.70 to 56.70): VX0  
Ion 69.00 (68.70 to 69.70): VX0  
Ion 84.00 (83.70 to 84.70): VX0


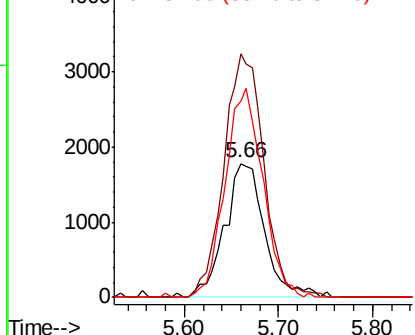



#33  
1,2-Dichloroethane-d4  
Concen: 53.83 ug/l  
RT: 6.07 min Scan# 899  
Delta R.T. 0.00 min  
Lab File: VX004148.D  
Acq: 20 Aug 2018 13:09

Tgt Ion: 65 Resp: 210774  
Ion Ratio Lower Upper  
65 100  
67 52.9 0.0 105.8



Abundance Ion 64.90 (64.60 to 65.60): VX0  
Ion 66.90 (66.60 to 67.60): VX0

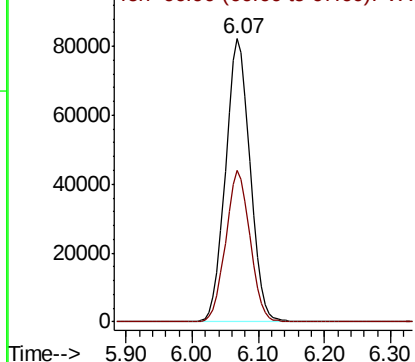

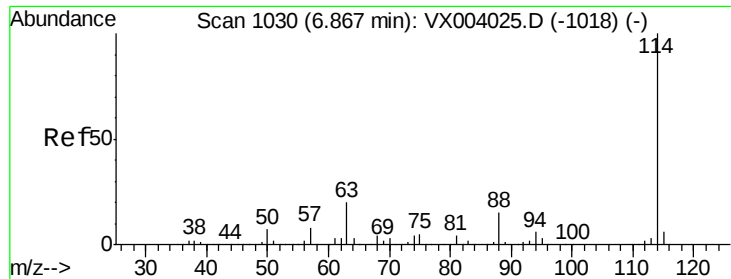

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.86 min Scan# 1029

Delta R.T. -0.01 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :

KY037MW097-180815


Tot Ion:114 Resp: 423722

Ion Ratio Lower Upper

114 100

63 20.2 0.0 39.0




88 15.3 0.0 32.0

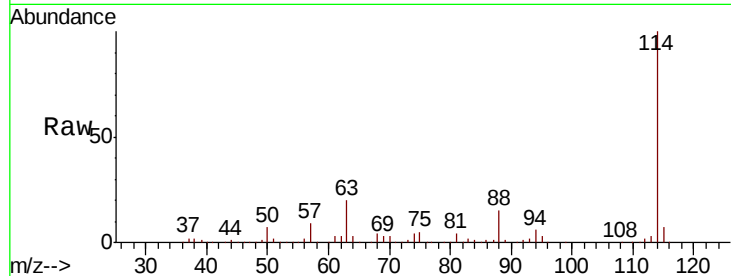

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

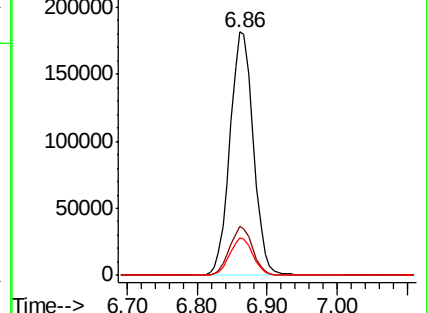

#35

Dibromofluoromethane

Concen: 57.42 ug/l

RT: 5.51 min Scan# 807

Delta R.T. 0.01 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09


Tgt Ion:113 Resp: 182099

Ion Ratio Lower Upper

113 100

111 101.5 82.0 123.0



192 24.0 19.0 28.4




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

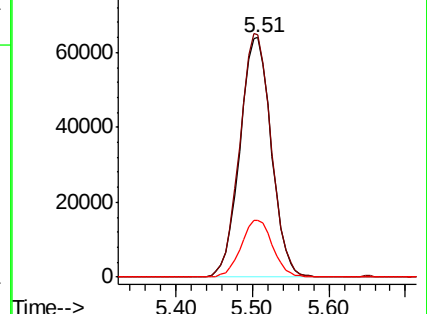

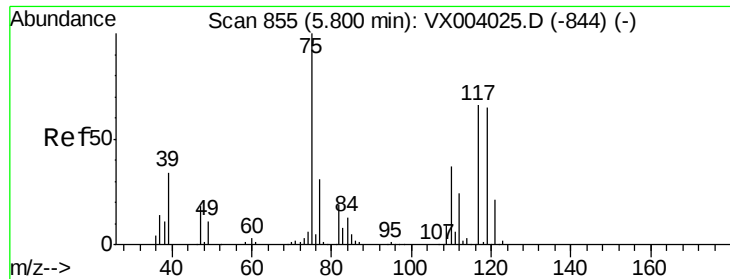

#36

1,1-Dichloropropene

Concen: 3.95 ug/l

RT: 5.66 min Scan# 832

Delta R.T. -0.14 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :

KY037MW097-180815


Tot Ion: 75 Resp: 19054

Ion Ratio Lower Upper

75 100

110 9.3 18.2 54.6#




77 0.0 25.0 37.4#

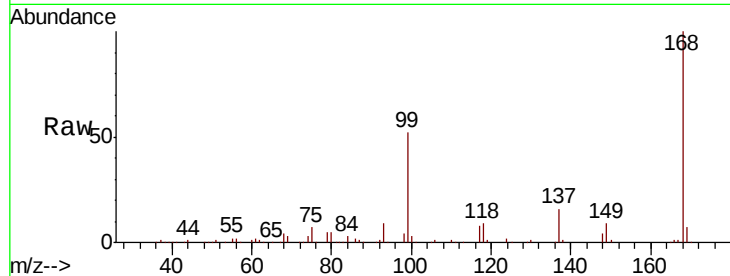

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

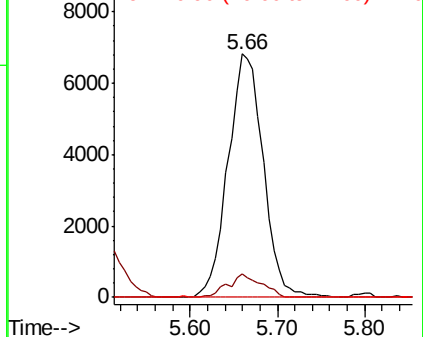

#38

Carbon Tetrachloride

Concen: 5.15 ug/l

RT: 5.67 min Scan# 833

Delta R.T. -0.12 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09


Tgt Ion: 117 Resp: 24142

Ion Ratio Lower Upper

117 100

119 8.9 79.5 119.3#



121 0.0 25.0 37.4#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

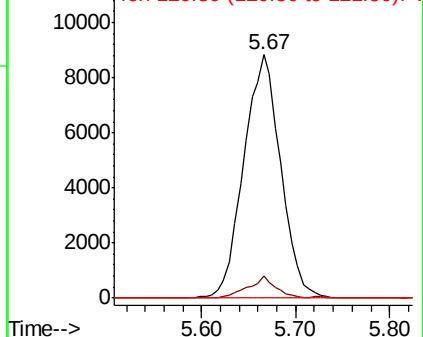

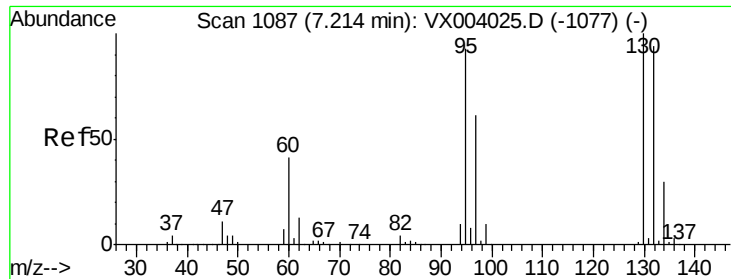

#44

Trichloroethene

Concen: 0.25 ug/l

RT: 7.21 min Scan# 1086

Delta R.T. -0.01 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :


KY037MW097-180815

Tot Ion:130 Resp: 982

Ion Ratio Lower Upper




130 100

95 85.1 0.0 199.4

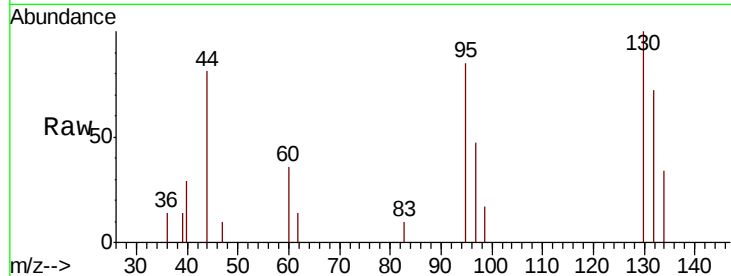

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

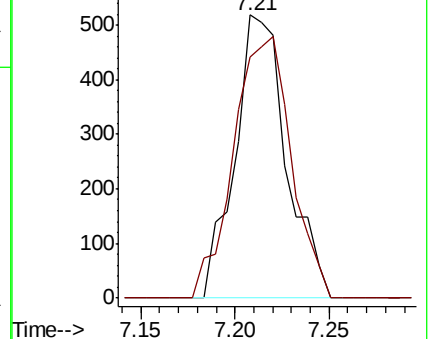

#50

Toluene-d8

Concen: 48.94 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX004148.D


Acq: 20 Aug 2018 13:09

Tgt Ion: 98 Resp: 629256

Ion Ratio Lower Upper



98 100


100 66.6 53.3 79.9



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V




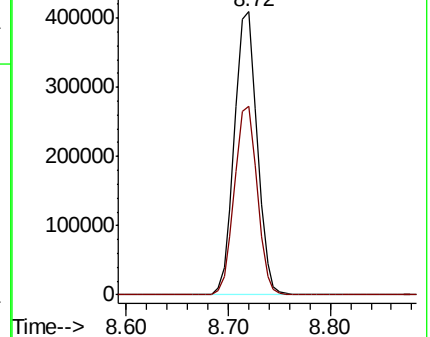




#60  
 Dibromochloromethane  
 Concen: 0.49 ug/l  
 RT: 9.34 min Scan# 1435  
 Delta R.T. -0.25 min  
 Lab File: VX004148.D  
 Acq: 20 Aug 2018 13:09




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 KY037MW097-180815


Tot Ion:129 Resp: 1794  
 Ion Ratio Lower Upper  
 129 100  
 127 0.0 38.8 116.3#

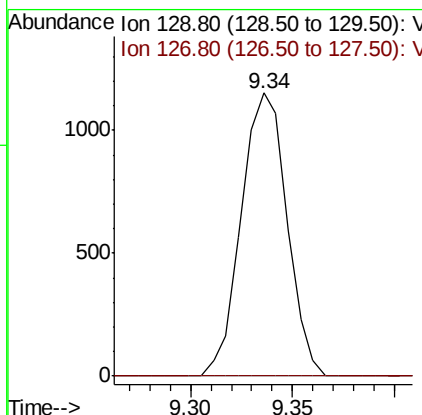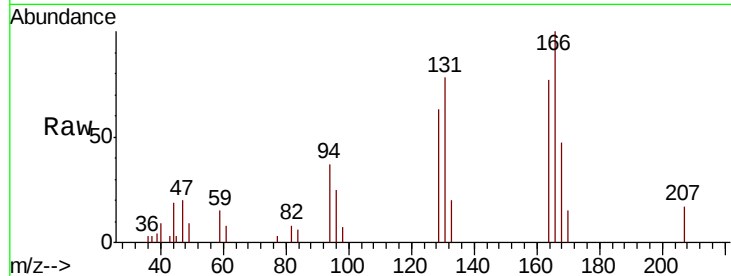

#62  
 4-Bromofluorobenzene  
 Concen: 43.17 ug/l  
 RT: 11.14 min Scan# 1731  
 Delta R.T. 0.00 min  
 Lab File: VX004148.D  
 Acq: 20 Aug 2018 13:09

Tgt Ion: 95 Resp: 201305  
 Ion Ratio Lower Upper  
 95 100  
 174 96.9 0.0 182.8  
 176 90.3 0.0 179.0

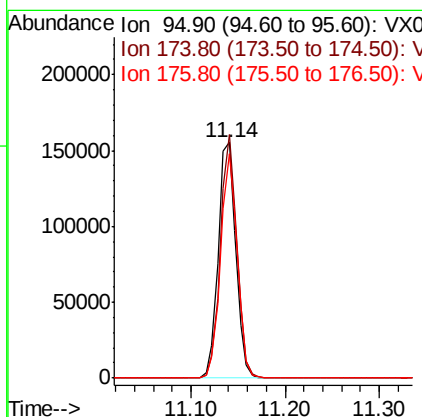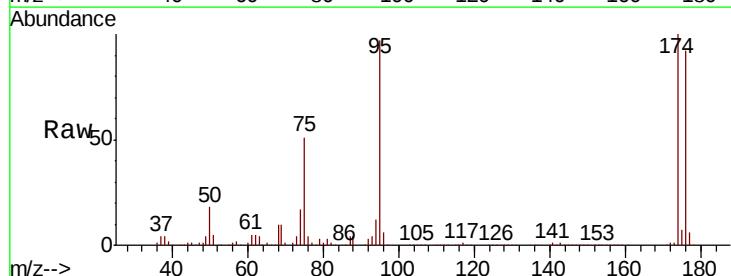


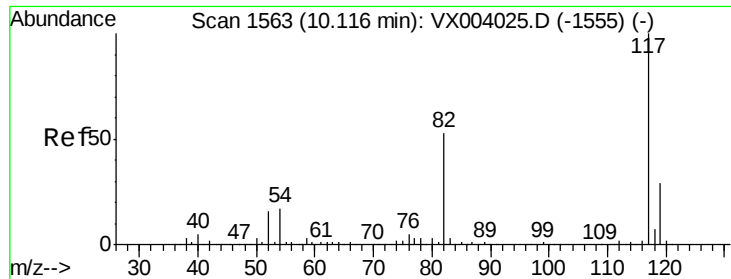




#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 10.12 min Scan# 1563  
Delta R.T. -0.00 min  
Lab File: VX004148.D  
Acq: 20 Aug 2018 13:09

Instrument :  
MSVOA\_X  
ClientSampleId :  
KY037MW097-180815

Tot Ion:117 Resp: 406254  
Ion Ratio Lower Upper  
117 100  
82 52.1 45.4 68.0  
119 32.3 26.6 40.0

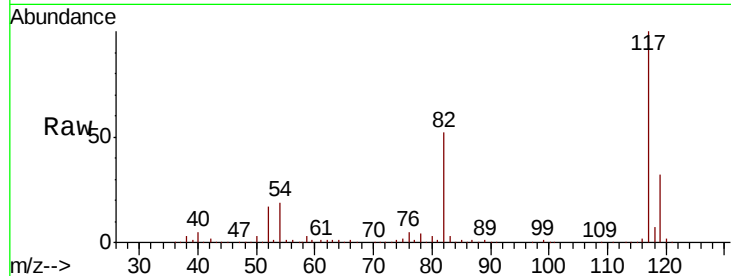


Abundance Ion 116.90 (116.60 to 117.60): V  
Ion 82.00 (81.70 to 82.70): VX0  
Ion 118.90 (118.60 to 119.60): V

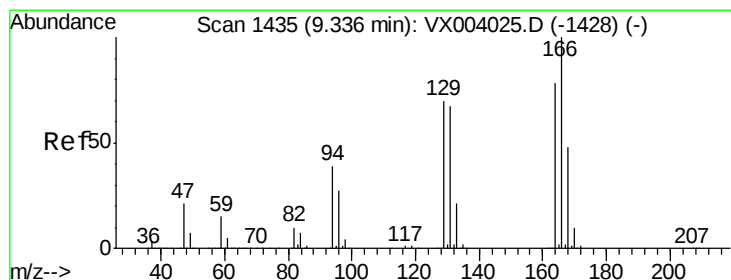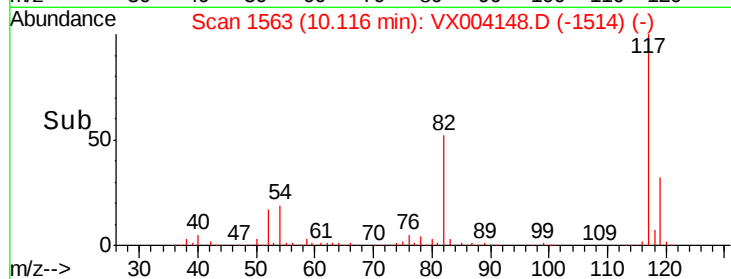
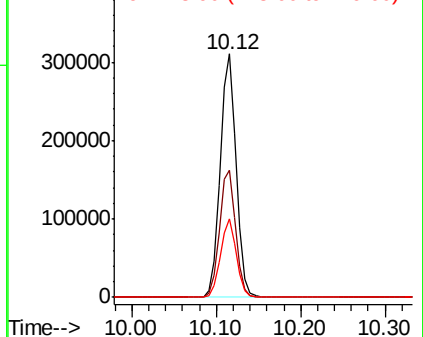



#64  
Tetrachloroethene  
Concen: 0.53 ug/l  
RT: 9.34 min Scan# 1435  
Delta R.T. -0.00 min  
Lab File: VX004148.D  
Acq: 20 Aug 2018 13:09

Tgt Ion:164 Resp: 2028  
Ion Ratio Lower Upper  
164 100  
166 129.2 98.0 147.0  
129 81.6 64.3 96.5  
131 100.3 66.8 100.2#



Abundance Ion 163.80 (163.50 to 164.50): V  
Ion 165.80 (165.50 to 166.50): V  
Ion 128.80 (128.50 to 129.50): V  
Ion 130.80 (130.50 to 131.50): V

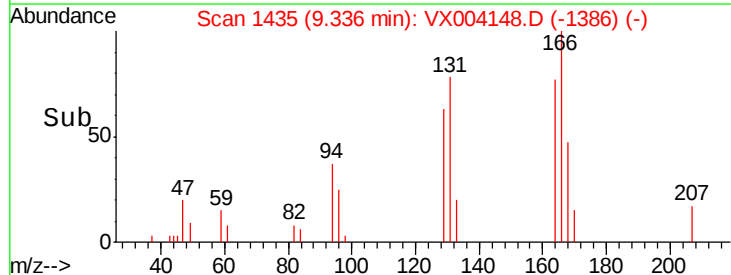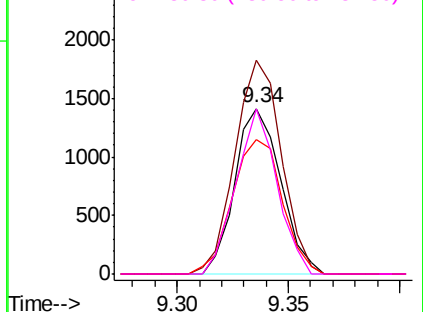



#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.08 min Scan# 1885

Delta R.T. 0.00 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :

KY037MW097-180815


Tot Ion:152 Resp: 213816

Ion Ratio Lower Upper

152 100

115 53.2 39.1 117.3




150 155.1 0.0 349.2

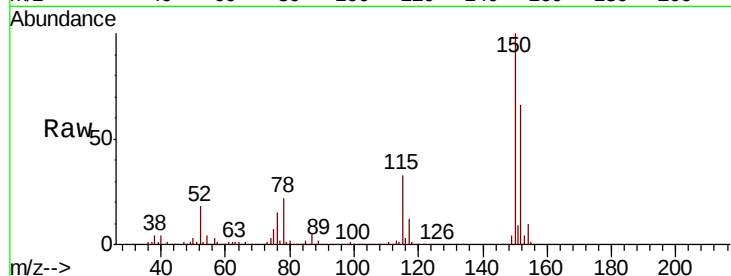

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

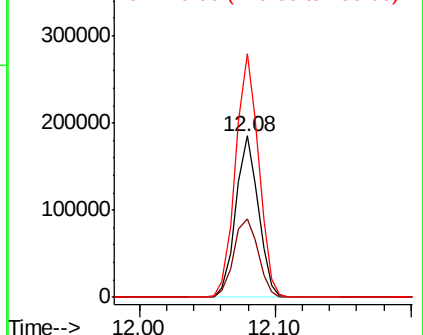

#76

1,2,3-Trichloropropane

Concen: 23.77 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX004148.D


Acq: 20 Aug 2018 13:09

Tgt Ion: 75 Resp: 101937

Ion Ratio Lower Upper



75 100


77 1.4 20.8 62.5#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

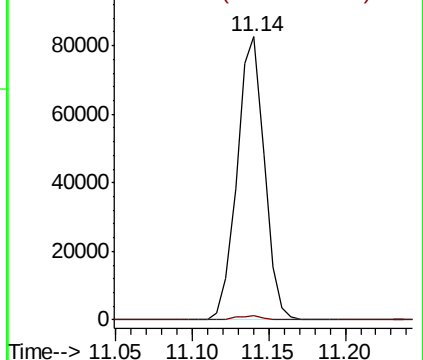



#81

trans-1,4-Dichloro-2-butene

Concen: 73.59 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09

Instrument :

MSVOA\_X

ClientSampleId :

KY037MW097-180815


Tot Ion: 75 Resp: 101937

Ion Ratio Lower Upper

75 100

53 0.2 80.3 120.5#




89 0.0 37.8 56.8#

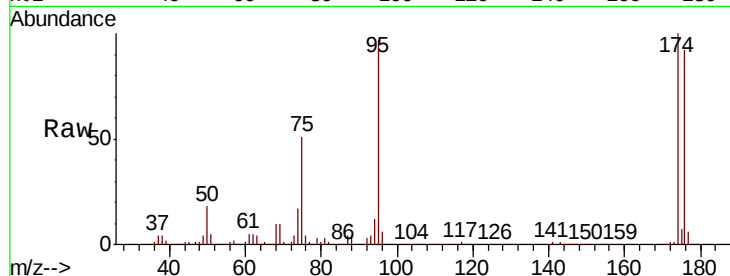

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

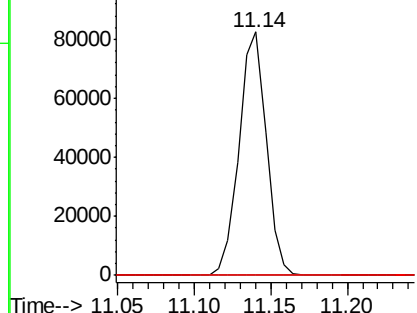

#95

Naphthalene

Concen: 1.18 ug/l

RT: 13.83 min Scan# 2173

Delta R.T. 0.00 min

Lab File: VX004148.D

Acq: 20 Aug 2018 13:09


Tgt Ion:128 Resp: 507

Ion Ratio Lower Upper

128 100

127 0.0 10.2 15.2#

129 4.3 8.8 13.2#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

