


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082018\  
 Data File : VX004143.D  
 Acq On : 20 Aug 2018 09:35  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampled :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X081418W.M  
 Title : SW846 8260  
 Last Update : Tue Aug 14 13:27:25 2018

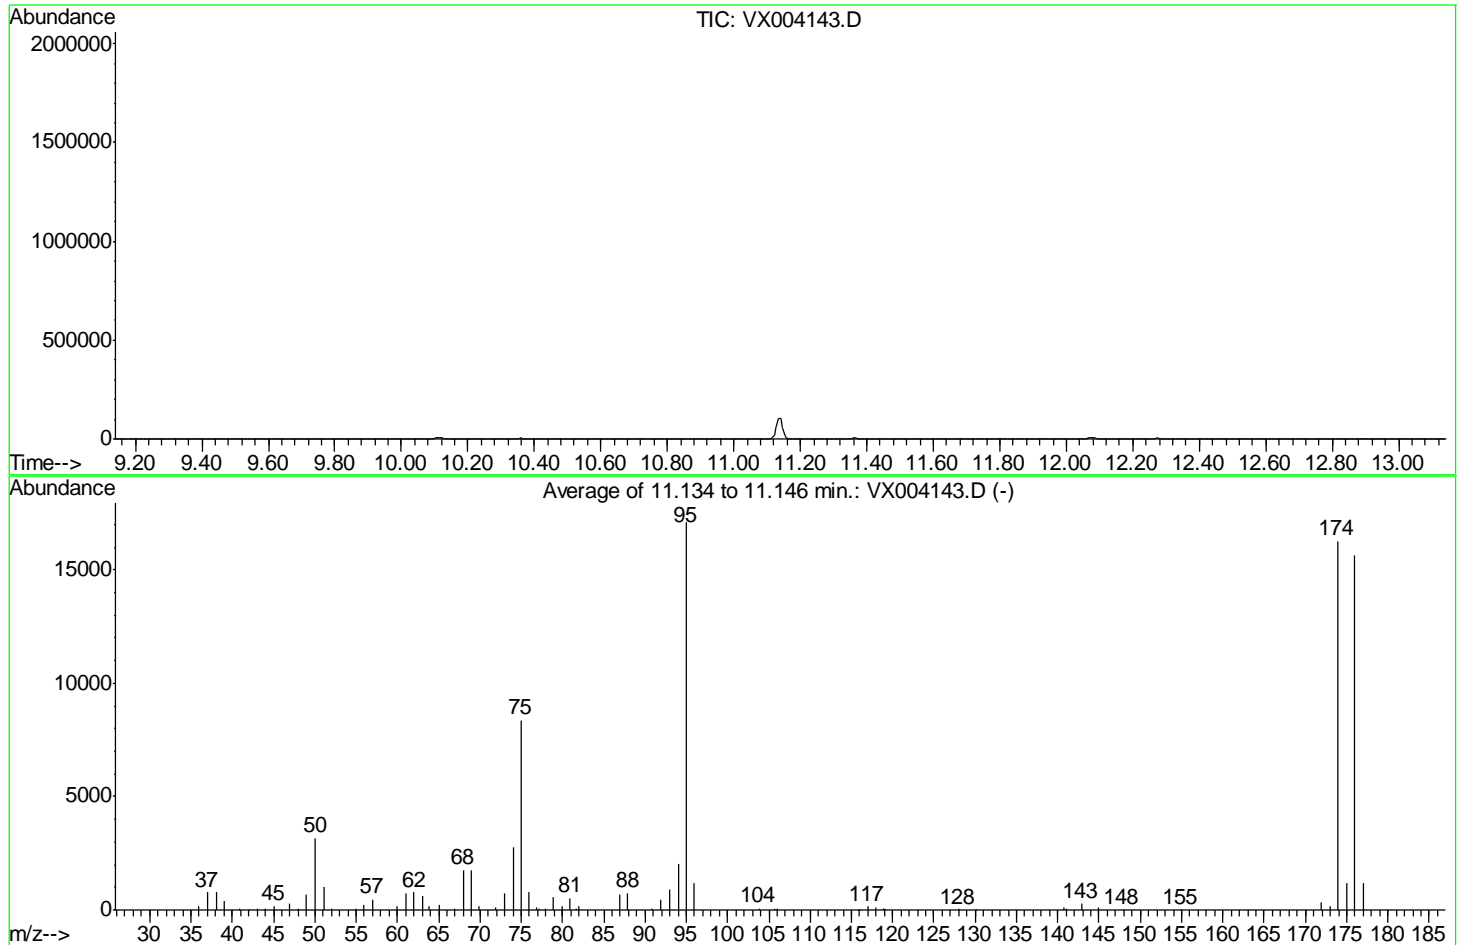

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	3173	PASS
75	95	30	60	48.9	8355	PASS
95	95	100	100	100.0	17093	PASS
96	95	5	9	7.1	1211	PASS
173	174	0.00	2	1.2	189	PASS
174	95	50	100	95.2	16274	PASS
175	174	5	9	7.4	1202	PASS
176	174	95	101	96.2	15658	PASS
177	176	5	9	7.7	1206	PASS