

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX082019\
 Data File : VX011672.D
 Acq On : 20 Aug 2019 10:13
 Operator : JC/SP
 Sample : VX0820MBL01
 Misc : 5.0g/10mL/100uL/10mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0820MBL01

Quant Time: Aug 20 13:21:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 04:15:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	395729	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	486175	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	469039	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	224958	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	197235	53.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.48%	
35) Dibromofluoromethane	5.49	113	166045	52.22	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.44%	
50) Toluene-d8	8.71	98	587810	59.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	118.66%	
62) 4-Bromofluorobenzene	11.13	95	216350	51.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.46%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX082019\
Data File : VX011672.D
Acq On : 20 Aug 2019 10:13
Operator : JC/SP
Sample : VX0820MBL01
Misc : 5.0g/10mL/100uL/10mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0820MBL01

Quant Time: Aug 20 13:21:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 04:15:26 2019
Response via : Initial Calibration

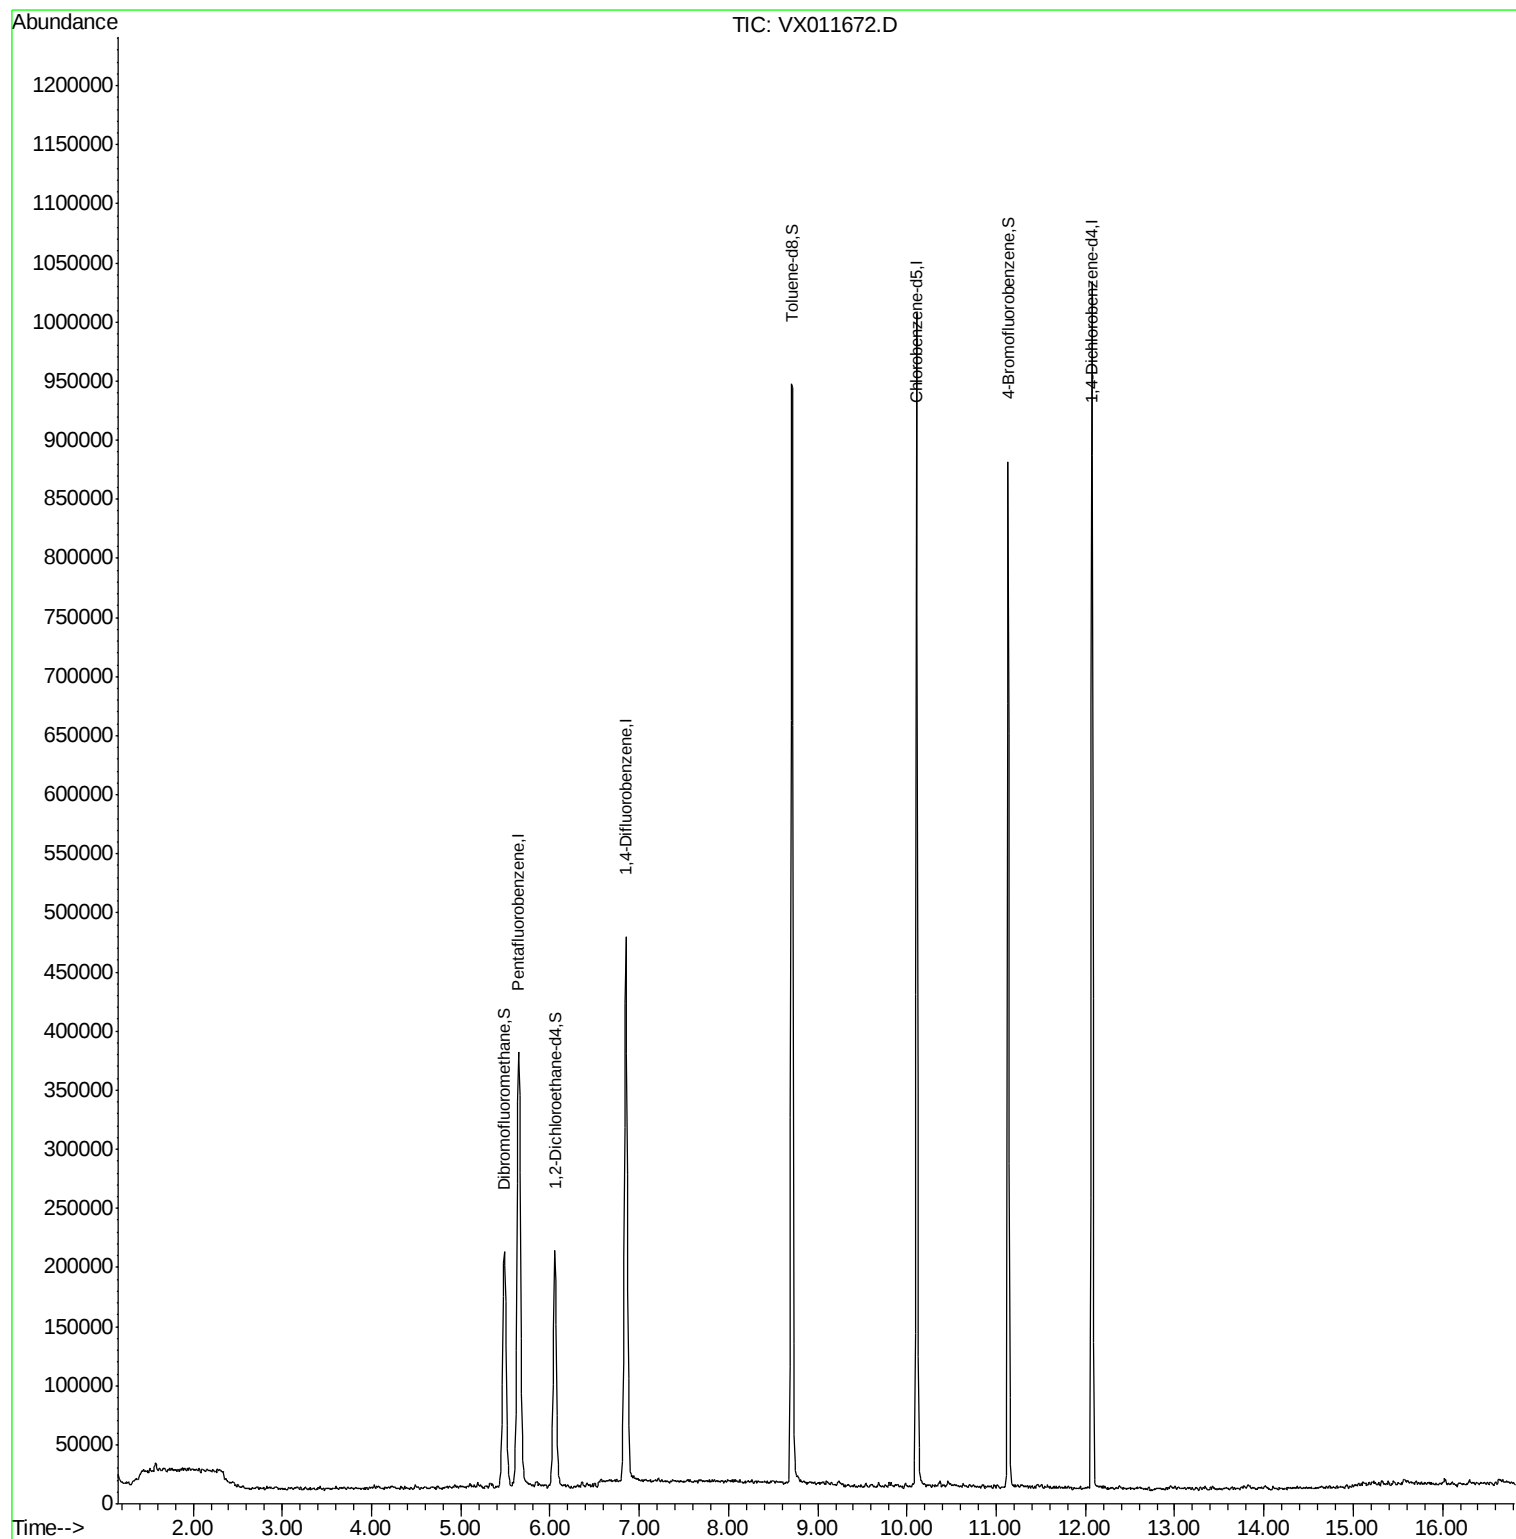

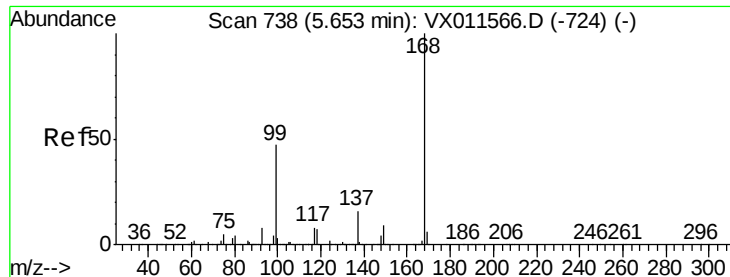

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 737

Delta R.T. -0.01 min

Lab File: VX011672.D

Acq: 20 Aug 2019 10:13

Instrument :

MSVOA_X

ClientSampleId :


VX0820MBL01

Tot Ion:168 Resp: 395729

Ion Ratio Lower Upper

168 100

99 48.1 37.3 55.9

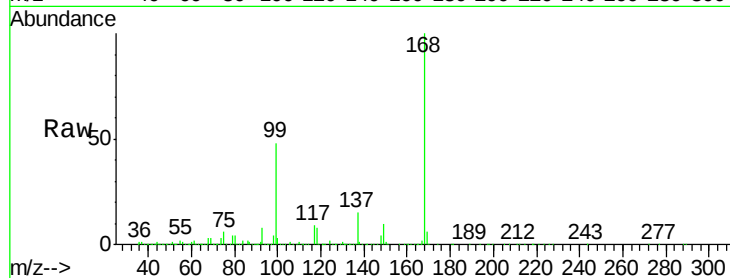

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

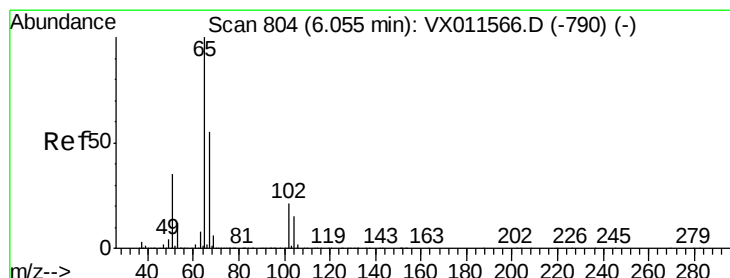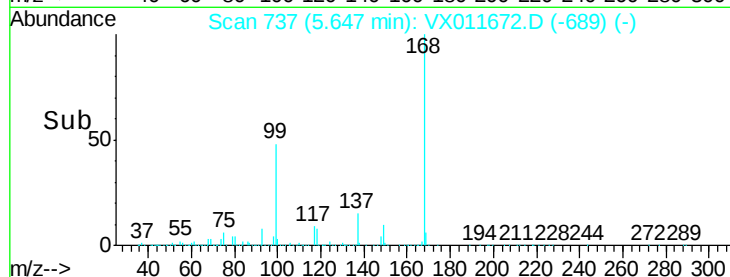

#33

1,2-Dichloroethane-d4

Concen: 53.745 ug/l

RT: 6.06 min Scan# 804

Delta R.T. 0.00 min

Lab File: VX011672.D


Acq: 20 Aug 2019 10:13

Tgt Ion: 65 Resp: 197235

Ion Ratio Lower Upper

65 100

67 51.5 0.0 107.6

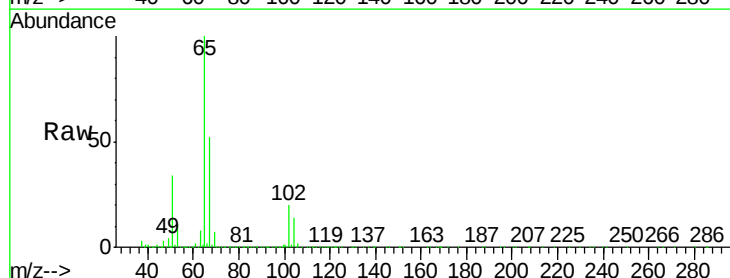

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.06

80000

60000


40000


20000

0

Time-->

5.90 6.00 6.10 6.20

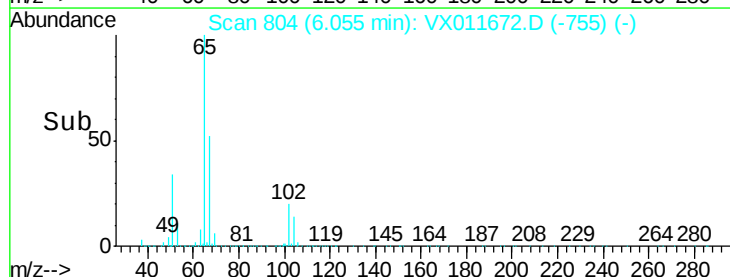

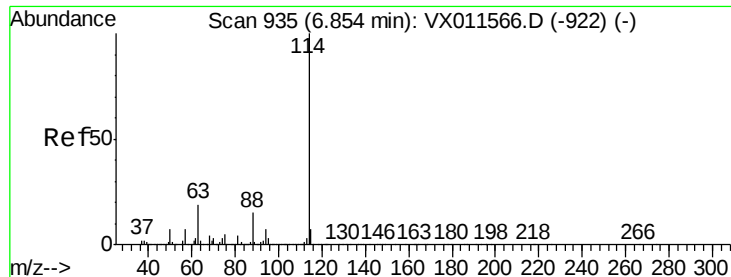

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 934

Delta R.T. -0.01 min

Lab File: VX011672.D

Acq: 20 Aug 2019 10:13

Instrument :

MSVOA_X

ClientSampleId :

VX0820MBL01


Tot Ion:114 Resp: 486175

Ion Ratio Lower Upper

114 100

63 19.4 0.0 37.8




88 15.8 0.0 30.2

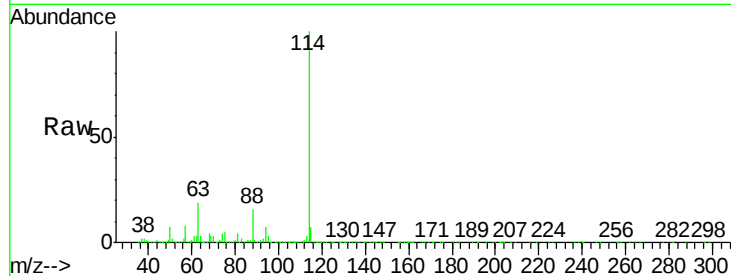

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

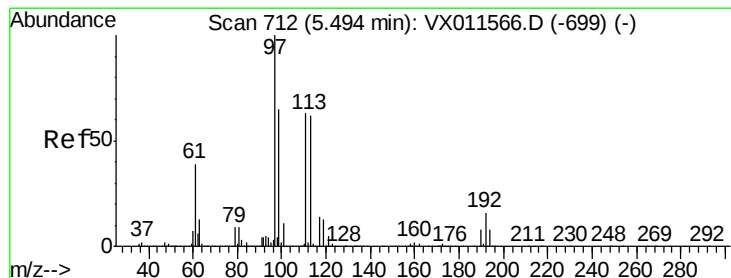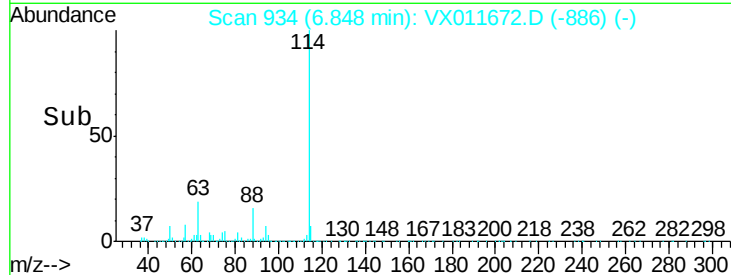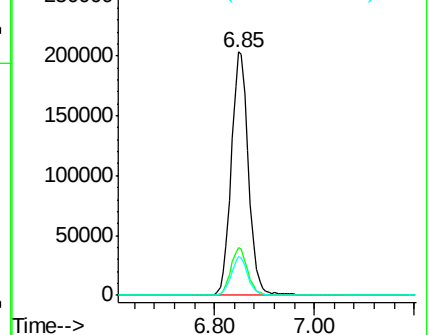

#35

Dibromofluoromethane

Concen: 52.217 ug/l

RT: 5.49 min Scan# 711

Delta R.T. -0.01 min

Lab File: VX011672.D

Acq: 20 Aug 2019 10:13


Tgt Ion:113 Resp: 166045

Ion Ratio Lower Upper

113 100

111 102.0 81.1 121.7



192 25.0 20.8 31.2

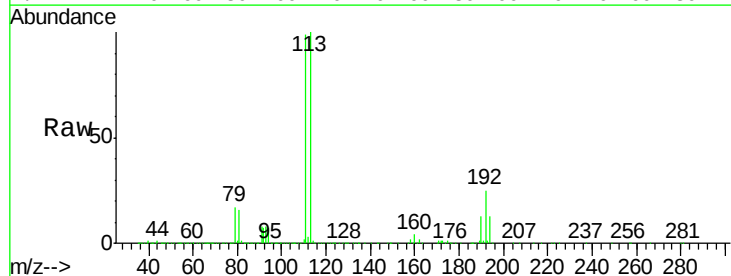


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

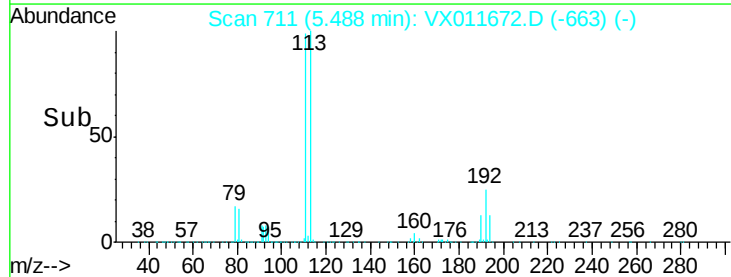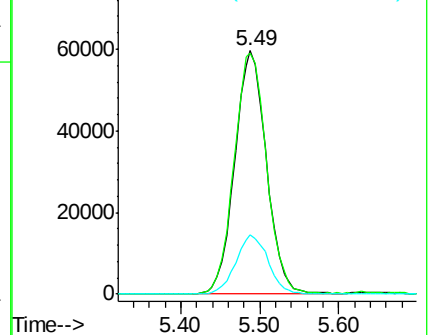

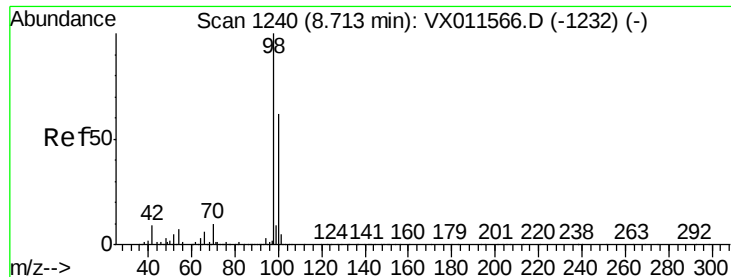

#50

Toluene-d8

Concen: 59.326 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX011672.D

Acq: 20 Aug 2019 10:13

Instrument :

MSVOA_X

ClientSampleId :





VX0820MBL01

Tot Ion: 98 Resp: 587810

Ion Ratio Lower Upper

98 100

100 64.3 52.4 78.6

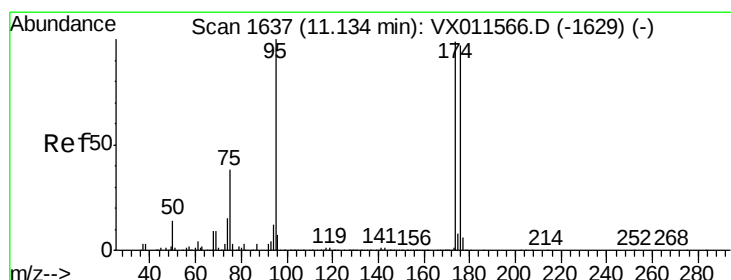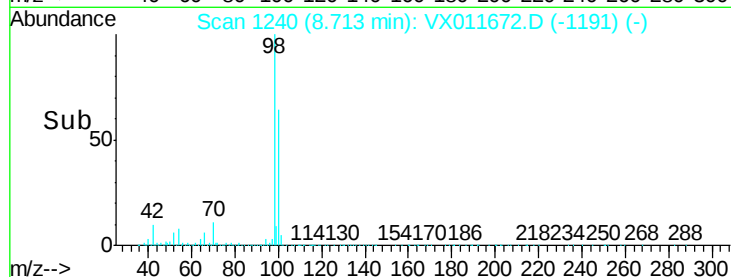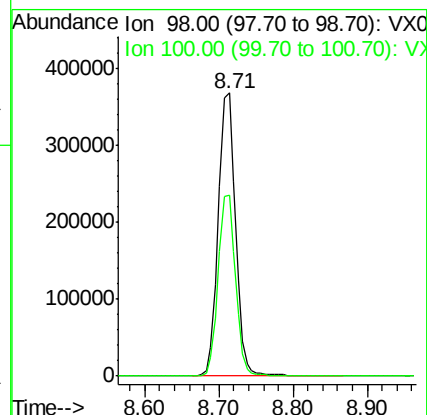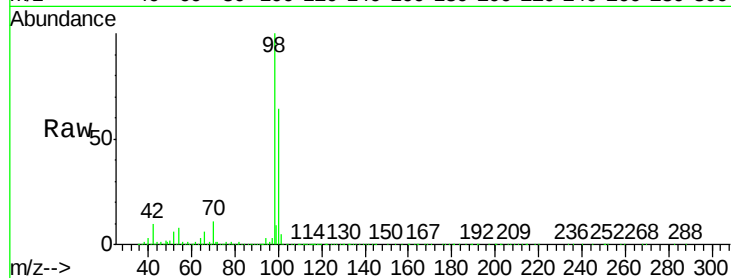

#62

4-Bromofluorobenzene

Concen: 51.733 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX011672.D

Acq: 20 Aug 2019 10:13




Tgt Ion: 95 Resp: 216350


Ion Ratio Lower Upper

95 100

174 96.1 0.0 200.6

176 93.5 0.0 196.6


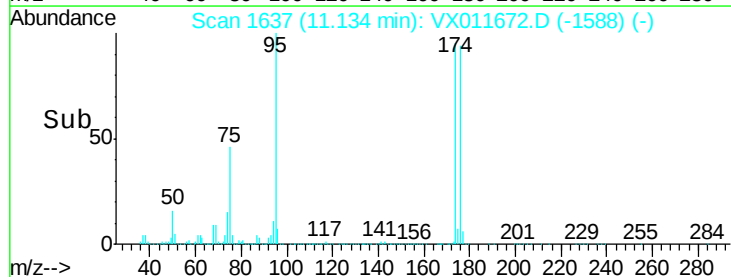
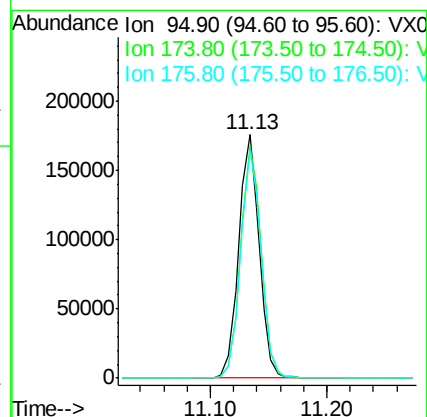
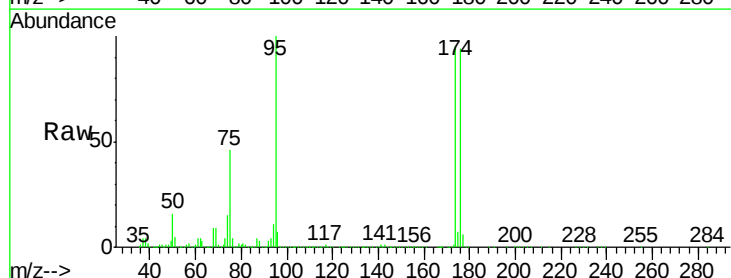


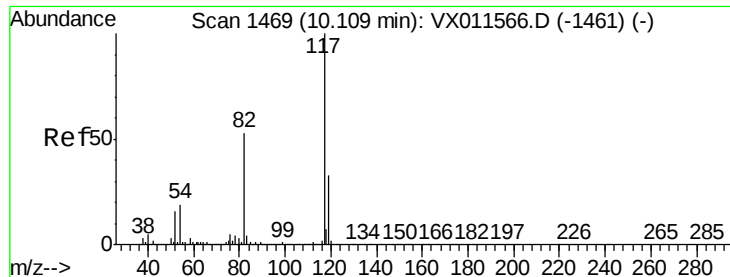

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX011672.D
Acq: 20 Aug 2019 10:13

Instrument :
MSVOA_X
ClientSampleId :
VX0820MBL01

Tot Ion	Ratio	Lower	Upper
117	100		
82	52.3	42.0	63.0
119	32.6	26.5	39.7

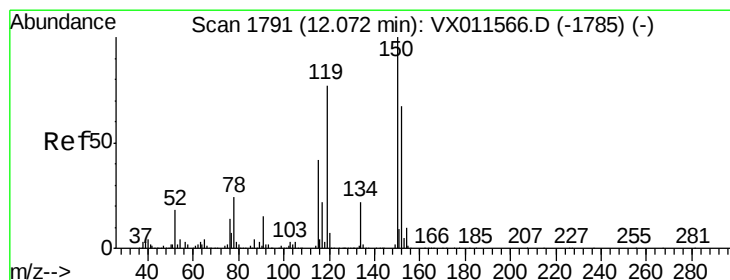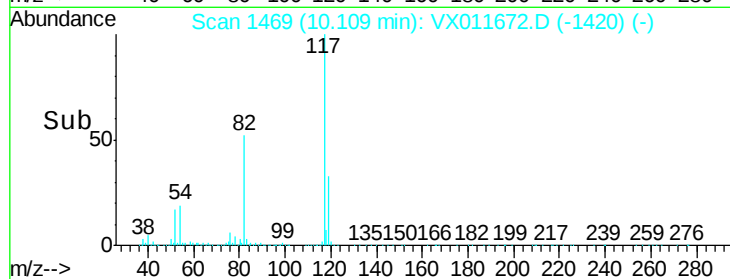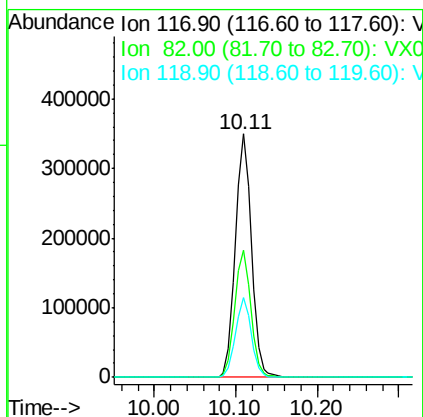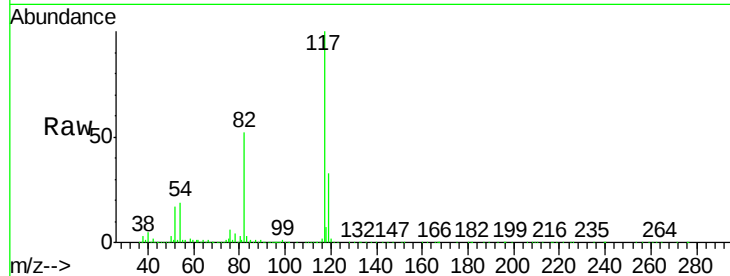

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1791
Delta R.T. 0.00 min
Lab File: VX011672.D
Acq: 20 Aug 2019 10:13

Tgt Ion	Ratio	Lower	Upper
152	100		
115	54.0	37.3	111.9
150	156.9	0.0	346.2

