


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082019\
 Data File : VX011694.D
 Acq On : 20 Aug 2019 19:19
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
 Title : SW846 8260
 Last Update : Fri Aug 16 04:15:26 2019

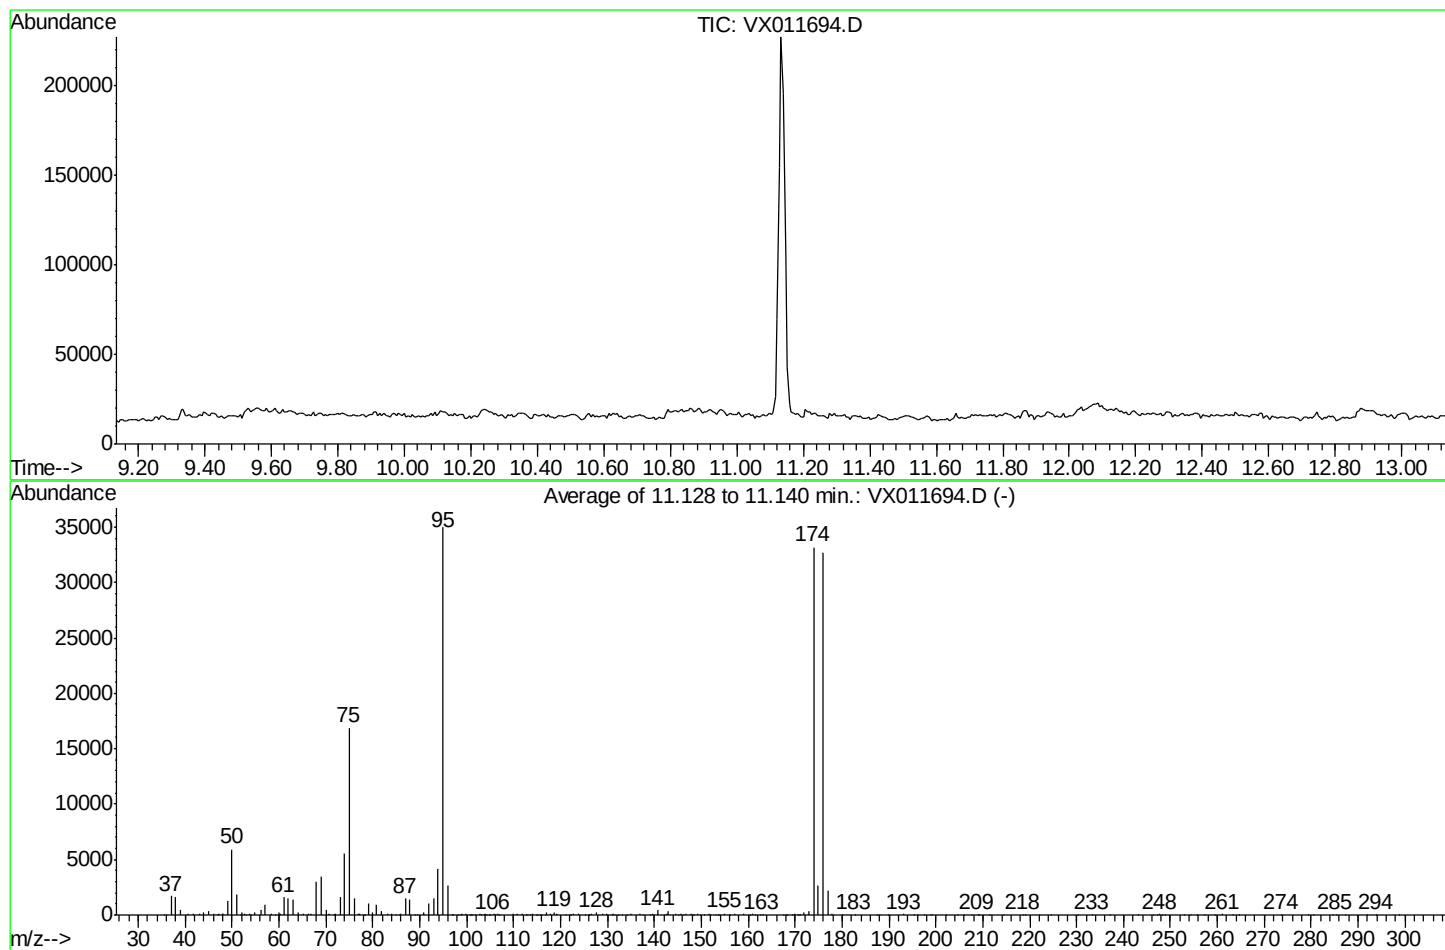

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	5949	PASS
75	95	30	60	48.2	16862	PASS
95	95	100	100	100.0	34973	PASS
96	95	5	9	7.5	2624	PASS
173	174	0.00	2	0.9	299	PASS
174	95	50	100	94.9	33178	PASS
175	174	5	9	8.2	2713	PASS
176	174	95	101	98.6	32701	PASS
177	176	5	9	6.6	2146	PASS