


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082020\
 Data File : VX018021.D
 Acq On : 20 Aug 2020 08:50
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081920W.M
 Title : SW846 8260
 Last Update : Wed Aug 19 05:36:51 2020

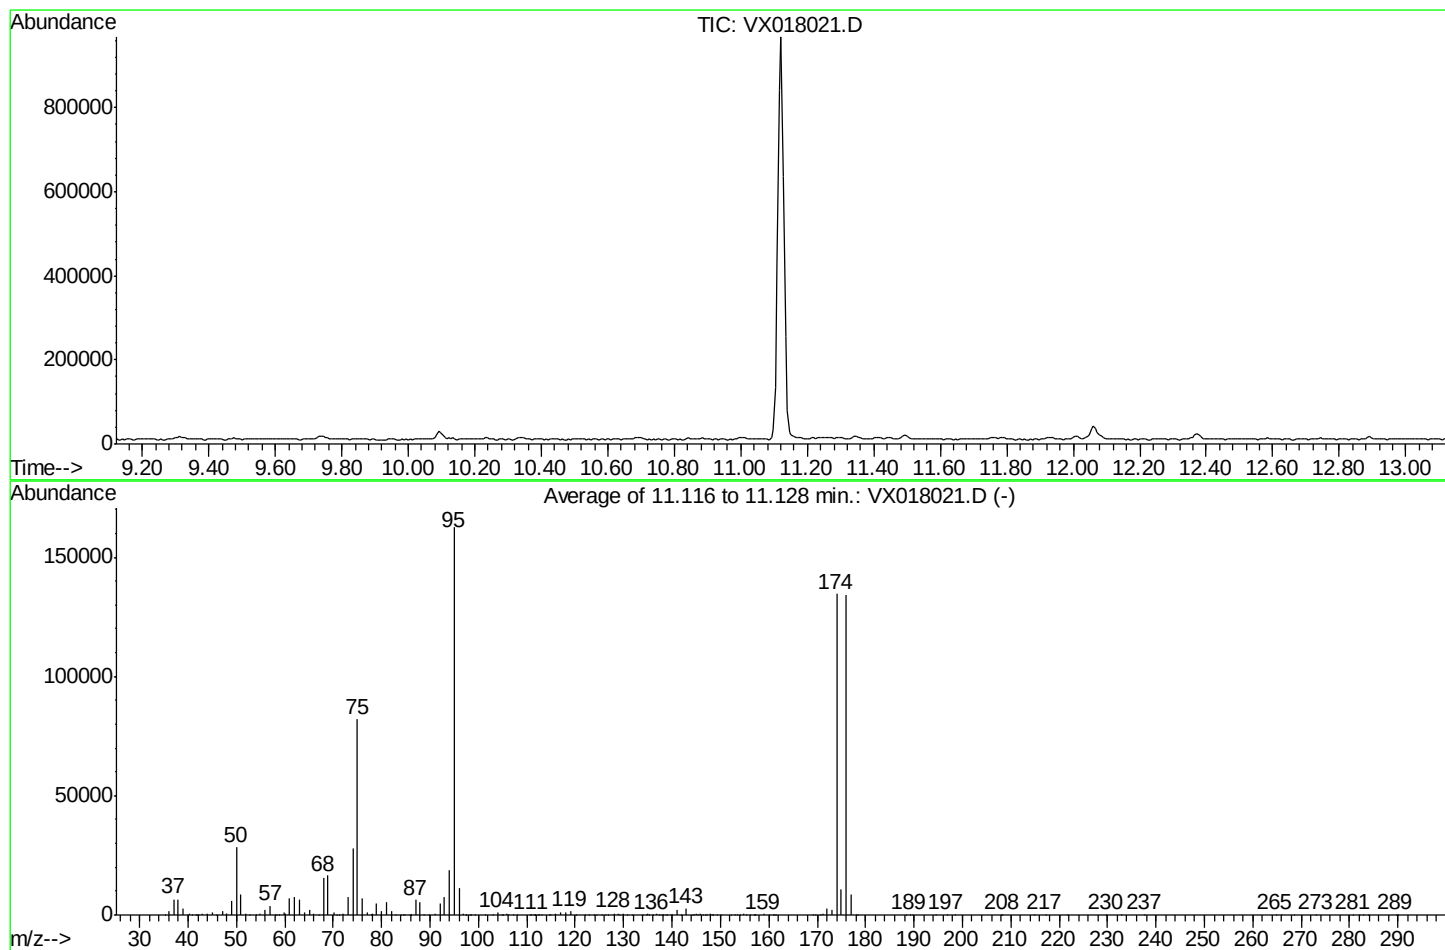

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	28433	PASS
75	95	30	60	50.4	81936	PASS
95	95	100	100	100.0	162533	PASS
96	95	5	9	6.8	11088	PASS
173	174	0.00	2	1.6	2199	PASS
174	95	50	100	82.8	134586	PASS
175	174	5	9	7.9	10584	PASS
176	174	95	101	99.6	133989	PASS
177	176	5	9	6.4	8580	PASS