

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082021\
 Data File : VX023855.D
 Acq On : 19 Aug 2021 22:07
 Operator : JC/MD
 Sample : M3483-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BB-TT-VPB-RW7-GW-340-342

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Title : SW846 8260

Signal : TIC: VX023855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	66	rBV	8882	11410	1.54%	0.301%
2	1.569	71	79	82	rBV3	4563	8167	1.10%	0.215%
3	2.550	235	240	252	rVB	8836	15922	2.15%	0.420%
4	5.397	693	707	721	rBV	85715	249429	33.68%	6.574%
5	5.562	721	734	750	rVB	138589	392914	53.05%	10.356%
6	5.970	789	801	819	rBV	96552	257767	34.80%	6.794%
7	6.769	920	932	946	rBV	228245	536526	72.44%	14.141%
8	8.653	1234	1241	1251	rBV	480184	740657	100.00%	19.521%
9	10.055	1465	1471	1482	rBV	471130	641872	86.66%	16.918%
10	11.085	1634	1640	1651	rBV	352345	451298	60.93%	11.895%
11	12.024	1789	1794	1804	rBV	398724	488155	65.91%	12.866%




Sum of corrected areas: 3794117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082021\
Data File : VX023855.D
Acq On : 19 Aug 2021 22:07
Operator : JC/MD
Sample : M3483-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BB-TT-VPB-RW7-GW-340-342

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

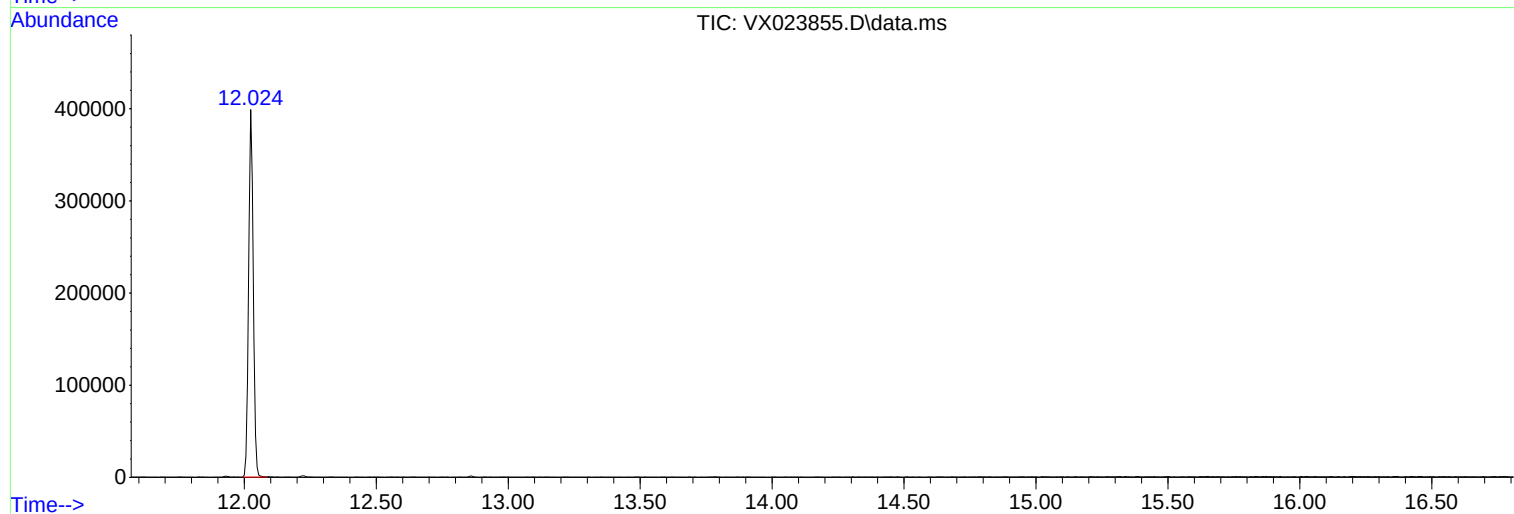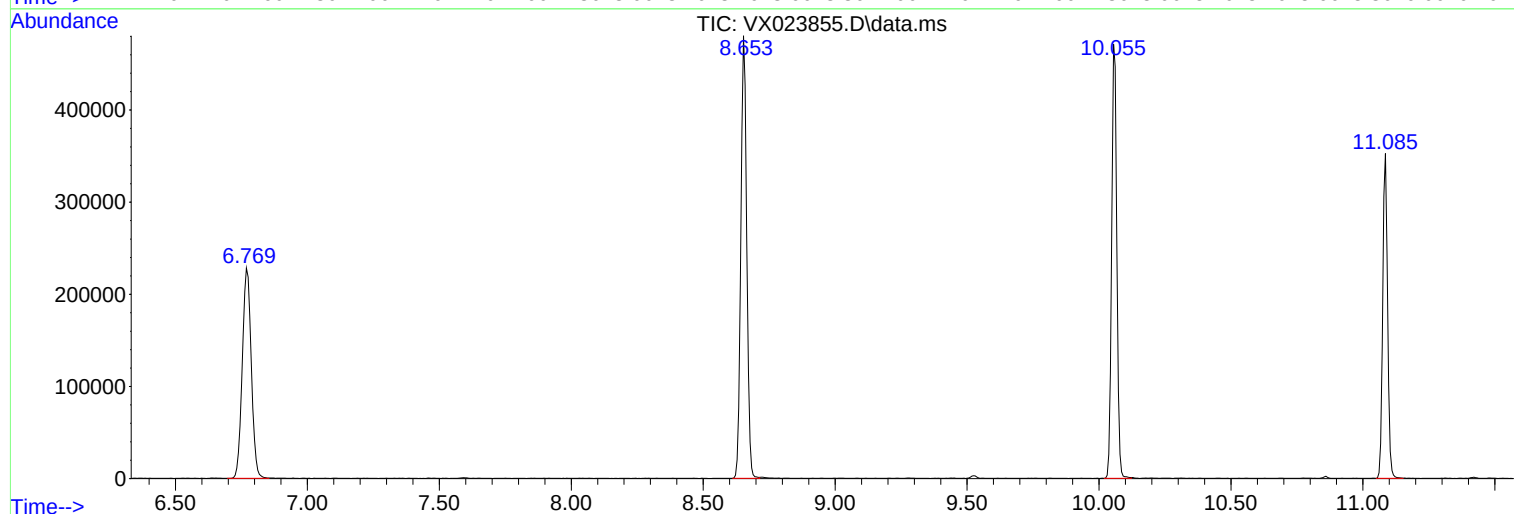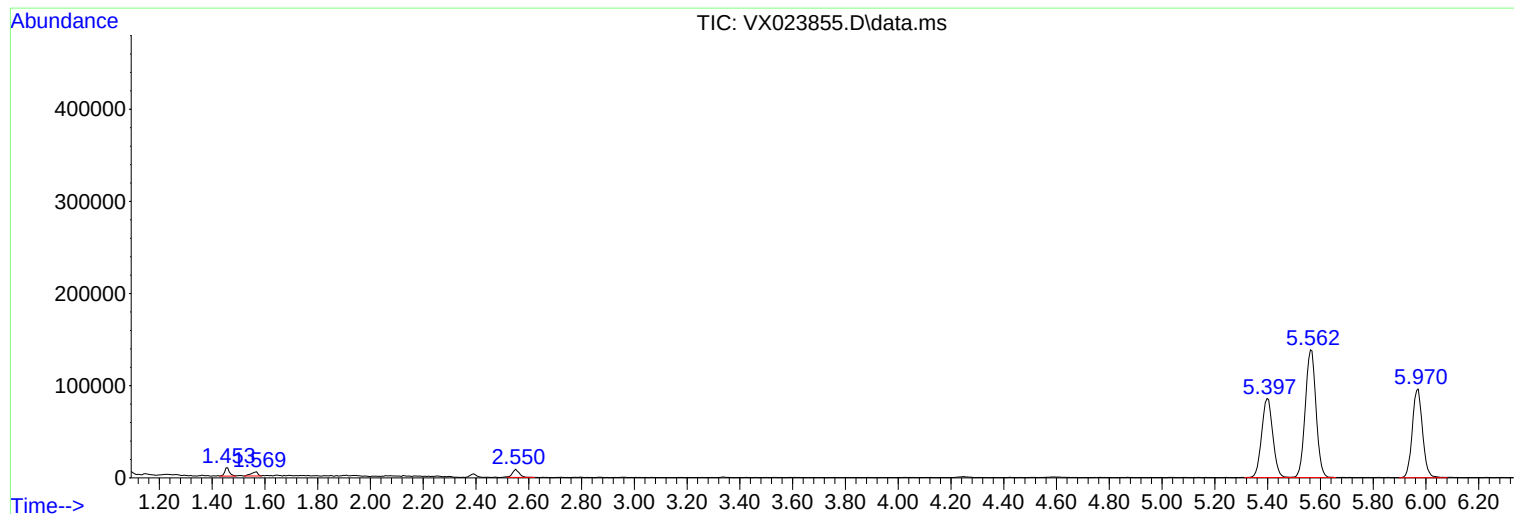

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082021\
Data File : VX023855.D
Acq On : 19 Aug 2021 22:07
Operator : JC/MD
Sample : M3483-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BB-TT-VPB-RW7-GW-340-342

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082021\
Data File : VX023855.D
Acq On : 19 Aug 2021 22:07
Operator : JC/MD
Sample : M3483-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BB-TT-VPB-RW7-GW-340-342

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
