

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082021\
 Data File : VX023858.D
 Acq On : 19 Aug 2021 23:17
 Operator : JC/MD
 Sample : M3484-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 022-OUTFALL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Title : SW846 8260

Signal : TIC: VX023858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	69	rBV	23174	28358	3.77%	0.656%
2	1.569	70	79	83	rVV2	4865	9054	1.20%	0.209%
3	2.063	155	160	165	rBV	9522	14204	1.89%	0.329%
4	2.300	195	199	204	rVB	5987	8417	1.12%	0.195%
5	2.386	207	213	229	rVB	68649	111061	14.77%	2.570%
6	3.587	402	410	416	rBV2	10352	24095	3.20%	0.558%
7	4.013	473	480	490	rBV4	4633	11673	1.55%	0.270%
8	4.245	509	518	519	rBV2	4333	8167	1.09%	0.189%
9	4.300	521	527	533	rVV2	9689	25984	3.46%	0.601%
10	4.379	535	540	549	rVB6	3546	10347	1.38%	0.239%
11	4.580	564	573	586	rBV	10917	31518	4.19%	0.729%
12	5.397	694	707	719	rBV	86751	253108	33.66%	5.857%
13	5.562	722	734	751	rVB2	138904	399112	53.08%	9.235%
14	5.964	790	800	812	rBV	98228	257694	34.27%	5.963%
15	6.769	923	932	949	rVB	229525	536552	71.35%	12.415%
16	7.470	1040	1047	1054	rBV2	5591	11996	1.60%	0.278%
17	7.586	1060	1066	1073	rVB3	4186	7588	1.01%	0.176%
18	8.580	1223	1229	1234	rBV2	11583	18829	2.50%	0.436%
19	8.653	1234	1241	1250	rBV	492160	751948	100.00%	17.399%
20	9.525	1378	1384	1391	rBV3	8879	13174	1.75%	0.305%
21	10.055	1465	1471	1488	rVB	492324	663402	88.22%	15.350%
22	10.659	1565	1570	1579	rVB	38957	49836	6.63%	1.153%
23	11.085	1634	1640	1653	rVB	385363	492374	65.48%	11.393%
24	11.756	1746	1750	1757	rVB	8250	10807	1.44%	0.250%
25	12.024	1789	1794	1806	rVB	459856	558575	74.28%	12.925%
26	12.219	1822	1826	1833	rBV2	9143	13861	1.84%	0.321%


Sum of corrected areas: 4321734

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082021\
Data File : VX023858.D
Acq On : 19 Aug 2021 23:17
Operator : JC/MD
Sample : M3484-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
O22-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

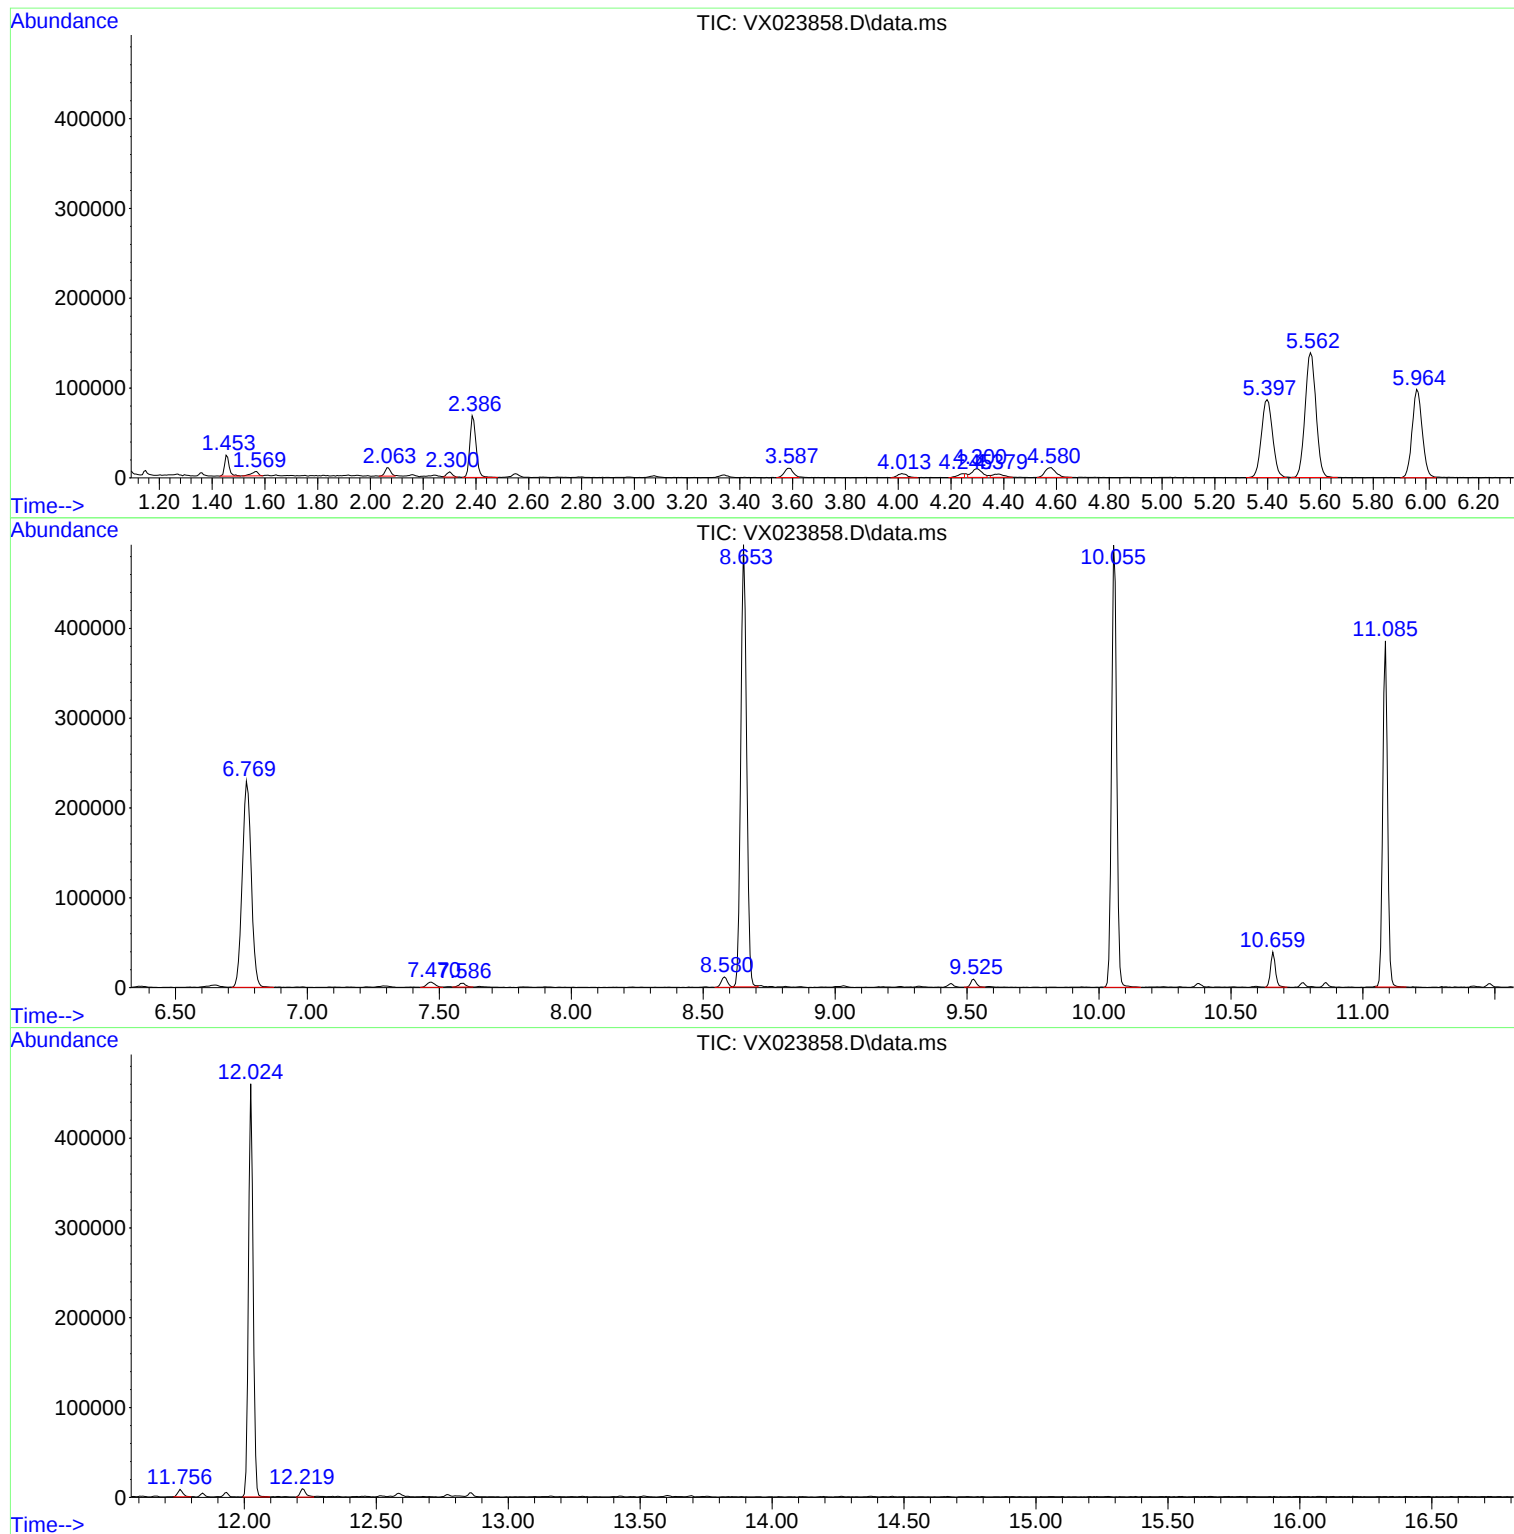

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082021\
Data File : VX023858.D
Acq On : 19 Aug 2021 23:17
Operator : JC/MD
Sample : M3484-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
O22-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082021\
Data File : VX023858.D
Acq On : 19 Aug 2021 23:17
Operator : JC/MD
Sample : M3484-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
O22-OUTFALL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
