


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082021\  
 Data File : VX023841.D  
 Acq On : 19 Aug 2021 16:00  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081721W.M  
 Title : SW846 8260  
 Last Update : Tue Aug 17 11:57:51 2021

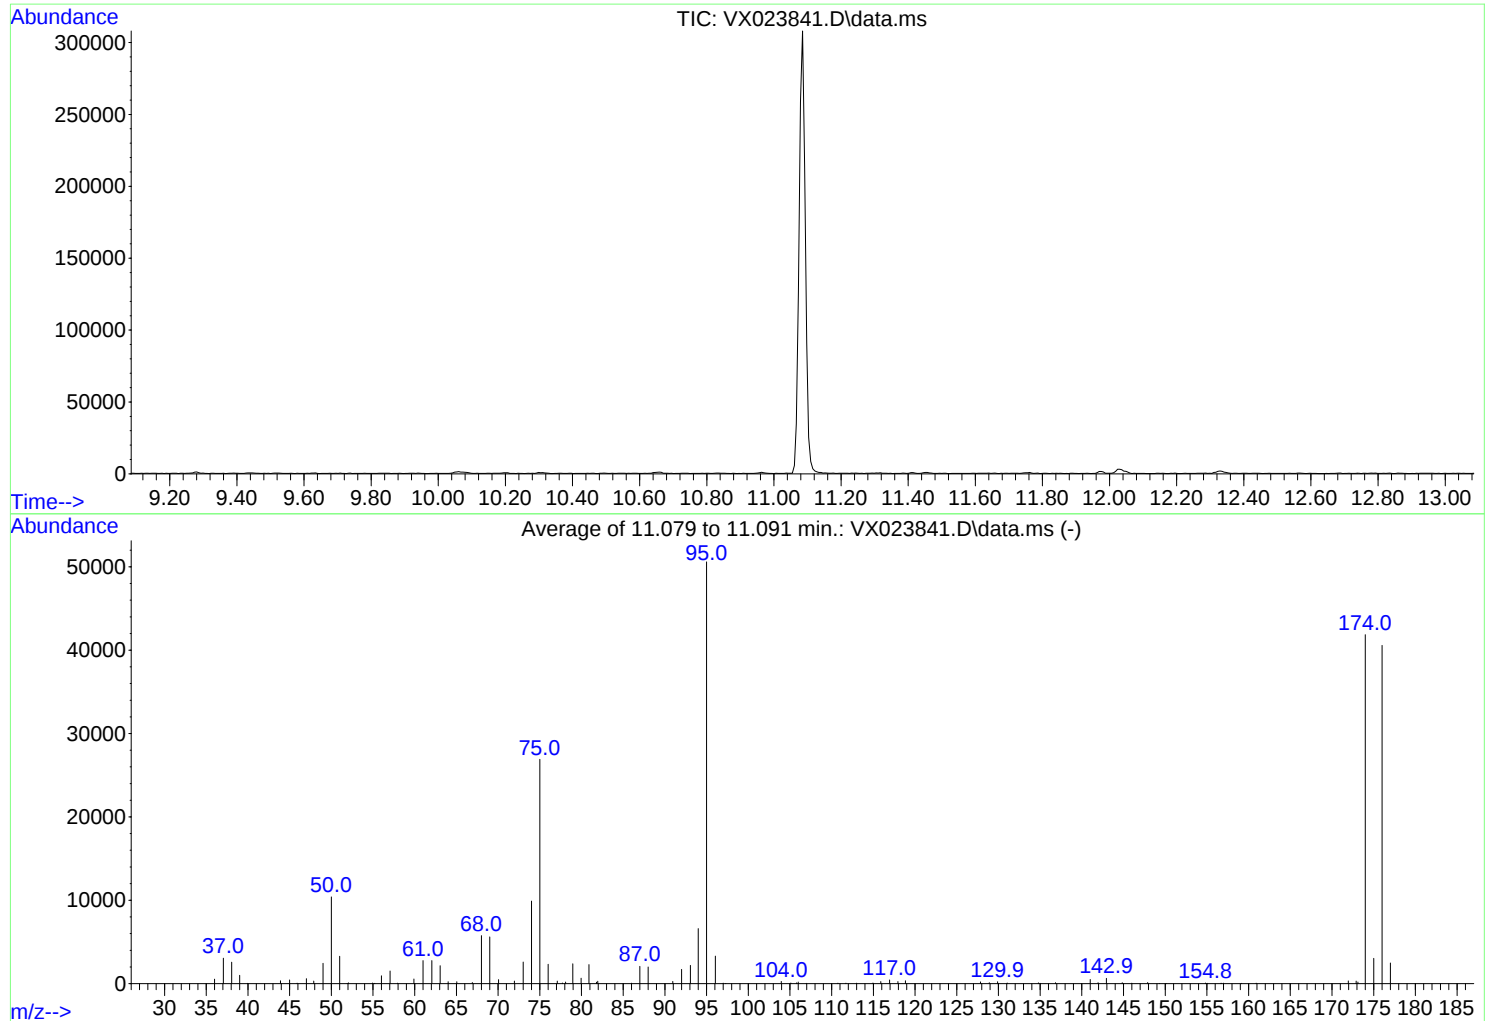

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.6         | 10400      | PASS                |
| 75             | 95              | 30              | 60              | 53.2         | 26901      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 50597      | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 3305       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.7          | 310        | PASS                |
| 174            | 95              | 50              | 100             | 82.7         | 41856      | PASS                |
| 175            | 174             | 5               | 9               | 7.3          | 3035       | PASS                |
| 176            | 174             | 95              | 101             | 97.0         | 40581      | PASS                |
| 177            | 176             | 5               | 9               | 6.1          | 2479       | PASS                |