

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082025\
 Data File : VX047451.D
 Acq On : 20 Aug 2025 18:18
 Operator : JC/MD
 Sample : Q2878-01DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-18B-57.5-081325DL

Quant Time: Aug 21 01:37:46 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.568	168	215725	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	432331	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	427580	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	219266	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	168273	55.735	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 111.480%			
35) Dibromofluoromethane	5.403	113	140124	49.940	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.880%			
50) Toluene-d8	8.653	98	502298	50.085	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 100.160%			
62) 4-Bromofluorobenzene	11.079	95	211301	57.095	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 114.180%			
Target Compounds						Qvalue
3) Chloromethane	1.307	50	1152	0.466	ug/l #	41
4) Vinyl Chloride	1.392	62	15518	4.998	ug/l #	55
6) Chloroethane	1.733	64	1277	0.672	ug/l #	60
9) 1,1,2-Trichlorotrifluo...	2.355	101	921	0.346	ug/l	88
10) Methyl Iodide	2.471	142	1038	0.227	ug/l #	85
11) Tert butyl alcohol	2.971	59	652	2.482	ug/l #	72
12) 1,1-Dichloroethene	2.337	96	2062	0.759	ug/l	98
16) Acetone	2.398	43	5950	5.243	ug/l	91
17) Carbon Disulfide	2.532	76	4859	0.593	ug/l	98
20) Methylene Chloride	2.812	84	959	0.319	ug/l #	78
21) trans-1,2-Dichloroethene	3.117	96	3018	1.047	ug/l #	87
24) 1,1-Dichloroethane	3.629	63	3602	0.683	ug/l #	93
27) cis-1,2-Dichloroethene	4.507	96	273342	81.407	ug/l	89
29) Tetrahydrofuran	5.056	42	1134	1.180	ug/l #	74
31) Cyclohexane	5.574	56	5229	1.076	ug/l #	5
36) 1,1-Dichloropropene	5.568	75	17674	3.990	ug/l #	47
38) Carbon Tetrachloride	5.568	117	22390	4.626	ug/l #	13
40) Benzene	6.062	78	8309	0.627	ug/l	94
41) Methacrylonitrile	5.056	41	895	0.462	ug/l #	30
44) Trichloroethene	7.135	130	49879	14.693	ug/l	94
52) Toluene	8.726	92	4849	0.592	ug/l	91
67) Ethyl Benzene	10.201	91	7353	0.420	ug/l	100
68) m/p-Xylenes	10.305	106	2534	0.389	ug/l	93
69) o-Xylene	10.646	106	1425	0.227	ug/l	98
70) Styrene	10.659	104	2487	0.235	ug/l #	68
76) 1,2,3-Trichloropropane	11.079	75	110102	27.378	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.079	75	110102	108.152	ug/l #	7
84) 1,2,4-Trimethylbenzene	11.756	105	3024	0.214	ug/l	96
95) Naphthalene	13.774	128	140385	9.645	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082025\
Data File : VX047451.D
Acq On : 20 Aug 2025 18:18
Operator : JC/MD
Sample : Q2878-01DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL

Quant Time: Aug 21 01:37:46 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration




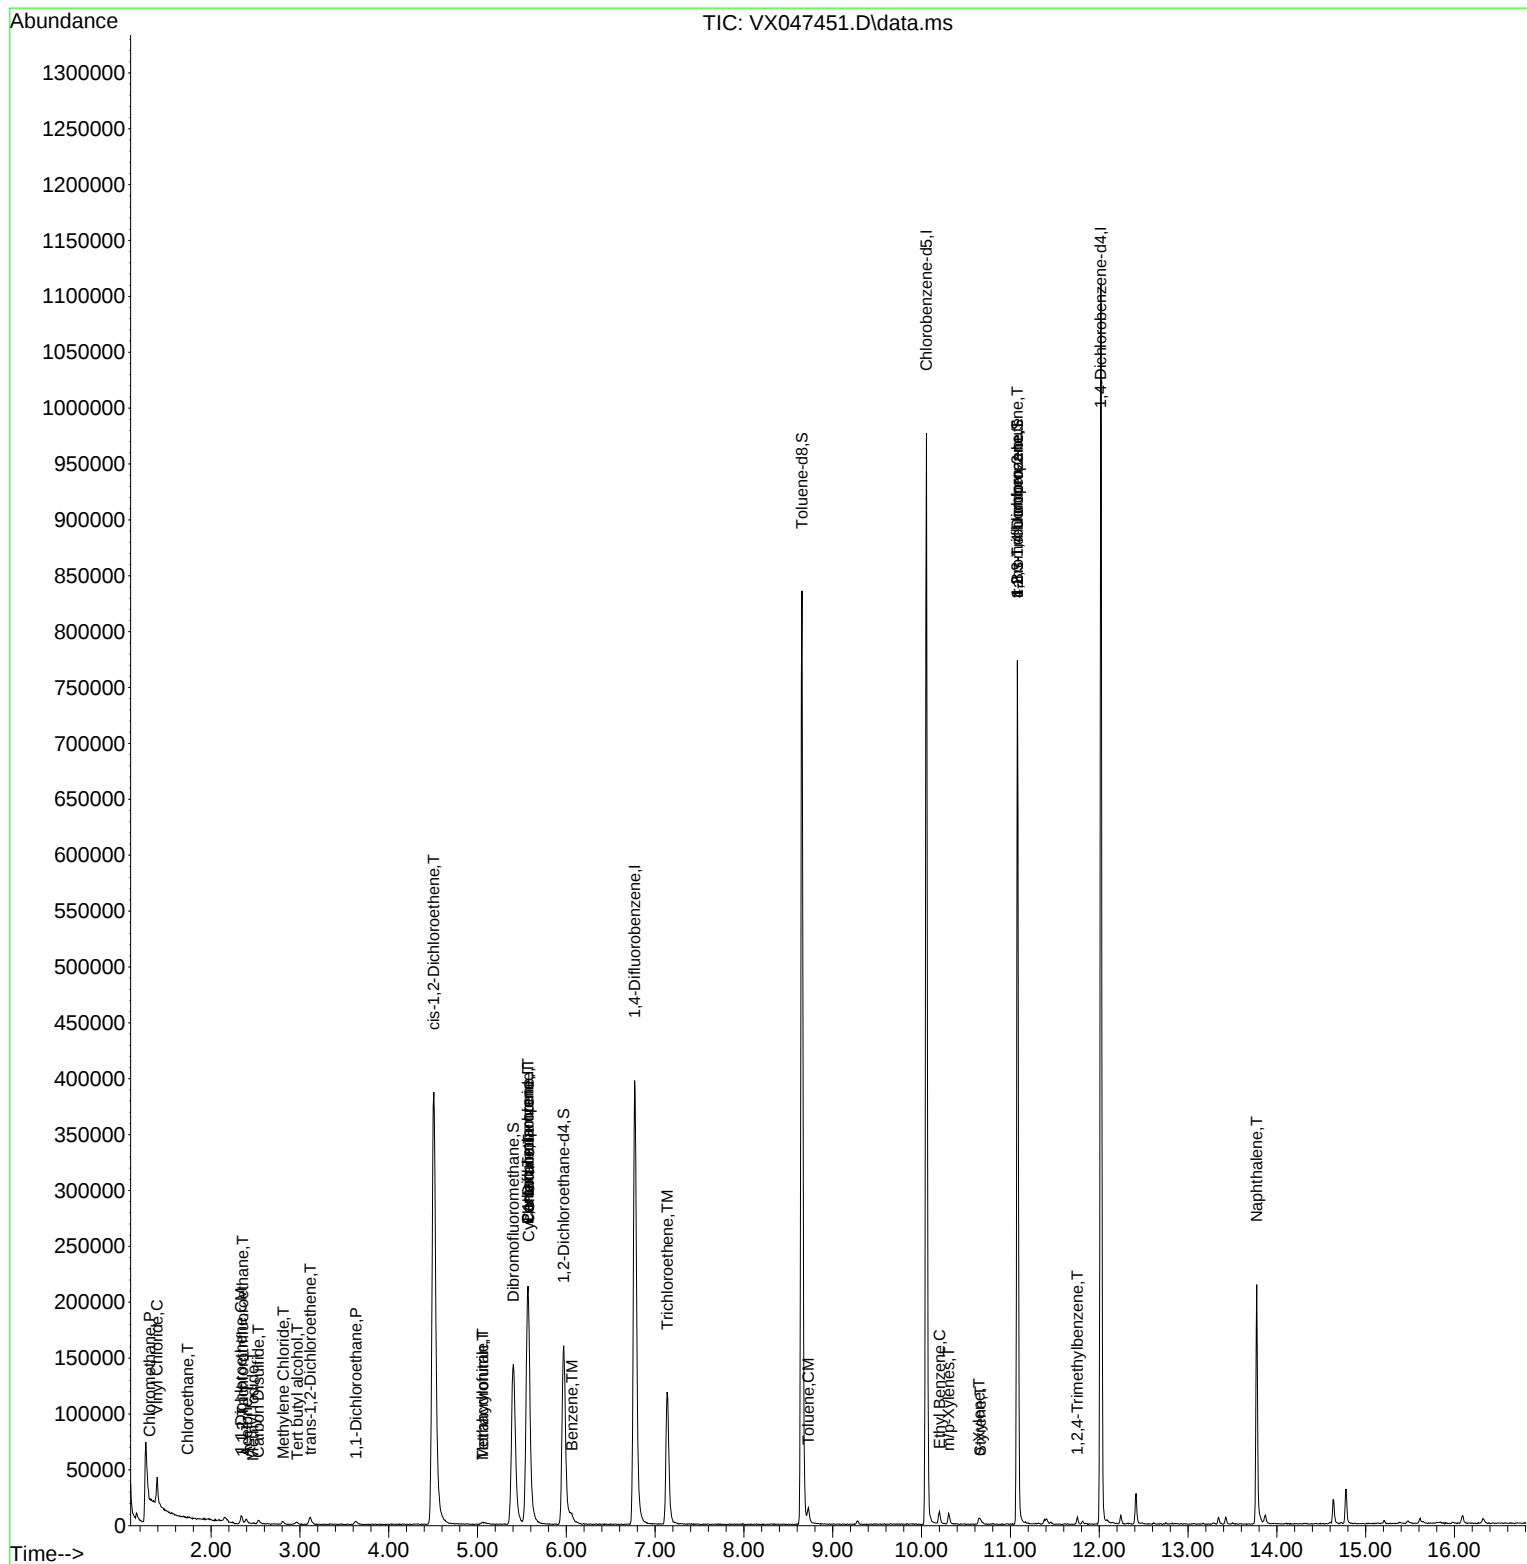




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.568 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion:168 Resp: 215725
Ion Ratio Lower Upper
168 100
99 60.7 47.9 71.9

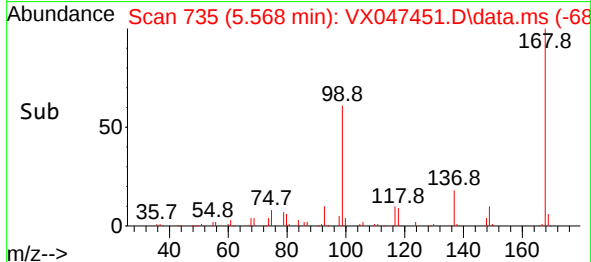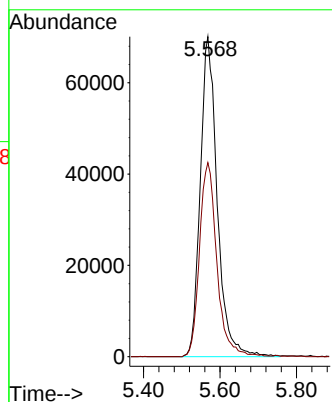

#3
Chloromethane
Concen: 0.466 ug/l
RT: 1.307 min Scan# 36
Delta R.T. -0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion: 50 Resp: 1152
Ion Ratio Lower Upper
50 100
52 0.0 27.0 40.4#



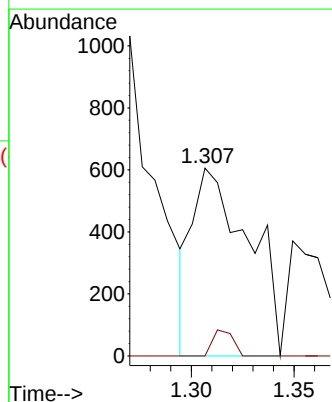
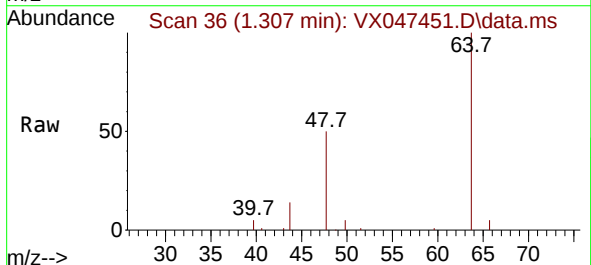


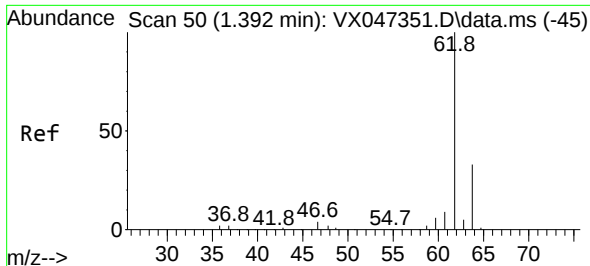

#4
 Vinyl Chloride
 Concen: 4.998 ug/l
 RT: 1.392 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: VX047451.D
 Acq: 20 Aug 2025 18:18




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-18B-57.5-081325DL


Tgt Ion: 62 Resp: 15518
 Ion Ratio Lower Upper
 62 100
 64 58.7 26.5 39.7#

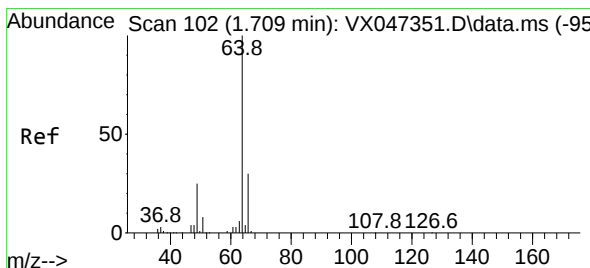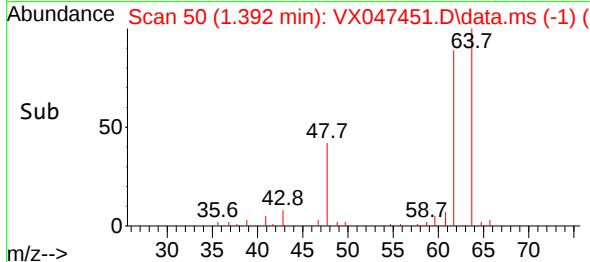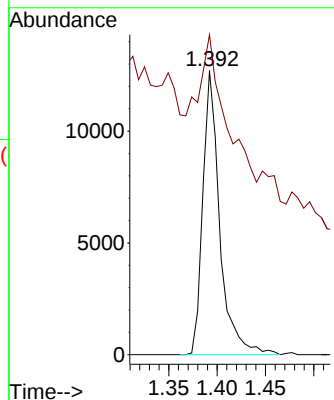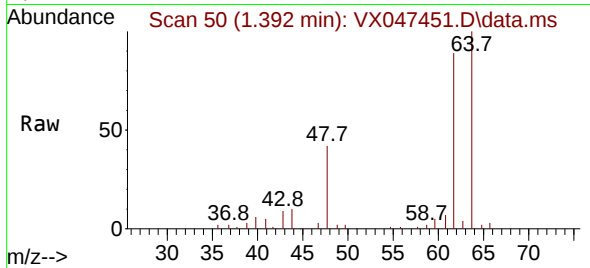

#6
 Chloroethane
 Concen: 0.672 ug/l
 RT: 1.733 min Scan# 106
 Delta R.T. 0.024 min
 Lab File: VX047451.D
 Acq: 20 Aug 2025 18:18

Tgt Ion: 64 Resp: 1277
 Ion Ratio Lower Upper
 64 100
 66 8.6 24.4 36.6#


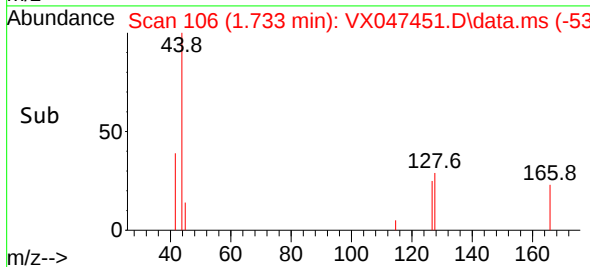
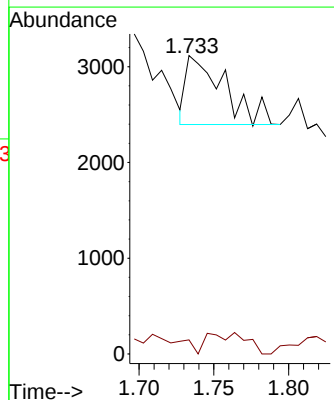
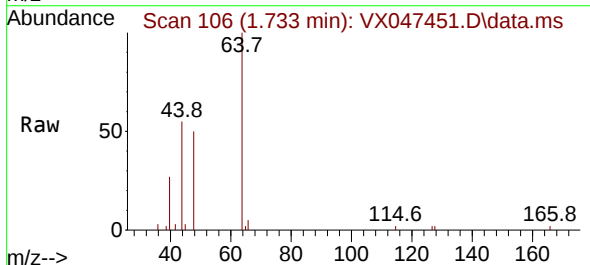




#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.346 ug/l
RT: 2.355 min Scan# 207
Delta R.T. 0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion:101 Resp: 921
Ion Ratio Lower Upper
101 100
85 46.0 34.3 51.5
151 87.9 59.2 88.8

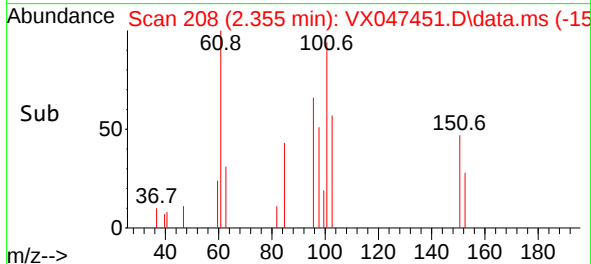

#10
Methyl Iodide
Concen: 0.227 ug/l
RT: 2.471 min Scan# 227
Delta R.T. 0.000 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion:142 Resp: 1038
Ion Ratio Lower Upper
142 100
127 32.8 36.1 54.1#
141 12.7 11.1 16.7


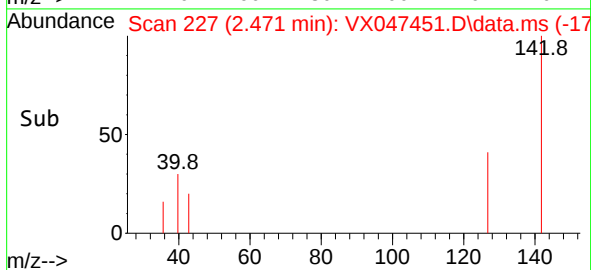




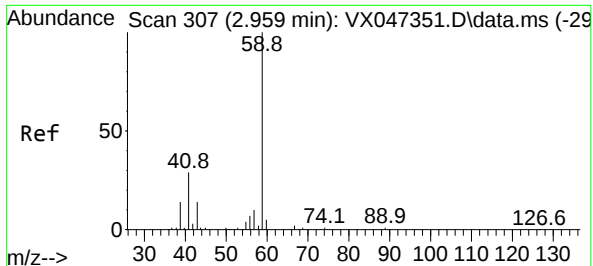

#11
Tert butyl alcohol
Concen: 2.482 ug/l
RT: 2.971 min Scan# 309
Delta R.T. 0.012 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion: 59 Resp: 652
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

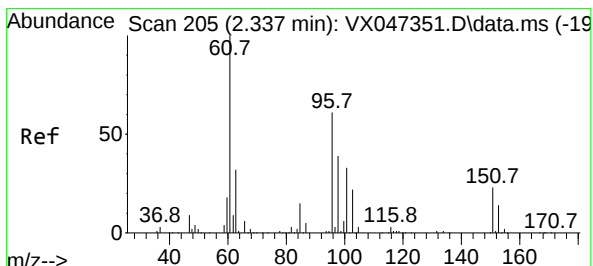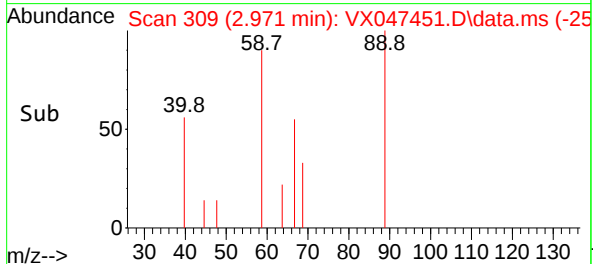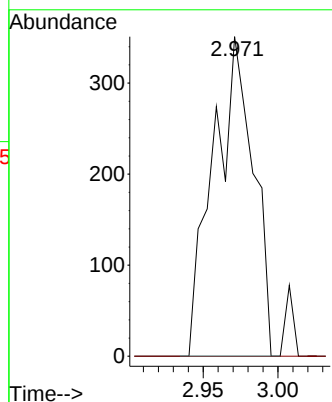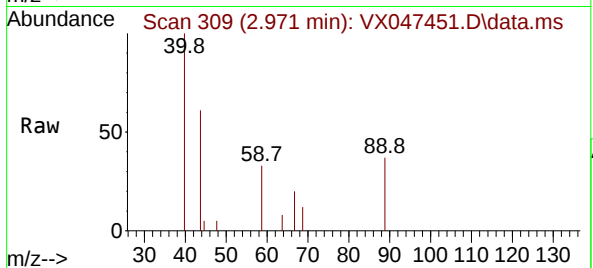

#12
1,1-Dichloroethene
Concen: 0.759 ug/l
RT: 2.337 min Scan# 205
Delta R.T. 0.000 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion: 96 Resp: 2062
Ion Ratio Lower Upper
96 100
61 163.1 132.2 198.2
98 62.6 51.2 76.8


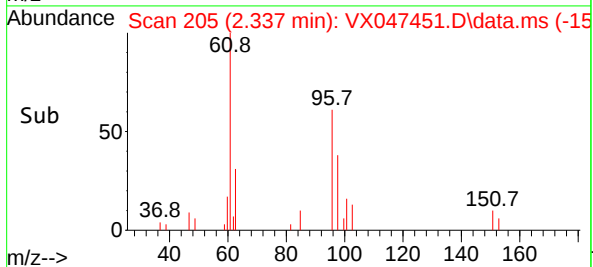
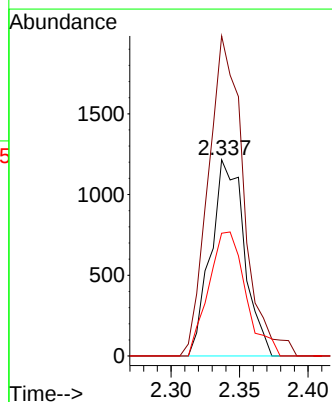
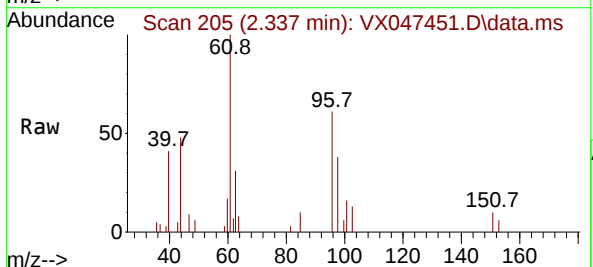




#16
Acetone
Concen: 5.243 ug/l
RT: 2.398 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion: 43 Resp: 5950
Ion Ratio Lower Upper
43 100
58 36.2 24.8 37.2

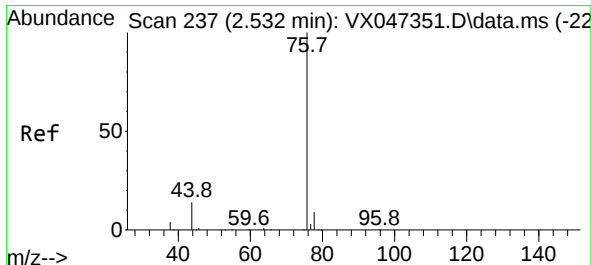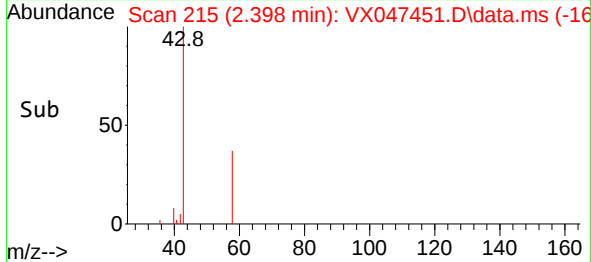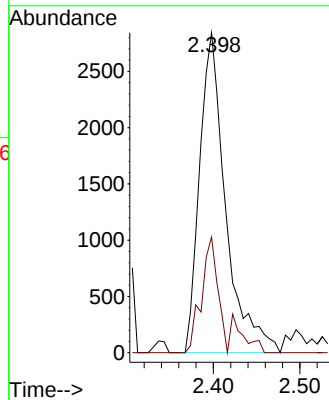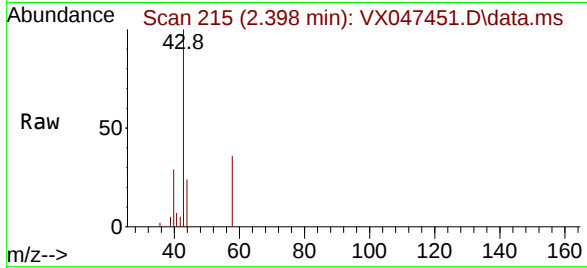

#17
Carbon Disulfide
Concen: 0.593 ug/l
RT: 2.532 min Scan# 237
Delta R.T. 0.000 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion: 76 Resp: 4859
Ion Ratio Lower Upper
76 100
78 9.6 7.2 10.8



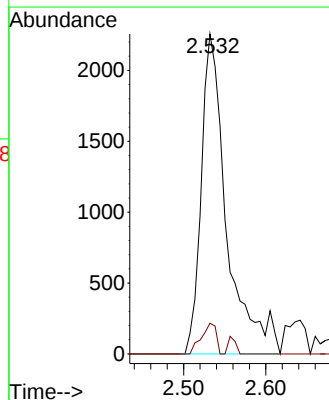
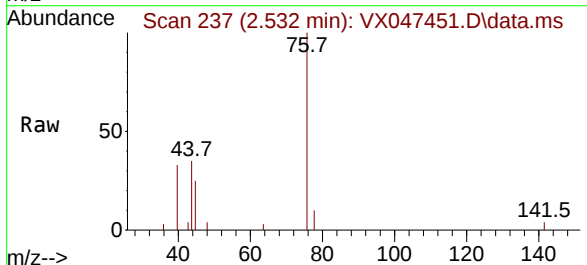




#20
Methylene Chloride
Concen: 0.319 ug/l
RT: 2.812 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion: 84	Resp: 959
Ion Ratio	Lower Upper
84	100
49	88.2 100.1 150.1#
51	30.3 29.5 44.3
86	57.5 51.8 77.8

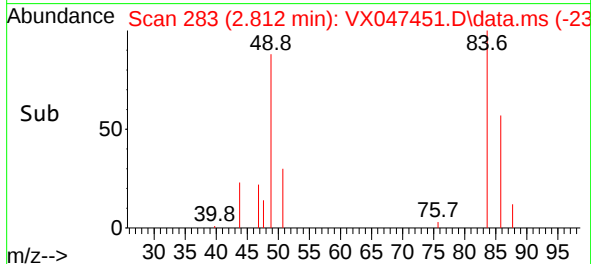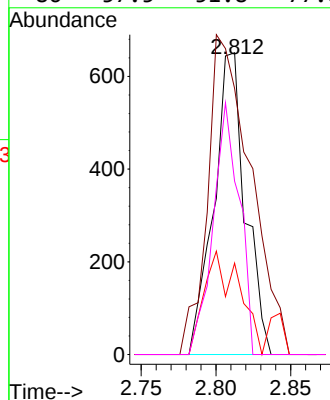

#21
trans-1,2-Dichloroethene
Concen: 1.047 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.012 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion: 96	Resp: 3018
Ion Ratio	Lower Upper
96	100
61	151.1 112.6 169.0
98	82.8 50.9 76.3#


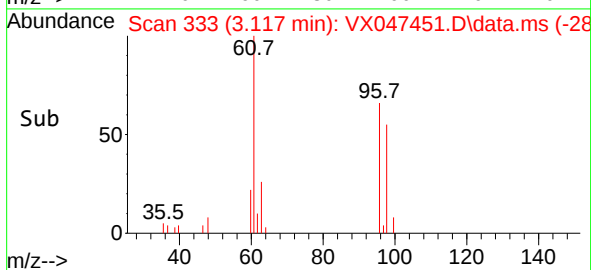
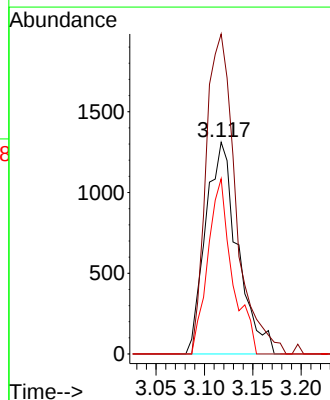





#24
1,1-Dichloroethane
Concen: 0.683 ug/l
RT: 3.629 min Scan# 416
Delta R.T. 0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion: 63 Resp: 3602
Ion Ratio Lower Upper
63 100
98 5.5 3.3 9.9
100 0.0 2.1 6.3#

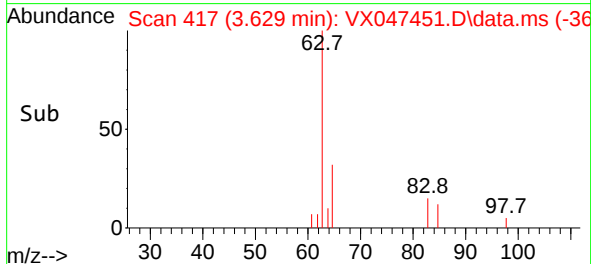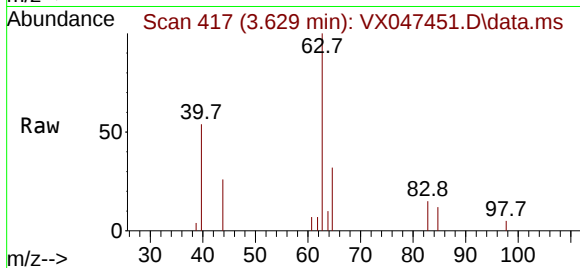

#27
cis-1,2-Dichloroethene
Concen: 81.407 ug/l
RT: 4.507 min Scan# 561
Delta R.T. 0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion: 96 Resp: 273342
Ion Ratio Lower Upper
96 100
61 129.7 0.0 296.6
98 63.7 0.0 130.4

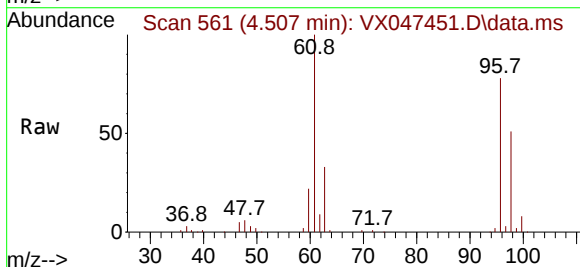

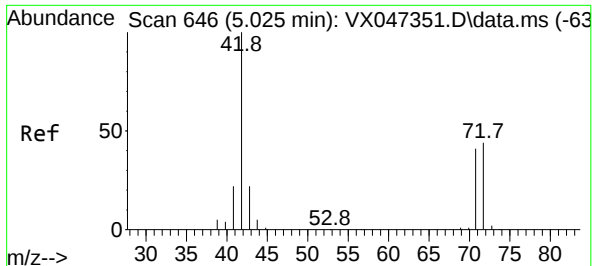

#29

Tetrahydrofuran

Concen: 1.180 ug/l

RT: 5.056 min Scan# 61

Delta R.T. 0.031 min

Lab File: VX047451.D

Acq: 20 Aug 2025 18:18





Instrument :

MSVOA_X

ClientSampleId :

MW-18B-57.5-081325DL

Tgt Ion:	42	Resp:	1134
Ion	Ratio	Lower	Upper
42	100		
72	14.3	34.6	51.8#
71	36.9	32.6	49.0

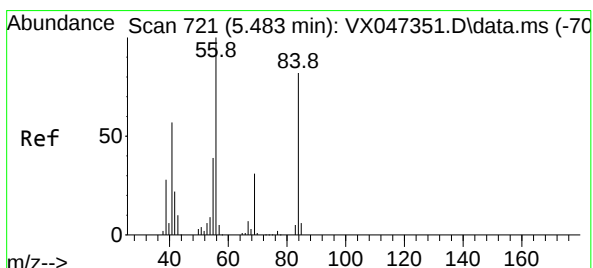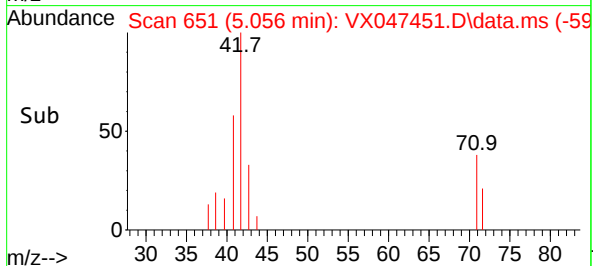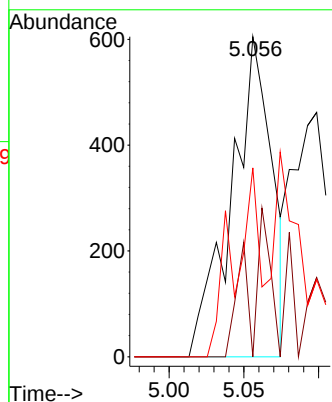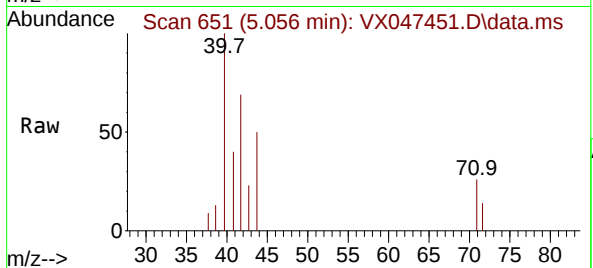

#31

Cyclohexane

Concen: 1.076 ug/l




RT: 5.574 min Scan# 736


Delta R.T. 0.092 min

Lab File: VX047451.D

Acq: 20 Aug 2025 18:18

Tgt Ion:	56	Resp:	5229
Ion	Ratio	Lower	Upper
56	100		
69	178.1	24.3	36.5#
84	107.8	65.3	97.9#


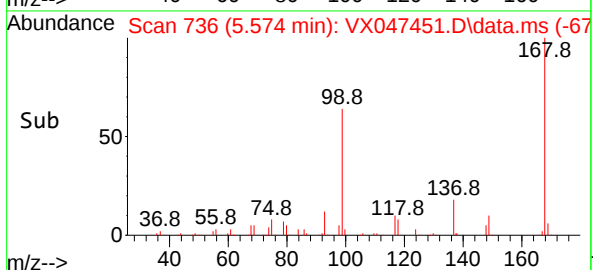

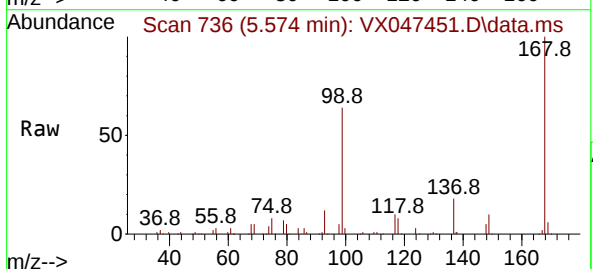




#33
 1,2-Dichloroethane-d4
 Concen: 55.735 ug/l
 RT: 5.970 min Scan# 801
 Delta R.T. 0.006 min
 Lab File: VX047451.D
 Acq: 20 Aug 2025 18:18




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-18B-57.5-081325DL


Tgt Ion: 65 Resp: 168273
 Ion Ratio Lower Upper
 65 100
 67 51.2 0.0 106.0

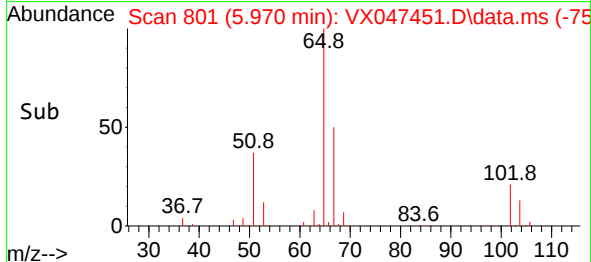

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.769 min Scan# 932
 Delta R.T. 0.000 min
 Lab File: VX047451.D
 Acq: 20 Aug 2025 18:18

Tgt Ion: 114 Resp: 432331
 Ion Ratio Lower Upper
 114 100
 63 22.3 0.0 42.4
 88 17.2 0.0 33.0




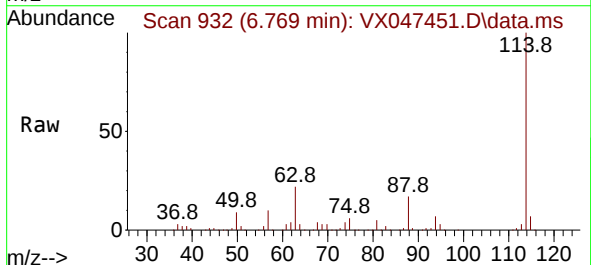




#35
Dibromofluoromethane
Concen: 49.940 ug/l
RT: 5.403 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion:113 Resp: 140124
Ion Ratio Lower Upper
113 100
111 102.0 81.4 122.2
192 18.4 14.1 21.1

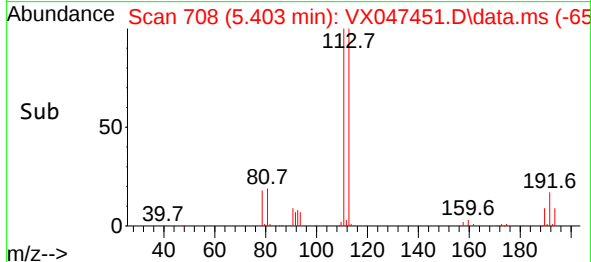

#36
1,1-Dichloropropene
Concen: 3.990 ug/l
RT: 5.568 min Scan# 735
Delta R.T. -0.140 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion: 75 Resp: 17674
Ion Ratio Lower Upper
75 100
110 5.8 17.4 52.2#
77 0.0 24.4 36.6#


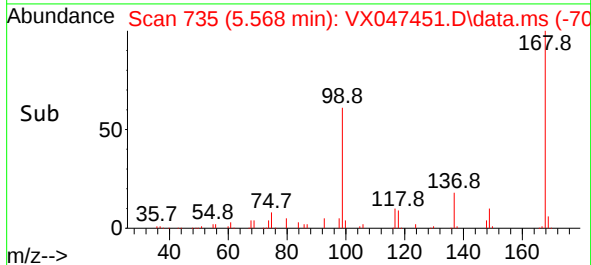






#38
Carbon Tetrachloride
Concen: 4.626 ug/l
RT: 5.568 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion:117 Resp: 22390
Ion Ratio Lower Upper
117 100
119 2.9 78.5 117.7#
121 0.0 24.7 37.1#

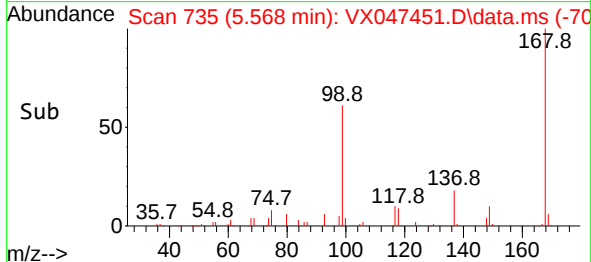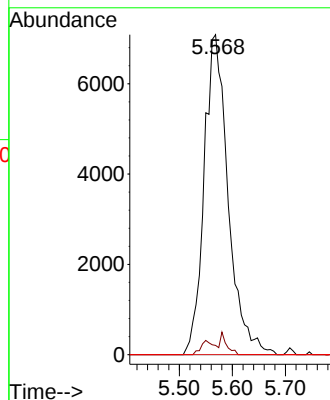

#40
Benzene
Concen: 0.627 ug/l
RT: 6.062 min Scan# 816
Delta R.T. 0.012 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion: 78 Resp: 8309
Ion Ratio Lower Upper
78 100
77 26.8 19.0 28.4



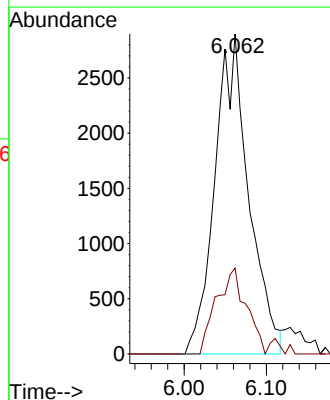
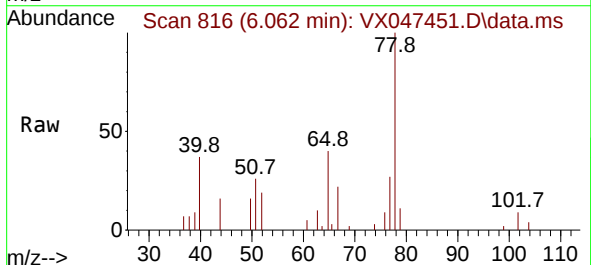


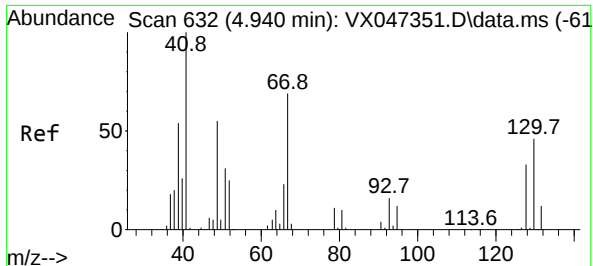

#41
Methacrylonitrile
Concen: 0.462 ug/l
RT: 5.056 min Scan# 61
Delta R.T. 0.116 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion: 41	Resp:	895
Ion	Ratio	Lower Upper
41	100	
39	21.5	45.4 68.2#
67	0.0	64.0 96.0#
52	0.0	27.0 40.6#

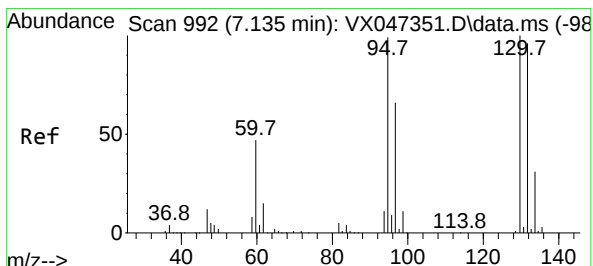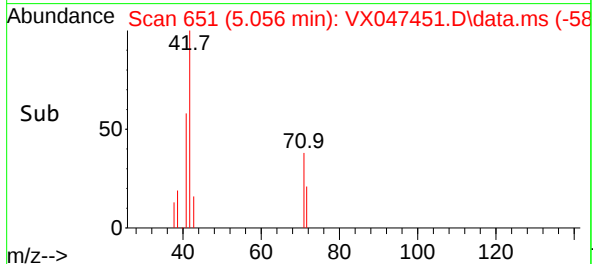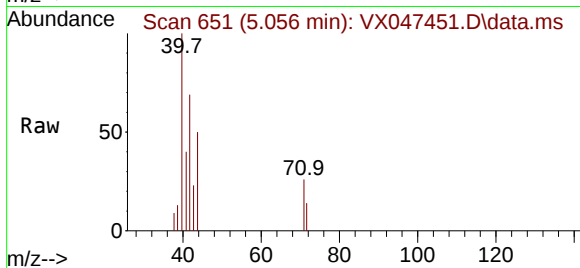

#44
Trichloroethene
Concen: 14.693 ug/l
RT: 7.135 min Scan# 992
Delta R.T. 0.000 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion: 130	Resp:	49879
Ion	Ratio	Lower Upper
130	100	
95	93.4	0.0 198.6


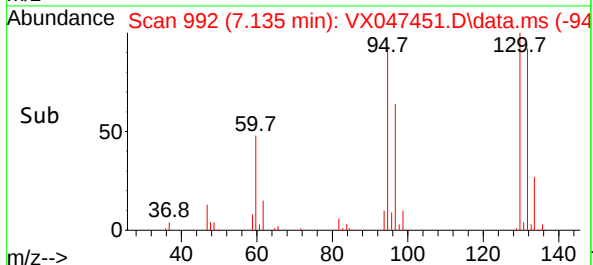
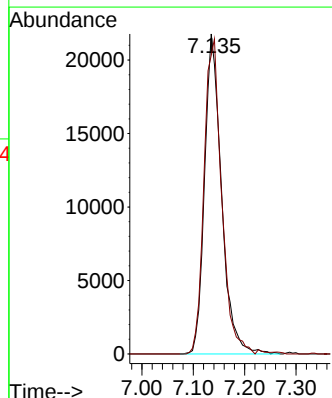
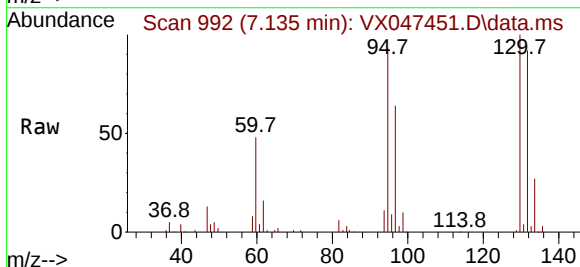


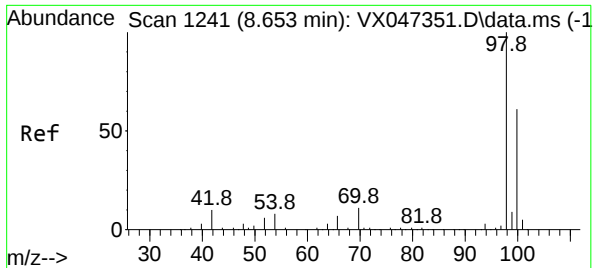

#50
Toluene-d8
Concen: 50.085 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion: 98 Resp: 502298
Ion Ratio Lower Upper
98 100
100 66.6 53.9 80.9

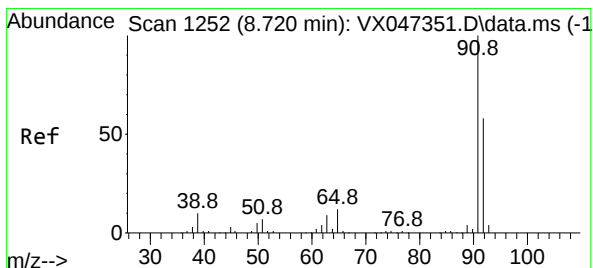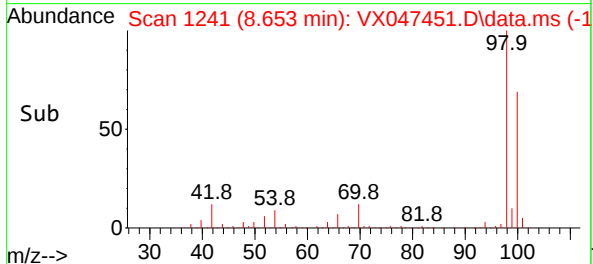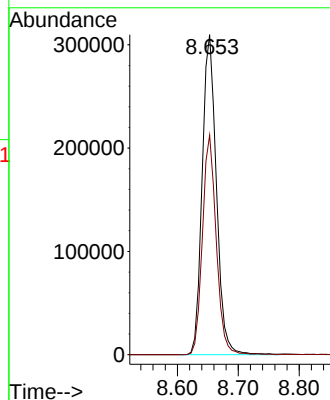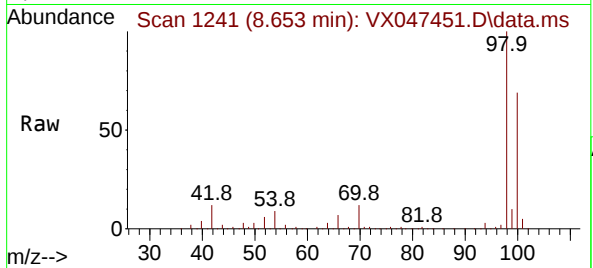

#52
Toluene
Concen: 0.592 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion: 92 Resp: 4849
Ion Ratio Lower Upper
92 100
91 182.9 136.3 204.5

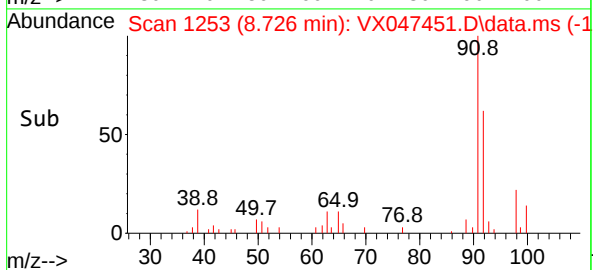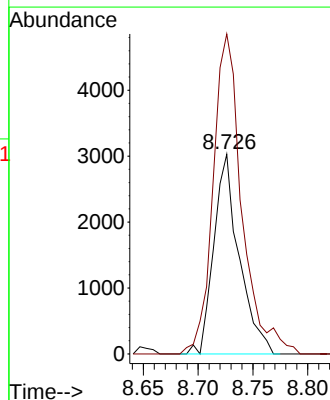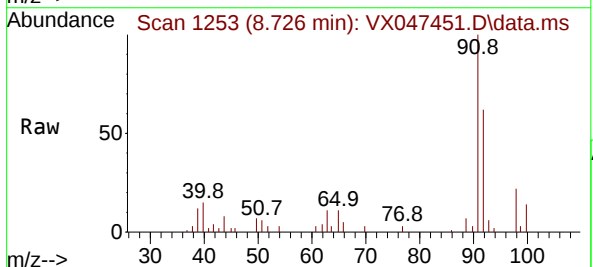



#62

4-Bromofluorobenzene

Concen: 57.095 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX047451.D

Acq: 20 Aug 2025 18:18

Instrument :

MSVOA_X

ClientSampleId :

MW-18B-57.5-081325DL





Tgt Ion: 95 Resp: 211301

Ion Ratio Lower Upper

95 100

174 73.3 0.0 148.0

176 69.5 0.0 145.4

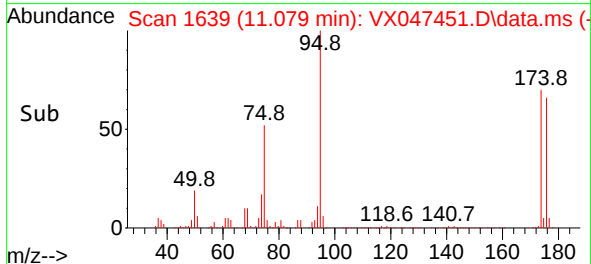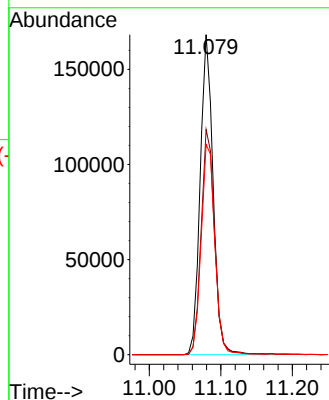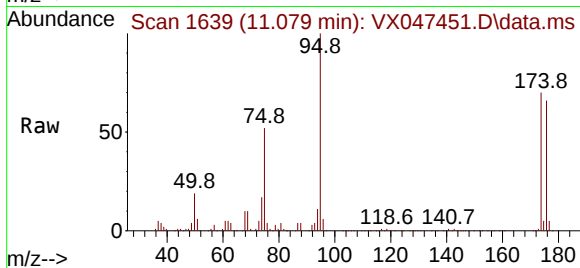

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX047451.D

Acq: 20 Aug 2025 18:18




Tgt Ion: 117 Resp: 427580


Ion Ratio Lower Upper

117 100

82 56.0 45.0 67.4

119 32.0 25.8 38.8

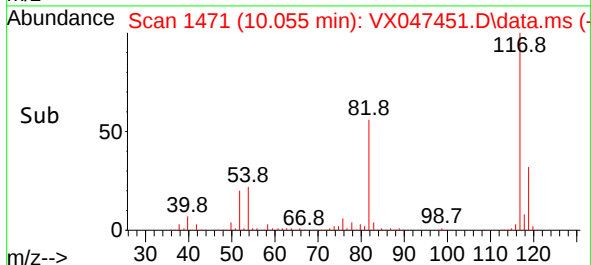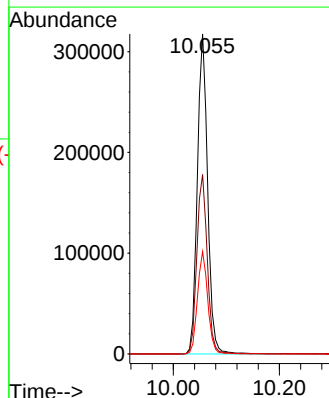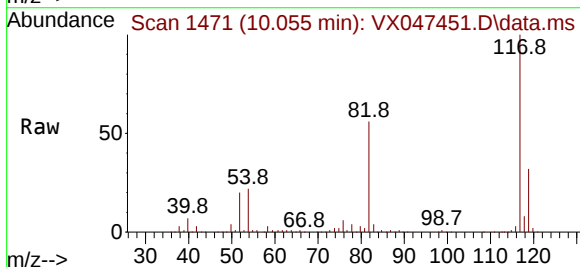



#67

Ethyl Benzene

Concen: 0.420 ug/l

RT: 10.201 min Scan# 1495

Delta R.T. 0.006 min

Lab File: VX047451.D

Acq: 20 Aug 2025 18:18

Instrument :

MSVOA_X

ClientSampleId :





MW-18B-57.5-081325DL

Tgt Ion: 91 Resp: 7353

Ion Ratio Lower Upper

91 100

106 30.4 24.4 36.6

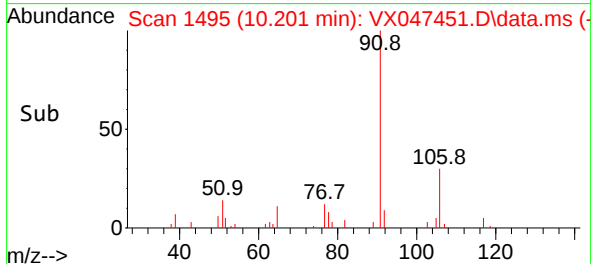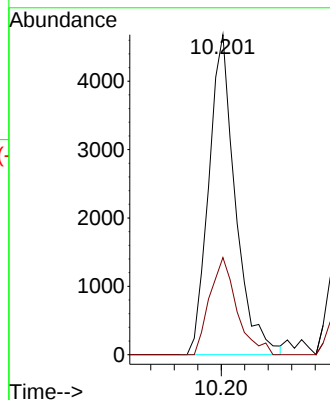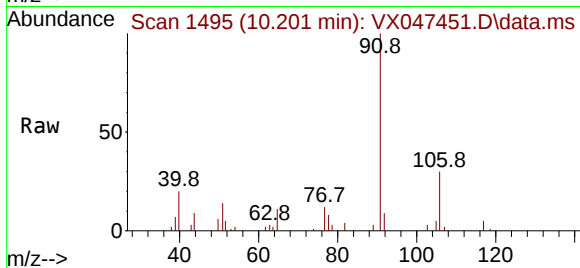

#68

m/p-Xylenes

Concen: 0.389 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.006 min

Lab File: VX047451.D




Acq: 20 Aug 2025 18:18


Tgt Ion: 106 Resp: 2534

Ion Ratio Lower Upper

106 100

91 216.9 164.7 247.1



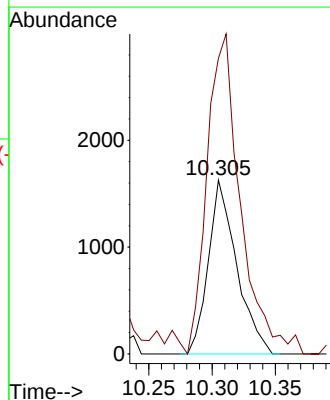
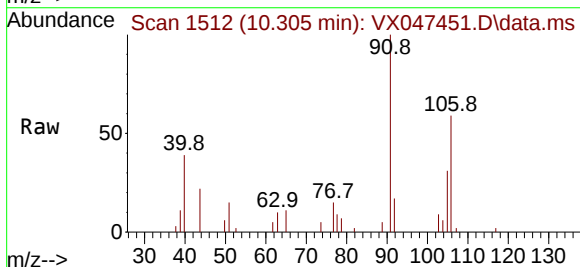




#69
o-Xylene
Concen: 0.227 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-081325DL


Tgt Ion:106 Resp: 1425
Ion Ratio Lower Upper
106 100
91 217.9 110.6 331.8

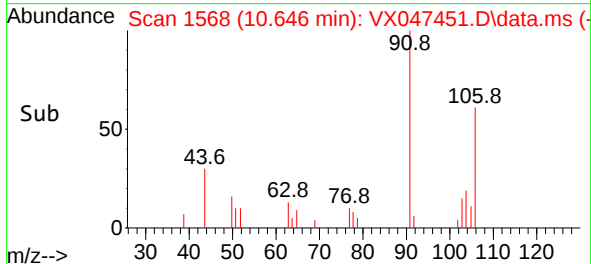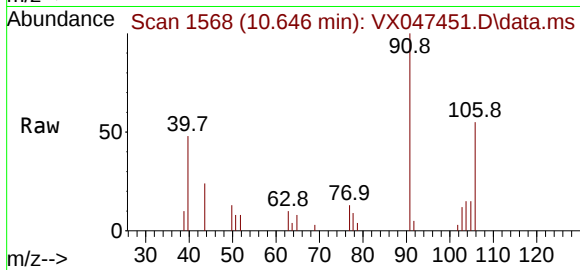

#70
Styrene
Concen: 0.235 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. 0.006 min
Lab File: VX047451.D
Acq: 20 Aug 2025 18:18

Tgt Ion:104 Resp: 2487
Ion Ratio Lower Upper
104 100
78 35.5 41.8 62.8#
103 25.1 43.6 65.4#


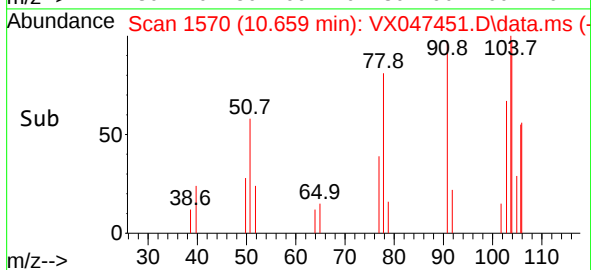

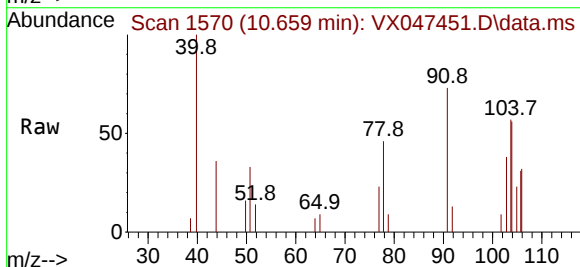




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VX047451.D
 Acq: 20 Aug 2025 18:18




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-18B-57.5-081325DL


Tgt Ion:152 Resp: 219266
 Ion Ratio Lower Upper
 152 100
 115 63.4 44.6 133.8
 150 156.6 0.0 349.8

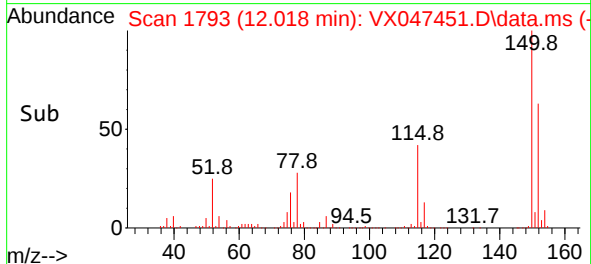

#76
 1,2,3-Trichloropropane
 Concen: 27.378 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.158 min
 Lab File: VX047451.D
 Acq: 20 Aug 2025 18:18

Tgt Ion: 75 Resp: 110102
 Ion Ratio Lower Upper
 75 100
 77 1.7 19.4 58.2#


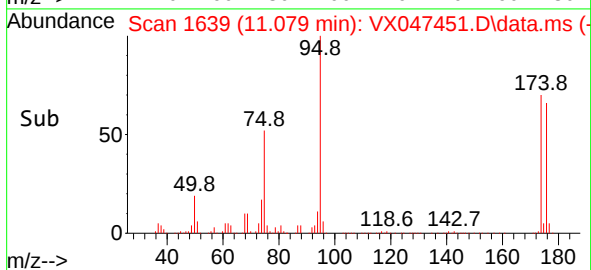






#81
 trans-1,4-Dichloro-2-butene
 Concen: 108.152 ug/l
 RT: 11.079 min Scan# 110102
 Delta R.T. 0.061 min
 Lab File: VX047451.D
 Acq: 20 Aug 2025 18:18




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-18B-57.5-081325DL


Tgt Ion: 75 Resp: 110102
 Ion Ratio Lower Upper
 75 100
 53 0.0 85.2 127.8#
 89 0.0 36.7 55.1#

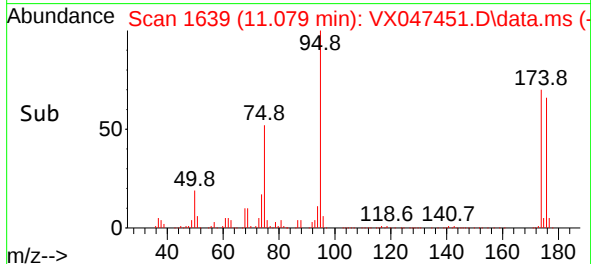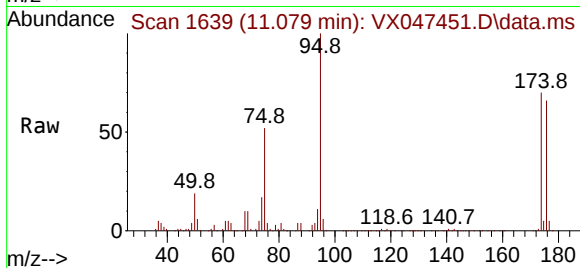

#84
 1,2,4-Trimethylbenzene
 Concen: 0.214 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.006 min
 Lab File: VX047451.D
 Acq: 20 Aug 2025 18:18

Tgt Ion:105 Resp: 3024
 Ion Ratio Lower Upper
 105 100
 120 46.1 21.9 65.7

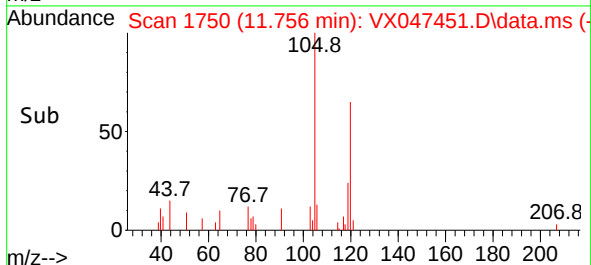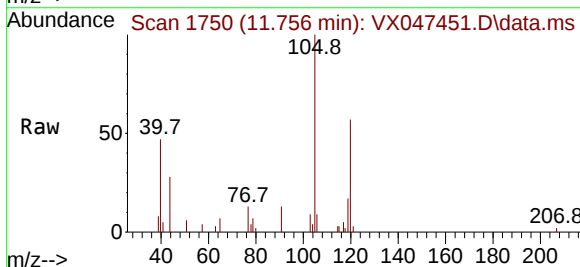



#95

Naphthalene

Concen: 9.645 ug/l

RT: 13.774 min Scan# 20

Delta R.T. 0.000 min

Lab File: VX047451.D


Acq: 20 Aug 2025 18:18

Instrument :

MSVOA_X

ClientSampleId :

MW-18B-57.5-081325DL

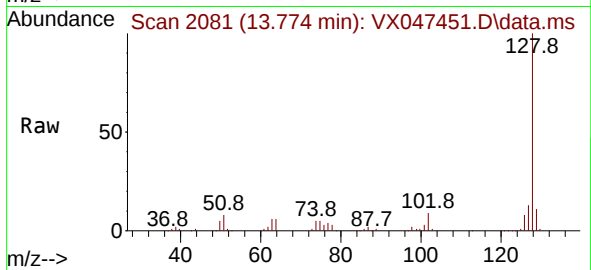

Tgt Ion:128 Resp: 140385

Ion Ratio Lower Upper

128 100

127 12.5 10.1 15.1

129 10.7 8.7 13.1

