


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082119\
Data File : VX011720.D
Acq On : 21 Aug 2019 08:22
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
Title : SW846 8260
Last Update : Fri Aug 16 04:15:26 2019

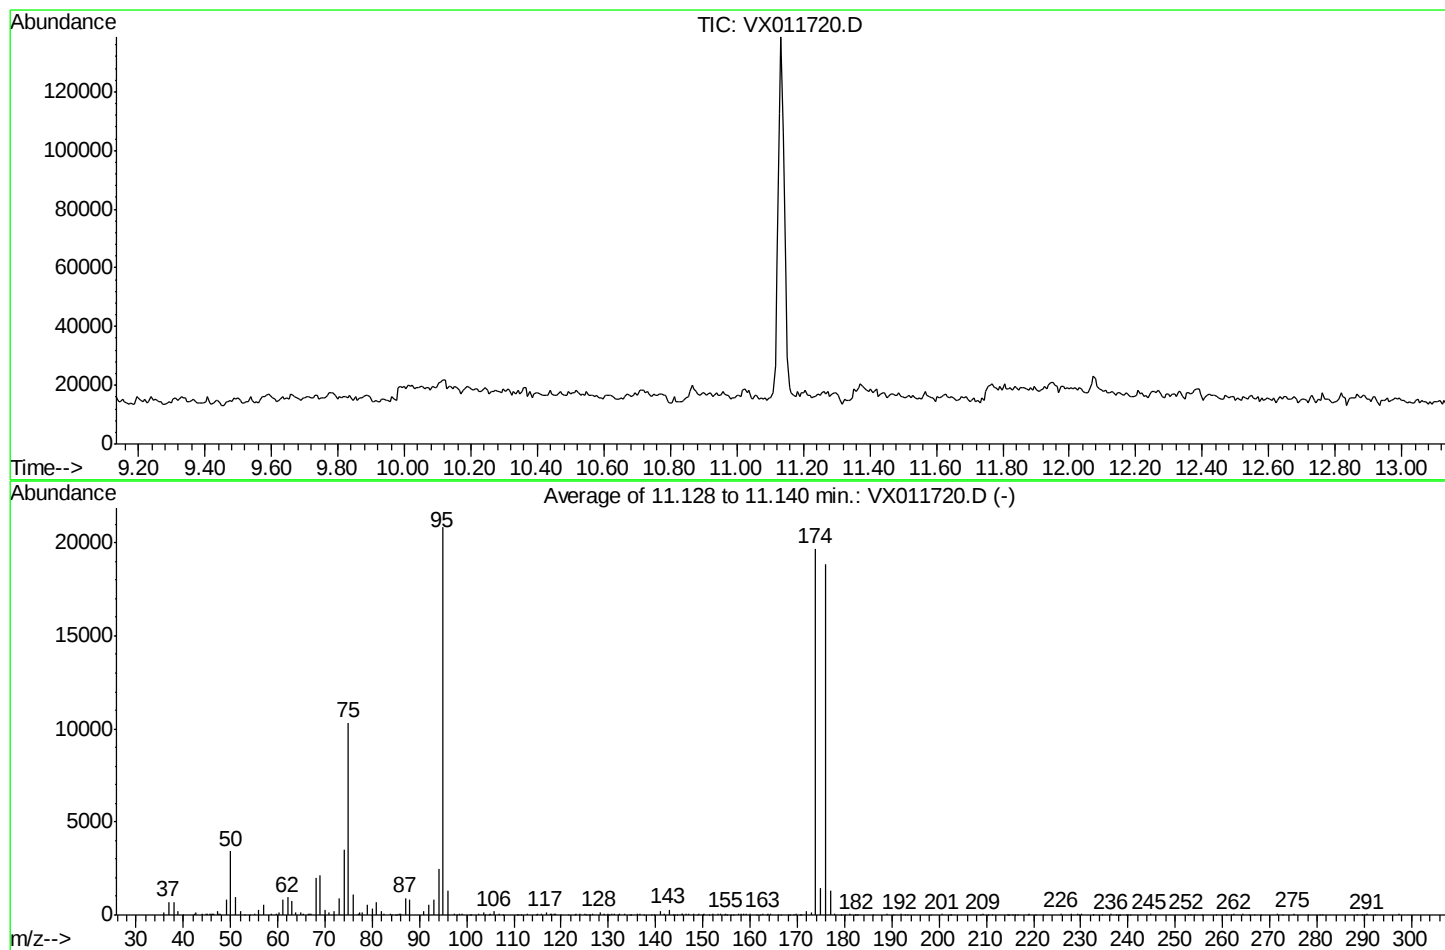

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	3418	PASS
75	95	30	60	49.6	10337	PASS
95	95	100	100	100.0	20828	PASS
96	95	5	9	6.3	1319	PASS
173	174	0.00	2	0.7	145	PASS
174	95	50	100	94.4	19669	PASS
175	174	5	9	7.3	1428	PASS
176	174	95	101	95.8	18851	PASS
177	176	5	9	6.8	1284	PASS