


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082119\
 Data File : VX011738.D
 Acq On : 21 Aug 2019 18:15
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
 Title : SW846 8260
 Last Update : Fri Aug 16 04:15:26 2019

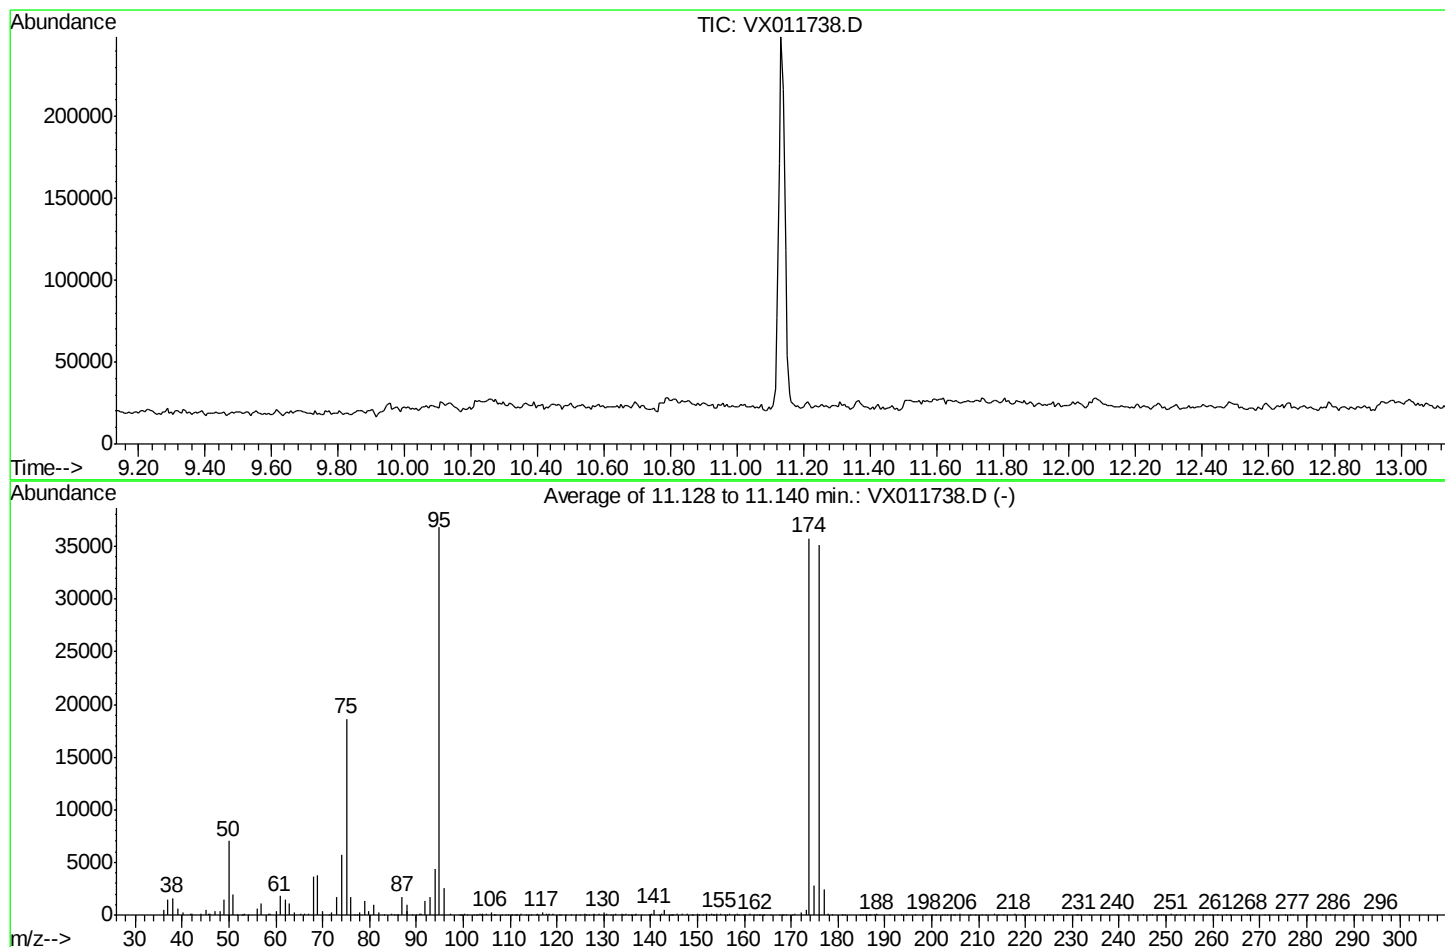

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	7018	PASS
75	95	30	60	50.7	18655	PASS
95	95	100	100	100.0	36821	PASS
96	95	5	9	6.9	2530	PASS
173	174	0.00	2	1.5	525	PASS
174	95	50	100	97.1	35747	PASS
175	174	5	9	7.7	2755	PASS
176	174	95	101	98.3	35144	PASS
177	176	5	9	7.1	2495	PASS