



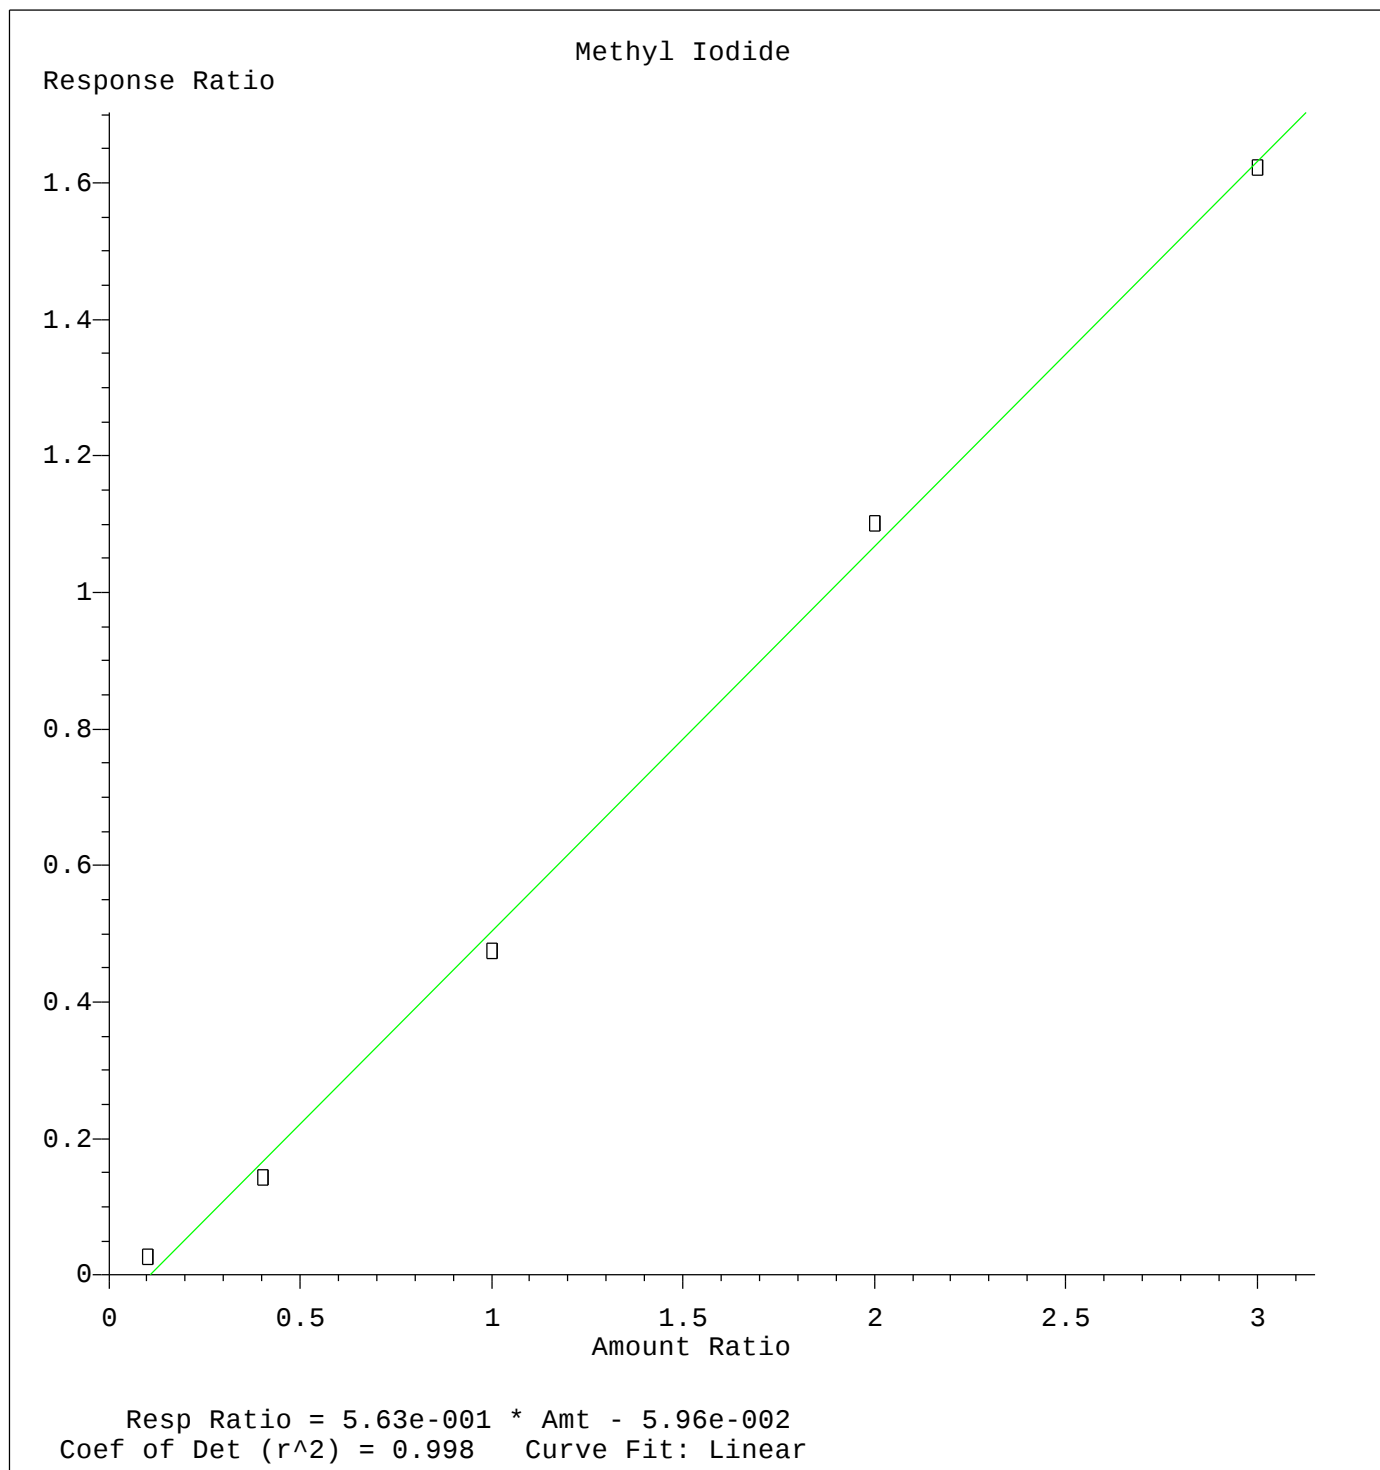

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082120W.M
Calibration Table Last Updated: Fri Aug 21 03:03:56 2020

Methylene Chloride

Response Ratio

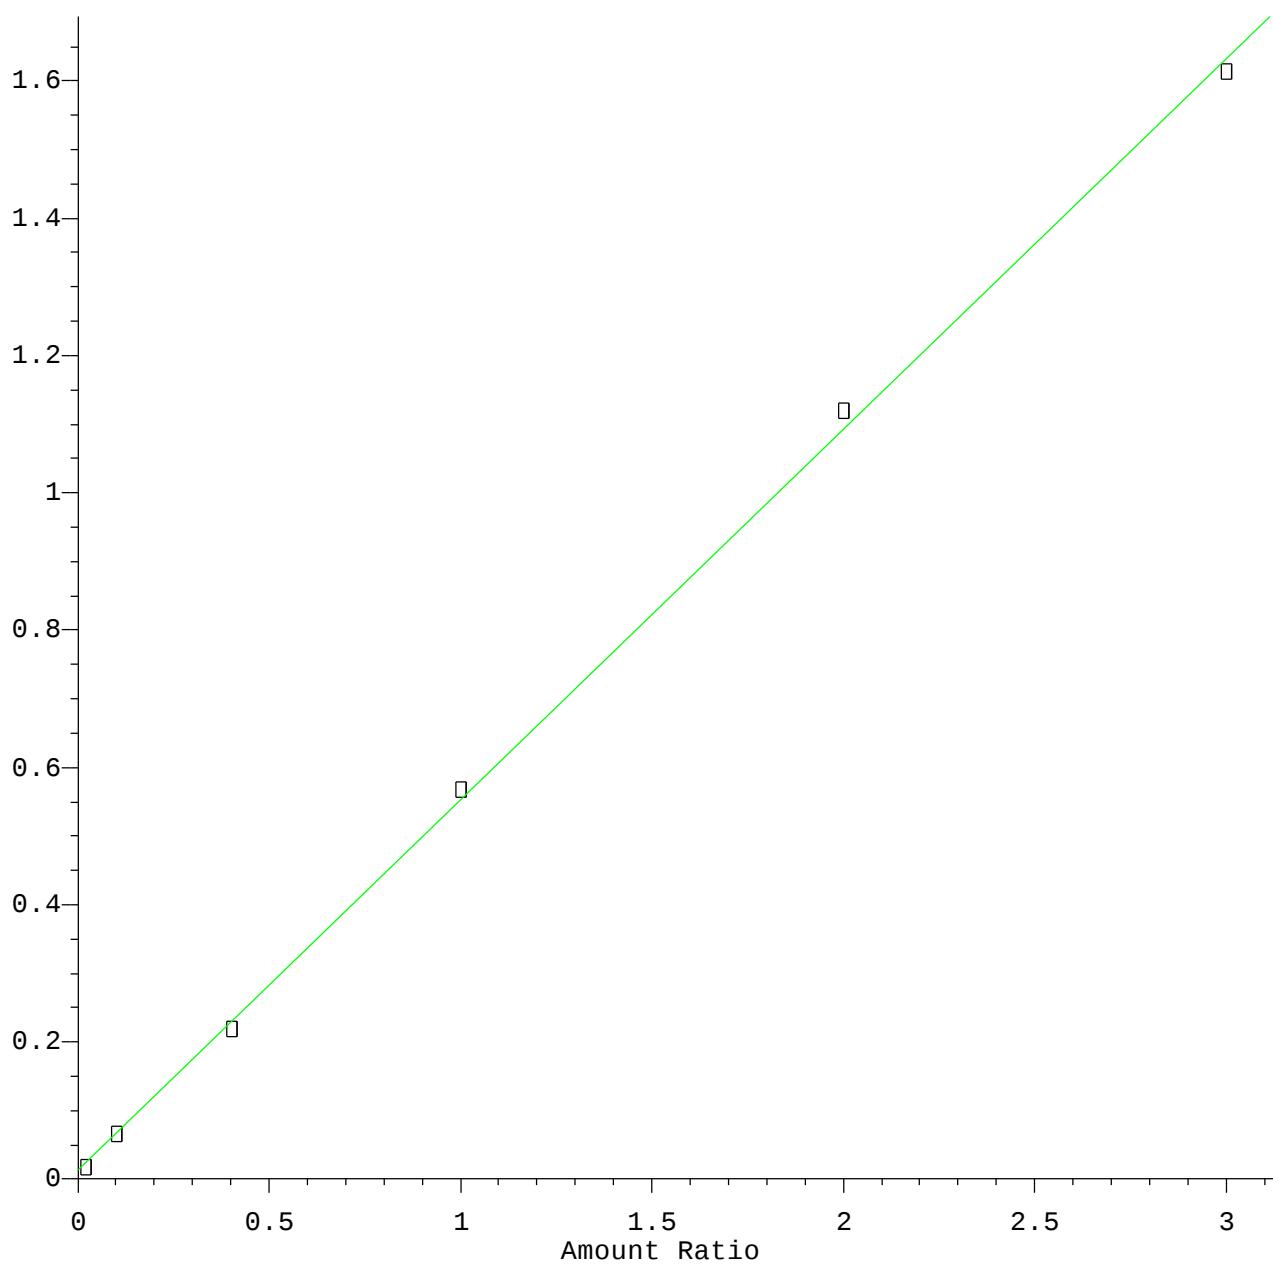

Resp Ratio = $5.40 \times 10^{-1} \times \text{Amt} + 1.29 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082120W.M
Calibration Table Last Updated: Fri Aug 21 03:03:56 2020