

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082121\
 Data File : VX023869.D
 Acq On : 20 Aug 2021 10:19
 Operator : JC/MD
 Sample : VX0821WBL01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK603

Quant Time: Aug 21 04:11:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR081921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 21 04:11:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	128721	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	121046	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	57776	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	21097	4.194	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.800%
7) Chloroethane-d5	1.672	69	27074	4.391	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.800%
11) 1,1-Dichloroethene-d2	2.306	63	47813	3.173	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%
20) 2-Butanone-d5	4.471	46	102781	50.396	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.800%
24) Chloroform-d	5.068	84	77885	4.499	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%
26) 1,2-Dichloroethane-d4	5.964	65	43023	4.599	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
32) Benzene-d6	5.983	84	152440	4.533	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	7.318	67	47706	4.545	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.800%
41) Toluene-d8	8.653	98	137092	4.288	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.800%
43) trans-1,3-Dichloroprop...	8.952	79	13383	4.581	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.600%
46) 2-Hexanone-d5	9.390	63	80960	50.254	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.500%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	34128	4.543	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	51185	4.718	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.400%
Target Compounds						Qvalue
16) Methylene chloride	2.794	84	3142	0.279	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082121\
Data File : VX023869.D
Acq On : 20 Aug 2021 10:19
Operator : JC/MD
Sample : VX0821WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK603

Quant Time: Aug 21 04:11:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR081921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 21 04:11:10 2021
Response via : Initial Calibration

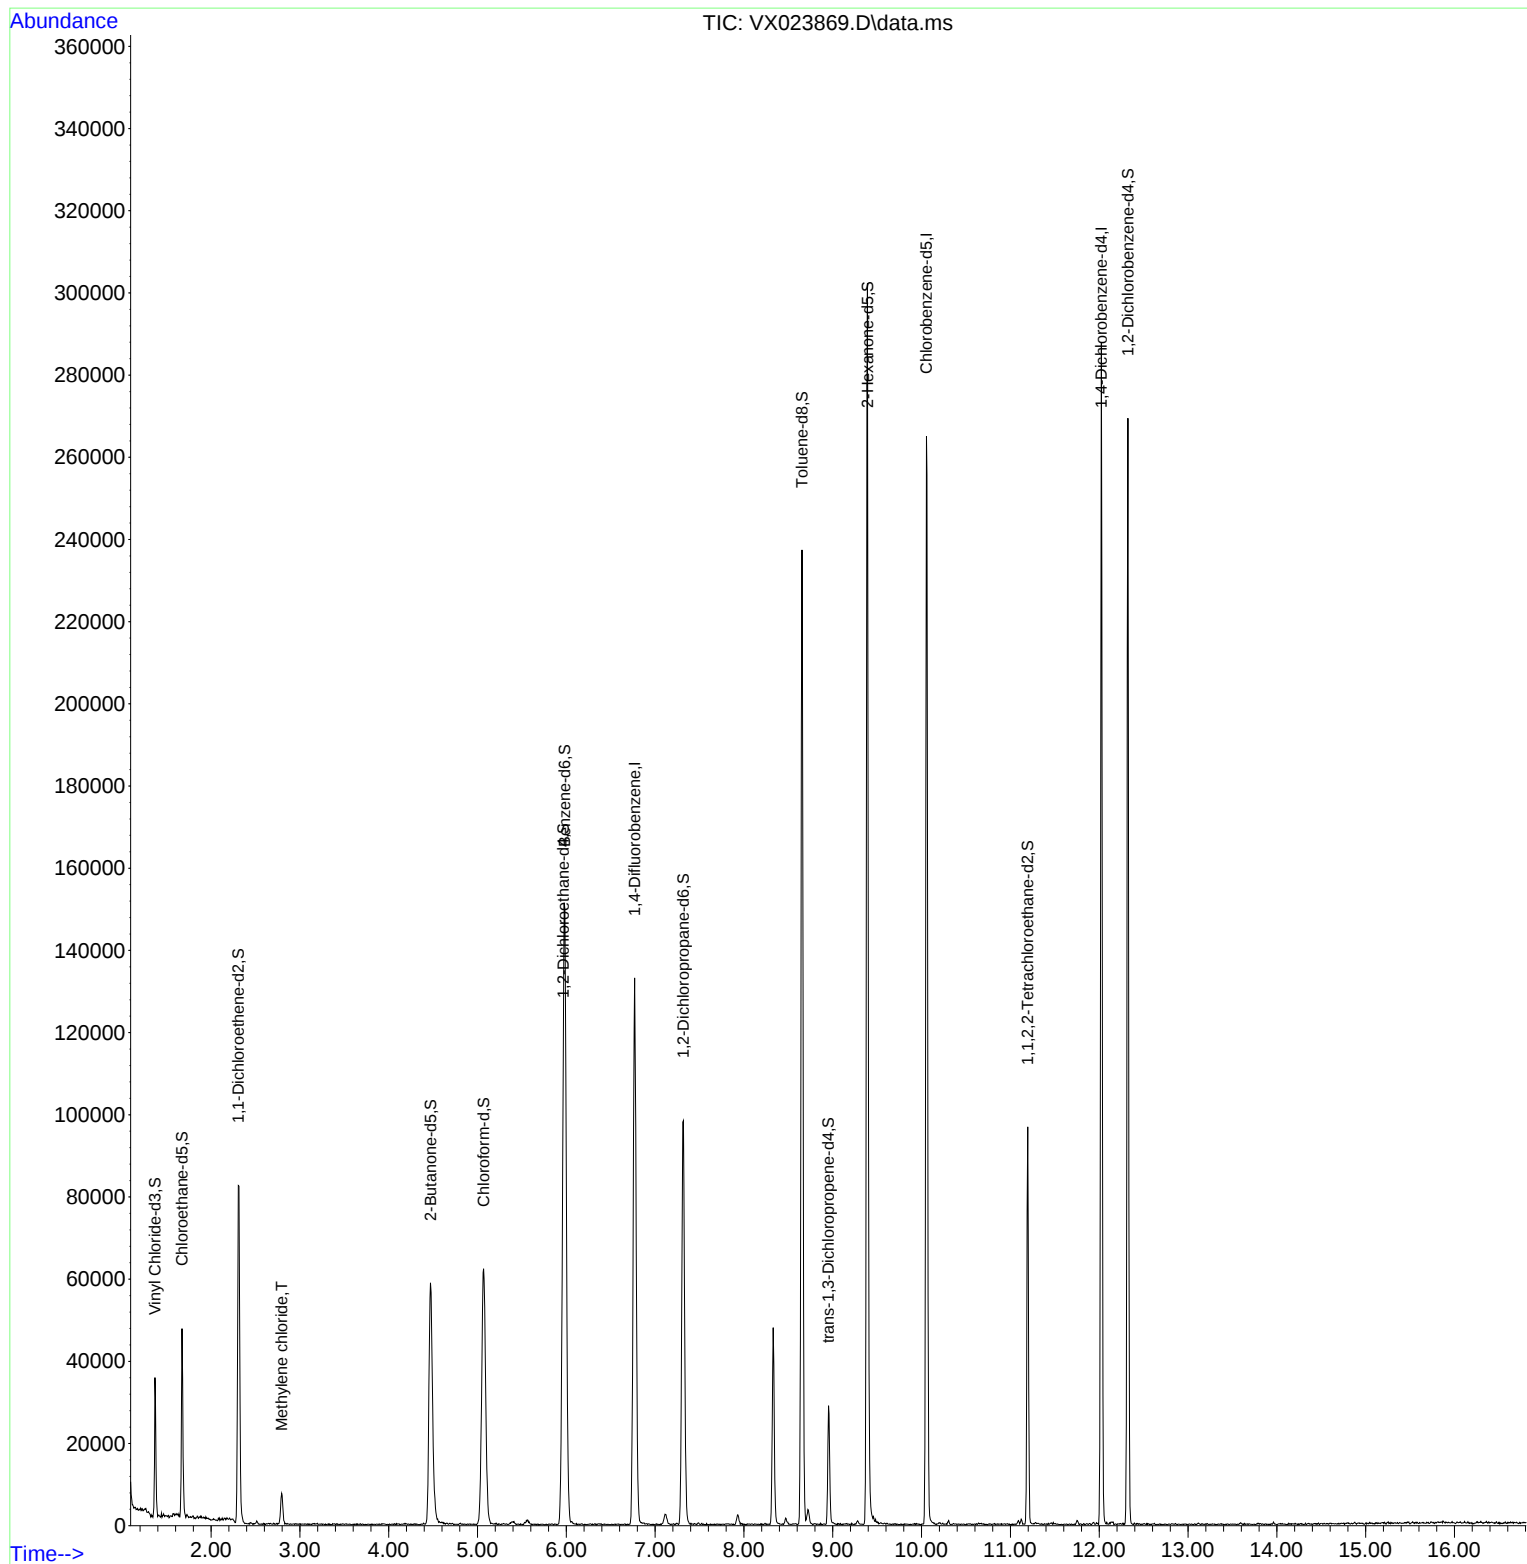

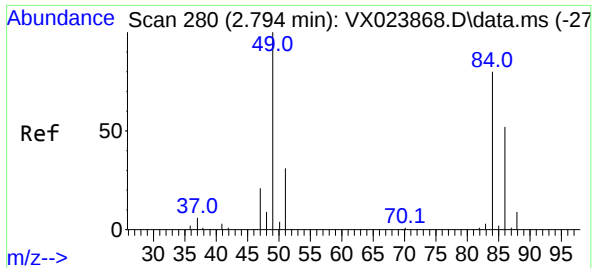

#16
Methylene chloride
Concen: 0.279 ug/L
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023869.D
Acq: 20 Aug 2021 10:19

Instrument :
MSVOA_X
ClientSampleId :
VBLK603

Tgt Ion:	84	Resp:	3142
Ion	Ratio	Lower	Upper
84	100		
86	66.5	44.6	82.8
49	144.2	79.5	147.6

