
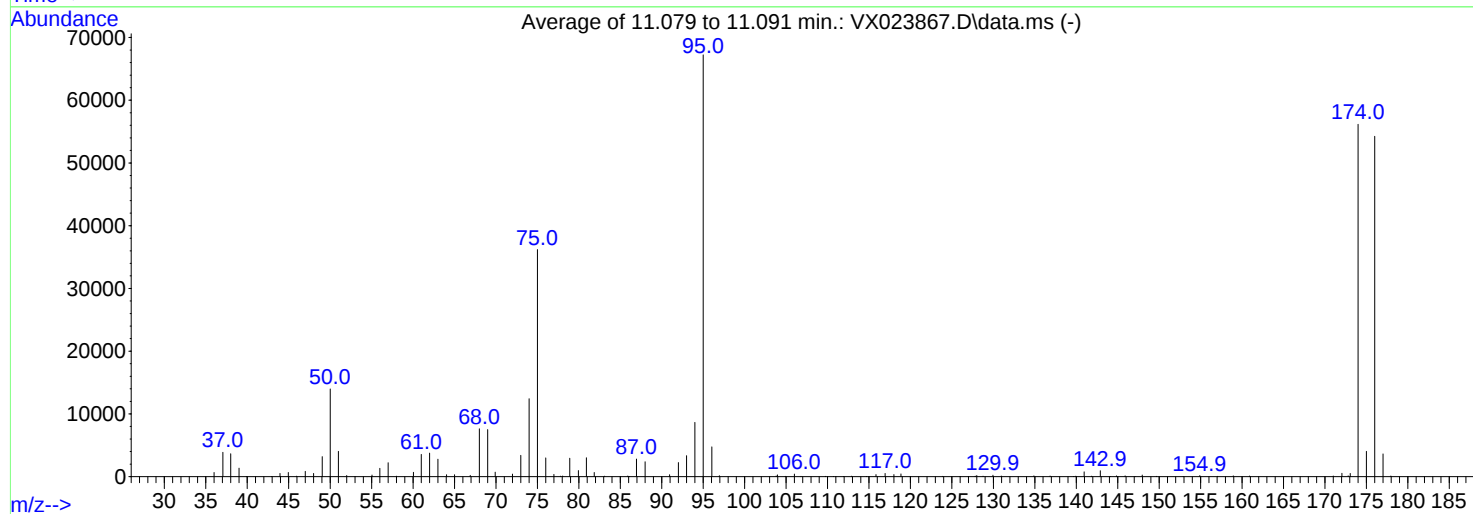


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082121\
Data File : VX023867.D
Acq On : 20 Aug 2021 08:57
Operator : JC/MD
Sample : BFB605
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB605

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR081921WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Aug 21 04:11:10 2021

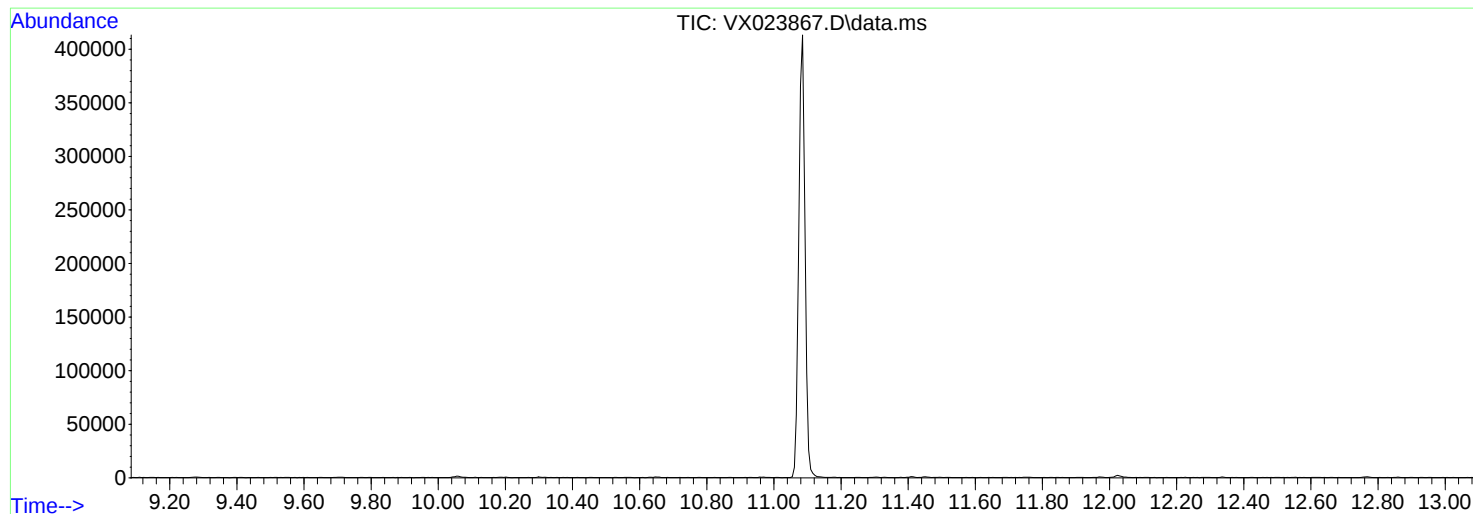

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	13976	PASS
75	95	30	80	53.8	36189	PASS
95	95	100	100	100.0	67235	PASS
96	95	5	9	7.1	4753	PASS
173	174	0.00	2	0.9	513	PASS
174	95	50	120	83.5	56171	PASS
175	174	5	9	7.2	4021	PASS
176	174	95	105	96.6	54259	PASS
177	176	5	10	6.7	3614	PASS

m/z	Abundance
36.00	695.0
37.10	4474.0
38.00	4310.0
39.00	1721.0
39.90	151.0
43.00	55.0
44.00	762.0
45.00	776.0
45.90	146.0
47.00	884.0
48.10	607.0
49.10	3859.0
50.00	16824.0
51.00	4685.0
52.00	217.0
53.00	50.0
55.00	243.0
56.00	1487.0
57.00	2976.0
58.00	150.0
60.00	831.0
61.00	4314.0
62.00	4596.0
63.00	3284.0
64.00	345.0
65.00	424.0
66.90	190.0
68.00	9186.0
69.00	8508.0
69.90	808.0
72.10	499.0
73.00	3869.0
74.00	14242.0
75.00	41872.0
76.00	3637.0
76.90	448.0
77.80	238.0
78.90	3376.0
79.90	965.0
80.90	3688.0
81.90	853.0
83.10	140.0
85.90	137.0
86.90	3518.0
88.00	2772.0
90.90	407.0
92.00	2737.0
93.00	4109.0
94.00	10556.0
95.00	78984.0
96.00	6072.0
96.90	161.0
104.00	570.0
105.90	436.0
106.80	100.0
109.70	59.0
110.70	91.0
112.00	58.0
112.90	69.0
115.00	50.0
115.90	440.0
116.90	628.0
117.90	407.0
118.90	646.0
123.90	122.0
127.00	60.0
128.00	388.0
128.80	73.0
130.00	197.0
130.90	76.0
134.90	181.0
136.80	116.0
139.90	111.0
141.00	1025.0
141.80	92.0
142.90	1003.0
144.10	53.0
144.80	174.0
146.00	206.0
147.10	57.0
148.00	314.0
149.70	64.0
154.90	240.0
157.00	140.0
159.00	98.0
160.90	88.0
171.00	144.0
172.00	691.0
173.00	668.0
174.00	66264.0
175.00	5091.0
176.00	66512.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

177.004455.0

178.00113.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

m/z	Abundance
35.90	357.0
37.00	2492.0
38.00	2375.0
39.00	962.0
39.90	142.0
44.00	499.0
45.00	492.0
47.00	549.0
47.90	272.0
49.00	2133.0
50.00	9197.0
51.00	2568.0
52.00	94.0
55.10	138.0
56.00	870.0
57.10	1175.0
60.00	546.0
61.00	2483.0
62.10	2498.0
63.10	1877.0
63.90	223.0
64.90	239.0
67.00	147.0
68.00	5191.0
69.00	5334.0
70.00	460.0
71.90	291.0
73.00	2638.0
74.00	8848.0
75.00	25512.0
76.00	1876.0
77.10	270.0
78.00	116.0
78.90	2080.0
80.00	857.0
80.90	2163.0
81.90	477.0
83.10	74.0
86.10	84.0
87.00	1978.0
88.00	1836.0
90.90	289.0
92.00	1604.0
93.10	2102.0
94.00	6138.0
95.10	48136.0
96.10	3228.0
96.90	145.0
103.90	251.0
106.00	352.0
112.90	79.0
115.90	217.0
116.90	373.0
118.10	203.0
118.80	341.0
128.00	155.0
128.70	83.0
130.00	223.0
131.00	73.0
134.90	129.0
136.90	71.0
139.70	65.0
140.90	563.0
141.80	55.0
142.90	712.0
145.00	59.0
145.80	105.0
147.90	231.0
154.90	149.0
159.00	129.0
160.90	95.0
171.10	87.0
172.00	312.0
172.80	405.0
174.00	48632.0
175.00	3154.0
176.00	47312.0
177.00	3034.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

m/z	Abundance
39.90	125.0
44.10	145.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

m/z	Abundance
36.00	923.0
37.00	4707.0
38.00	4251.0
39.00	1406.0
40.00	180.0
42.90	61.0
43.90	683.0
44.90	753.0
46.10	64.0
47.00	1096.0
48.00	645.0
49.00	3561.0
50.00	15906.0
51.00	4835.0
52.00	237.0
55.10	360.0
56.00	1599.0
57.00	2482.0
58.00	73.0
60.10	685.0
61.00	3849.0
62.00	4134.0
63.00	3200.0
64.20	333.0
65.00	295.0
66.80	252.0
68.00	8481.0
69.00	8688.0
69.90	845.0
72.00	439.0
73.00	3658.0
74.00	14162.0
75.00	41184.0
76.00	3457.0
77.10	394.0
78.10	200.0
78.90	3383.0
79.90	1062.0
80.90	3183.0
81.80	632.0
85.90	138.0
87.00	2897.0
88.00	2527.0
91.00	213.0
92.00	2405.0
93.00	3786.0
94.00	9217.0
95.00	74584.0
96.10	4960.0
97.10	160.0
103.80	299.0
104.90	189.0
106.10	450.0
106.80	79.0
109.80	79.0
111.00	79.0
111.90	50.0
112.90	61.0
114.70	56.0
115.00	52.0
115.80	311.0
117.00	569.0
118.00	361.0
118.90	306.0
123.90	72.0
126.00	52.0
127.80	208.0
128.70	52.0
129.90	293.0
130.90	140.0
134.90	109.0
136.90	116.0
140.00	93.0
140.90	709.0
141.90	90.0
142.90	1115.0
144.90	159.0
145.90	108.0
147.90	207.0
149.70	73.0
152.90	54.0
154.90	121.0
157.20	57.0
158.90	144.0
160.90	95.0
170.90	69.0
172.10	575.0
173.10	872.0
174.00	53616.0
175.00	3817.0
176.00	48952.0
177.00	3354.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

177.90

179.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605