

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082123\
 Data File : VX037124.D
 Acq On : 21 Aug 2023 11:51
 Operator : JC/MD
 Sample : VX0821MBL01
 Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0821MBL01

Quant Time: Aug 22 05:53:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	158353	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	275132	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	258056	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	121276	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	116399	50.986	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	101.980%
35) Dibromofluoromethane	5.385	113	89599	49.173	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.340%
50) Toluene-d8	8.647	98	325394	49.231	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.460%
62) 4-Bromofluorobenzene	11.079	95	129314	49.785	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.560%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082123\
Data File : VX037124.D
Acq On : 21 Aug 2023 11:51
Operator : JC/MD
Sample : VX0821MBL01
Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0821MBL01

Quant Time: Aug 22 05:53:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration




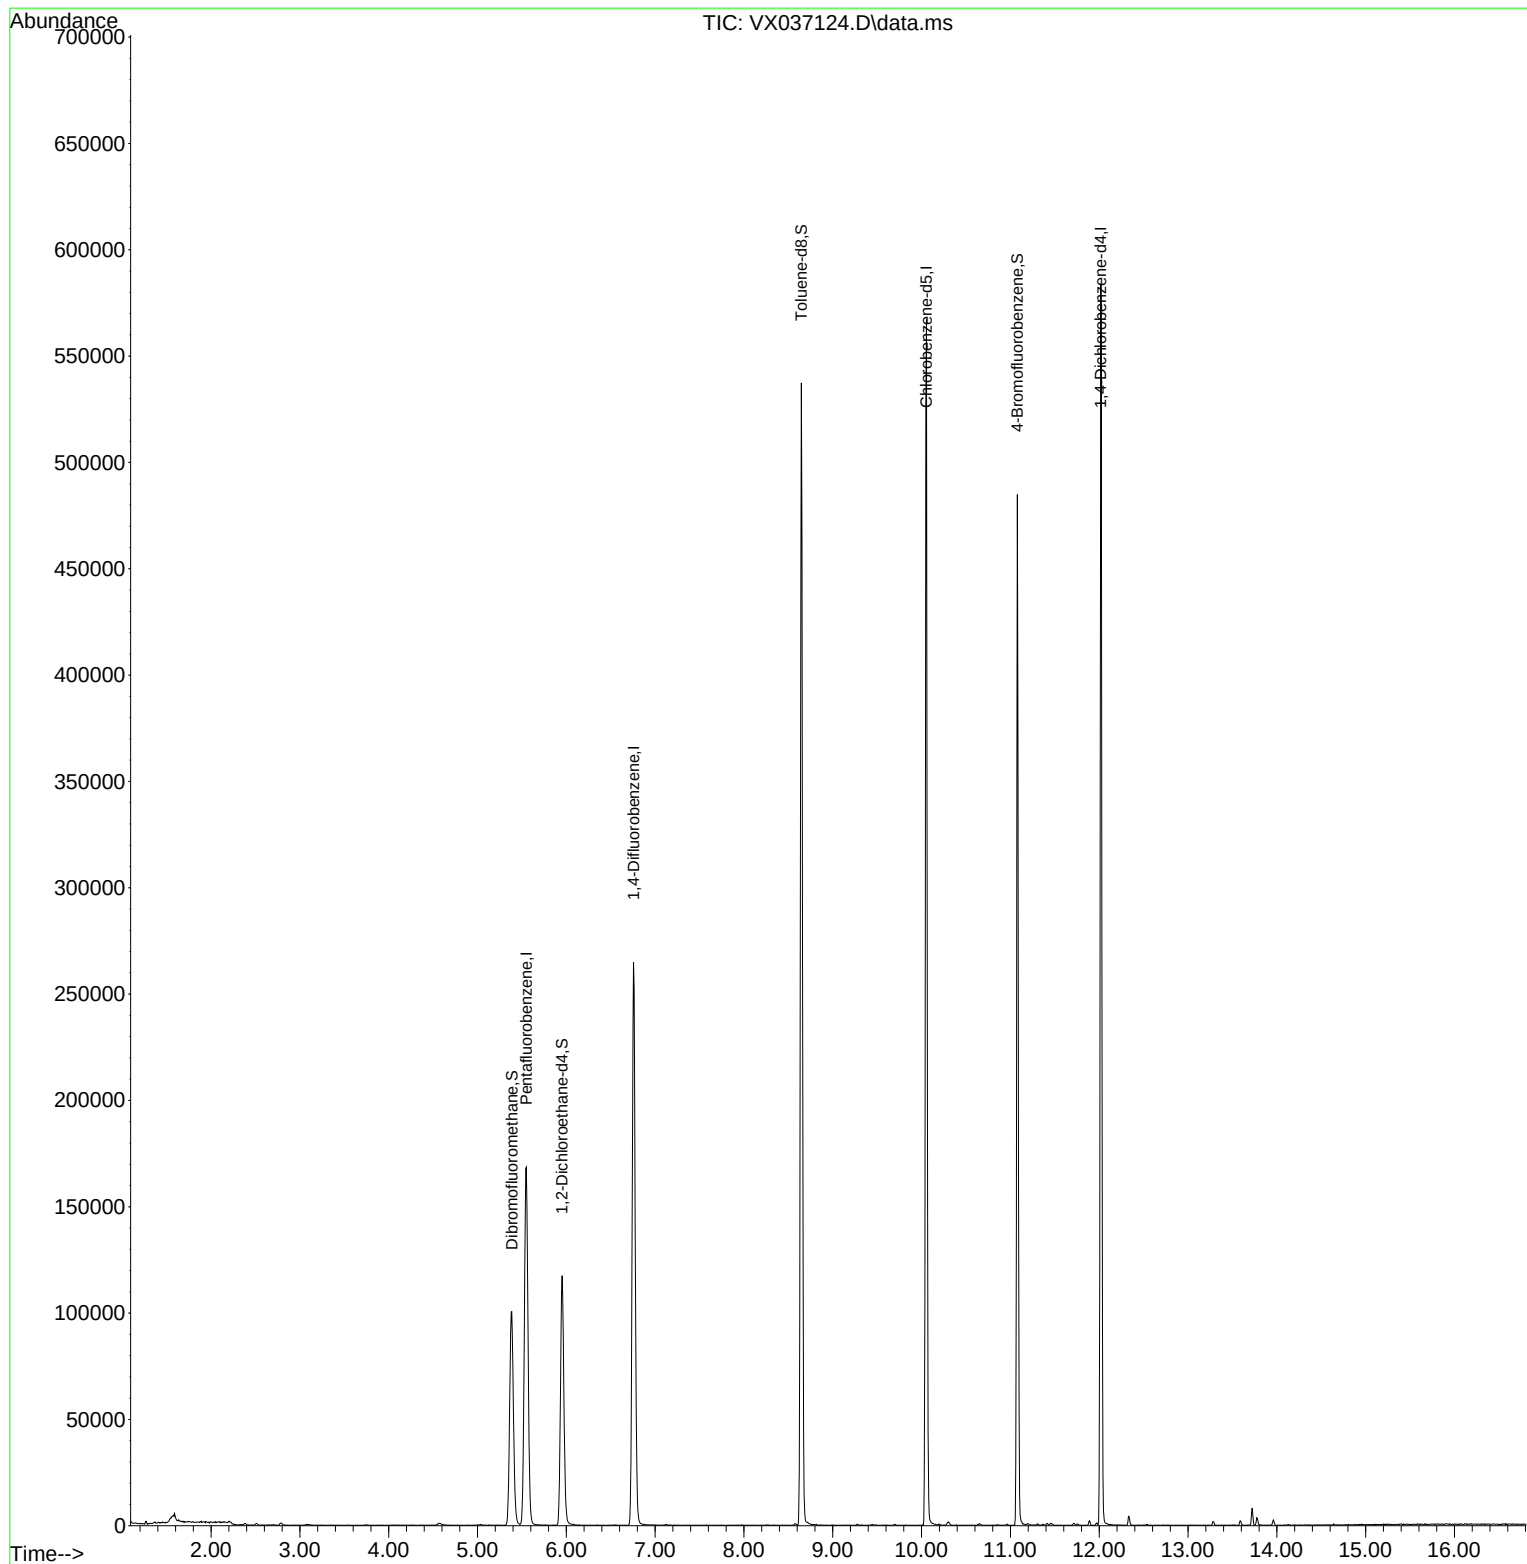


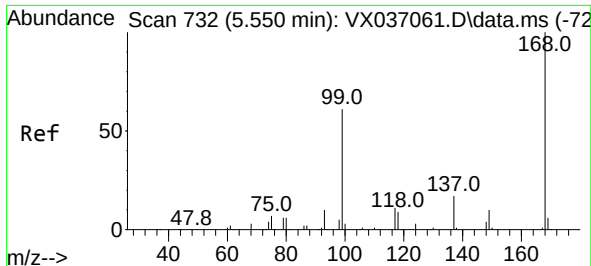

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX037124.D
Acq: 21 Aug 2023 11:51




Instrument :
MSVOA_X
ClientSampleId :
VX0821MBL01


Tgt Ion:168 Resp: 158353
Ion Ratio Lower Upper
168 100
99 62.0 56.6 85.0

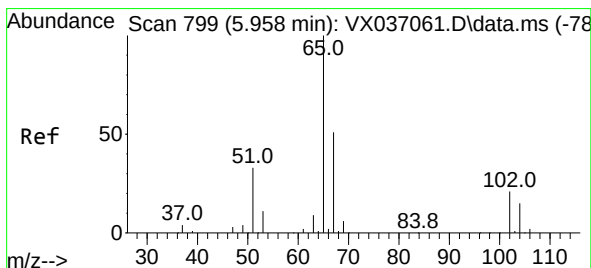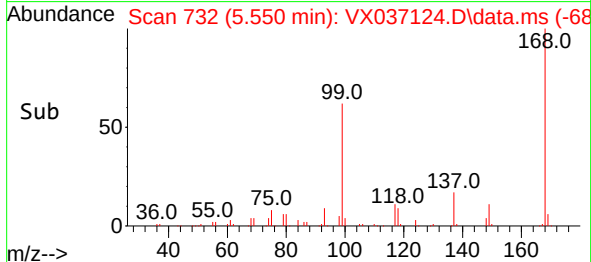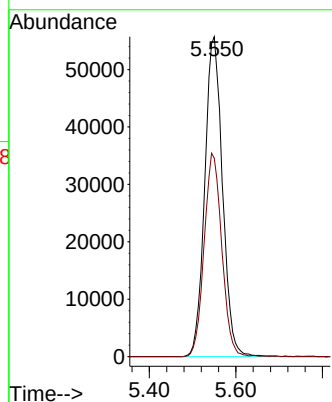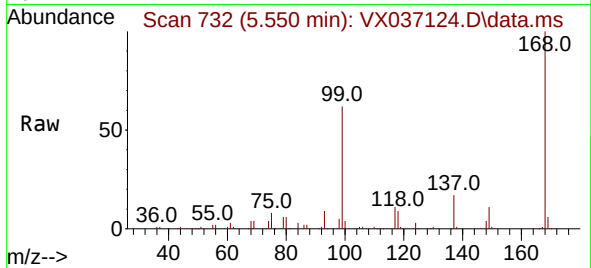

#33
1,2-Dichloroethane-d4
Concen: 50.986 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX037124.D
Acq: 21 Aug 2023 11:51

Tgt Ion: 65 Resp: 116399
Ion Ratio Lower Upper
65 100
67 51.1 0.0 100.2


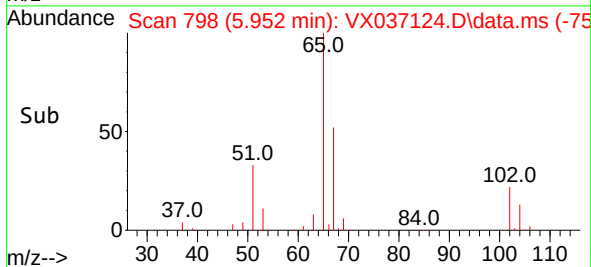
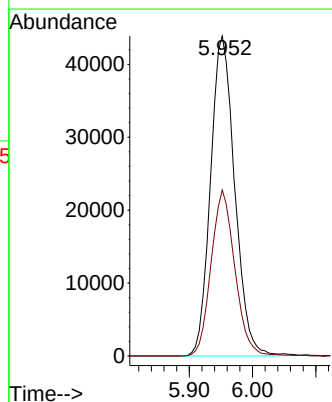
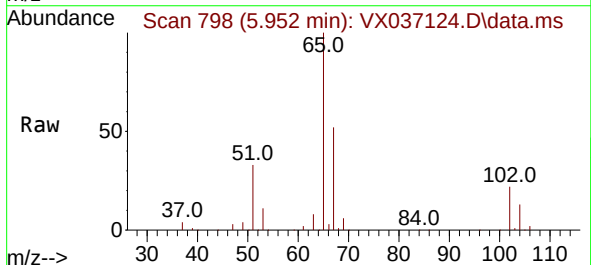


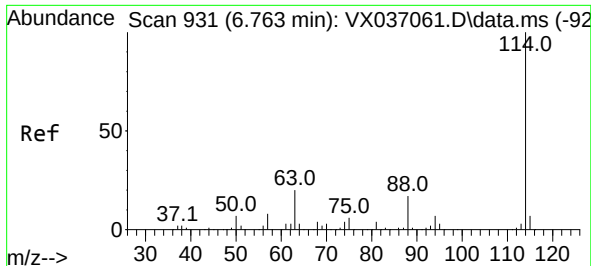

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. -0.006 min
Lab File: VX037124.D
Acq: 21 Aug 2023 11:51




Instrument :
MSVOA_X
ClientSampleId :
VX0821MBL01


Tgt Ion:114 Resp: 275132
Ion Ratio Lower Upper
114 100
63 20.3 0.0 45.0
88 16.5 0.0 36.6

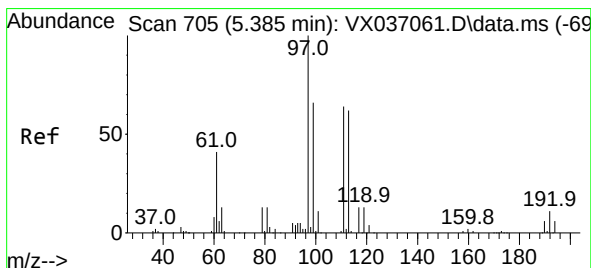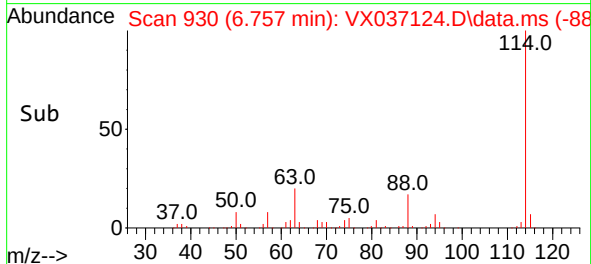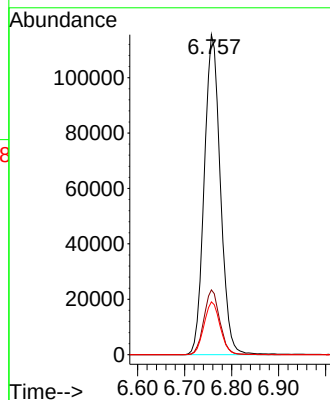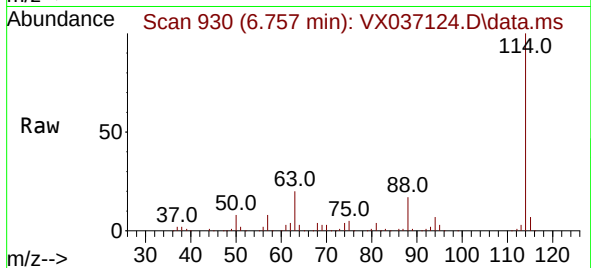

#35
Dibromofluoromethane
Concen: 49.173 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037124.D
Acq: 21 Aug 2023 11:51

Tgt Ion:113 Resp: 89599
Ion Ratio Lower Upper
113 100
111 102.9 82.9 124.3
192 18.5 13.3 19.9


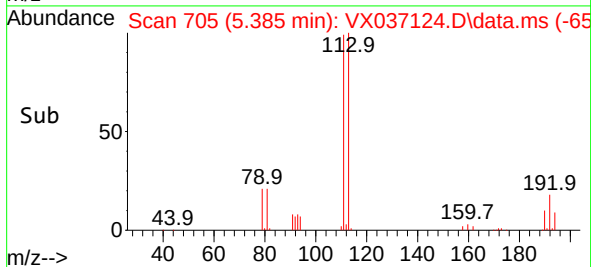
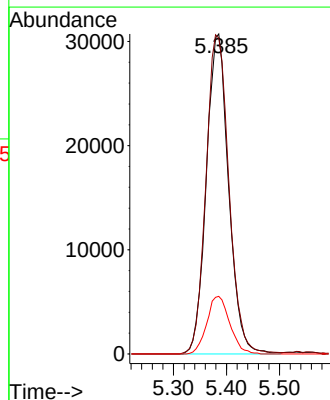
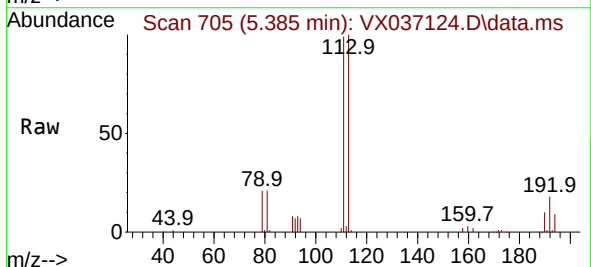


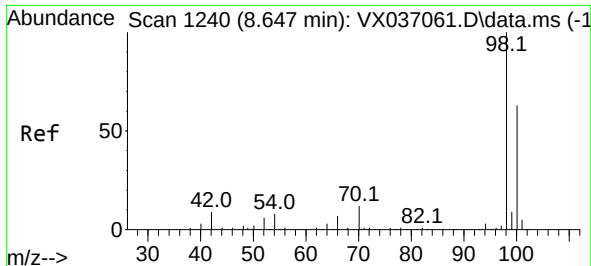

#50
Toluene-d8
Concen: 49.231 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037124.D
Acq: 21 Aug 2023 11:51




Instrument :
MSVOA_X
ClientSampleId :
VX0821MBL01


Tgt Ion: 98 Resp: 325394
Ion Ratio Lower Upper
98 100
100 66.1 53.1 79.7

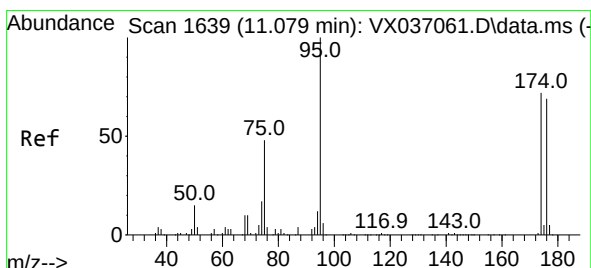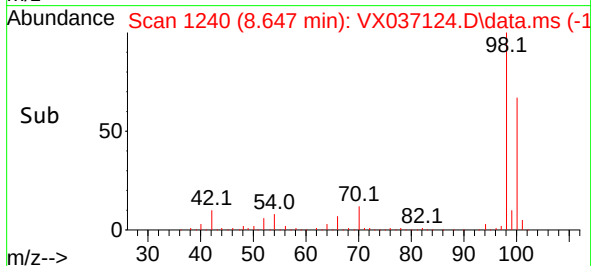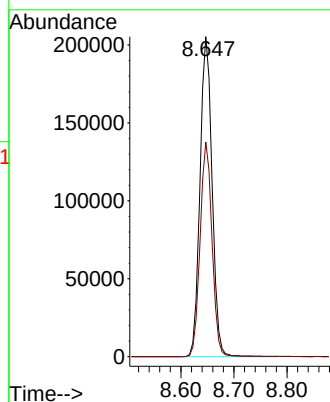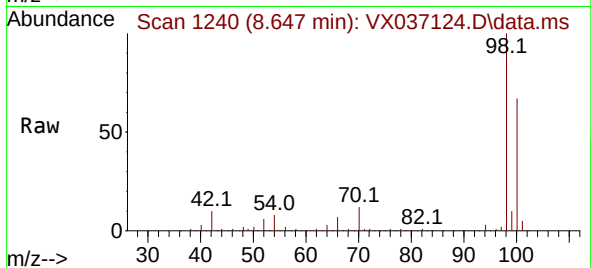

#62
4-Bromofluorobenzene
Concen: 49.785 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037124.D
Acq: 21 Aug 2023 11:51

Tgt Ion: 95 Resp: 129314
Ion Ratio Lower Upper
95 100
174 73.1 0.0 135.6
176 70.6 0.0 131.0


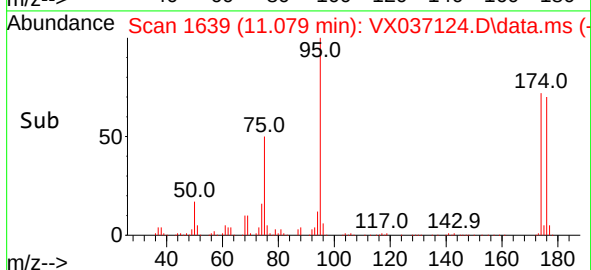
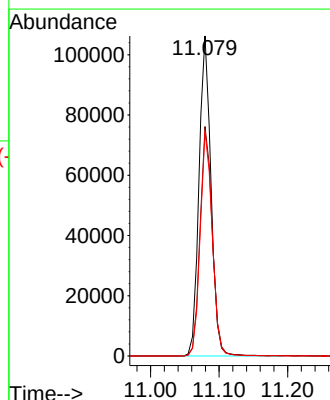
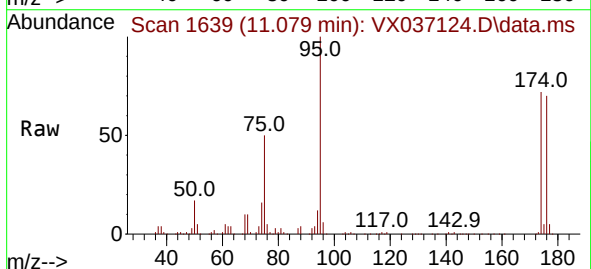


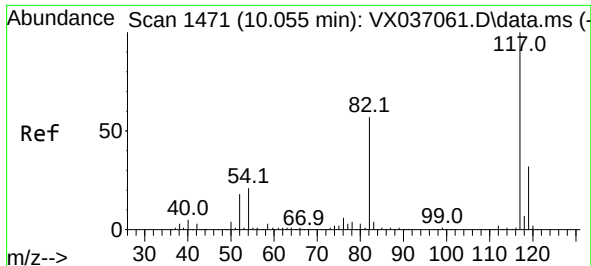

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX037124.D
Acq: 21 Aug 2023 11:51

Instrument :
MSVOA_X
ClientSampleId :
VX0821MBL01

Tgt Ion:117 Resp: 258056
Ion Ratio Lower Upper
117 100
82 54.7 46.2 69.4
119 32.5 25.5 38.3

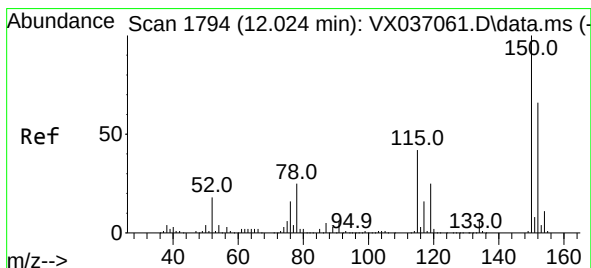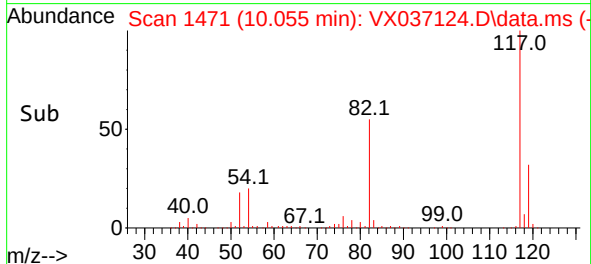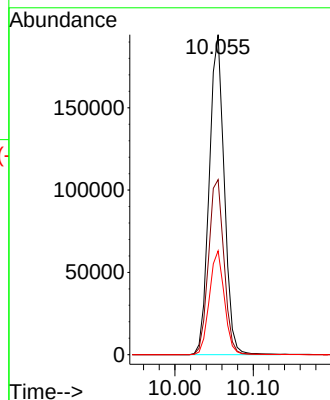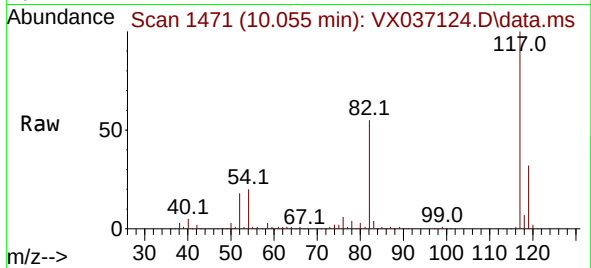

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX037124.D
Acq: 21 Aug 2023 11:51

Tgt Ion:152 Resp: 121276
Ion Ratio Lower Upper
152 100
115 63.6 43.3 129.9
150 157.9 0.0 345.0

