

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082124\
 Data File : VX043076.D
 Acq On : 21 Aug 2024 10:20
 Operator : JC/MD
 Sample : VX0821WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0821WBL01

Quant Time: Aug 22 03:28:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081424W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 15 04:22:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	127497	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	241255	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	208859	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	90356	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	94462	56.384	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	112.760%
35) Dibromofluoromethane	5.385	113	75072	50.300	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.600%
50) Toluene-d8	8.647	98	293877	51.008	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.020%
62) 4-Bromofluorobenzene	11.079	95	106759	51.104	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	102.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082124\
Data File : VX043076.D
Acq On : 21 Aug 2024 10:20
Operator : JC/MD
Sample : VX0821WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0821WBL01

Quant Time: Aug 22 03:28:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081424W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 15 04:22:11 2024
Response via : Initial Calibration




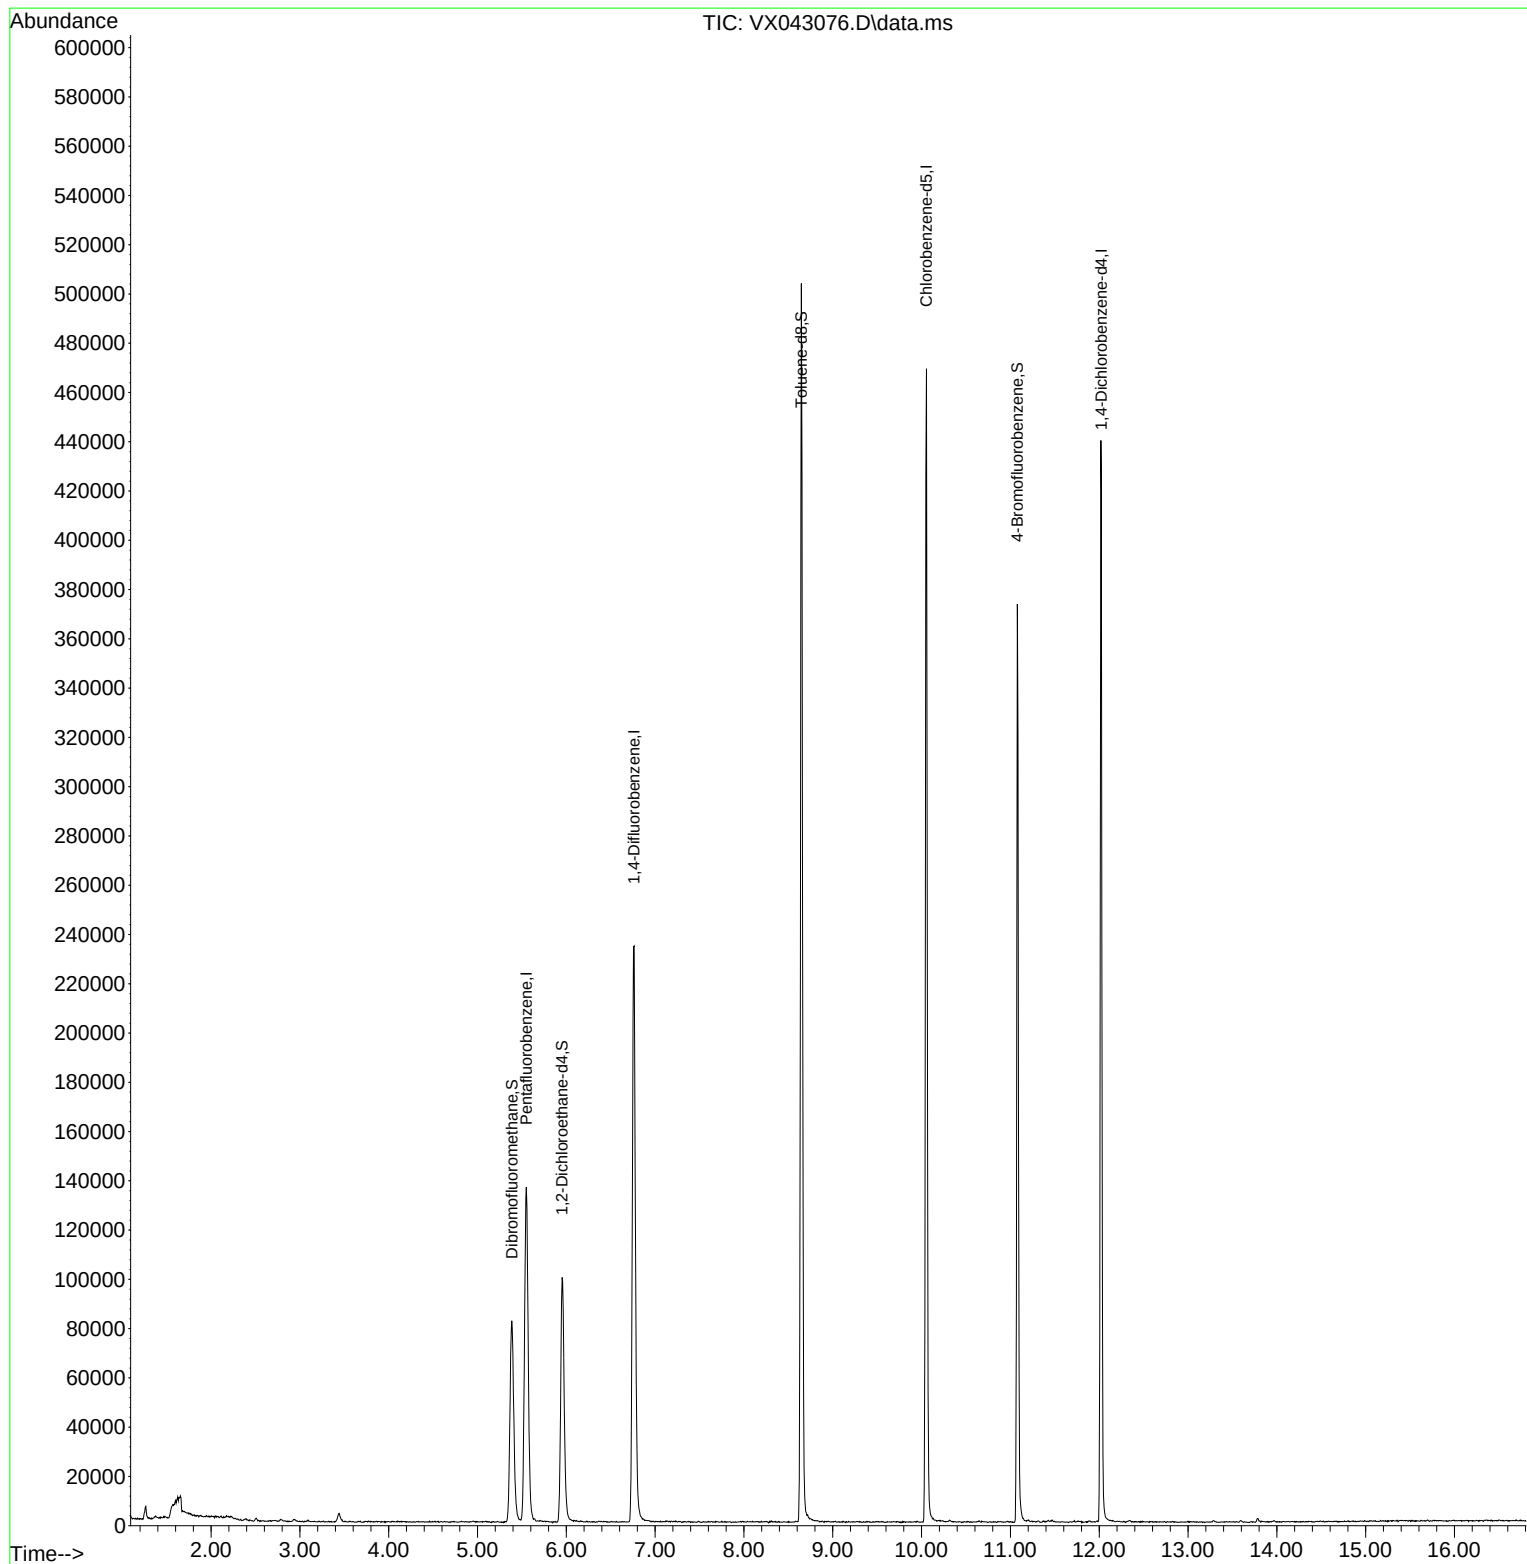


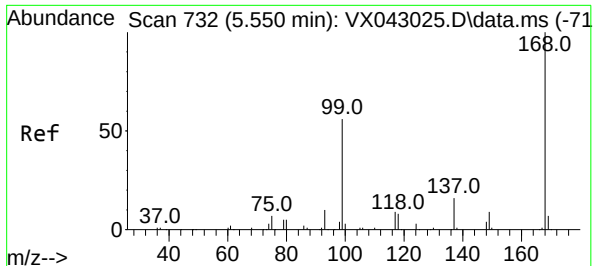

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX043076.D
Acq: 21 Aug 2024 10:20




Instrument :
MSVOA_X
ClientSampleId :
VX0821WBL01


Tgt Ion:168 Resp: 127497
Ion Ratio Lower Upper
168 100
99 63.6 56.6 85.0

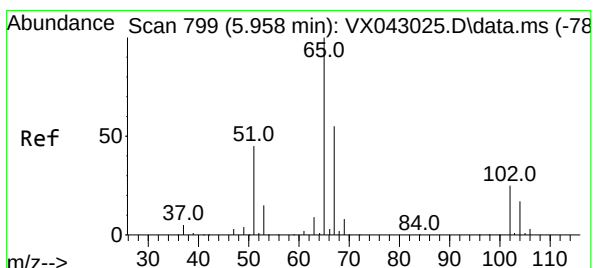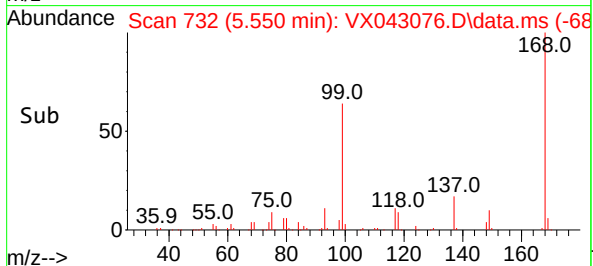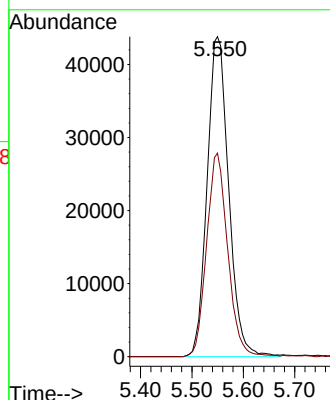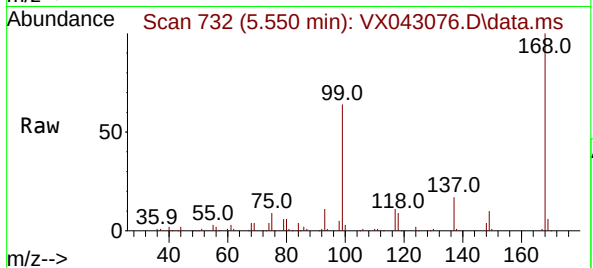

#33
1,2-Dichloroethane-d4
Concen: 56.384 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX043076.D
Acq: 21 Aug 2024 10:20

Tgt Ion: 65 Resp: 94462
Ion Ratio Lower Upper
65 100
67 54.2 0.0 100.2


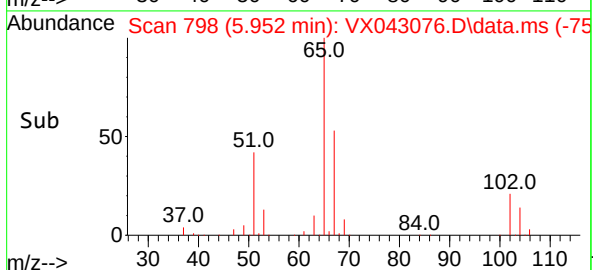
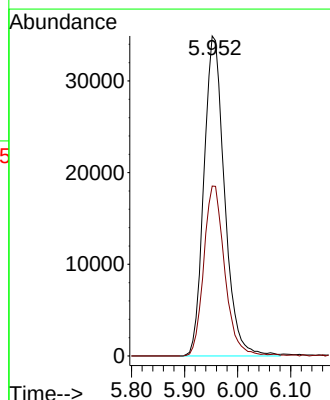
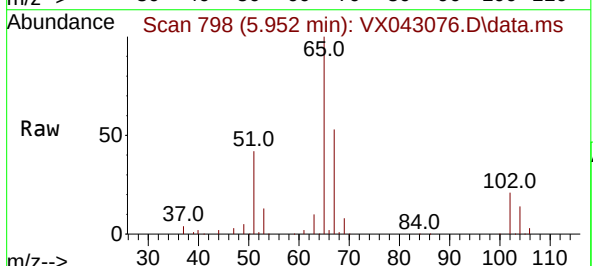


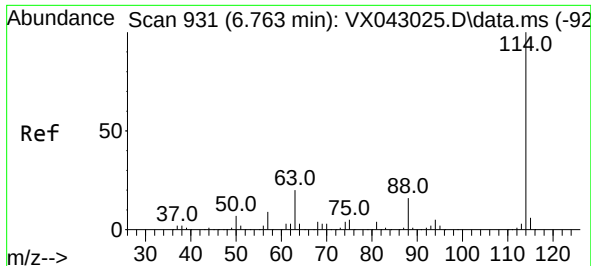

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX043076.D
Acq: 21 Aug 2024 10:20




Instrument :
MSVOA_X
ClientSampleId :
VX0821WBL01


Tgt Ion:114 Resp: 241255
Ion Ratio Lower Upper
114 100
63 21.6 0.0 45.0
88 17.2 0.0 36.6

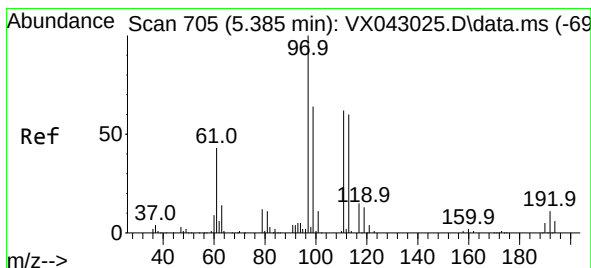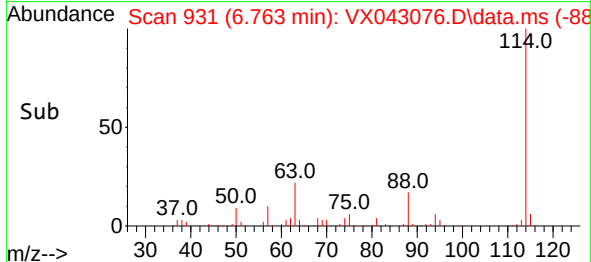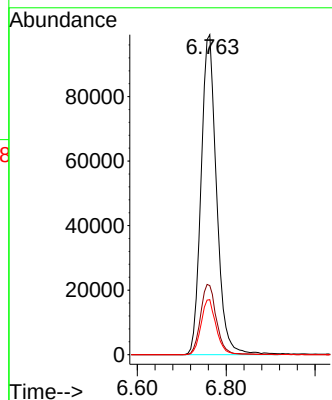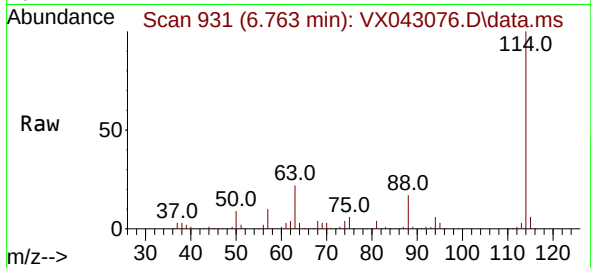

#35
Dibromofluoromethane
Concen: 50.300 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX043076.D
Acq: 21 Aug 2024 10:20

Tgt Ion:113 Resp: 75072
Ion Ratio Lower Upper
113 100
111 104.3 82.9 124.3
192 18.2 13.3 19.9


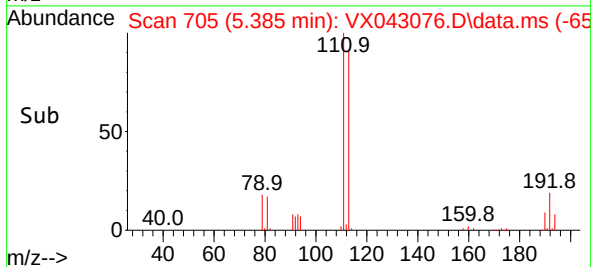
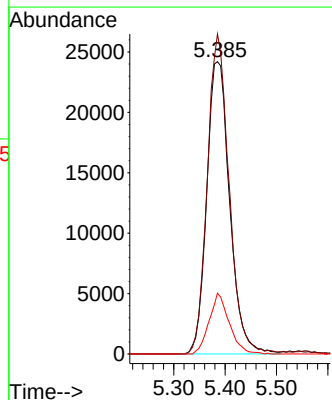
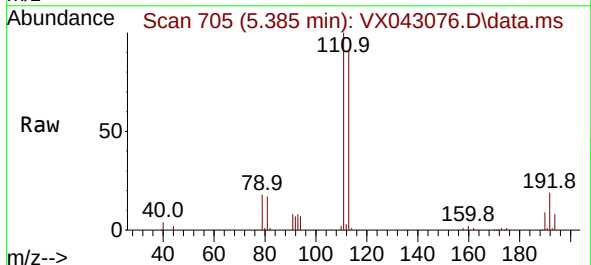


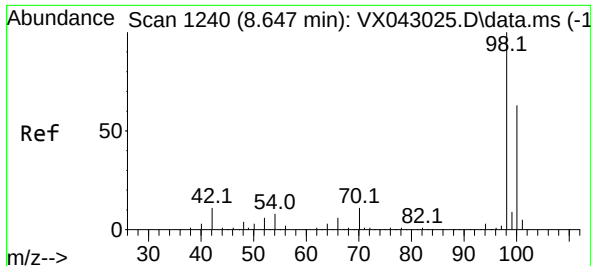

#50
Toluene-d8
Concen: 51.008 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX043076.D
Acq: 21 Aug 2024 10:20




Instrument :
MSVOA_X
ClientSampleId :
VX0821WBL01


Tgt Ion: 98 Resp: 293877
Ion Ratio Lower Upper
98 100
100 66.0 53.1 79.7

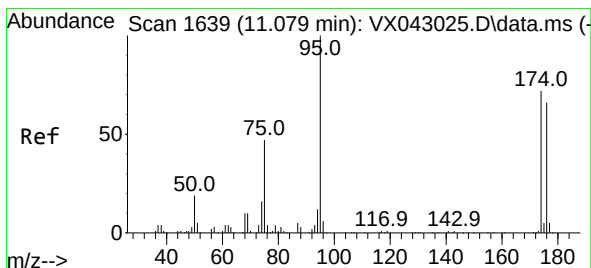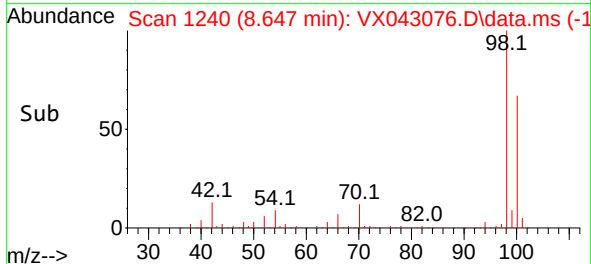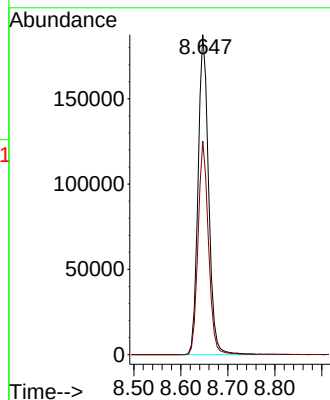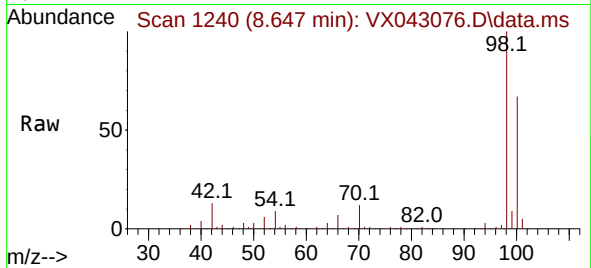

#62
4-Bromofluorobenzene
Concen: 51.104 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX043076.D
Acq: 21 Aug 2024 10:20

Tgt Ion: 95 Resp: 106759
Ion Ratio Lower Upper
95 100
174 67.7 0.0 135.6
176 65.1 0.0 131.0

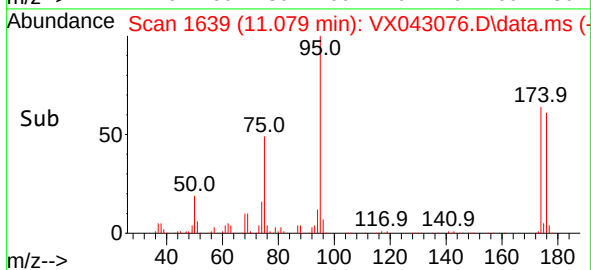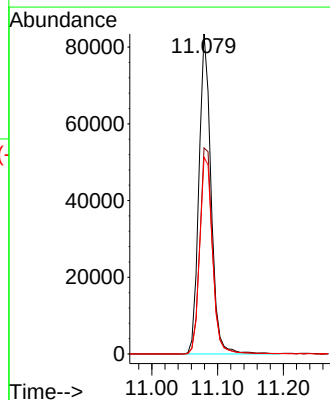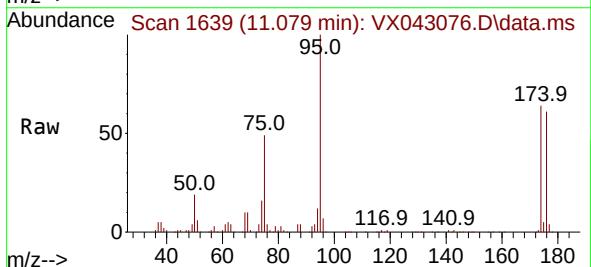

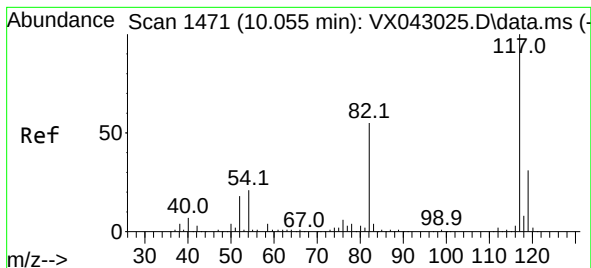

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX043076.D

Acq: 21 Aug 2024 10:20

Instrument :

MSVOA_X

ClientSampleId :

VX0821WBL01





Tgt Ion:117 Resp: 208859

Ion Ratio Lower Upper

117 100

82 58.3 46.2 69.4

119 31.7 25.5 38.3

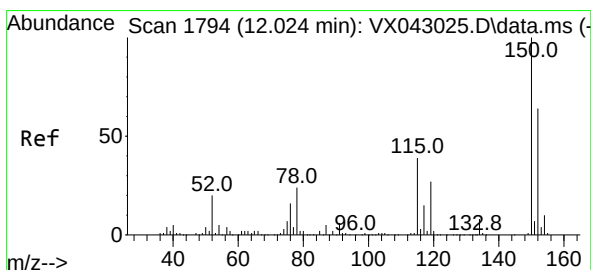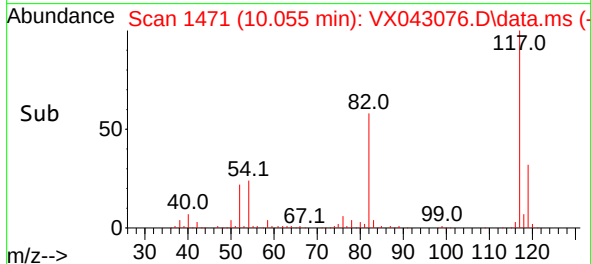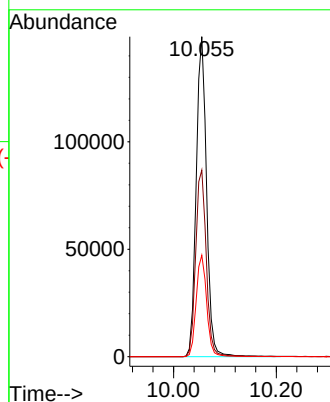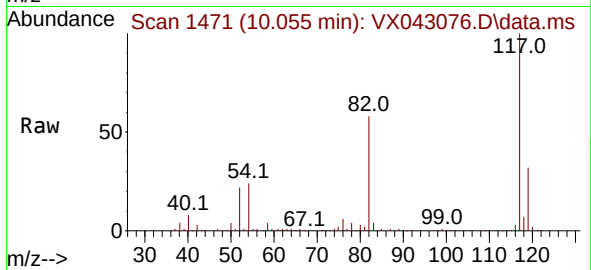

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX043076.D

Acq: 21 Aug 2024 10:20

Tgt Ion:152 Resp: 90356

Ion Ratio Lower Upper

152 100

115 62.1 43.3 129.9

150 156.3 0.0 345.0

