

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082125\
 Data File : VX047465.D
 Acq On : 21 Aug 2025 13:25
 Operator : JC/MD
 Sample : Q2900-05DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11C-081825DL

Quant Time: Aug 22 03:45:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	217485	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	440392	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	436547	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	229381	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	164181	53.940	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 107.880%			
35) Dibromofluoromethane	5.397	113	136895	47.896	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 95.800%			
50) Toluene-d8	8.653	98	495256	48.479	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 96.960%			
62) 4-Bromofluorobenzene	11.079	95	212086	56.258	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 112.520%			
Target Compounds						Qvalue
4) Vinyl Chloride	1.392	62	15069	4.814	ug/l	95
10) Methyl Iodide	2.477	142	1419	0.308	ug/l #	64
11) Tert butyl alcohol	2.959	59	258	0.974	ug/l #	72
16) Acetone	2.392	43	1537	1.343	ug/l #	86
21) trans-1,2-Dichloroethene	3.111	96	74912	25.775	ug/l	95
27) cis-1,2-Dichloroethene	4.507	96	28358	8.377	ug/l	89
31) Cyclohexane	5.562	56	4882	0.997	ug/l #	51
36) 1,1-Dichloropropene	5.562	75	17656	3.913	ug/l #	51
38) Carbon Tetrachloride	5.562	117	23192	4.704	ug/l #	15
40) Benzene	6.050	78	796444	58.975	ug/l	98
42) 1,2-Dichloroethane	6.044	62	7158	1.496	ug/l #	75
44) Trichloroethene	7.141	130	3593	1.039	ug/l	84
52) Toluene	8.720	92	117616	14.094	ug/l	99
53) t-1,3-Dichloropropene	8.720	75	1517	0.341	ug/l #	1
55) 1,1,2-Trichloroethane	9.025	97	834	0.263	ug/l #	26
67) Ethyl Benzene	10.195	91	181825	10.183	ug/l	98
68) m/p-Xylenes	10.305	106	36436	5.473	ug/l	97
69) o-Xylene	10.640	106	46169	7.206	ug/l	96
70) Styrene	10.653	104	60840	5.620	ug/l	99
73) Isopropylbenzene	10.963	105	11263	0.627	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	110269	26.210	ug/l #	39
78) n-propylbenzene	11.305	91	5869	0.274	ug/l	97
79) 2-Chlorotoluene	11.402	91	4933	0.381	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	13510	0.915	ug/l	93
81) trans-1,4-Dichloro-2-b...	11.079	75	110269	103.875	ug/l #	7
83) tert-Butylbenzene	11.750	119	7598	0.516	ug/l #	46
84) 1,2,4-Trimethylbenzene	11.750	105	61775	4.183	ug/l	99
85) sec-Butylbenzene	11.750	105	61775	3.382	ug/l #	57
90) Hexachloroethane	12.408	117	43124	15.906	ug/l #	15
95) Naphthalene	13.774	128	1637289	107.525	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082125\
Data File : VX047465.D
Acq On : 21 Aug 2025 13:25
Operator : JC/MD
Sample : Q2900-05DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL

Quant Time: Aug 22 03:45:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration




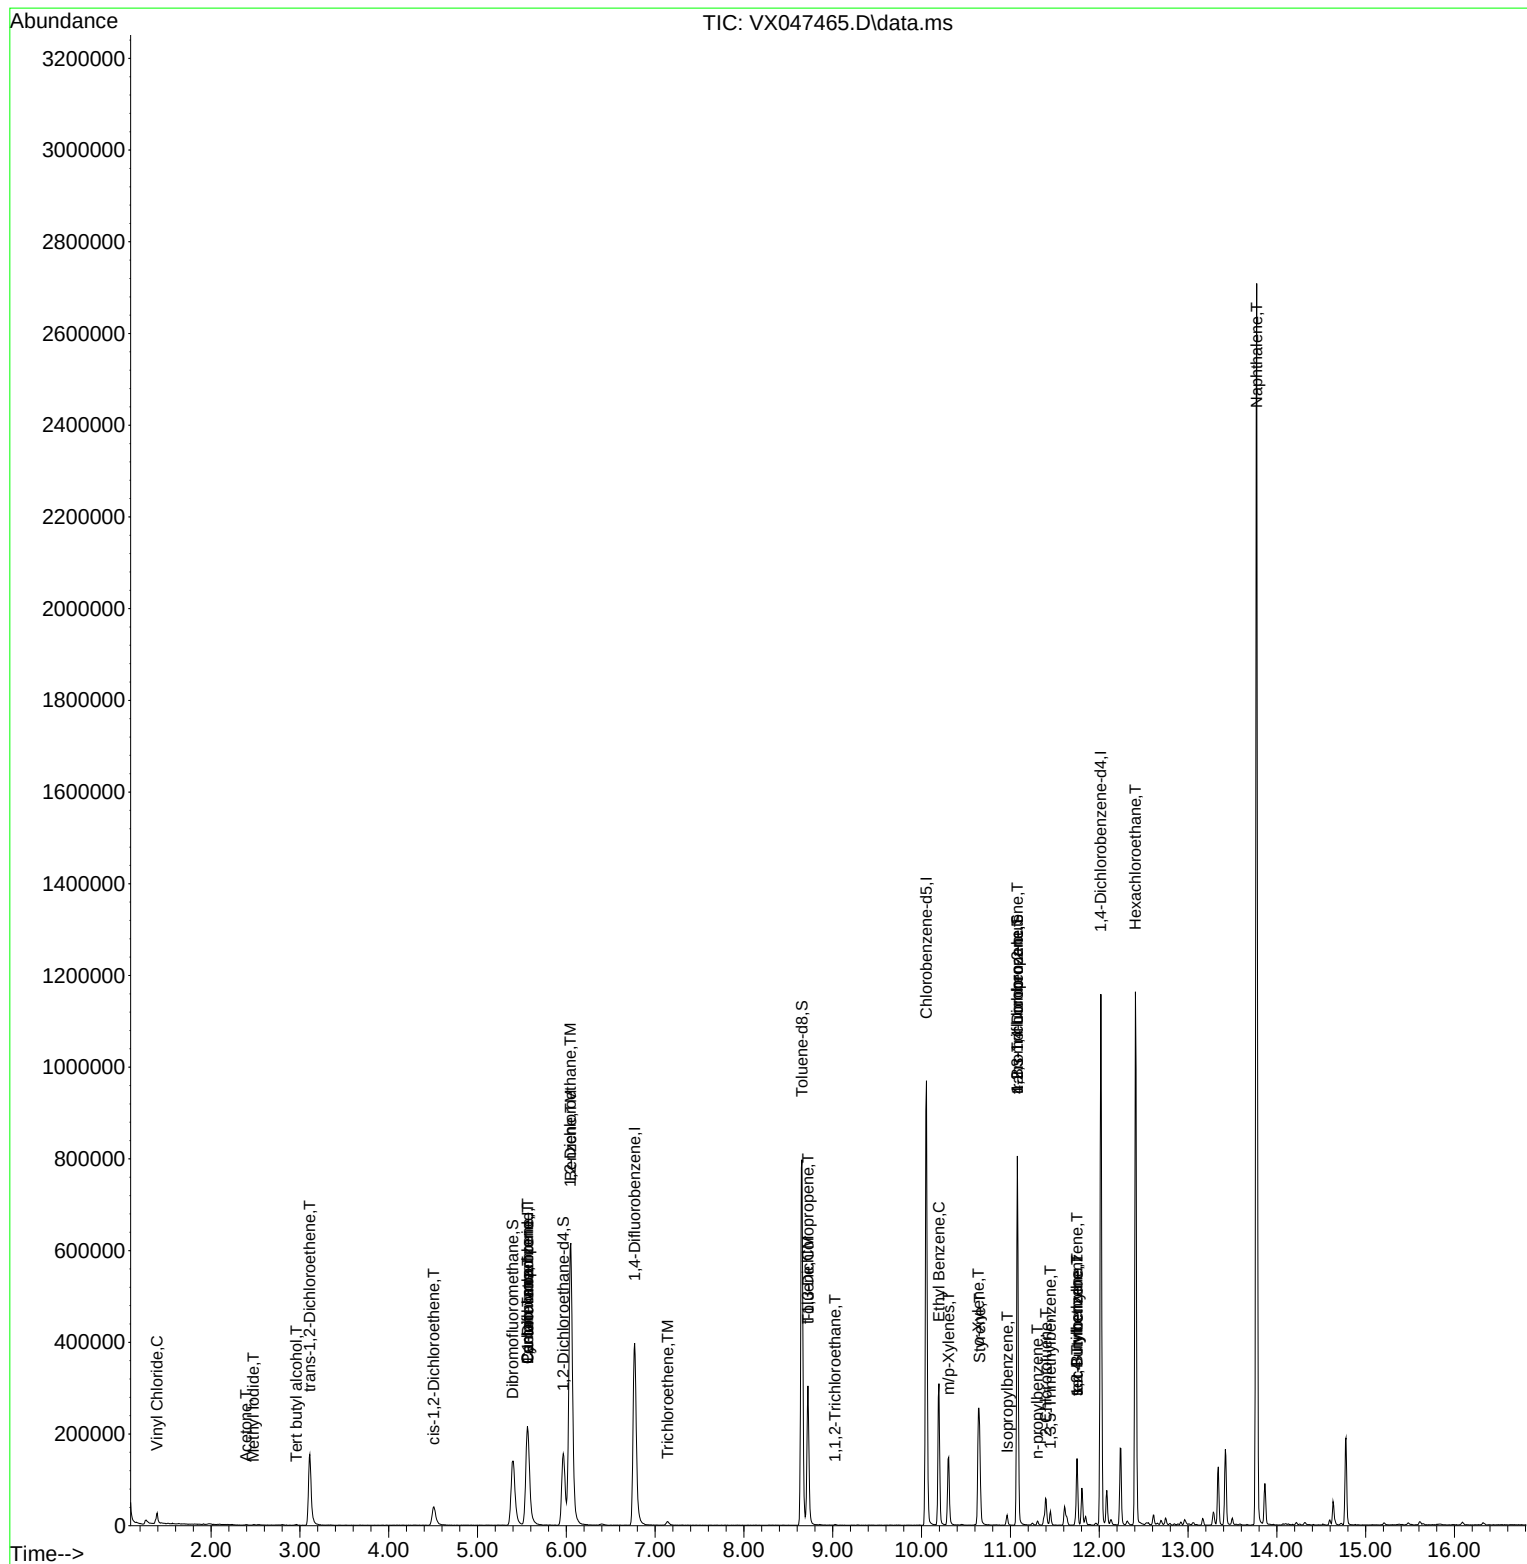




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion:168 Resp: 217485
Ion Ratio Lower Upper
168 100
99 60.4 47.9 71.9

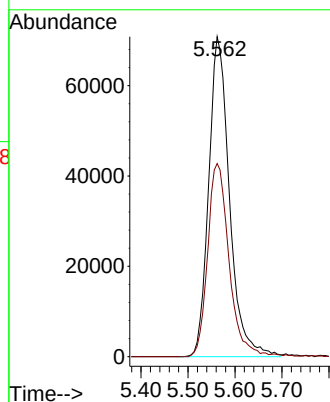

#4
Vinyl Chloride
Concen: 4.814 ug/l
RT: 1.392 min Scan# 50
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion: 62 Resp: 15069
Ion Ratio Lower Upper
62 100
64 36.0 26.5 39.7


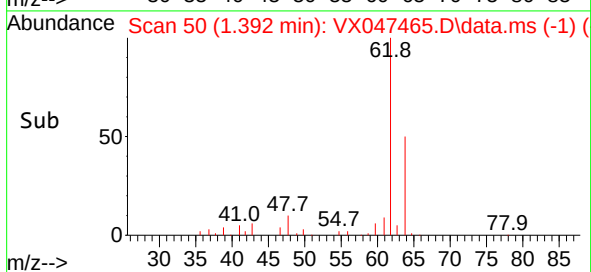
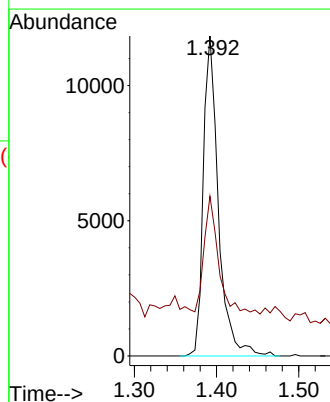





#10
Methyl Iodide
Concen: 0.308 ug/l
RT: 2.477 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion:142 Resp: 1419
Ion Ratio Lower Upper
142 100
127 72.7 36.1 54.1#
141 6.9 11.1 16.7#

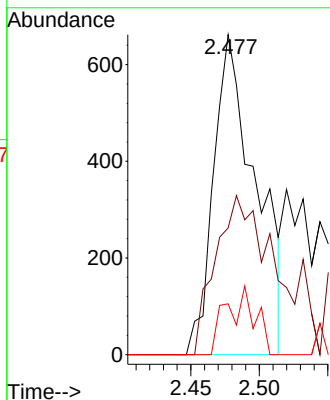

#11
Tert butyl alcohol
Concen: 0.974 ug/l
RT: 2.959 min Scan# 307
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion: 59 Resp: 258
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#



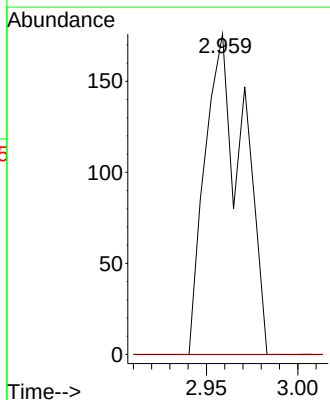





#16
Acetone
Concen: 1.343 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion: 43 Resp: 1537
Ion Ratio Lower Upper
43 100
58 23.4 24.8 37.2#

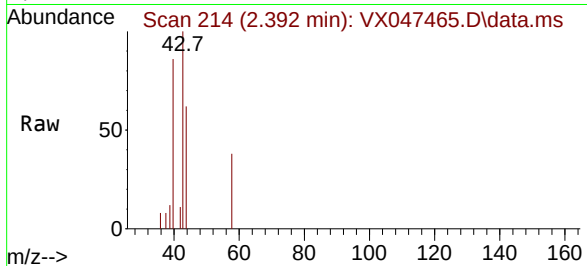

#21
trans-1,2-Dichloroethene
Concen: 25.775 ug/l
RT: 3.111 min Scan# 332
Delta R.T. 0.006 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion: 96 Resp: 74912
Ion Ratio Lower Upper
96 100
61 136.0 112.6 169.0
98 57.5 50.9 76.3

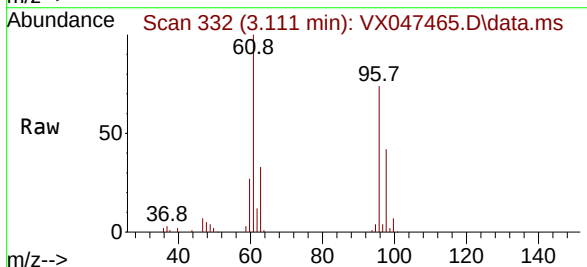



#27

cis-1,2-Dichloroethene

Concen: 8.377 ug/l

RT: 4.507 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25

Instrument :

MSVOA_X

ClientSampleId :

MW-11C-081825DL





Tgt Ion: 96 Resp: 28358

Ion Ratio Lower Upper

96 100

61 130.2 0.0 296.6

98 62.8 0.0 130.4

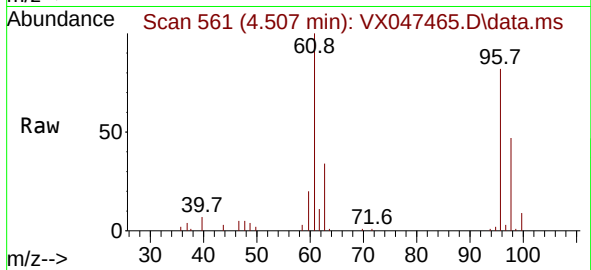

#31

Cyclohexane

Concen: 0.997 ug/l

RT: 5.562 min Scan# 734

Delta R.T. 0.079 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25




Tgt Ion: 56 Resp: 4882


Ion Ratio Lower Upper

56 100

69 122.3 24.3 36.5#

84 77.7 65.3 97.9

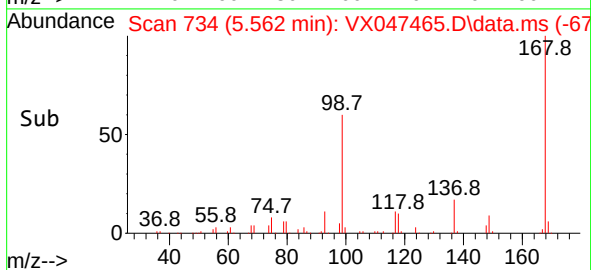

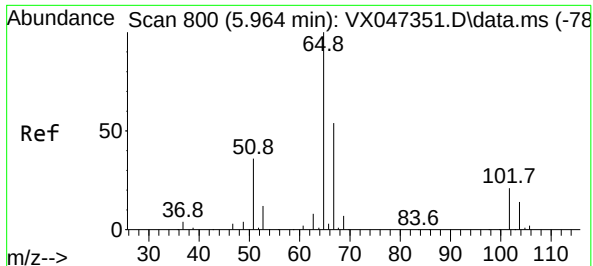

#33

1,2-Dichloroethane-d4

Concen: 53.940 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25

Instrument :

MSVOA_X

ClientSampleId :





MW-11C-081825DL

Tgt Ion: 65 Resp: 164181

Ion Ratio Lower Upper

65 100

67 51.3 0.0 106.0

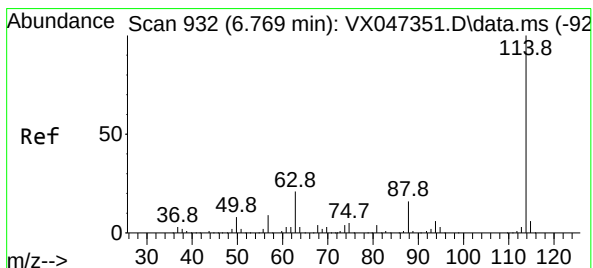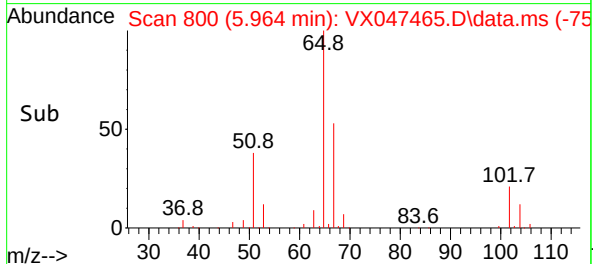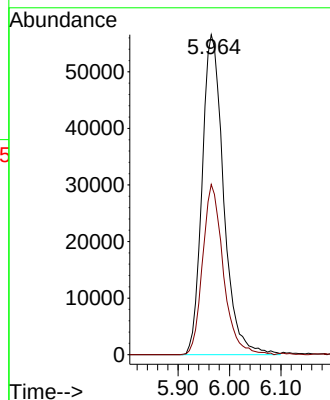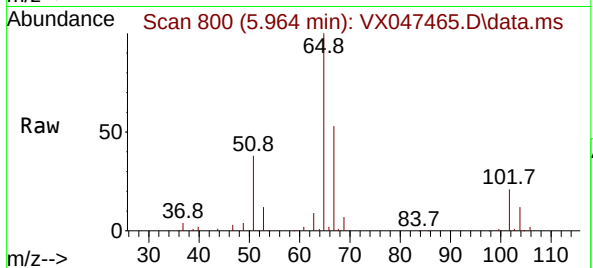

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25




Tgt Ion: 114 Resp: 440392


Ion Ratio Lower Upper

114 100

63 21.8 0.0 42.4

88 16.9 0.0 33.0

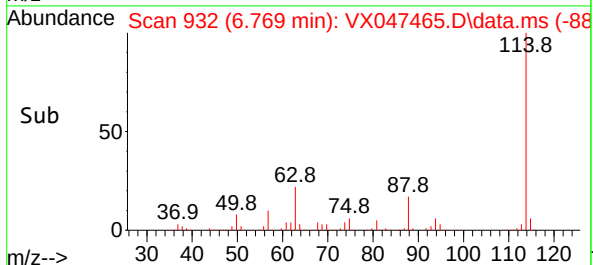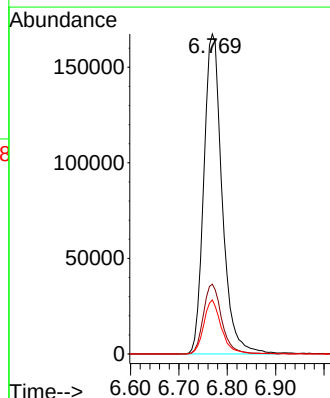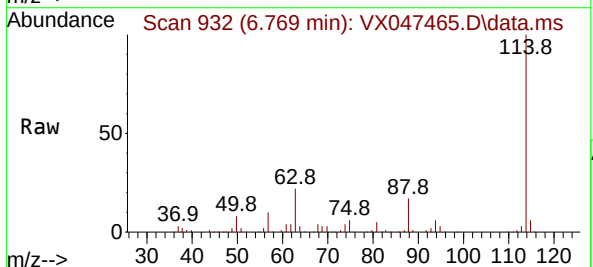

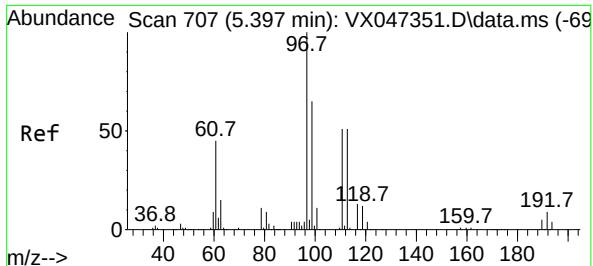

#35

Dibromofluoromethane

Concen: 47.896 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.000 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25

Instrument :

MSVOA_X

ClientSampleId :

MW-11C-081825DL





Tgt Ion:113 Resp: 136895

Ion Ratio Lower Upper

113 100

111 104.6 81.4 122.2

192 19.1 14.1 21.1

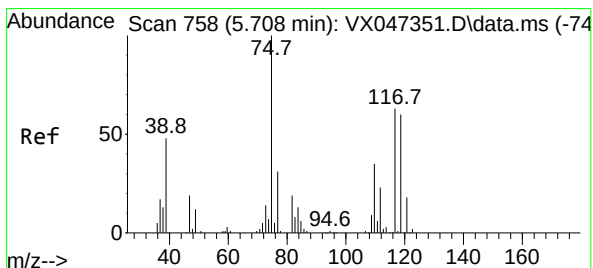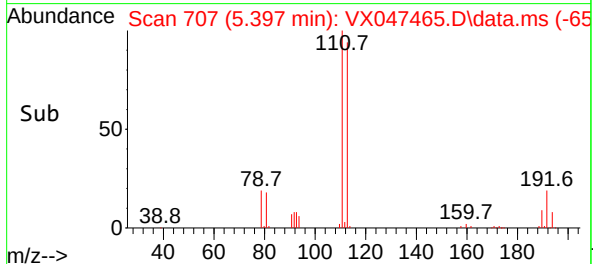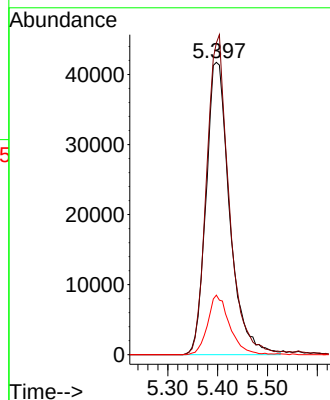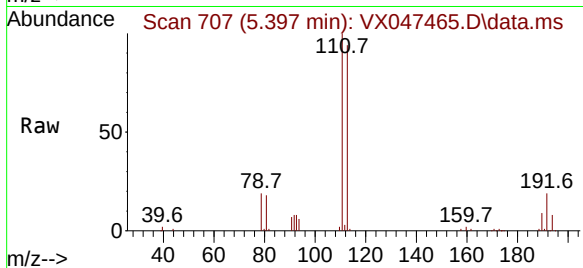

#36

1,1-Dichloropropene

Concen: 3.913 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.146 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25




Tgt Ion: 75 Resp: 17656


Ion Ratio Lower Upper

75 100

110 10.4 17.4 52.2#


77 0.0 24.4 36.6#

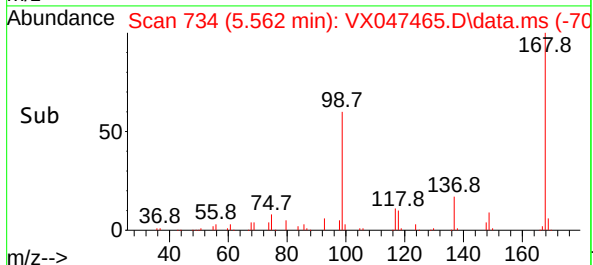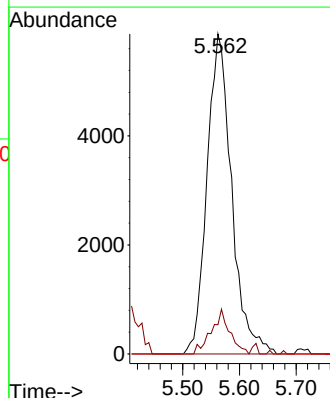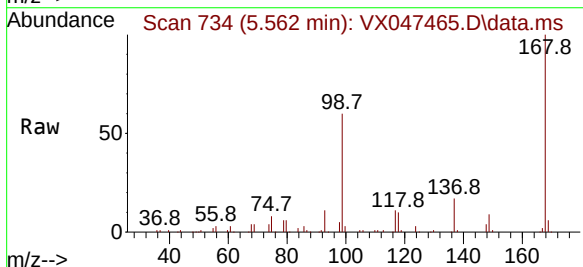






#38
Carbon Tetrachloride
Concen: 4.704 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL



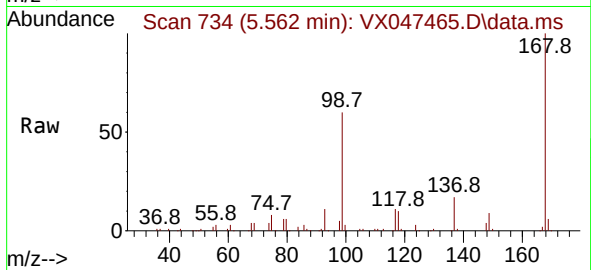



Tgt Ion:117 Resp: 23192
Ion Ratio Lower Upper
117 100
119 5.1 78.5 117.7#
121 0.0 24.7 37.1#

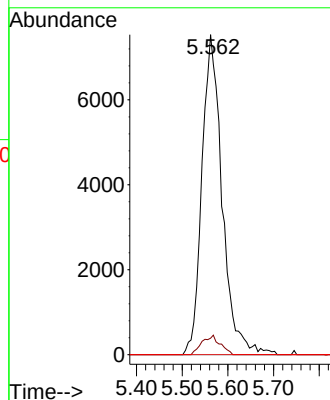

#40
Benzene
Concen: 58.975 ug/l
RT: 6.050 min Scan# 814
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion: 78 Resp: 796444
Ion Ratio Lower Upper
78 100
77 22.9 19.0 28.4


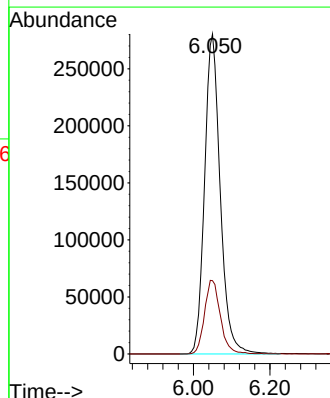






#42
1,2-Dichloroethane
Concen: 1.496 ug/l
RT: 6.044 min Scan# 81
Delta R.T. -0.055 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion: 62 Resp: 7158
Ion Ratio Lower Upper
62 100
98 0.0 0.0 18.0



#44
Trichloroethene
Concen: 1.039 ug/l
RT: 7.141 min Scan# 993
Delta R.T. 0.006 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion:130 Resp: 3593
Ion Ratio Lower Upper
130 100
95 115.0 0.0 198.6









#50
Toluene-d8
Concen: 48.479 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion: 98 Resp: 495256
Ion Ratio Lower Upper
98 100
100 66.6 53.9 80.9

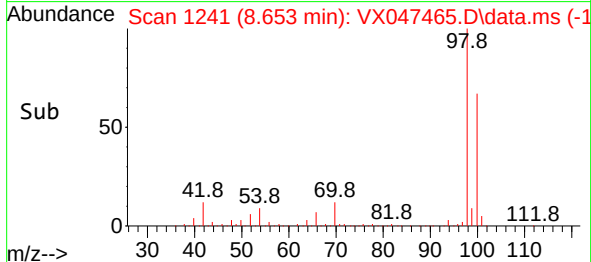

#52
Toluene
Concen: 14.094 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion: 92 Resp: 117616
Ion Ratio Lower Upper
92 100
91 169.0 136.3 204.5

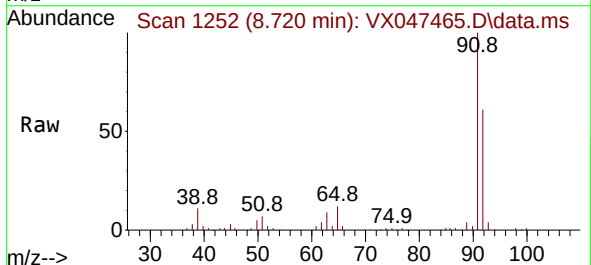

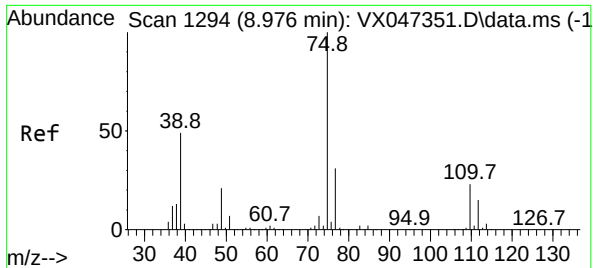

#53

t-1,3-Dichloropropene

Concen: 0.341 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.256 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25

Instrument :

MSVOA_X

ClientSampleId :





MW-11C-081825DL

Tgt Ion: 75 Resp: 1517

Ion Ratio Lower Upper

75 100

77 137.4 24.7 37.1#

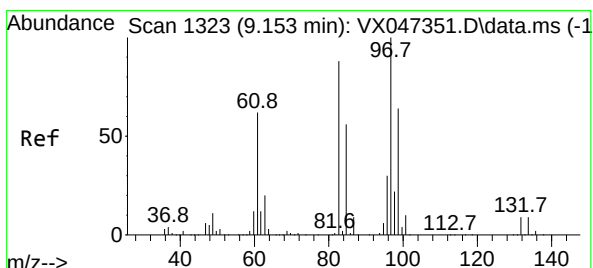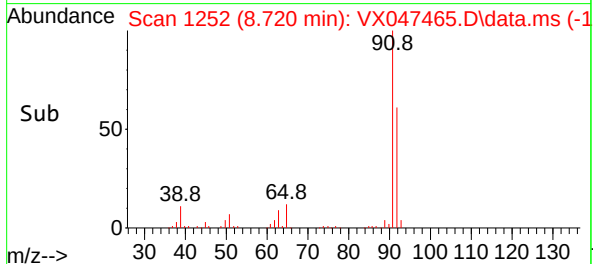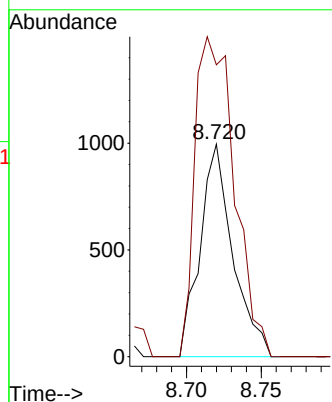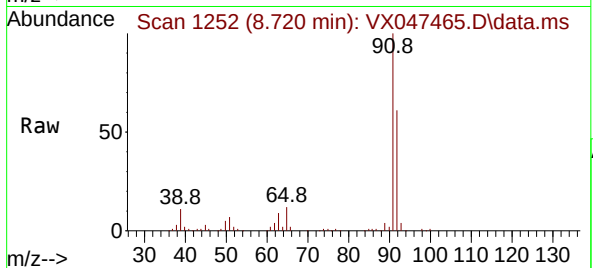

#55

1,1,2-Trichloroethane

Concen: 0.263 ug/l

RT: 9.025 min Scan# 1302

Delta R.T. -0.128 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25

Tgt Ion: 97 Resp: 834




Ion Ratio Lower Upper


97 100

83 0.0 70.6 106.0#

85 0.0 44.7 67.1#

99 30.6 51.2 76.8#


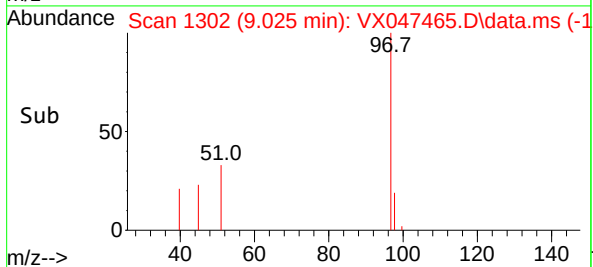

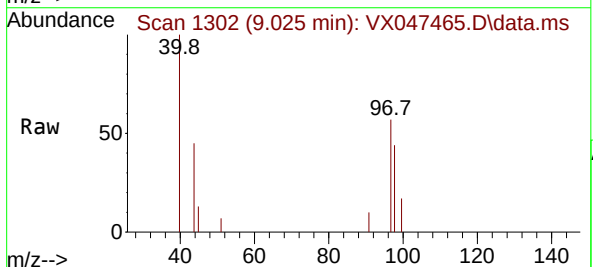




#62
4-Bromofluorobenzene
Concen: 56.258 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion: 95 Resp: 212086
Ion Ratio Lower Upper
95 100
174 74.9 0.0 148.0
176 70.7 0.0 145.4

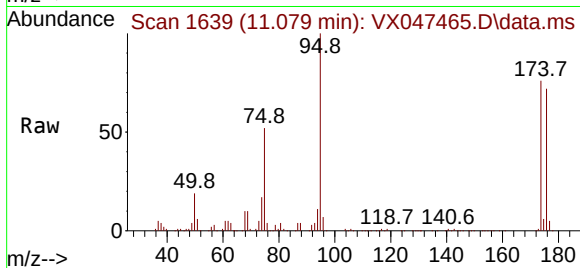

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion: 117 Resp: 436547
Ion Ratio Lower Upper
117 100
82 56.5 45.0 67.4
119 33.1 25.8 38.8

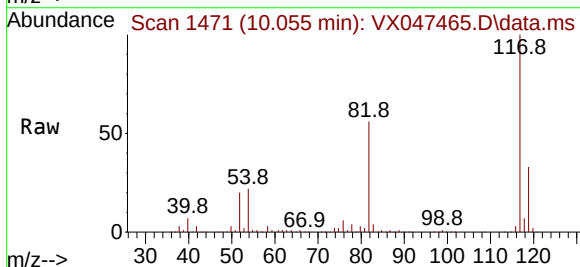



#67

Ethyl Benzene

Concen: 10.183 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25

Instrument :

MSVOA_X

ClientSampleId :





MW-11C-081825DL

Tgt Ion: 91 Resp: 181825

Ion Ratio Lower Upper

91 100

106 29.3 24.4 36.6



#68

m/p-Xylenes

Concen: 5.473 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.006 min

Lab File: VX047465.D




Acq: 21 Aug 2025 13:25


Tgt Ion: 106 Resp: 36436

Ion Ratio Lower Upper

106 100

91 210.8 164.7 247.1

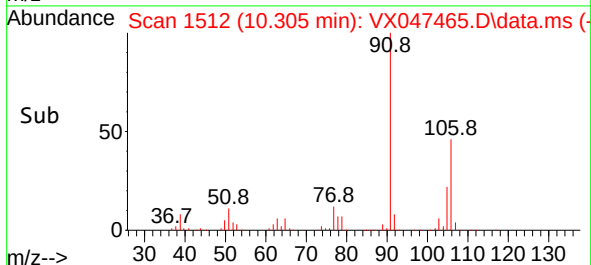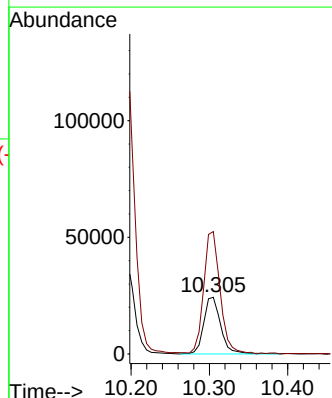



#69

o-Xylene

Concen: 7.206 ug/l

RT: 10.640 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25

Instrument :

MSVOA_X

ClientSampleId :





MW-11C-081825DL

Tgt Ion:106 Resp: 46169

Ion Ratio Lower Upper

106 100

91 227.8 110.6 331.8

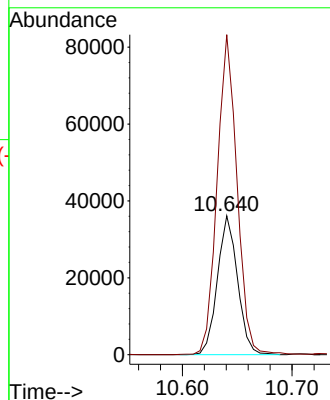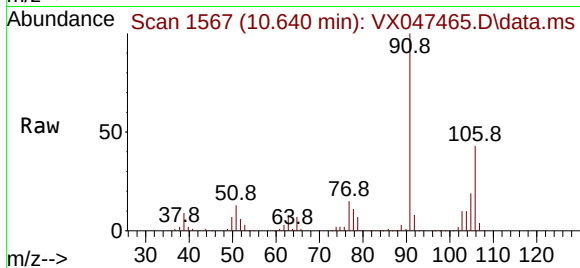

#70

Styrene

Concen: 5.620 ug/l

RT: 10.653 min Scan# 1569

Delta R.T. 0.000 min

Lab File: VX047465.D

Acq: 21 Aug 2025 13:25




Tgt Ion:104 Resp: 60840


Ion Ratio Lower Upper

104 100

78 53.7 41.8 62.8

103 54.6 43.6 65.4


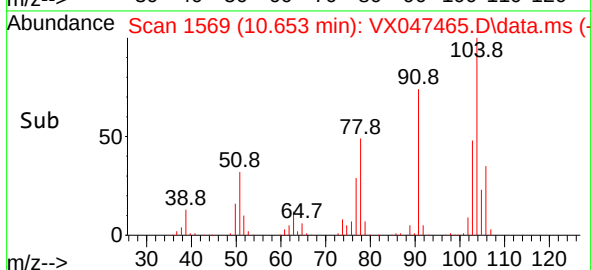
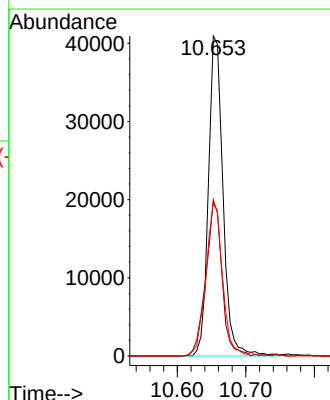
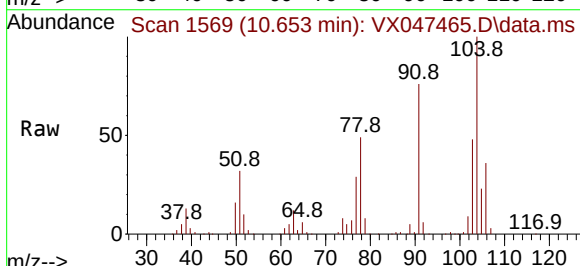




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion:152 Resp: 229381
Ion Ratio Lower Upper
152 100
115 61.8 44.6 133.8
150 156.1 0.0 349.8

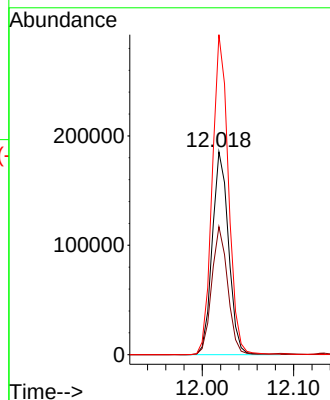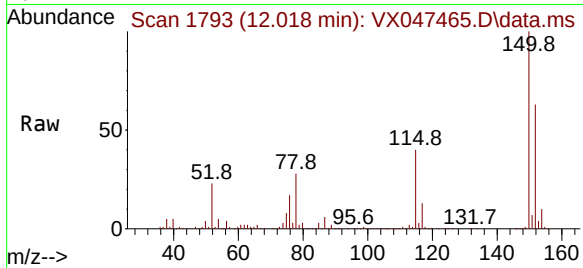

#73
Isopropylbenzene
Concen: 0.627 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion:105 Resp: 11263
Ion Ratio Lower Upper
105 100
120 25.4 12.9 38.6


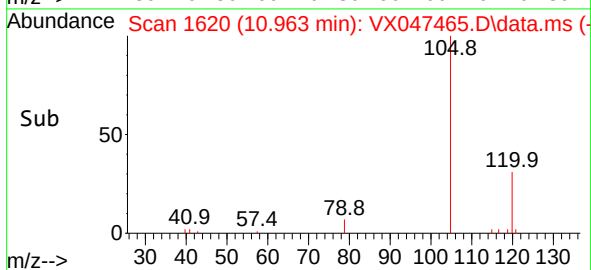
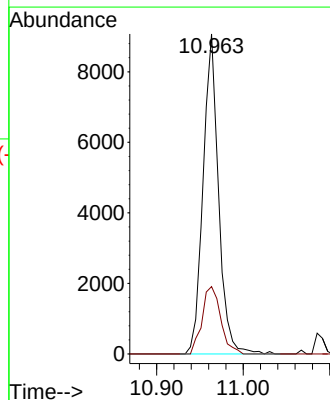
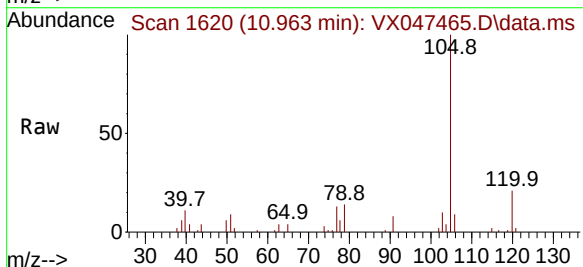




#76
1,2,3-Trichloropropane
Concen: 26.210 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion: 75 Resp: 110269
Ion Ratio Lower Upper
75 100
77 1.4 19.4 58.2#

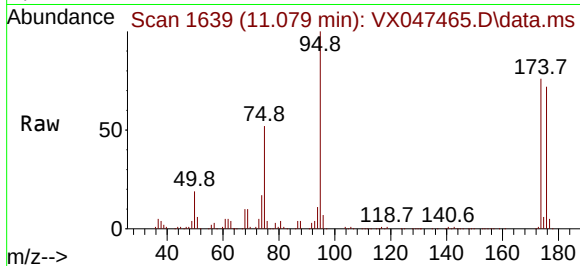

#78
n-propylbenzene
Concen: 0.274 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.006 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion: 91 Resp: 5869
Ion Ratio Lower Upper
91 100
120 23.5 11.0 33.0




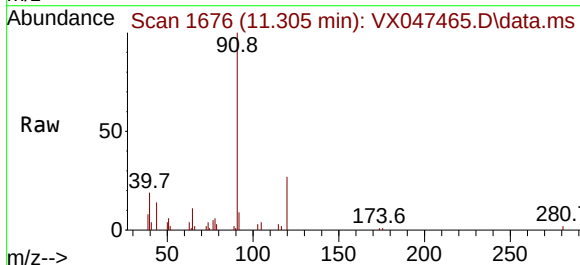




#79
2-Chlorotoluene
Concen: 0.381 ug/l
RT: 11.402 min Scan# 11
Delta R.T. 0.043 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion: 91 Resp: 4933
Ion Ratio Lower Upper
91 100
126 0.0 16.7 50.1#

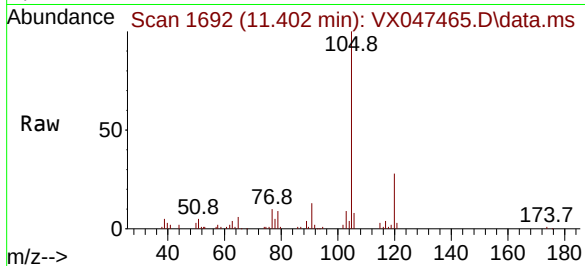

#80
1,3,5-Trimethylbenzene
Concen: 0.915 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion: 105 Resp: 13510
Ion Ratio Lower Upper
105 100
120 42.8 23.9 71.7


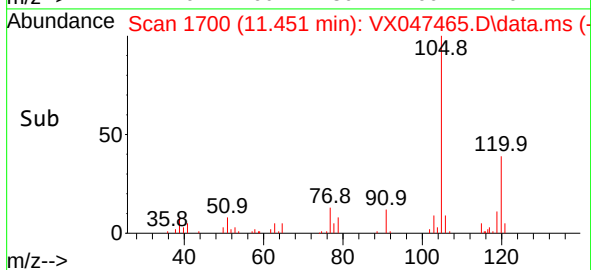

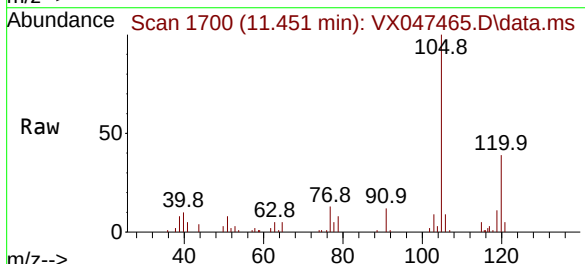




#81
trans-1,4-Dichloro-2-butene
Concen: 103.875 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion: 75 Resp: 110269
Ion Ratio Lower Upper
75 100
53 0.0 85.2 127.8#
89 0.0 36.7 55.1#

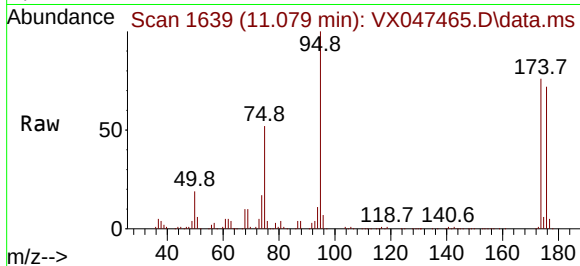

#83
tert-Butylbenzene
Concen: 0.516 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.037 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion: 119 Resp: 7598
Ion Ratio Lower Upper
119 100
91 100.4 29.1 87.4#
134 0.0 11.3 33.9#




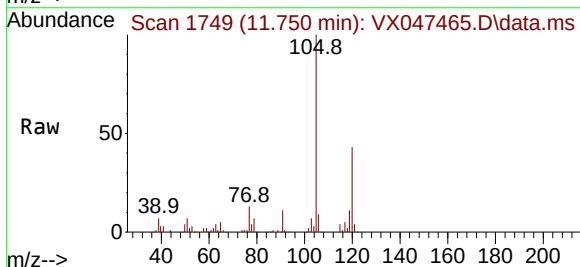




#84
1,2,4-Trimethylbenzene
Concen: 4.183 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25




Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL


Tgt Ion:105 Resp: 61775
Ion Ratio Lower Upper
105 100
120 44.3 21.9 65.7

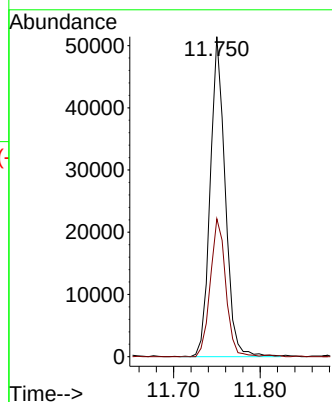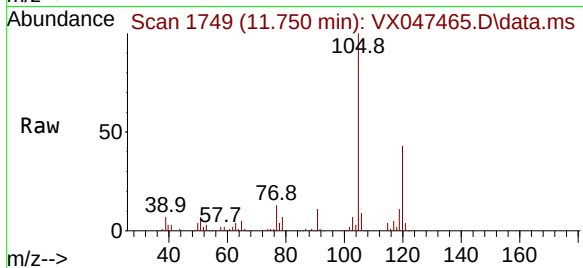

#85
sec-Butylbenzene
Concen: 3.382 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion:105 Resp: 61775
Ion Ratio Lower Upper
105 100
134 0.0 9.8 29.5#



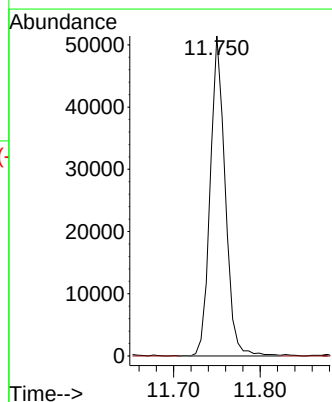
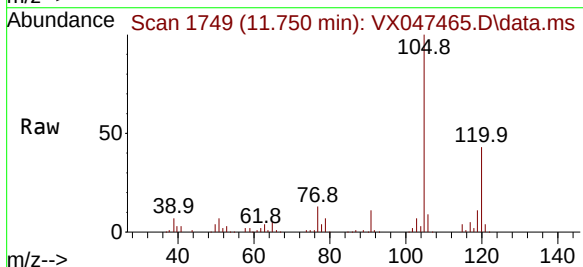




#90
Hexachloroethane
Concen: 15.906 ug/l
RT: 12.408 min Scan# 117
Delta R.T. -0.128 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Instrument :
MSVOA_X
ClientSampleId :
MW-11C-081825DL

Tgt Ion:117 Resp: 43124
Ion Ratio Lower Upper
117 100
201 0.0 35.1 105.3#

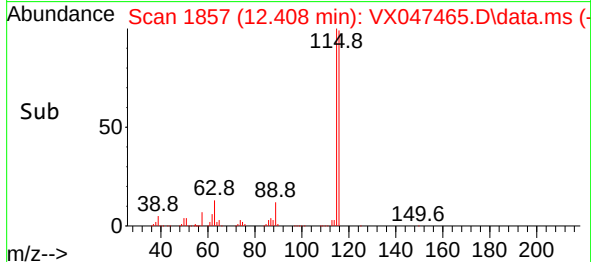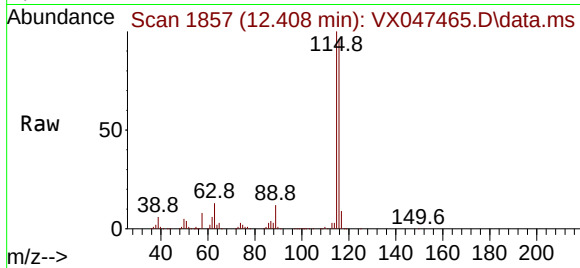

#95
Naphthalene
Concen: 107.525 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX047465.D
Acq: 21 Aug 2025 13:25

Tgt Ion:128 Resp: 1637289
Ion Ratio Lower Upper
128 100
127 12.7 10.1 15.1
129 10.9 8.7 13.1

