

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082125\
 Data File : VX047468.D
 Acq On : 21 Aug 2025 14:28
 Operator : JC/MD
 Sample : Q2869-04 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11A-13.5-081325DL

Quant Time: Aug 22 03:47:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	195089	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	386665	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	376333	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	185836	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	145202	53.181	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 106.360%	
35) Dibromofluoromethane	5.397	113	121502	48.417	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.840%	
50) Toluene-d8	8.653	98	434529	48.445	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 96.880%	
62) 4-Bromofluorobenzene	11.079	95	175623	53.059	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 106.120%	
Target Compounds						Qvalue
4) Vinyl Chloride	1.392	62	1334	0.475	ug/l	100
5) Bromomethane	1.636	94	425	0.375	ug/l	83
9) 1,1,2-Trichlorotrifluo...	2.349	101	10607	4.402	ug/l	96
10) Methyl Iodide	2.477	142	3663	0.887	ug/l #	88
11) Tert butyl alcohol	2.971	59	797	3.355	ug/l #	72
12) 1,1-Dichloroethene	2.343	96	996	0.405	ug/l #	40
13) Acrolein	2.258	56	147	0.293	ug/l #	31
15) Acrylonitrile	3.093	53	446	0.389	ug/l #	28
16) Acetone	2.392	43	1061	1.034	ug/l	91
17) Carbon Disulfide	2.532	76	1736	0.234	ug/l	96
20) Methylene Chloride	2.800	84	1198	0.441	ug/l #	73
21) trans-1,2-Dichloroethene	3.111	96	853	0.327	ug/l #	75
24) 1,1-Dichloroethane	3.623	63	1305	0.274	ug/l #	83
27) cis-1,2-Dichloroethene	4.507	96	227423	74.896	ug/l	89
29) Tetrahydrofuran	5.056	42	254	0.292	ug/l #	69
31) Cyclohexane	5.562	56	4227	0.962	ug/l #	1
36) 1,1-Dichloropropene	5.562	75	16014	4.042	ug/l #	49
38) Carbon Tetrachloride	5.562	117	20950	4.839	ug/l #	14
44) Trichloroethene	7.129	130	286321	94.305	ug/l	99
49) 1,4-Dioxane	7.708	88	81	2.717	ug/l #	43
60) Dibromochloromethane	9.281	129	1851	0.560	ug/l #	11
64) Tetrachloroethene	9.275	164	1793	0.659	ug/l	95
76) 1,2,3-Trichloropropane	11.079	75	91579	26.868	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	91579	106.285	ug/l #	7
89) n-Butylbenzene	12.335	91	2666	0.229	ug/l	98
93) 1,2,4-Trichlorobenzene	13.591	180	1530	0.354	ug/l	97
94) Hexachlorobutadiene	13.725	225	1654	1.076	ug/l	90
95) Naphthalene	13.780	128	13704	1.111	ug/l	97
96) 1,2,3-Trichlorobenzene	13.963	180	1546	0.380	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082125\
Data File : VX047468.D
Acq On : 21 Aug 2025 14:28
Operator : JC/MD
Sample : Q2869-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL

Quant Time: Aug 22 03:47:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration




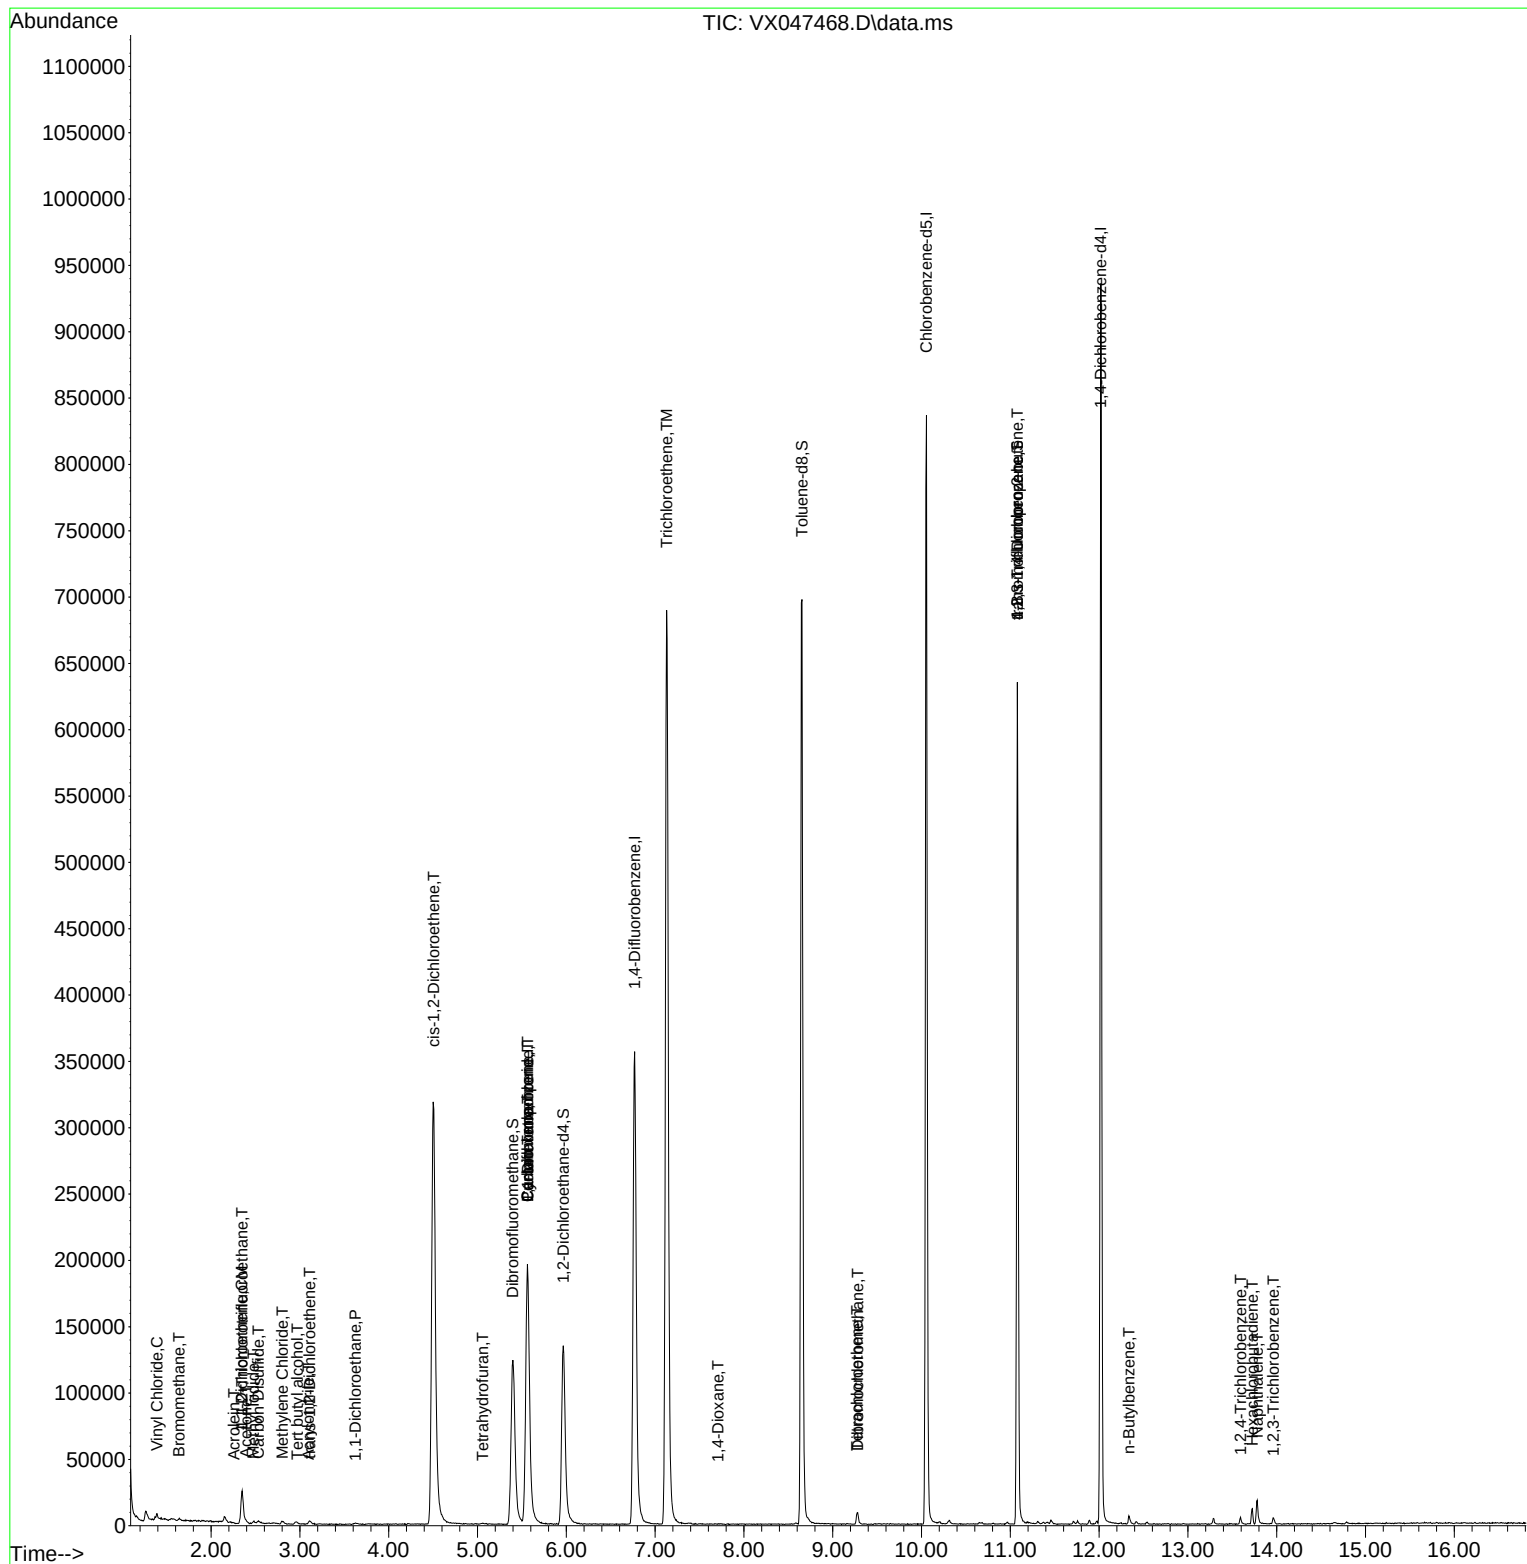




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion:168 Resp: 195089
Ion Ratio Lower Upper
168 100
99 64.4 47.9 71.9

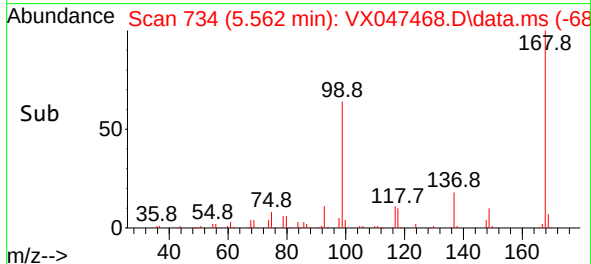

#4
Vinyl Chloride
Concen: 0.475 ug/l
RT: 1.392 min Scan# 50
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion: 62 Resp: 1334
Ion Ratio Lower Upper
62 100
64 33.0 26.5 39.7




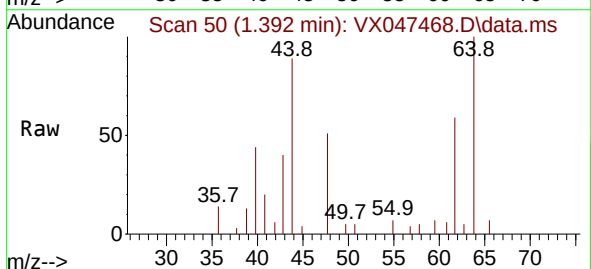


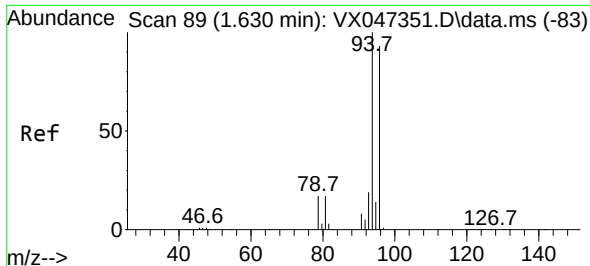

#5
Bromomethane
Concen: 0.375 ug/l
RT: 1.636 min Scan# 90
Delta R.T. 0.006 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion: 94 Resp: 425
Ion Ratio Lower Upper
94 100
96 76.7 74.7 112.1

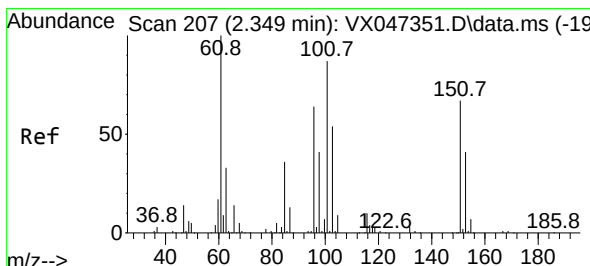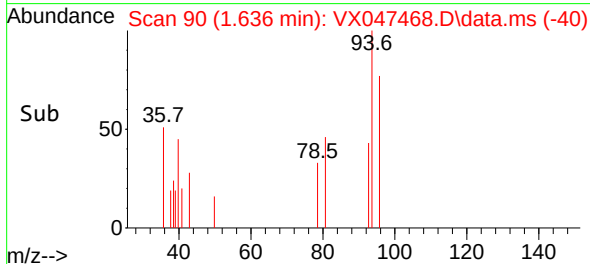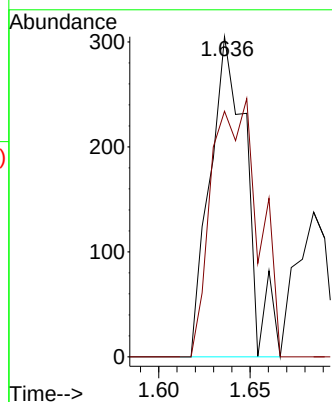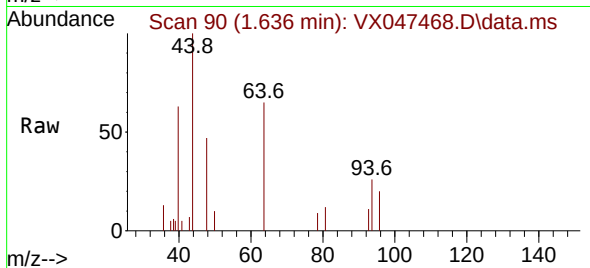

#9
1,1,2-Trichlorotrifluoroethane
Concen: 4.402 ug/l
RT: 2.349 min Scan# 207
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion: 101 Resp: 10607
Ion Ratio Lower Upper
101 100
85 38.5 34.3 51.5
151 71.8 59.2 88.8


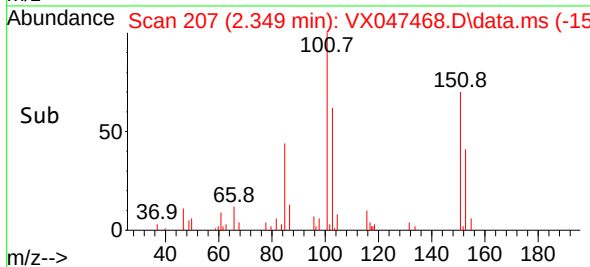
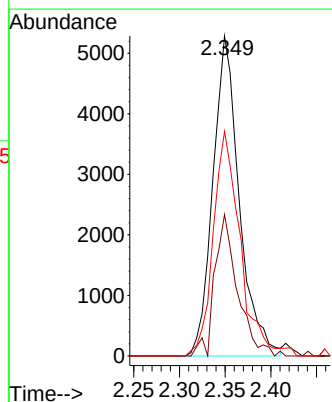
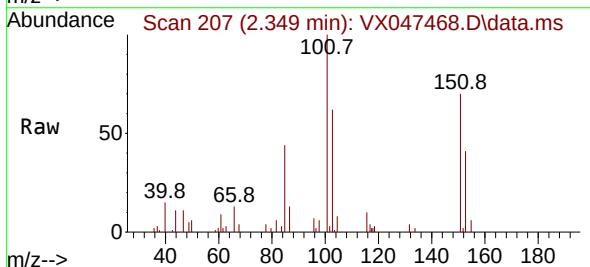




#10
Methyl Iodide
Concen: 0.887 ug/l
RT: 2.477 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion:142 Resp: 3663
Ion Ratio Lower Upper
142 100
127 36.0 36.1 54.1#
141 11.0 11.1 16.7#

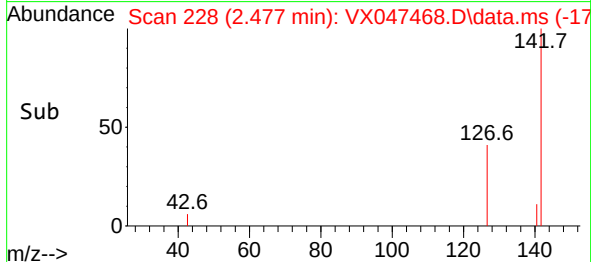

#11
Tert butyl alcohol
Concen: 3.355 ug/l
RT: 2.971 min Scan# 309
Delta R.T. 0.012 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion: 59 Resp: 797
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

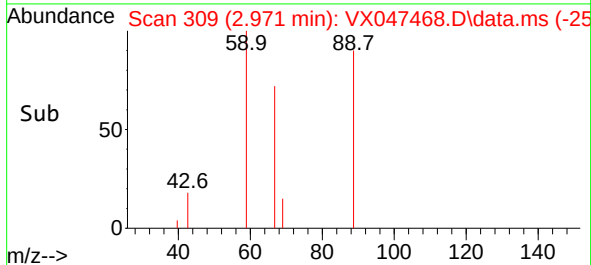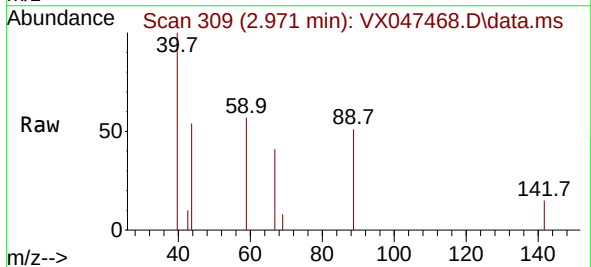

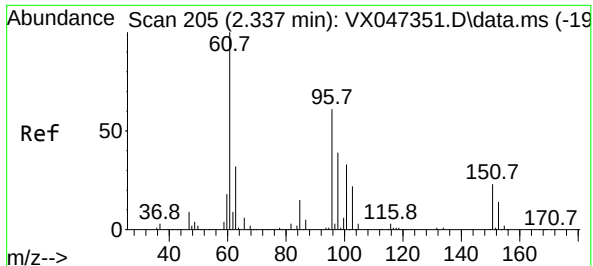

#12

1,1-Dichloroethene

Concen: 0.405 ug/l

RT: 2.343 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX047468.D

Acq: 21 Aug 2025 14:28

Instrument :

MSVOA_X

ClientSampleId :

MW-11A-13.5-081325DL





Tgt Ion: 96 Resp: 996

Ion Ratio Lower Upper

96 100

61 95.6 132.2 198.2#

98 0.0 51.2 76.8#

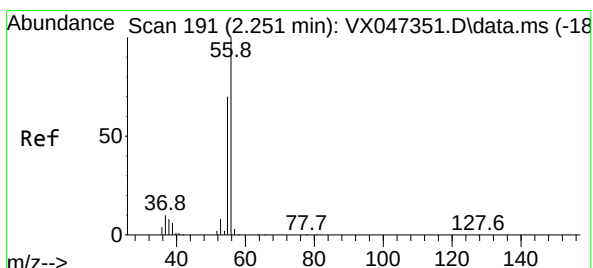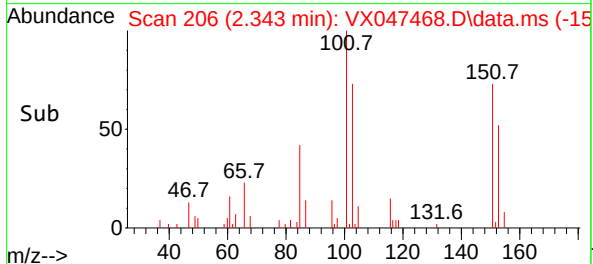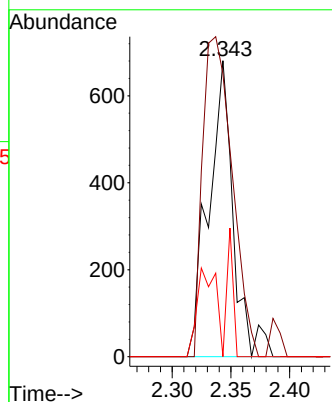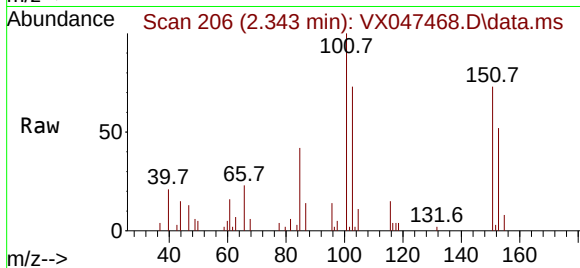

#13

Acrolein

Concen: 0.293 ug/l

RT: 2.258 min Scan# 192

Delta R.T. 0.006 min

Lab File: VX047468.D




Acq: 21 Aug 2025 14:28


Tgt Ion: 56 Resp: 147

Ion Ratio Lower Upper

56 100

55 12.9 55.5 83.3#


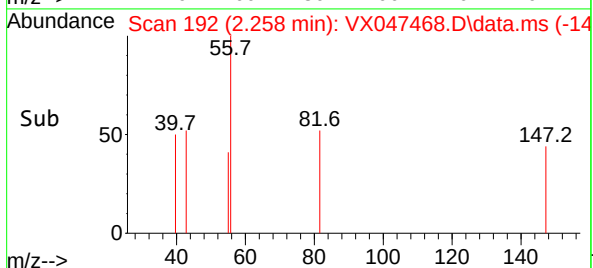

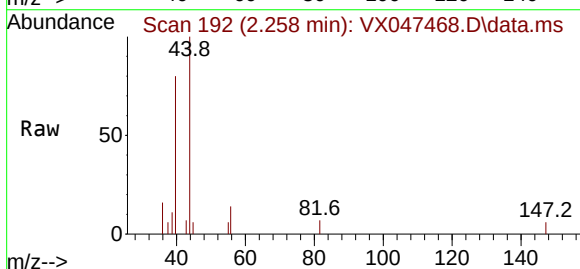




#15
Acrylonitrile
Concen: 0.389 ug/l
RT: 3.093 min Scan# 31
Delta R.T. 0.012 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion: 53 Resp: 446
Ion Ratio Lower Upper
53 100
52 13.9 65.8 98.6#
51 0.0 28.2 42.2#

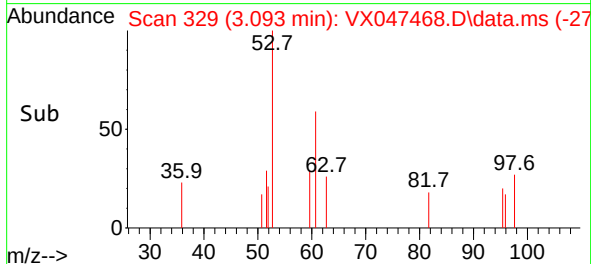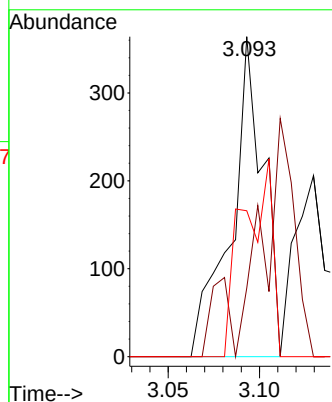

#16
Acetone
Concen: 1.034 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion: 43 Resp: 1061
Ion Ratio Lower Upper
43 100
58 26.0 24.8 37.2

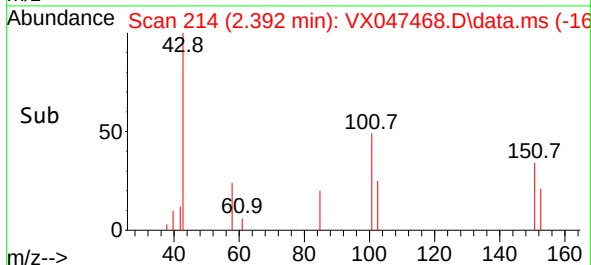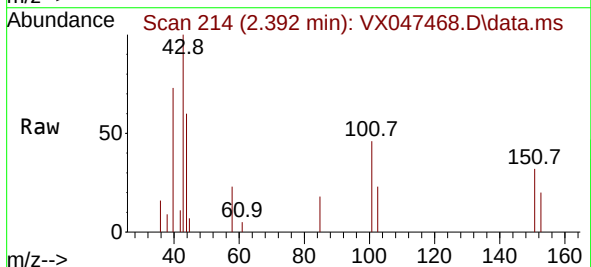



#17

Carbon Disulfide

Concen: 0.234 ug/l

RT: 2.532 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX047468.D

Acq: 21 Aug 2025 14:28

Instrument :

MSVOA_X

ClientSampleId :





MW-11A-13.5-081325DL

Tgt Ion: 76 Resp: 1736

Ion Ratio Lower Upper

76 100

78 10.3 7.2 10.8

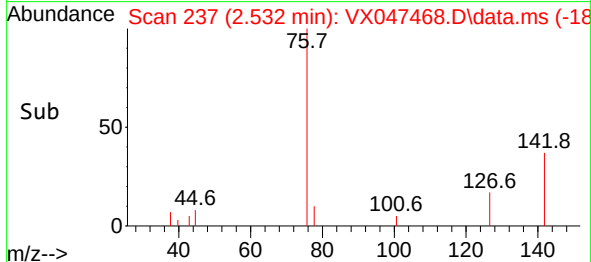

#20

Methylene Chloride

Concen: 0.441 ug/l

RT: 2.800 min Scan# 281

Delta R.T. -0.006 min

Lab File: VX047468.D

Acq: 21 Aug 2025 14:28

Tgt Ion: 84 Resp: 1198




Ion Ratio Lower Upper


84 100

49 95.1 100.1 150.1#

51 41.5 29.5 44.3

86 34.9 51.8 77.8#


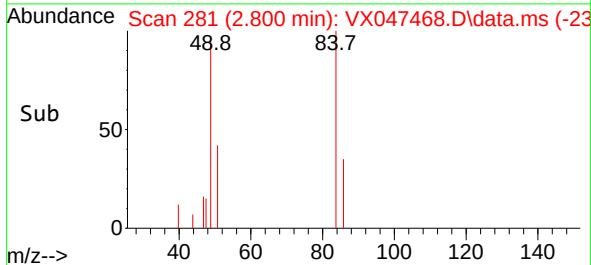

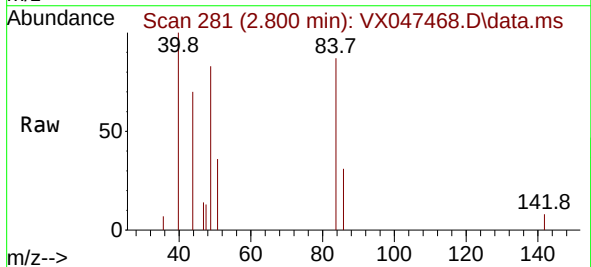




#21
trans-1,2-Dichloroethene
Concen: 0.327 ug/l
RT: 3.111 min Scan# 311
Delta R.T. 0.006 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion: 96 Resp: 853
Ion Ratio Lower Upper
96 100
61 106.2 112.6 169.0#
98 49.9 50.9 76.3#

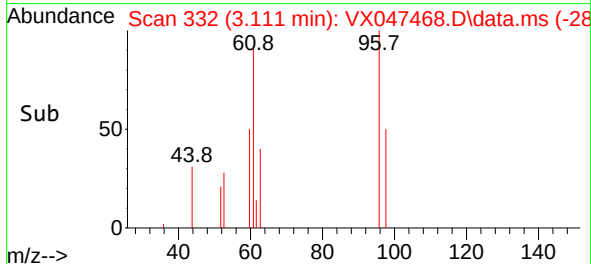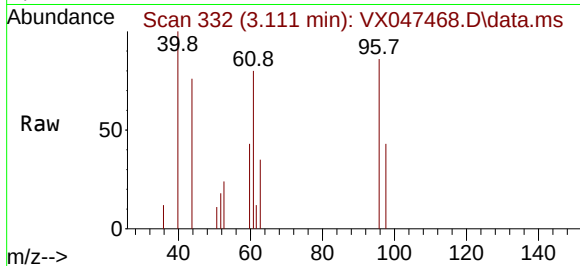

#24
1,1-Dichloroethane
Concen: 0.274 ug/l
RT: 3.623 min Scan# 416
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion: 63 Resp: 1305
Ion Ratio Lower Upper
63 100
98 0.0 3.3 9.9#
100 0.0 2.1 6.3#

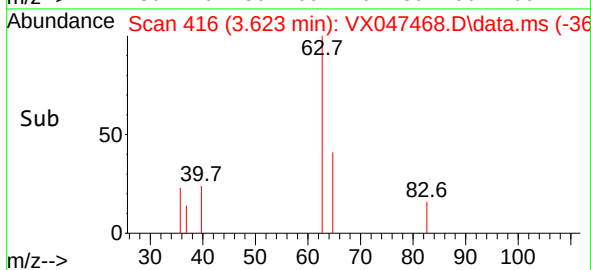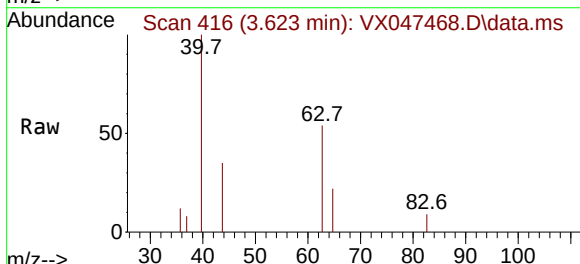



#27

cis-1,2-Dichloroethene

Concen: 74.896 ug/l

RT: 4.507 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX047468.D

Acq: 21 Aug 2025 14:28

Instrument :

MSVOA_X

ClientSampleId :

MW-11A-13.5-081325DL





Tgt Ion: 96 Resp: 227423

Ion Ratio Lower Upper

96 100

61 129.5 0.0 296.6

98 64.0 0.0 130.4

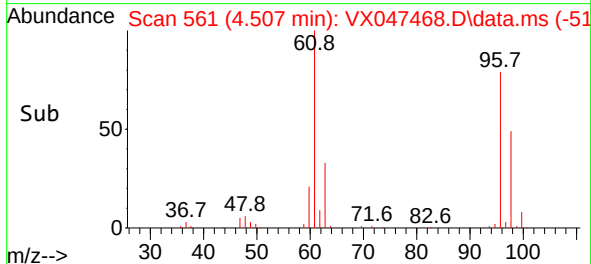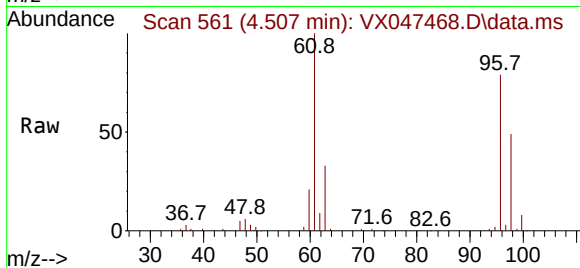

#29

Tetrahydrofuran

Concen: 0.292 ug/l

RT: 5.056 min Scan# 651

Delta R.T. 0.031 min

Lab File: VX047468.D

Acq: 21 Aug 2025 14:28




Tgt Ion: 42 Resp: 254


Ion Ratio Lower Upper

42 100

72 7.9 34.6 51.8#


71 43.7 32.6 49.0

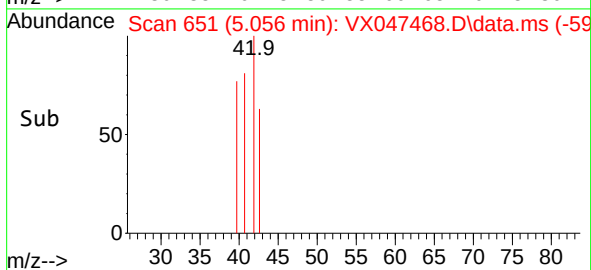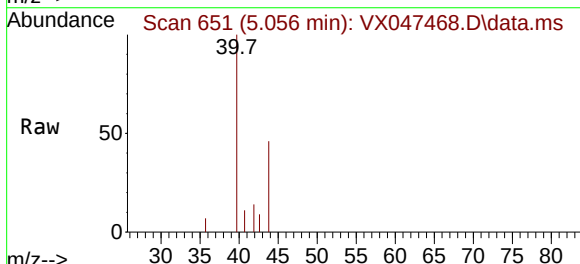






#31
Cyclohexane
Concen: 0.962 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.079 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL







Tgt Ion: 56 Resp: 4227
Ion Ratio Lower Upper
56 100
69 177.9 24.3 36.5#
84 120.4 65.3 97.9#

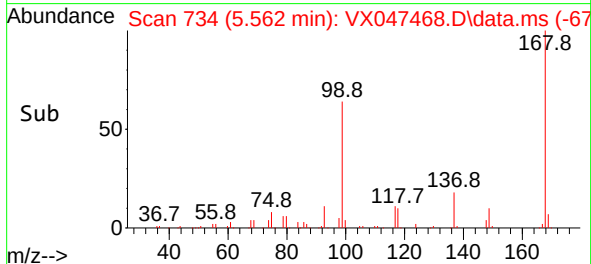

#33
1,2-Dichloroethane-d4
Concen: 53.181 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion: 65 Resp: 145202
Ion Ratio Lower Upper
65 100
67 50.6 0.0 106.0



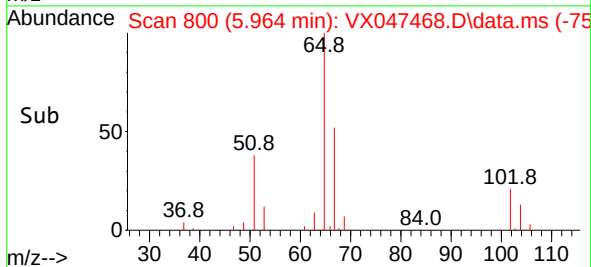
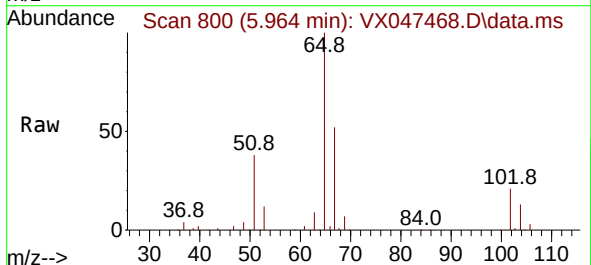




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion:114 Resp: 386665
Ion Ratio Lower Upper
114 100
63 22.1 0.0 42.4
88 17.0 0.0 33.0



#35
Dibromofluoromethane
Concen: 48.417 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion:113 Resp: 121502
Ion Ratio Lower Upper
113 100
111 103.5 81.4 122.2
192 17.8 14.1 21.1

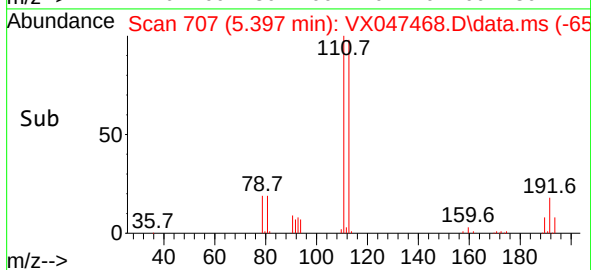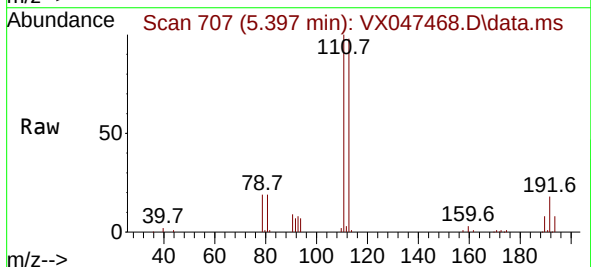



#36

1,1-Dichloropropene

Concen: 4.042 ug/l

RT: 5.562 min Scan# 71

Delta R.T. -0.146 min

Lab File: VX047468.D


Acq: 21 Aug 2025 14:28

Instrument :




MSVOA_X

ClientSampleId :

MW-11A-13.5-081325DL

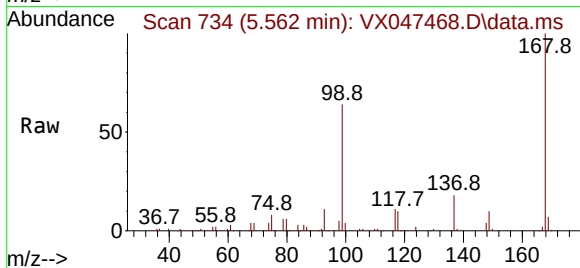

Tgt Ion: 75	Resp: 16014
Ion Ratio	Lower Upper
75	100
110	7.4 17.4 52.2#
77	0.0 24.4 36.6#

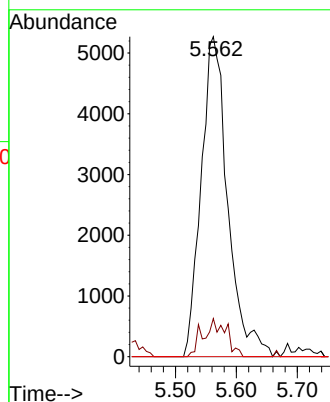

#38

Carbon Tetrachloride

Concen: 4.839 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.128 min

Lab File: VX047468.D

Acq: 21 Aug 2025 14:28

Tgt Ion: 117	Resp: 20950
Ion Ratio	Lower Upper
117	100
119	3.6 78.5 117.7#
121	0.0 24.7 37.1#



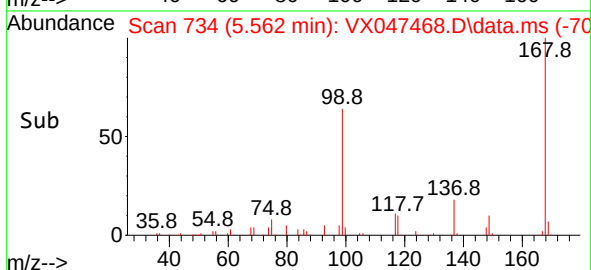
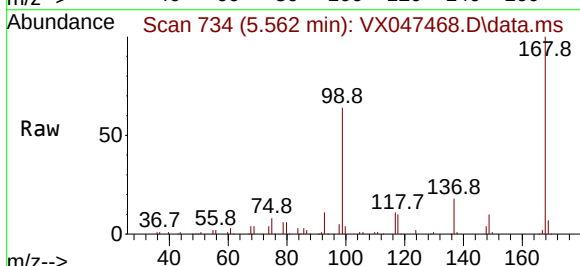


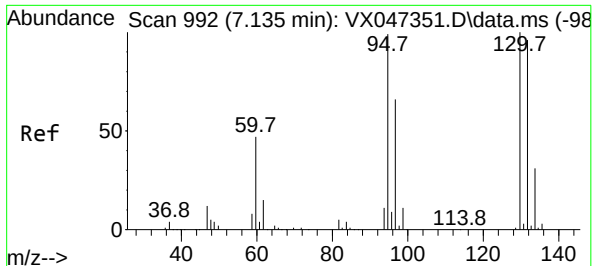

#44
Trichloroethene
Concen: 94.305 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.006 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion:130 Resp: 286321
Ion Ratio Lower Upper
130 100
95 100.7 0.0 198.6

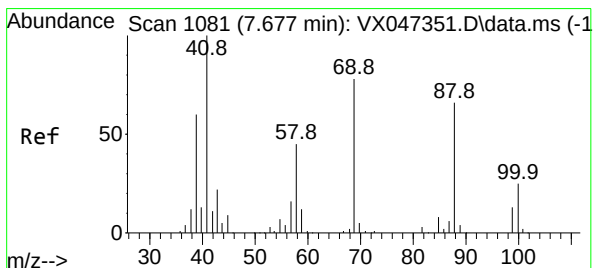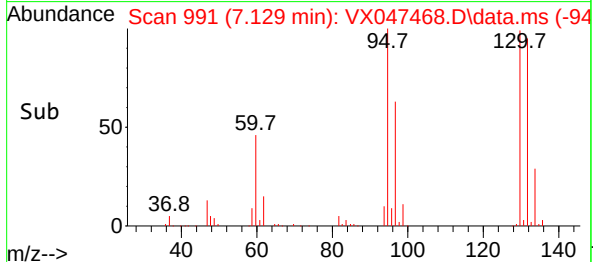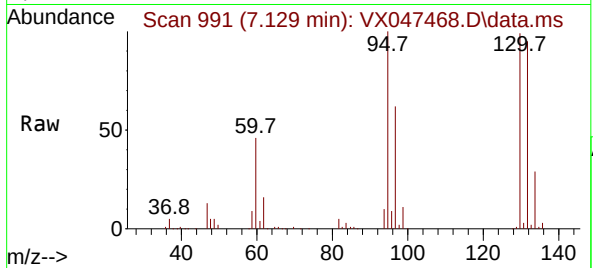

#49
1,4-Dioxane
Concen: 2.717 ug/l
RT: 7.708 min Scan# 1086
Delta R.T. 0.031 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion: 88 Resp: 81
Ion Ratio Lower Upper
88 100
43 35.8 32.4 48.6
58 0.0 56.9 85.3#


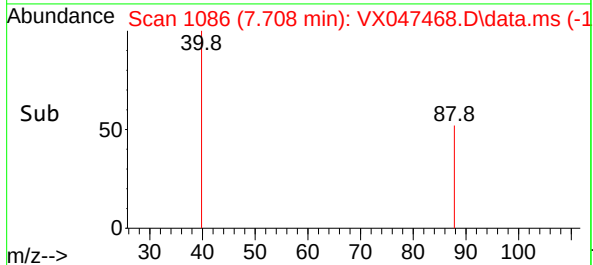

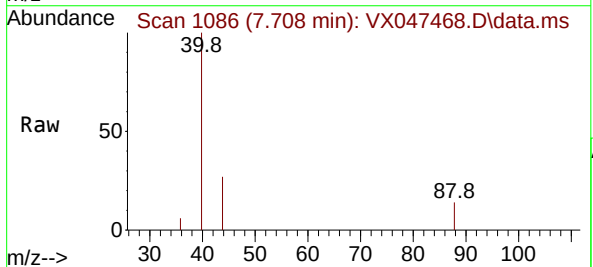


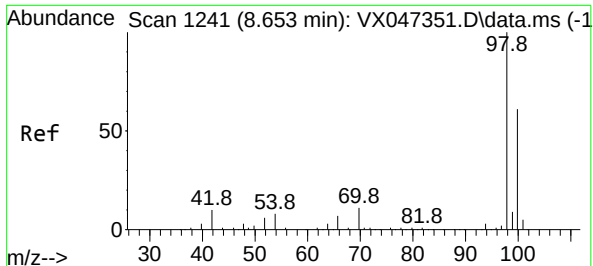

#50
Toluene-d8
Concen: 48.445 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion: 98 Resp: 434529
Ion Ratio Lower Upper
98 100
100 67.0 53.9 80.9

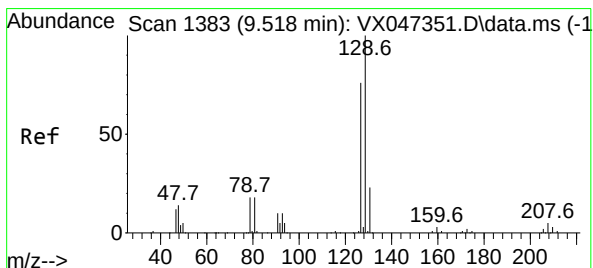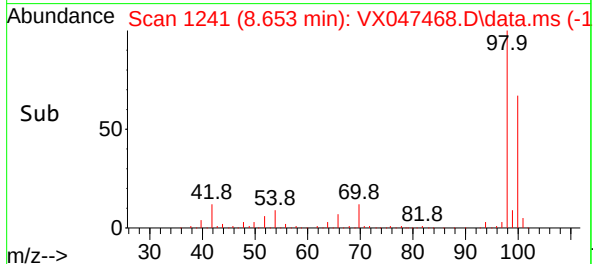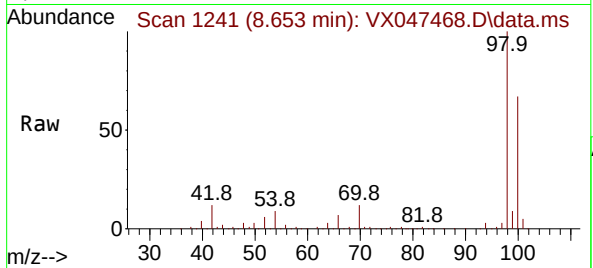

#60
Dibromochloromethane
Concen: 0.560 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.238 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion:129 Resp: 1851
Ion Ratio Lower Upper
129 100
127 0.0 38.9 116.6#


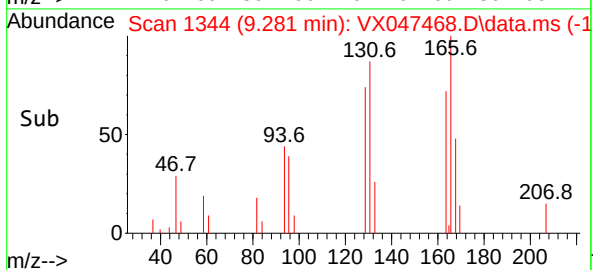

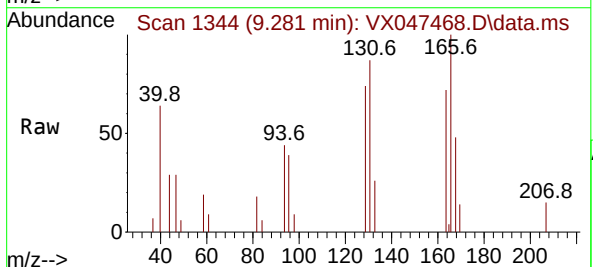




#62
4-Bromofluorobenzene
Concen: 53.059 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion: 95 Resp: 175623
Ion Ratio Lower Upper
95 100
174 72.3 0.0 148.0
176 70.7 0.0 145.4

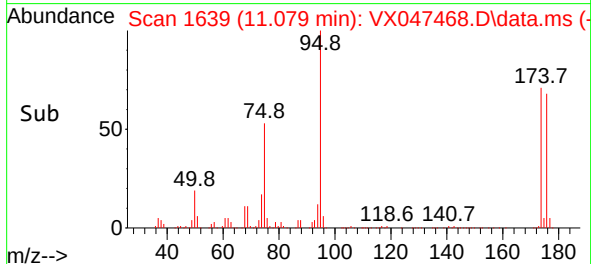

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion: 117 Resp: 376333
Ion Ratio Lower Upper
117 100
82 56.4 45.0 67.4
119 32.7 25.8 38.8

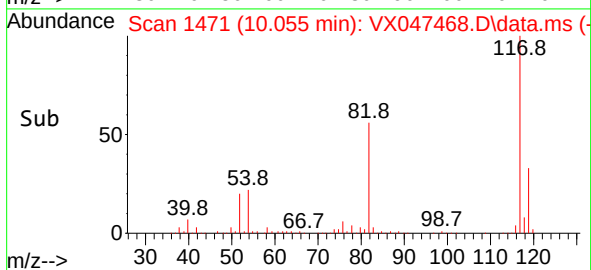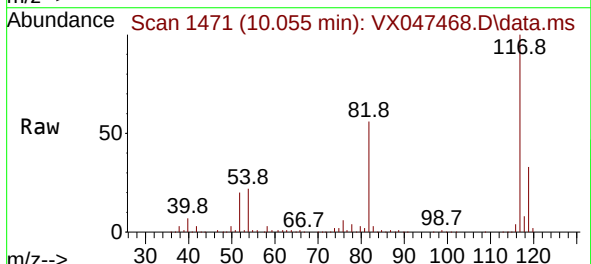







#64
Tetrachloroethene
Concen: 0.659 ug/l
RT: 9.275 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL

Tgt Ion:164 Resp: 1793




Ion	Ratio	Lower	Upper
164	100		
166	132.4	100.3	150.5
129	91.4	77.7	116.5
131	90.5	74.8	112.2

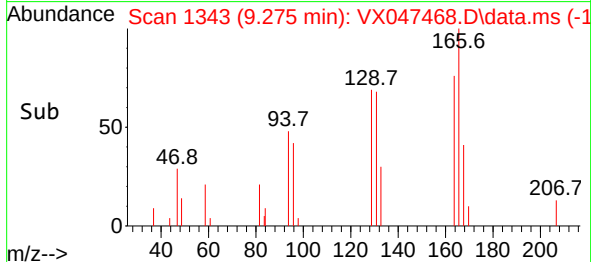


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion:152 Resp: 185836

Ion	Ratio	Lower	Upper
152	100		
115	61.2	44.6	133.8
150	155.6	0.0	349.8

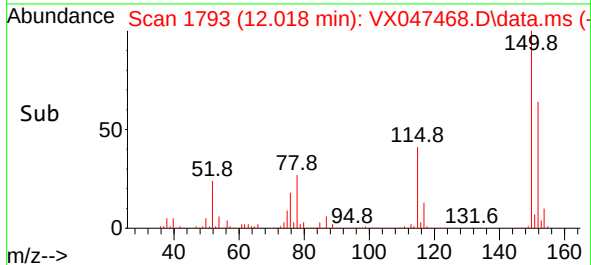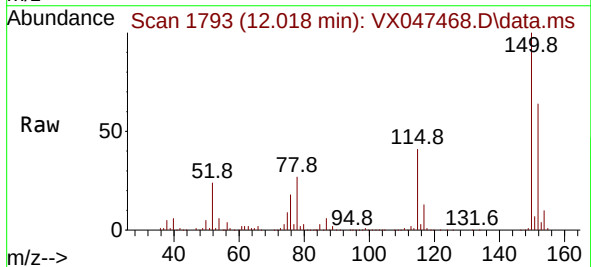



#76

1,2,3-Trichloropropane

Concen: 26.868 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX047468.D

Acq: 21 Aug 2025 14:28

Instrument :

MSVOA_X

ClientSampleId :





MW-11A-13.5-081325DL

Tgt Ion: 75 Resp: 91579

Ion Ratio Lower Upper

75 100

77 1.2 19.4 58.2#

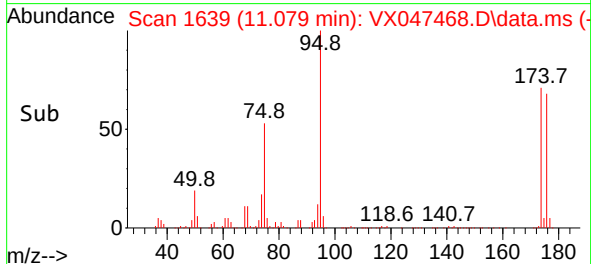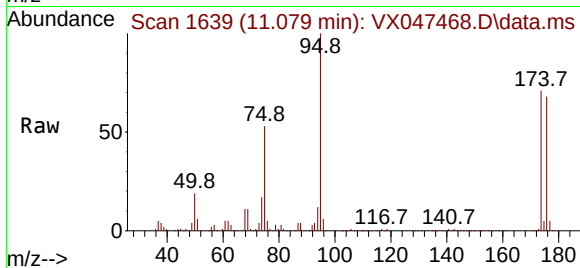

#81

trans-1,4-Dichloro-2-butene

Concen: 106.285 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX047468.D

Acq: 21 Aug 2025 14:28




Tgt Ion: 75 Resp: 91579


Ion Ratio Lower Upper

75 100

53 0.0 85.2 127.8#

89 0.0 36.7 55.1#


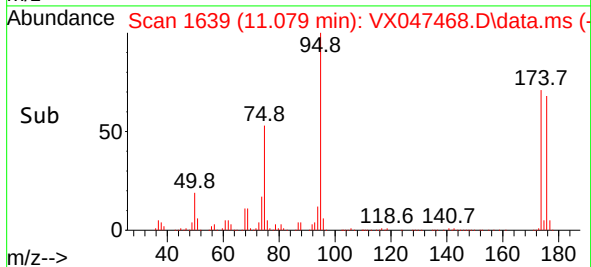

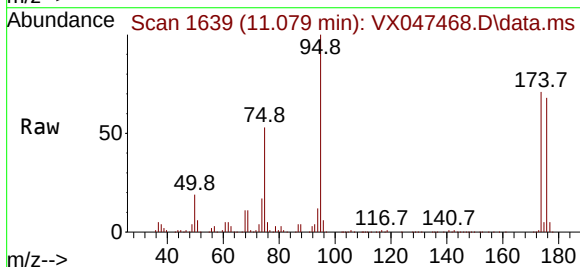




#89
n-Butylbenzene
Concen: 0.229 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.006 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion:	91	Resp:	2666
Ion	Ratio	Lower	Upper
91	100		
92	55.9	27.2	81.5
134	24.0	12.6	37.8

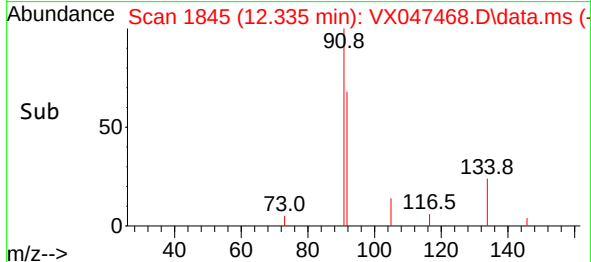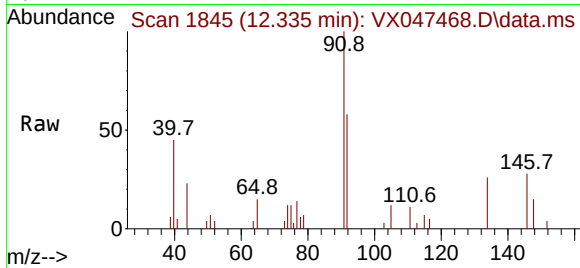

#93
1,2,4-Trichlorobenzene
Concen: 0.354 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28

Tgt Ion:	180	Resp:	1530
Ion	Ratio	Lower	Upper
180	100		
182	99.4	48.1	144.4
145	30.1	16.2	48.5


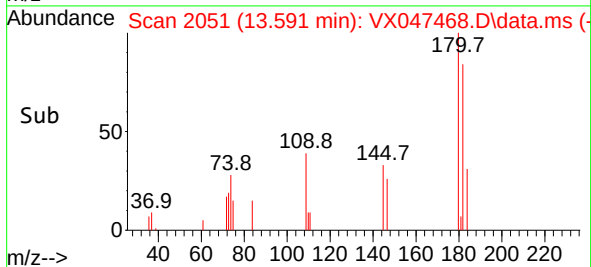

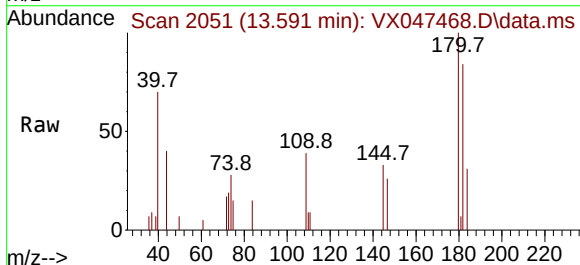




#94
Hexachlorobutadiene
Concen: 1.076 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. 0.000 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28




Instrument :
MSVOA_X
ClientSampleId :
MW-11A-13.5-081325DL


Tgt Ion:	225	Resp:	1654
Ion	Ratio	Lower	Upper
225	100		
223	54.5	32.2	96.6
227	69.6	31.6	95.0

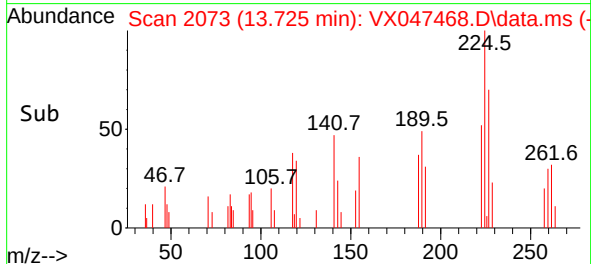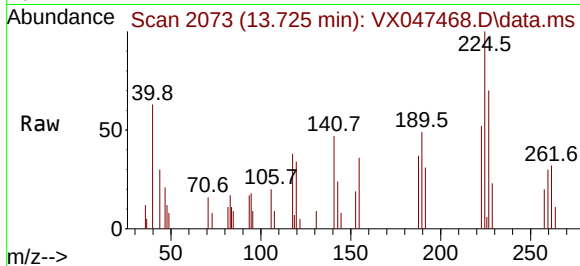

#95
Naphthalene
Concen: 1.111 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX047468.D
Acq: 21 Aug 2025 14:28


Tgt Ion:	128	Resp:	13704
Ion	Ratio	Lower	Upper
128	100		
127	14.4	10.1	15.1
129	10.0	8.7	13.1

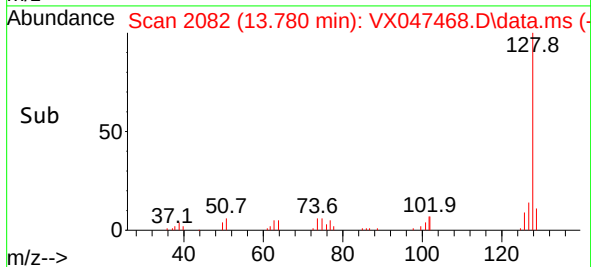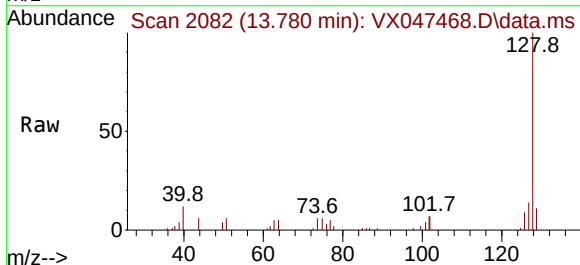



#96
 1,2,3-Trichlorobenzene
 Concen: 0.380 ug/l
 RT: 13.963 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX047468.D
 Acq: 21 Aug 2025 14:28

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11A-13.5-081325DL

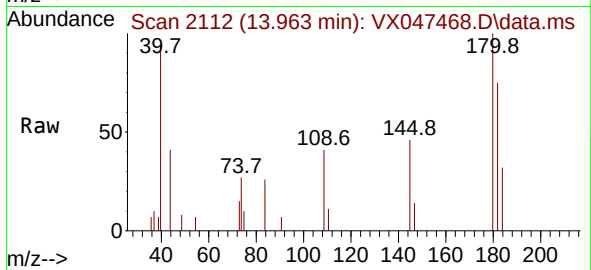

Tgt Ion	Ratio	Lower	Upper
180	100		
182	100.7	48.0	144.2
145	34.5	17.4	52.2

