


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX082218\
Data File : VX004189.D
Acq On : 22 Aug 2018 09:48
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Title : SW846 8260
Last Update : Mon Aug 13 01:34:27 2018

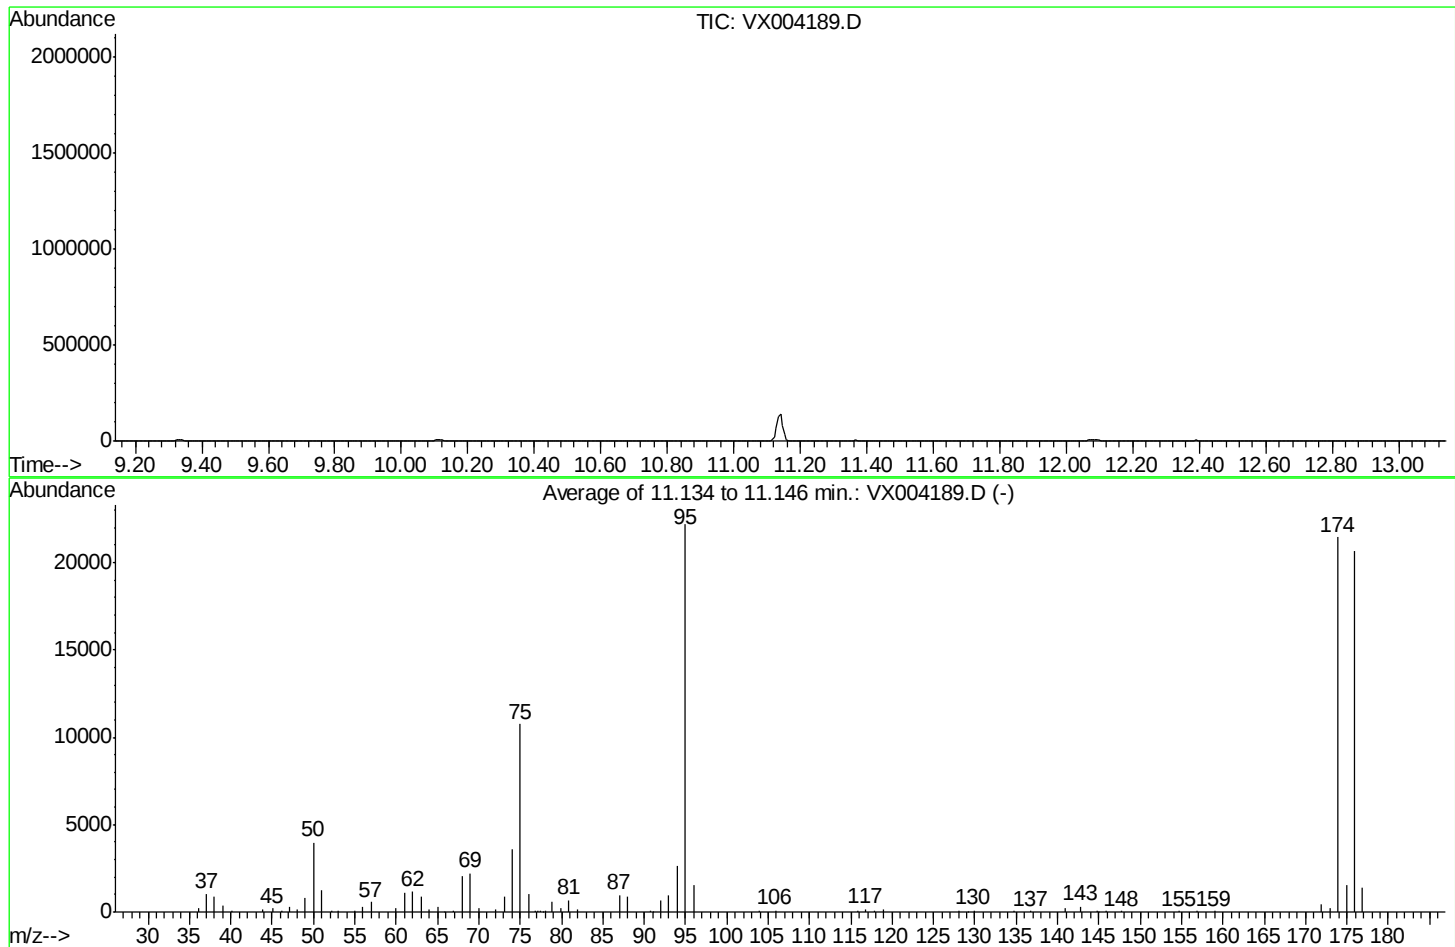

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	3975	PASS
75	95	30	60	48.4	10737	PASS
95	95	100	100	100.0	22185	PASS
96	95	5	9	7.0	1551	PASS
173	174	0.00	2	1.2	247	PASS
174	95	50	100	96.7	21456	PASS
175	174	5	9	7.3	1569	PASS
176	174	95	101	96.2	20636	PASS
177	176	5	9	6.6	1359	PASS