


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082219\
 Data File : VX011755.D
 Acq On : 22 Aug 2019 12:01
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082219W.M
 Title : SW846 8260
 Last Update : Fri Aug 23 01:48:12 2019

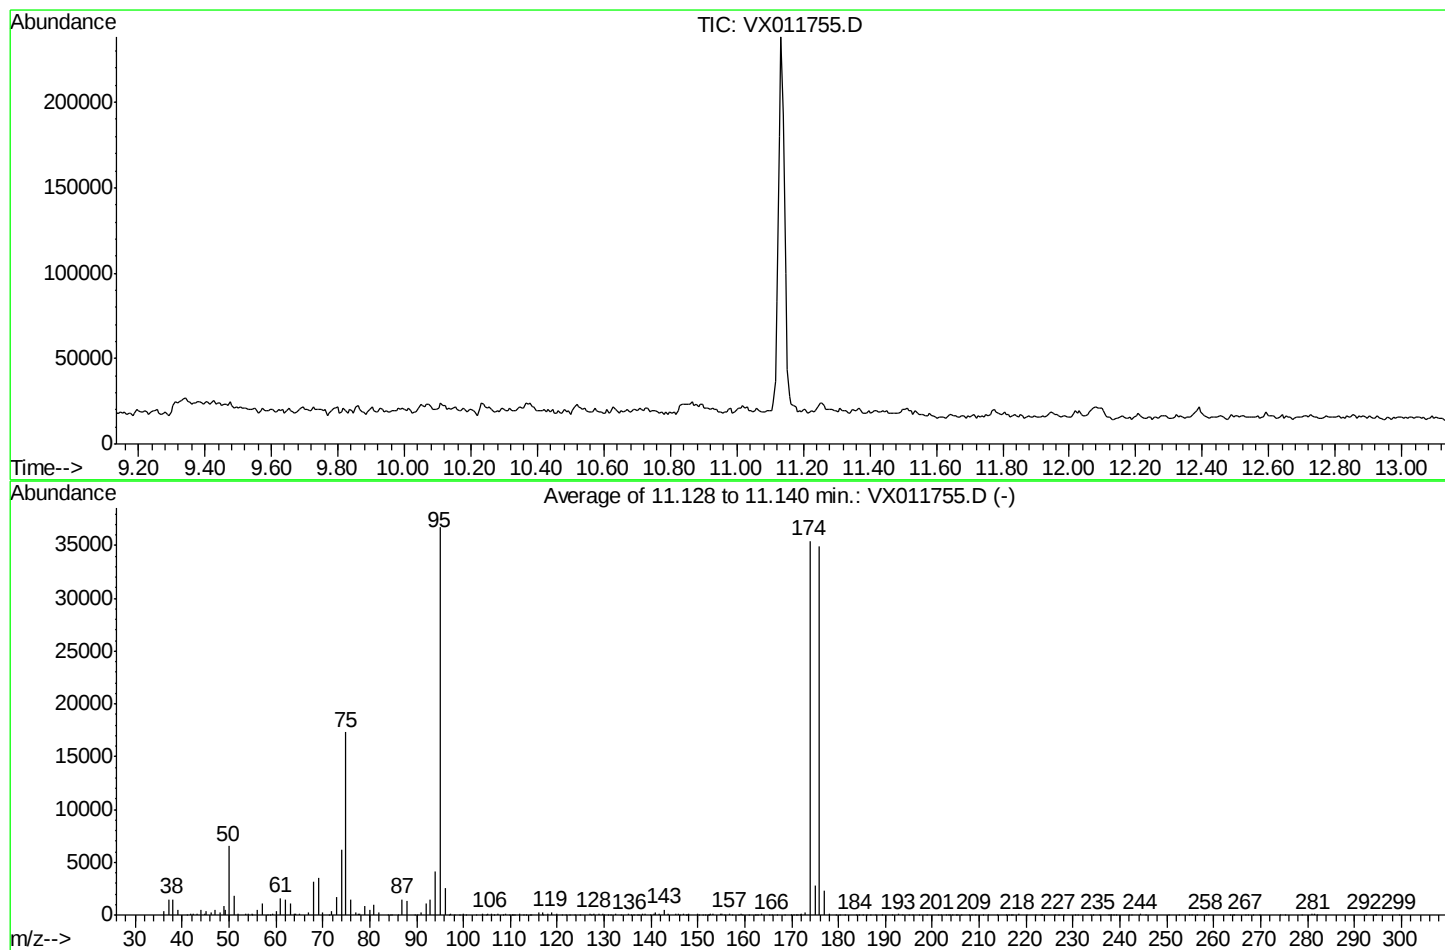

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	6512	PASS
75	95	30	60	47.1	17300	PASS
95	95	100	100	100.0	36728	PASS
96	95	5	9	7.0	2561	PASS
173	174	0.00	2	0.6	205	PASS
174	95	50	100	96.4	35421	PASS
175	174	5	9	7.8	2771	PASS
176	174	95	101	98.5	34888	PASS
177	176	5	9	6.6	2311	PASS