

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082221\
 Data File : VX023887.D
 Acq On : 20 Aug 2021 19:08
 Operator : JC/MD
 Sample : M3511-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M

Title : SW846 8260

Signal : TIC: VX023887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	24	27	34	rVB	74284	69711	8.91%	1.666%
2	1.568	71	79	83	rVB2	5003	9436	1.21%	0.226%
3	2.550	230	240	248	rBV	15070	27871	3.56%	0.666%
4	5.397	695	707	719	rBV	90556	261675	33.44%	6.255%
5	5.562	722	734	749	rVB	147508	416086	53.17%	9.946%
6	5.964	790	800	813	rBV	101488	268206	34.28%	6.411%
7	6.769	921	932	947	rBV	239189	564867	72.19%	13.503%
8	8.653	1234	1241	1252	rBV	518711	782503	100.00%	18.705%
9	10.055	1465	1471	1480	rBV	499718	693372	88.61%	16.575%
10	11.085	1634	1640	1652	rVB	413580	514817	65.79%	12.306%
11	12.024	1788	1794	1806	rBV	481759	574755	73.45%	13.739%




Sum of corrected areas: 4183299

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082221\
Data File : VX023887.D
Acq On : 20 Aug 2021 19:08
Operator : JC/MD
Sample : M3511-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

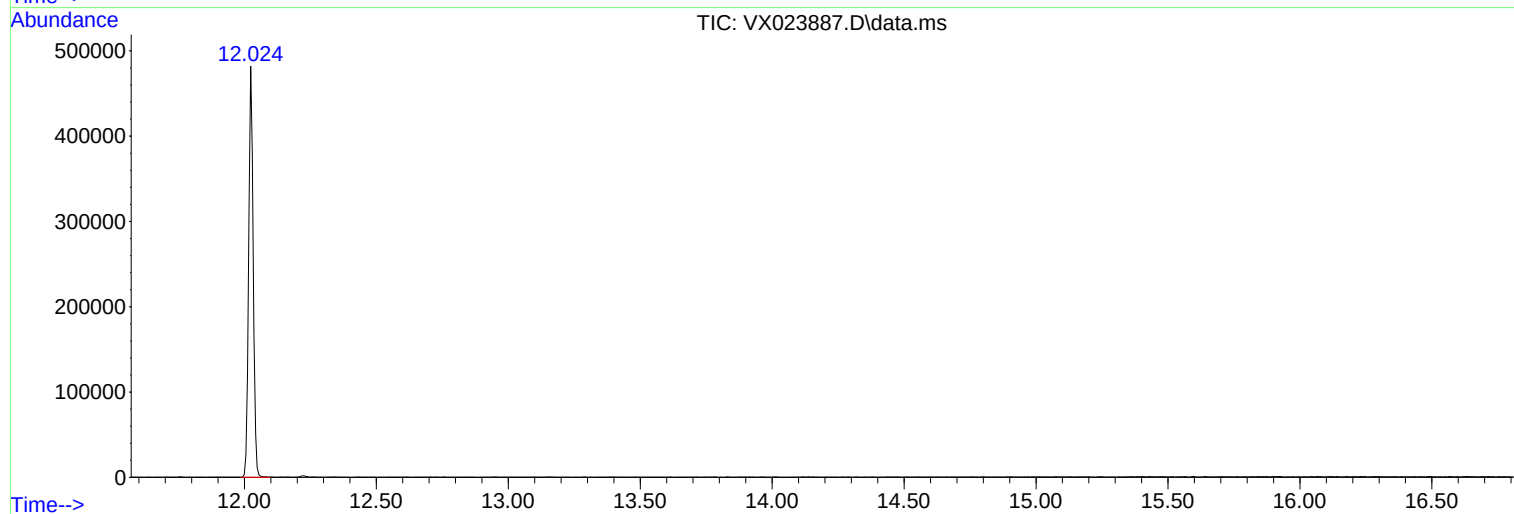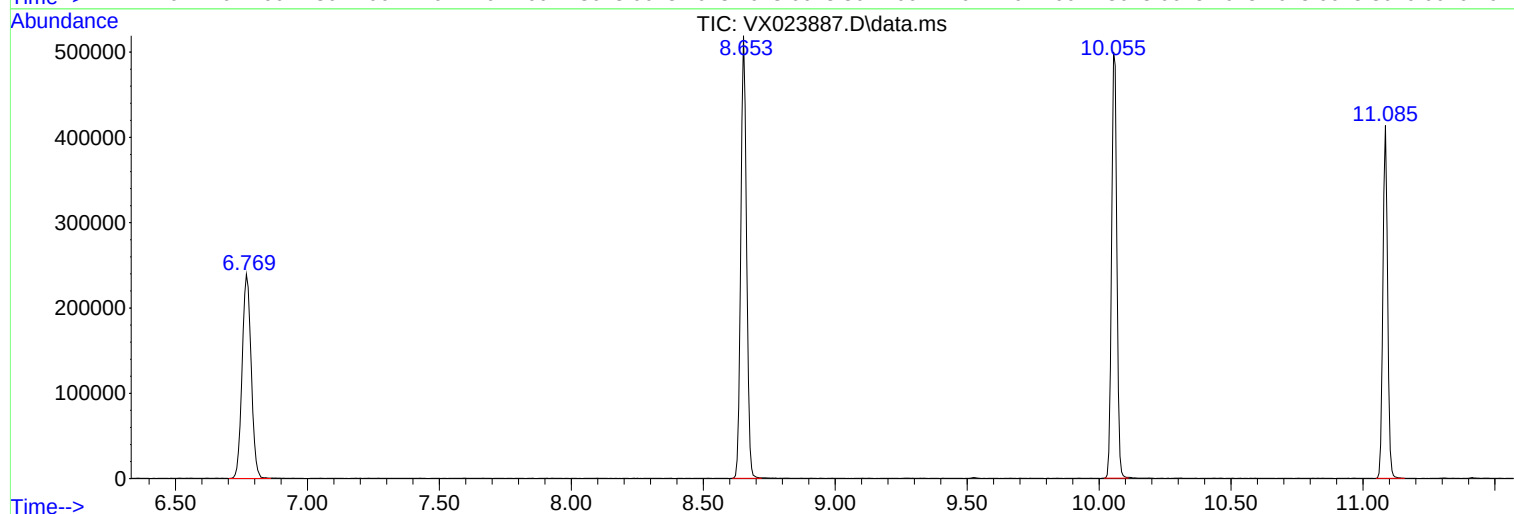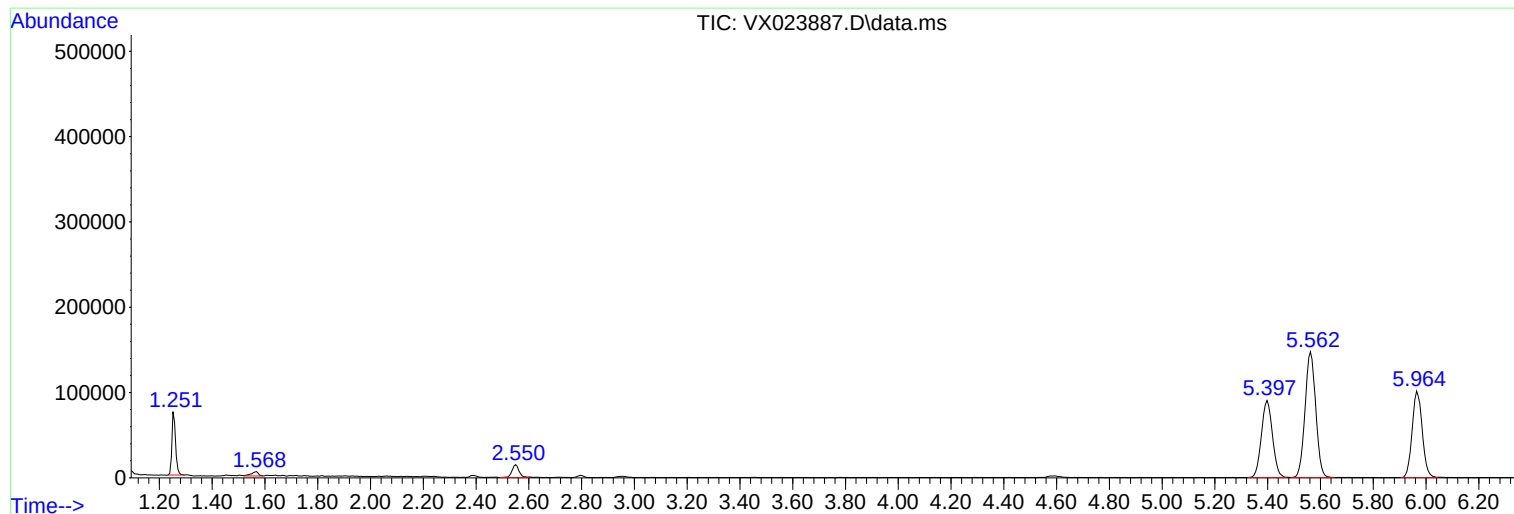

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082221\
Data File : VX023887.D
Acq On : 20 Aug 2021 19:08
Operator : JC/MD
Sample : M3511-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082221\
Data File : VX023887.D
Acq On : 20 Aug 2021 19:08
Operator : JC/MD
Sample : M3511-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
