

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082221\
 Data File : VX023895.D
 Acq On : 20 Aug 2021 22:16
 Operator : JC/MD
 Sample : M3479-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 210818092-02-VOA

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX023895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.392	205	214	226	rBV2	86102	163889	1.84%	0.495%
2	2.983	296	311	327	rBV	3978786	8887624	100.00%	26.853%
3	4.611	561	578	605	rBV	2664284	8814619	99.18%	26.633%
4	4.910	617	627	634	rBV2	83586	241931	2.72%	0.731%
5	5.013	634	644	663	rVB	1343681	4042419	45.48%	12.214%
6	5.964	790	800	809	rBV	90867	238487	2.68%	0.721%
7	6.099	809	822	830	rVV7	27262	128393	1.44%	0.388%
8	6.245	838	846	856	rVB	71525	197437	2.22%	0.597%
9	6.769	920	932	946	rVB	199319	474855	5.34%	1.435%
10	7.909	1112	1119	1125	rBV2	48222	90222	1.02%	0.273%
11	8.653	1234	1241	1247	rBV	415887	653532	7.35%	1.975%
12	8.720	1247	1252	1261	rVB2	78018	127468	1.43%	0.385%
13	8.805	1261	1266	1271	rBV	91801	143030	1.61%	0.432%
14	9.378	1352	1360	1366	rBV	120992	184356	2.07%	0.557%
15	10.055	1459	1471	1476	rBV	416829	622374	7.00%	1.880%
16	10.305	1503	1512	1518	rVV	156811	249937	2.81%	0.755%
17	10.646	1563	1568	1580	rBV	89957	144012	1.62%	0.435%
18	11.085	1634	1640	1646	rBV	338340	465836	5.24%	1.407%
19	11.482	1698	1705	1707	rVV3	65196	116855	1.31%	0.353%
20	11.890	1769	1772	1776	rVB	90446	110158	1.24%	0.333%
21	11.951	1777	1782	1788	rBV2	106072	149817	1.69%	0.453%
22	12.427	1854	1860	1864	rBV	131211	168555	1.90%	0.509%
23	12.524	1872	1876	1882	rBV4	90885	154137	1.73%	0.466%
24	12.579	1882	1885	1889	rVB	114510	129690	1.46%	0.392%
25	12.768	1908	1916	1921	rBV	433911	608391	6.85%	1.838%
26	12.908	1928	1939	1943	rBV	1076599	1441431	16.22%	4.355%
27	12.945	1943	1945	1946	rVV	127624	124158	1.40%	0.375%
28	12.969	1946	1949	1958	rVB	186233	284909	3.21%	0.861%
29	13.268	1995	1998	2001	rBV	84985	108758	1.22%	0.329%
30	13.384	2008	2017	2020	rBV3	57931	106525	1.20%	0.322%
31	13.426	2020	2024	2028	rVV3	71331	103776	1.17%	0.314%
32	13.475	2028	2032	2035	rVV2	277905	394135	4.43%	1.191%
33	13.512	2035	2038	2046	rVB	244200	312712	3.52%	0.945%
34	13.591	2046	2051	2060	rBV2	356048	513416	5.78%	1.551%
35	13.774	2077	2081	2088	rVB2	340504	458886	5.16%	1.386%
36	13.926	2101	2106	2109	rVV4	60724	129057	1.45%	0.390%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082221\
Data File : VX023895.D
Acq On : 20 Aug 2021 22:16
Operator : JC/MD
Sample : M3479-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210818092-02-VOA

Integration Parameters: RTEINT3.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

37	14.237	2151	2157	2165	rBV4	47564	94090	1.06%	0.284%
38	14.317	2166	2170	2175	rVV3	68102	92018	1.04%	0.278%
39	14.414	2182	2186	2194	rBV2	45079	114775	1.29%	0.347%
40	14.609	2214	2218	2220	rBV2	72669	99577	1.12%	0.301%
41	14.640	2220	2223	2231	rVB	303075	400376	4.50%	1.210%
42	14.719	2231	2236	2240	rBV	430634	555694	6.25%	1.679%
43	14.762	2240	2243	2244	rVV	104046	132951	1.50%	0.402%
44	14.780	2244	2246	2254	rVB	264227	321646	3.62%	0.972%




Sum of corrected areas: 33096914

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082221\
Data File : VX023895.D
Acq On : 20 Aug 2021 22:16
Operator : JC/MD
Sample : M3479-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210818092-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

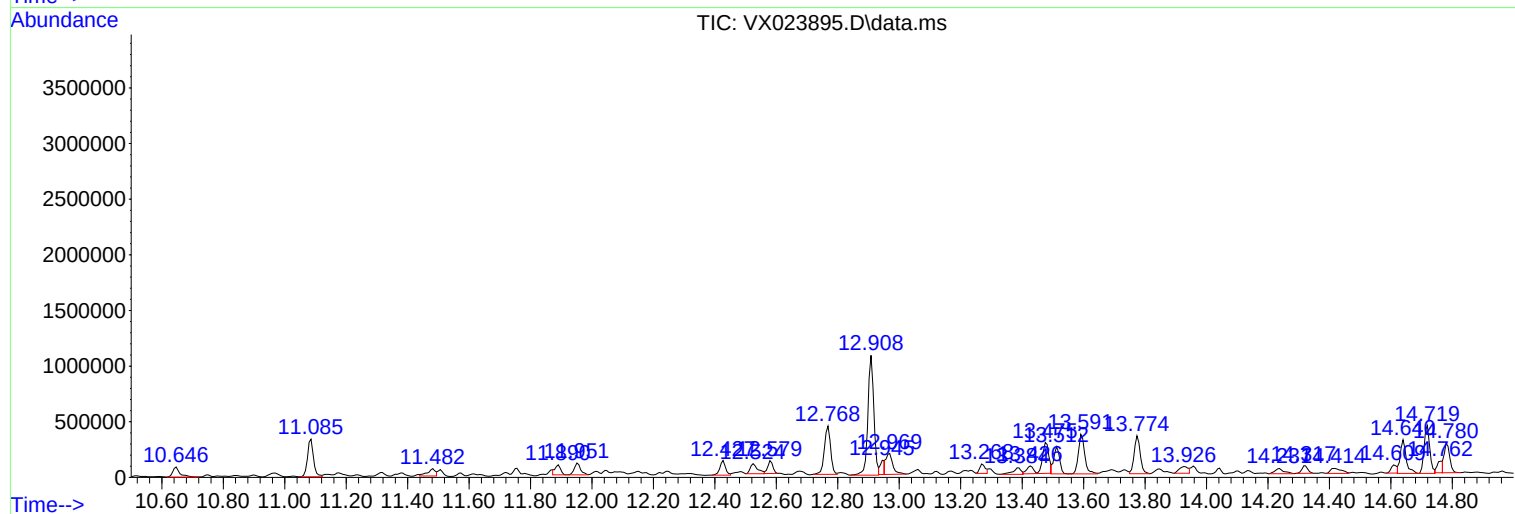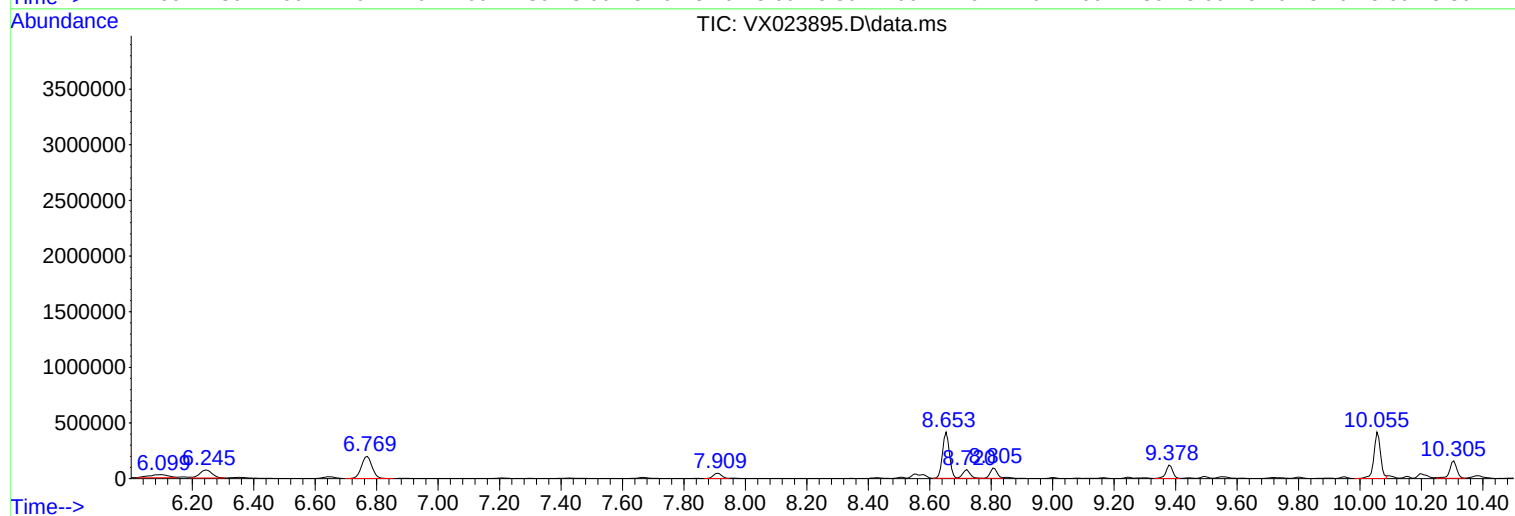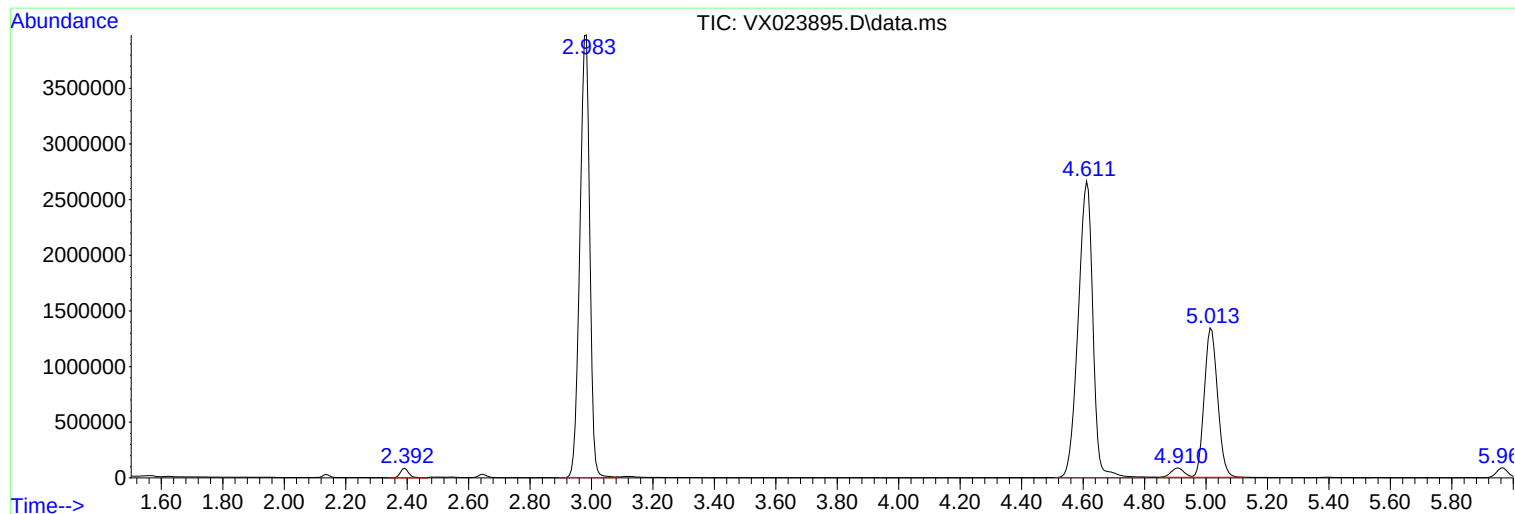

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082221\
Data File : VX023895.D
Acq On : 20 Aug 2021 22:16
Operator : JC/MD
Sample : M3479-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210818092-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082221\
Data File : VX023895.D
Acq On : 20 Aug 2021 22:16
Operator : JC/MD
Sample : M3479-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210818092-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------