

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030708.D
 Acq On : 22 Aug 2022 11:29
 Operator : JC/MD
 Sample : VX0822MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK694

Quant Time: Aug 23 02:06:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 23 02:05:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	321554	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	286478	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	132682	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	85581	41.444	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	82.880%		
7) Chloroethane-d5	1.666	69	68326	46.937	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.880%		
11) 1,1-Dichloroethene-d2	2.307	63	128846	32.986	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.980%		
21) 2-Butanone-d5	4.459	46	171341	89.553	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.550%		
24) Chloroform-d	5.056	84	191001	44.933	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.860%		
26) 1,2-Dichloroethane-d4	5.952	65	120394	41.712	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.420%		
32) Benzene-d6	5.971	84	395847	48.238	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.480%		
36) 1,2-Dichloropropane-d6	7.312	67	130508	49.019	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.040%		
41) Toluene-d8	8.647	98	353777	45.736	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.480%		
43) trans-1,3-Dichloroprop...	8.952	79	59466	44.897	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.800%		
47) 2-Hexanone-d5	9.385	63	129740	95.602	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	95.600%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	185147	52.936	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	105.880%		
66) 1,2-Dichlorobenzene-d4	12.323	152	129909	50.479	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.960%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	8.946	75	2944	0.826	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030708.D
Acq On : 22 Aug 2022 11:29
Operator : JC/MD
Sample : VX0822MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK694

Quant Time: Aug 23 02:06:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 23 02:05:32 2022
Response via : Initial Calibration

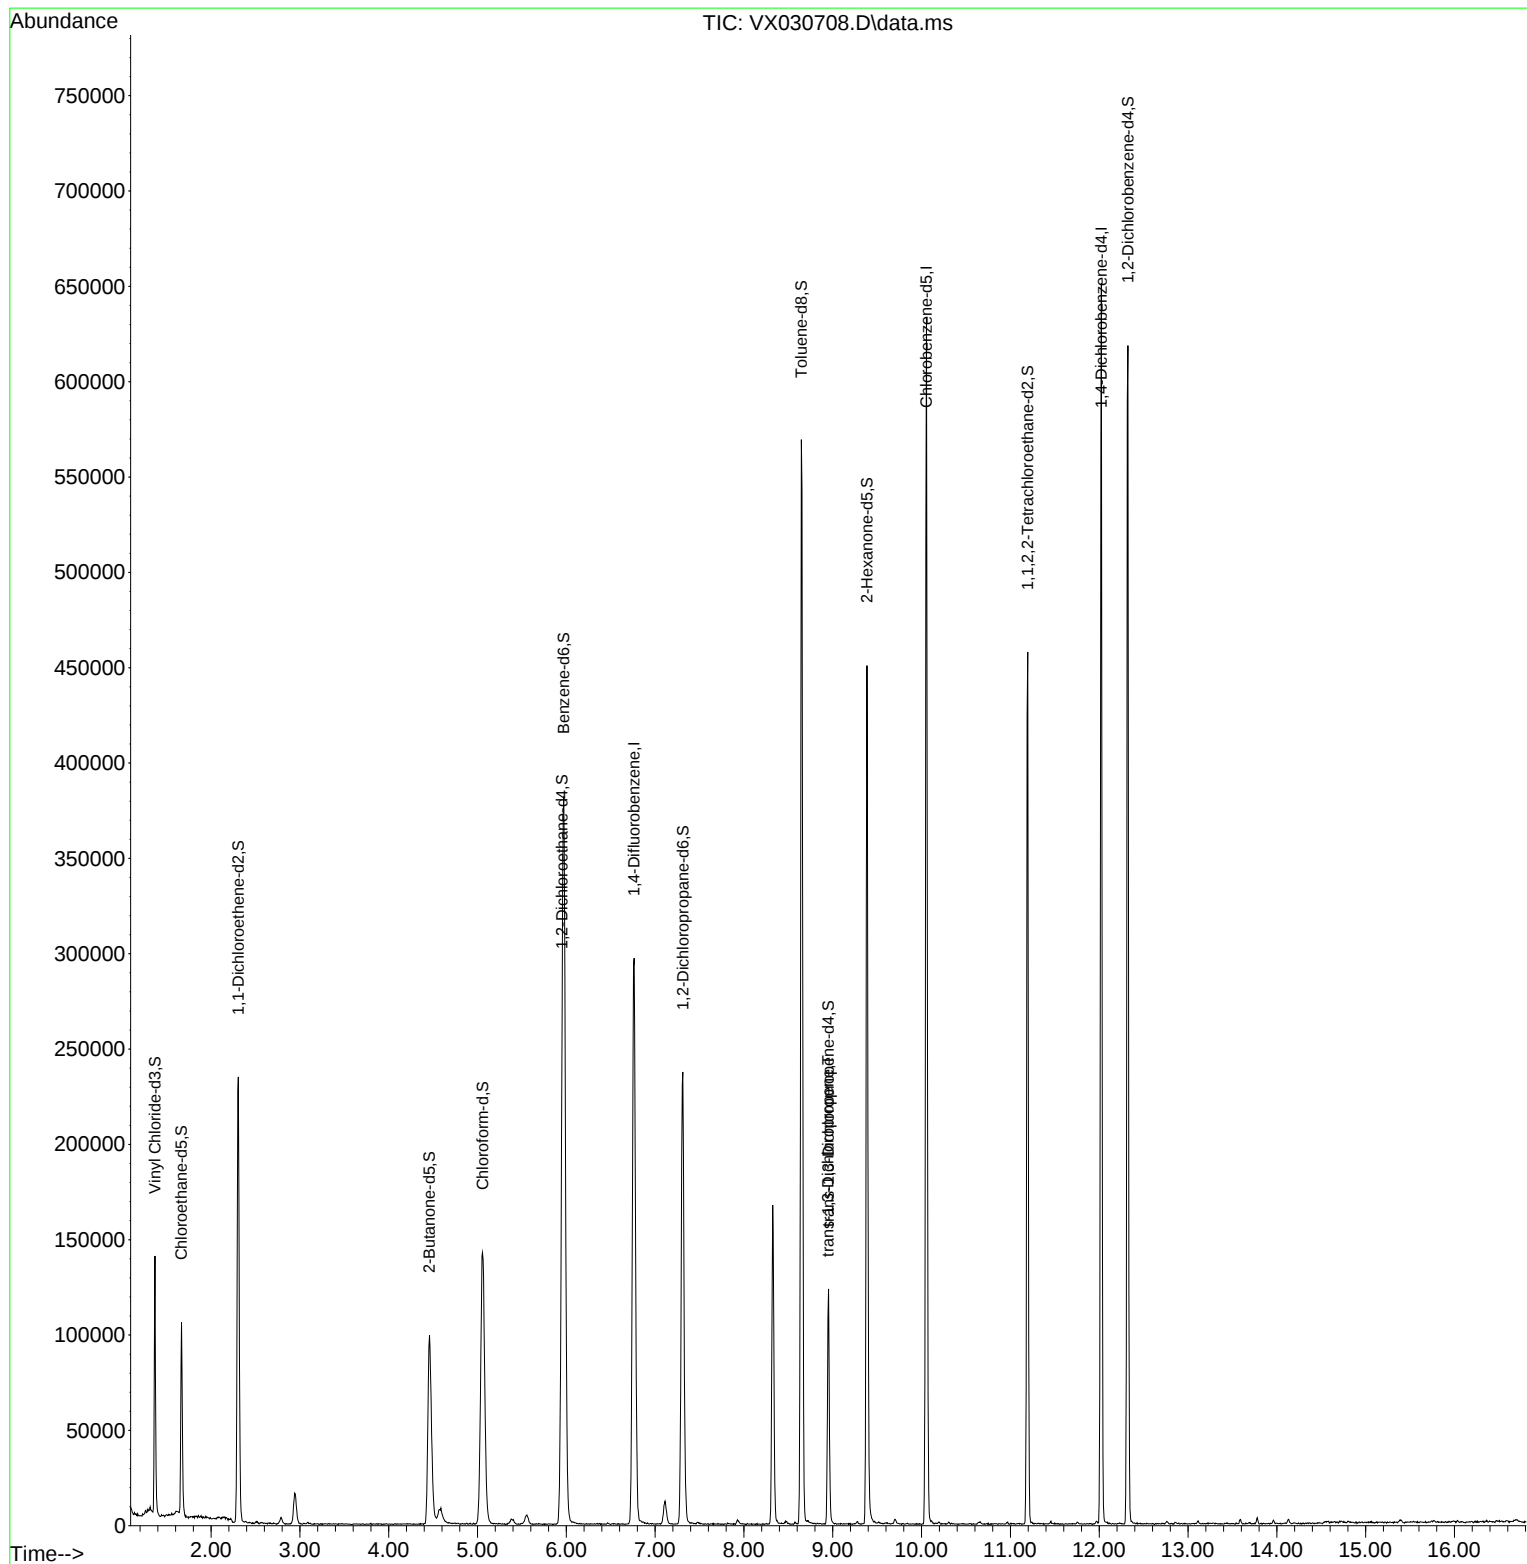

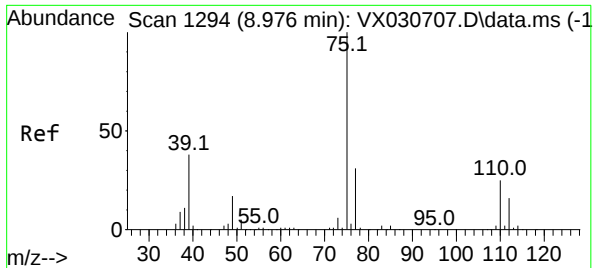

#44
 trans-1,3-Dichloropropene
 Concen: 0.826 ug/L
 RT: 8.946 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VX030708.D
 Acq: 22 Aug 2022 11:29

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK694

Tgt Ion: 75 Resp: 2944
 Ion Ratio Lower Upper
 75 100
 77 25.7 22.5 41.7

