

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030714.D
 Acq On : 22 Aug 2022 14:46
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK675

Quant Time: Aug 23 02:07:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 23 02:05:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	284335	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	265935	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	121329	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	70086	38.383	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.760%		
7) Chloroethane-d5	1.666	69	50681	39.373	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	78.740%		
11) 1,1-Dichloroethene-d2	2.300	63	107261	31.054	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.100%		
21) 2-Butanone-d5	4.471	46	172209	101.788	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.790%		
24) Chloroform-d	5.056	84	182943	48.671	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.340%		
26) 1,2-Dichloroethane-d4	5.952	65	118501	46.431	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.860%		
32) Benzene-d6	5.977	84	367288	48.216	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.440%		
36) 1,2-Dichloropropane-d6	7.306	67	126509	51.187	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.380%		
41) Toluene-d8	8.647	98	321225	44.736	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.480%		
43) trans-1,3-Dichloroprop...	8.952	79	55982	45.532	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.060%		
47) 2-Hexanone-d5	9.385	63	130292	103.426	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	103.430%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	182638	56.253	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	112.500%		
66) 1,2-Dichlorobenzene-d4	12.323	152	123696	52.563	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.120%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	8.952	75	2375	0.718	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030714.D
Acq On : 22 Aug 2022 14:46
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK675

Quant Time: Aug 23 02:07:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 23 02:05:32 2022
Response via : Initial Calibration

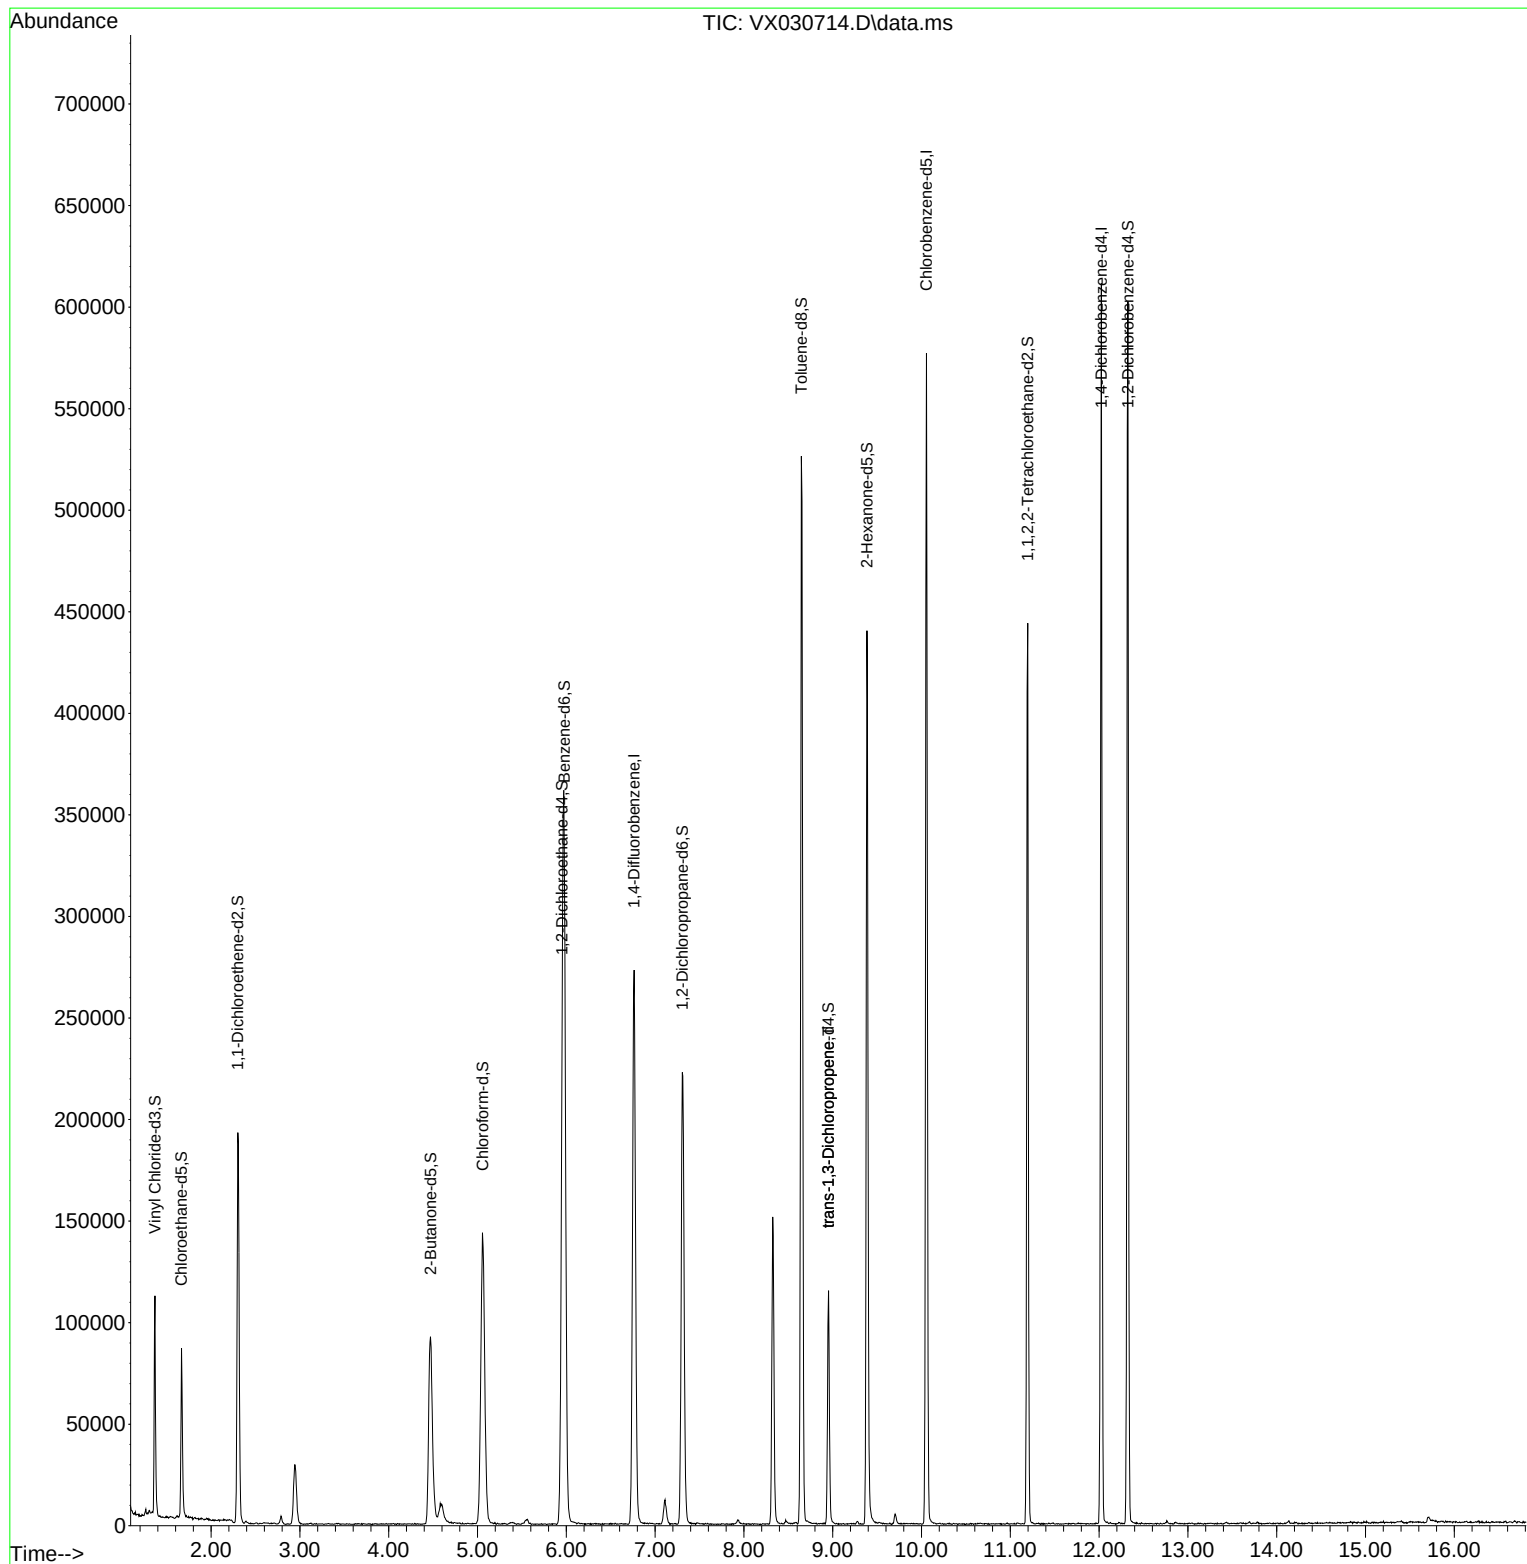

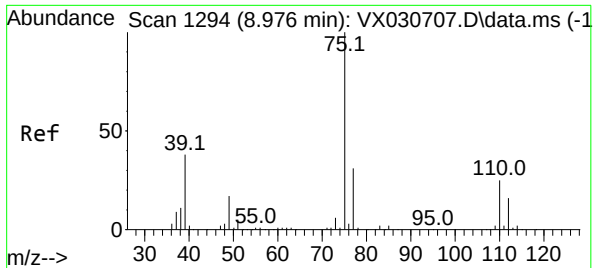

#44
 trans-1,3-Dichloropropene
 Concen: 0.718 ug/L
 RT: 8.952 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VX030714.D
 Acq: 22 Aug 2022 14:46

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK675

Tgt Ion: 75 Resp: 2375
 Ion Ratio Lower Upper
 75 100
 77 40.1 22.5 41.7

