

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030708.D
 Acq On : 22 Aug 2022 11:29
 Operator : JC/MD
 Sample : VX0822MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK694

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	136654	141006	12.55%	1.589%
2	1.666	91	95	102	rVB	101974	128328	11.42%	1.446%
3	2.307	194	200	211	rVB	233479	364437	32.44%	4.107%
4	2.654	254	257	258	rBV2	543	570	0.05%	0.006%
5	2.703	263	265	270	rVB2	708	892	0.08%	0.010%
6	2.788	270	279	287	rVB5	3625	7633	0.68%	0.086%
7	2.941	296	304	313	rBV	16278	37635	3.35%	0.424%
8	3.087	325	328	330	rVV2	758	756	0.07%	0.009%
9	3.233	349	352	353	rBV	450	405	0.04%	0.005%
10	3.825	447	449	453	rBV2	368	610	0.05%	0.007%
11	3.861	453	455	458	rVB2	397	354	0.03%	0.004%
12	3.971	471	473	477	rVV2	442	476	0.04%	0.005%
13	4.282	523	524	528	rBV2	341	393	0.03%	0.004%
14	4.398	542	543	544	rBV	509	354	0.03%	0.004%
15	4.459	544	553	566	rBV	98661	281172	25.03%	3.169%
16	4.879	620	622	624	rVB2	541	512	0.05%	0.006%
17	4.916	626	628	633	rVB3	622	624	0.06%	0.007%
18	4.952	633	634	636	rBV2	571	356	0.03%	0.004%
19	5.056	639	651	669	rVV2	142238	456786	40.66%	5.148%
20	5.343	697	698	699	rBV	597	397	0.04%	0.004%
21	5.379	699	704	707	rBV3	2273	4112	0.37%	0.046%
22	5.556	724	733	742	rVV5	4885	13432	1.20%	0.151%
23	5.690	753	755	759	rVV2	441	367	0.03%	0.004%
24	5.751	762	765	766	rVB2	431	373	0.03%	0.004%
25	5.769	766	768	770	rBV2	472	460	0.04%	0.005%
26	5.861	781	783	784	rBV	373	366	0.03%	0.004%
27	5.971	787	801	816	rBV2	381796	1123527	100.00%	12.662%
28	6.373	865	867	869	rVB2	514	421	0.04%	0.005%
29	6.464	879	882	888	rVB2	806	1110	0.10%	0.013%
30	6.525	888	892	893	rBV2	434	547	0.05%	0.006%
31	6.763	920	931	942	rBV	296614	719030	64.00%	8.103%
32	6.915	954	956	959	rVB	706	586	0.05%	0.007%
33	6.946	959	961	963	rBV2	377	364	0.03%	0.004%
34	7.111	980	988	999	rBV6	12048	29262	2.60%	0.330%
35	7.312	1011	1021	1036	rBV	237129	518145	46.12%	5.839%
36	7.476	1046	1048	1053	rVB4	950	1437	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030708.D
 Acq On : 22 Aug 2022 11:29
 Operator : JC/MD
 Sample : VX0822MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK694

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.562	1060	1062	1065	rBV2	354	353	0.03%	0.004%
38	7.671	1078	1080	1082	rBV2	480	595	0.05%	0.007%
39	7.818	1102	1104	1105	rBV	651	404	0.04%	0.005%
40	7.927	1118	1122	1129	rBV5	2428	4719	0.42%	0.053%
41	8.037	1138	1140	1142	rBV	593	516	0.05%	0.006%
42	8.147	1156	1158	1159	rBV	538	352	0.03%	0.004%
43	8.324	1180	1187	1198	rVV	167247	273201	24.32%	3.079%
44	8.470	1207	1211	1215	rVV4	1489	2055	0.18%	0.023%
45	8.574	1225	1228	1232	rBV3	1247	1426	0.13%	0.016%
46	8.647	1234	1240	1250	rBV	568488	904293	80.49%	10.191%
47	8.830	1267	1270	1273	rBV2	457	428	0.04%	0.005%
48	8.952	1284	1290	1301	rBV	123457	179132	15.94%	2.019%
49	9.092	1312	1313	1316	rBV	543	435	0.04%	0.005%
50	9.183	1327	1328	1331	rVB	594	441	0.04%	0.005%
51	9.275	1339	1343	1346	rBV4	1277	1623	0.14%	0.018%
52	9.385	1355	1361	1374	rBV	450010	622752	55.43%	7.018%
53	9.702	1409	1413	1421	rVB5	2377	4151	0.37%	0.047%
54	9.793	1425	1428	1431	rBV2	641	890	0.08%	0.010%
55	9.939	1450	1452	1453	rBV2	522	340	0.03%	0.004%
56	10.055	1465	1471	1479	rBV	632684	826468	73.56%	9.314%
57	10.153	1485	1487	1489	rBV	440	373	0.03%	0.004%
58	10.305	1508	1512	1515	rVB2	1151	1451	0.13%	0.016%
59	10.336	1515	1517	1519	rBV2	620	529	0.05%	0.006%
60	10.659	1564	1570	1576	rBV5	1354	2880	0.26%	0.032%
61	10.872	1603	1605	1608	rBV2	396	515	0.05%	0.006%
62	10.970	1617	1621	1624	rVB4	1176	1366	0.12%	0.015%
63	11.079	1636	1639	1640	rBV	354	417	0.04%	0.005%
64	11.195	1652	1658	1664	rBV	457262	584096	51.99%	6.582%
65	11.274	1670	1671	1675	rBV	444	486	0.04%	0.005%
66	11.311	1675	1677	1681	rVV3	487	648	0.06%	0.007%
67	11.390	1688	1690	1692	rBV	336	395	0.04%	0.004%
68	11.457	1699	1701	1703	rVB2	1202	771	0.07%	0.009%
69	11.659	1733	1734	1738	rBV	295	328	0.03%	0.004%
70	11.750	1747	1749	1754	rVB	996	1293	0.12%	0.015%
71	11.969	1778	1785	1788	rBV2	1614	2856	0.25%	0.032%
72	12.024	1788	1794	1804	rBV	650224	790359	70.35%	8.907%
73	12.152	1812	1815	1818	rBV2	353	444	0.04%	0.005%
74	12.207	1822	1824	1826	rBV	413	384	0.03%	0.004%
75	12.323	1837	1843	1849	rBV	617818	791640	70.46%	8.921%
76	12.427	1858	1860	1861	rVB	718	344	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030708.D
 Acq On : 22 Aug 2022 11:29
 Operator : JC/MD
 Sample : VX0822MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK694

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.445	1861	1863	1865	rBV2	387	403	0.04%	0.005%
78	12.634	1892	1894	1895	rBV2	513	406	0.04%	0.005%
79	12.762	1911	1915	1919	rBV4	1480	2369	0.21%	0.027%
80	12.853	1928	1930	1935	rBV4	1055	1907	0.17%	0.021%
81	12.920	1939	1941	1944	rVB2	431	458	0.04%	0.005%
82	12.957	1944	1947	1948	rBV	533	451	0.04%	0.005%
83	13.116	1969	1973	1978	rVB4	1614	2247	0.20%	0.025%
84	13.542	2041	2043	2046	rBV	779	785	0.07%	0.009%
85	13.591	2047	2051	2055	rVB2	2453	3530	0.31%	0.040%
86	13.780	2078	2082	2086	rVB2	3300	3898	0.35%	0.044%
87	13.823	2086	2089	2091	rVB	534	459	0.04%	0.005%
88	13.853	2091	2094	2097	rBV2	621	824	0.07%	0.009%
89	13.926	2105	2106	2108	rBV	538	420	0.04%	0.005%
90	13.963	2109	2112	2115	rVB4	1921	2288	0.20%	0.026%
91	14.067	2126	2129	2130	rBV	327	380	0.03%	0.004%
92	14.134	2135	2140	2145	rVB2	2382	3924	0.35%	0.044%
93	14.243	2156	2158	2161	rVB2	590	425	0.04%	0.005%
94	14.298	2164	2167	2169	rBV2	537	574	0.05%	0.006%
95	14.323	2169	2171	2173	rBV	479	463	0.04%	0.005%
96	14.530	2202	2205	2206	rBV2	875	858	0.08%	0.010%
97	14.603	2216	2217	2219	rBV2	597	538	0.05%	0.006%
98	14.707	2232	2234	2235	rBV2	1079	807	0.07%	0.009%
99	14.798	2247	2249	2253	rBV4	853	1150	0.10%	0.013%
100	16.225	2481	2483	2484	rBV	842	557	0.05%	0.006%


Sum of corrected areas: 8873505

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030708.D
Acq On : 22 Aug 2022 11:29
Operator : JC/MD
Sample : VX0822MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK694

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

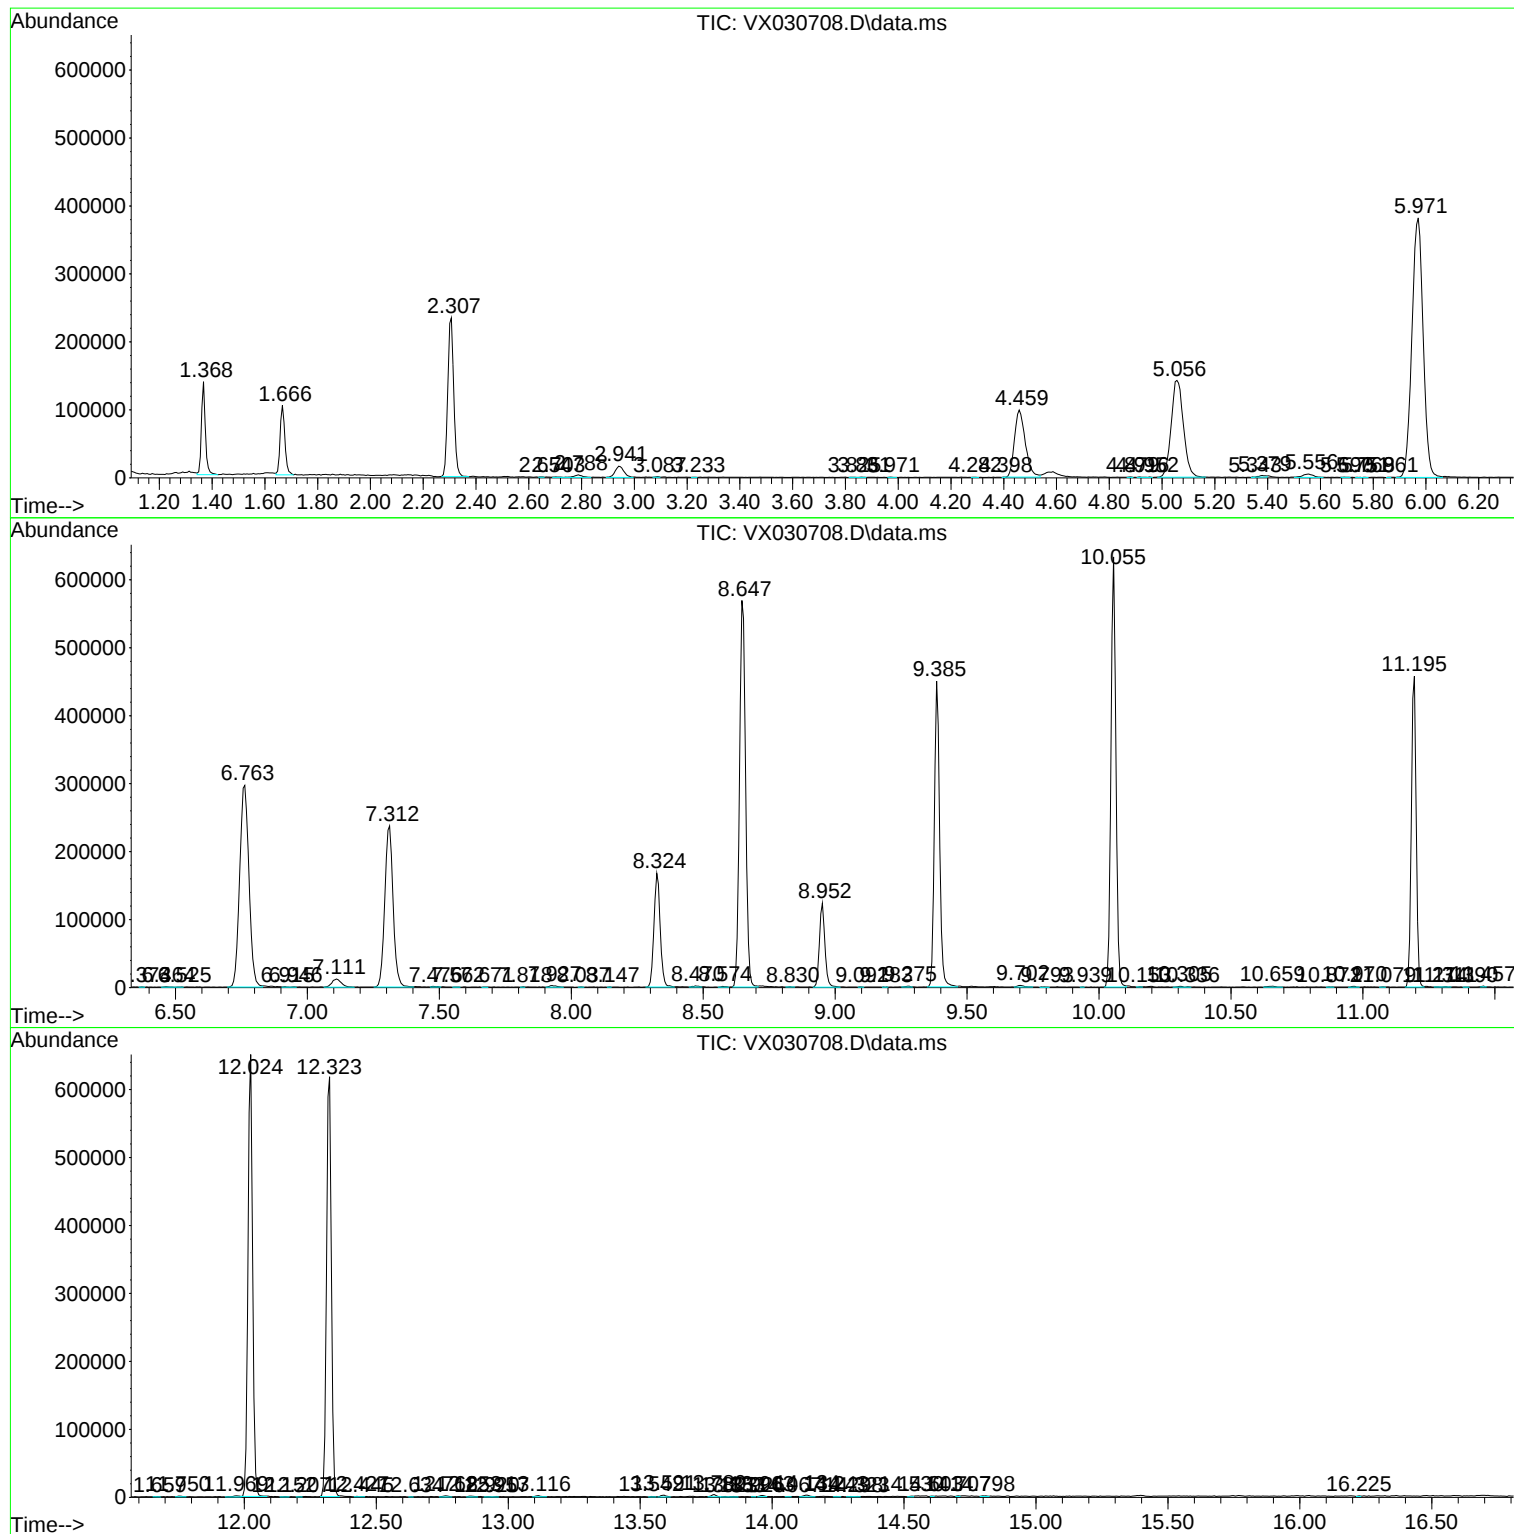

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030708.D
Acq On : 22 Aug 2022 11:29
Operator : JC/MD
Sample : VX0822MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK694

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030708.D
Acq On : 22 Aug 2022 11:29
Operator : JC/MD
Sample : VX0822MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK694

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc