

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030710.D
 Acq On : 22 Aug 2022 12:28
 Operator : JC/MD
 Sample : N4221-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	53	rVB	119616	121687	11.71%	1.475%
2	1.666	91	95	102	rVB	98962	115462	11.11%	1.400%
3	2.306	193	200	210	rVV	208107	329310	31.70%	3.993%
4	2.379	210	212	217	rVB4	1063	1560	0.15%	0.019%
5	2.568	239	243	244	rBV2	894	1143	0.11%	0.014%
6	2.788	274	279	283	rBV4	2589	4136	0.40%	0.050%
7	2.946	295	305	313	rVV	21562	51962	5.00%	0.630%
8	3.068	323	325	327	rBV2	358	380	0.04%	0.005%
9	3.172	340	342	346	rVB2	466	473	0.05%	0.006%
10	3.337	368	369	371	rBV2	436	366	0.04%	0.004%
11	3.385	375	377	381	rVB2	351	443	0.04%	0.005%
12	3.446	384	387	389	rBV2	399	444	0.04%	0.005%
13	3.477	390	392	396	rVV3	495	502	0.05%	0.006%
14	3.702	427	429	431	rBV	320	332	0.03%	0.004%
15	3.977	471	474	475	rBV2	375	336	0.03%	0.004%
16	4.330	531	532	534	rBV	400	369	0.04%	0.004%
17	4.367	536	538	540	rBV2	346	332	0.03%	0.004%
18	4.458	542	553	565	rBV	95171	272847	26.26%	3.308%
19	4.916	624	628	629	rBV3	529	593	0.06%	0.007%
20	4.934	629	631	633	rVV2	380	337	0.03%	0.004%
21	4.983	635	639	640	rBV2	366	406	0.04%	0.005%
22	5.056	640	651	669	rBV	139723	425804	40.99%	5.162%
23	5.239	678	681	682	rVB2	492	439	0.04%	0.005%
24	5.483	719	721	723	rBV2	406	341	0.03%	0.004%
25	5.537	727	730	732	rBV2	1620	2120	0.20%	0.026%
26	5.623	742	744	747	rBV2	301	355	0.03%	0.004%
27	5.647	747	748	750	rBV	336	340	0.03%	0.004%
28	5.970	788	801	815	rBV2	353759	1038917	100.00%	12.596%
29	6.293	852	854	858	rBV2	433	706	0.07%	0.009%
30	6.330	858	860	861	rBV	584	446	0.04%	0.005%
31	6.464	879	882	885	rVB3	635	755	0.07%	0.009%
32	6.501	885	888	889	rBV2	411	390	0.04%	0.005%
33	6.604	902	905	906	rBV2	353	341	0.03%	0.004%
34	6.763	921	931	943	rBV	280899	673082	64.79%	8.160%
35	6.976	962	966	969	rBV3	445	629	0.06%	0.008%
36	7.043	975	977	979	rBV2	375	421	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030710.D
 Acq On : 22 Aug 2022 12:28
 Operator : JC/MD
 Sample : N4221-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.104	980	987	998	rVV3	11409	27498	2.65%	0.333%
38	7.311	1011	1021	1033	rBV	221246	483113	46.50%	5.857%
39	7.549	1058	1060	1062	rBV	519	537	0.05%	0.007%
40	7.653	1075	1077	1080	rVV2	393	317	0.03%	0.004%
41	7.732	1088	1090	1093	rBV	375	447	0.04%	0.005%
42	7.799	1099	1101	1103	rVB	529	426	0.04%	0.005%
43	7.927	1118	1122	1129	rVV3	2023	3380	0.33%	0.041%
44	8.067	1143	1145	1146	rBV	586	467	0.04%	0.006%
45	8.250	1174	1175	1178	rVB2	389	339	0.03%	0.004%
46	8.323	1181	1187	1199	rVB	148172	250453	24.11%	3.036%
47	8.470	1209	1211	1215	rBV2	957	1052	0.10%	0.013%
48	8.580	1226	1229	1233	rBV4	735	1076	0.10%	0.013%
49	8.653	1234	1241	1252	rBV	511809	825299	79.44%	10.006%
50	8.951	1284	1290	1301	rBV	115199	164844	15.87%	1.999%
51	9.092	1311	1313	1315	rVV	543	380	0.04%	0.005%
52	9.183	1325	1328	1331	rVB2	658	829	0.08%	0.010%
53	9.275	1340	1343	1348	rVB3	1167	1554	0.15%	0.019%
54	9.323	1349	1351	1353	rVB	421	352	0.03%	0.004%
55	9.384	1356	1361	1374	rBV	426436	598748	57.63%	7.259%
56	9.701	1409	1413	1422	rVB3	5263	8485	0.82%	0.103%
57	9.957	1453	1455	1457	rVB2	684	484	0.05%	0.006%
58	10.055	1465	1471	1487	rBV	591057	782889	75.36%	9.492%
59	10.287	1507	1509	1510	rBV	406	328	0.03%	0.004%
60	10.299	1510	1511	1513	rBV2	748	515	0.05%	0.006%
61	10.451	1533	1536	1538	rBV2	533	759	0.07%	0.009%
62	10.512	1545	1546	1549	rBV	541	356	0.03%	0.004%
63	10.555	1551	1553	1554	rBV	465	456	0.04%	0.006%
64	10.628	1563	1565	1566	rBV2	333	337	0.03%	0.004%
65	10.652	1567	1569	1575	rVB3	865	1328	0.13%	0.016%
66	10.768	1584	1588	1591	rVB2	594	748	0.07%	0.009%
67	10.805	1591	1594	1595	rBV2	417	481	0.05%	0.006%
68	11.085	1638	1640	1644	rVB3	606	551	0.05%	0.007%
69	11.195	1652	1658	1665	rBV	412738	545132	52.47%	6.609%
70	11.347	1681	1683	1686	rVB2	416	317	0.03%	0.004%
71	11.439	1696	1698	1699	rBV	552	414	0.04%	0.005%
72	11.457	1699	1701	1703	rVB2	826	534	0.05%	0.006%
73	11.542	1713	1715	1717	rBV	395	427	0.04%	0.005%
74	11.634	1728	1730	1734	rBV3	351	446	0.04%	0.005%
75	11.713	1739	1743	1744	rBV	646	497	0.05%	0.006%
76	11.750	1747	1749	1750	rBV	700	363	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030710.D
 Acq On : 22 Aug 2022 12:28
 Operator : JC/MD
 Sample : N4221-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.872	1765	1769	1771	rBV2	465	662	0.06%	0.008%
78	11.975	1782	1786	1788	rBV2	779	876	0.08%	0.011%
79	12.024	1788	1794	1804	rVV	609419	747773	71.98%	9.066%
80	12.164	1815	1817	1821	rVB	697	729	0.07%	0.009%
81	12.225	1821	1827	1831	rBV3	1192	2183	0.21%	0.026%
82	12.323	1837	1843	1851	rBV	591552	727983	70.07%	8.826%
83	12.561	1880	1882	1884	rBV2	428	464	0.04%	0.006%
84	12.719	1906	1908	1911	rBV2	325	384	0.04%	0.005%
85	13.213	1985	1989	1992	rBV	301	558	0.05%	0.007%
86	13.396	2016	2019	2021	rVB	464	409	0.04%	0.005%
87	13.426	2021	2024	2025	rBV	500	473	0.05%	0.006%
88	13.469	2030	2031	2034	rBV	523	541	0.05%	0.007%
89	13.560	2044	2046	2047	rBV	430	319	0.03%	0.004%
90	13.682	2065	2066	2070	rBV2	474	562	0.05%	0.007%
91	13.780	2078	2082	2085	rVV2	835	1013	0.10%	0.012%
92	13.822	2087	2089	2091	rVB2	459	369	0.04%	0.004%
93	14.133	2136	2140	2142	rBV	1601	2086	0.20%	0.025%
94	14.261	2159	2161	2164	rBV2	480	579	0.06%	0.007%
95	14.292	2164	2166	2168	rVB	699	387	0.04%	0.005%
96	14.572	2210	2212	2214	rBV2	881	1048	0.10%	0.013%
97	14.682	2228	2230	2232	rBV3	622	725	0.07%	0.009%
98	16.090	2460	2461	2462	rBV	798	427	0.04%	0.005%
99	16.578	2539	2541	2544	rBV2	870	784	0.08%	0.010%
100	16.670	2555	2556	2560	rBV5	1186	1385	0.13%	0.017%




Sum of corrected areas: 8248183

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030710.D
Acq On : 22 Aug 2022 12:28
Operator : JC/MD
Sample : N4221-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

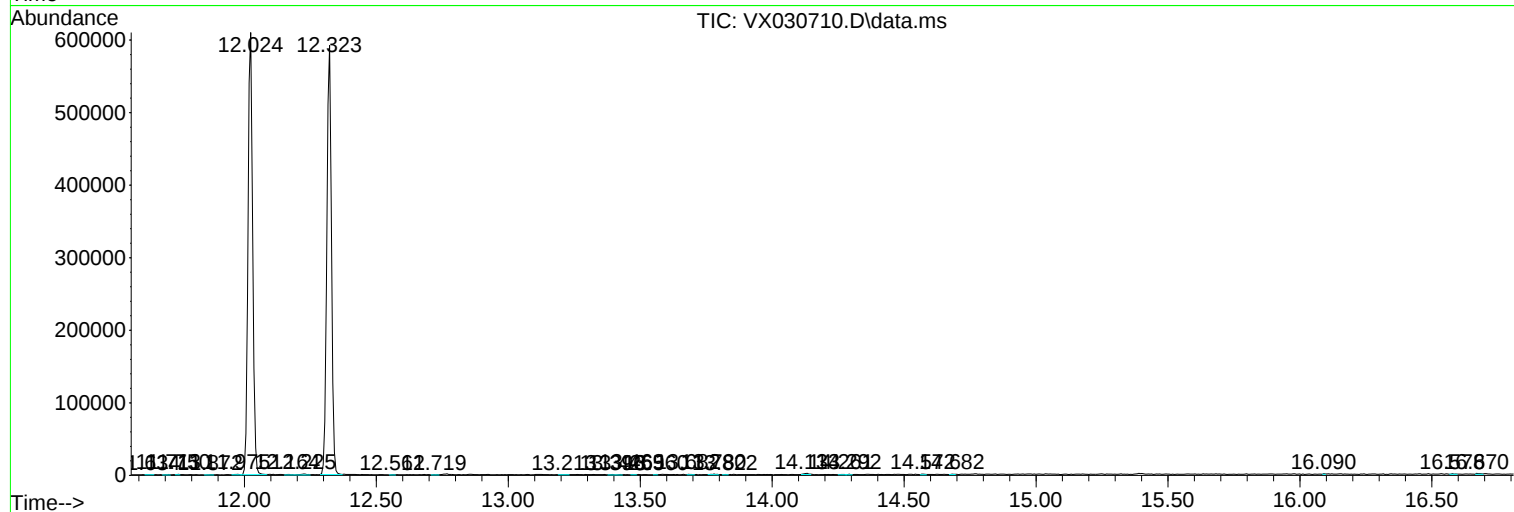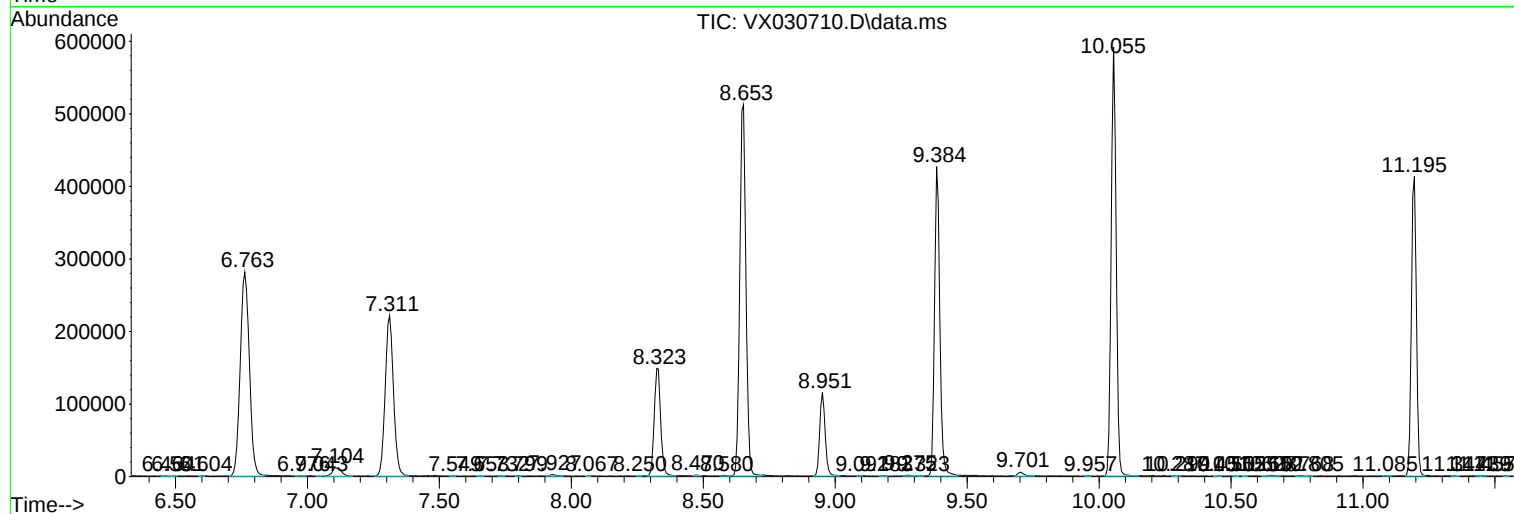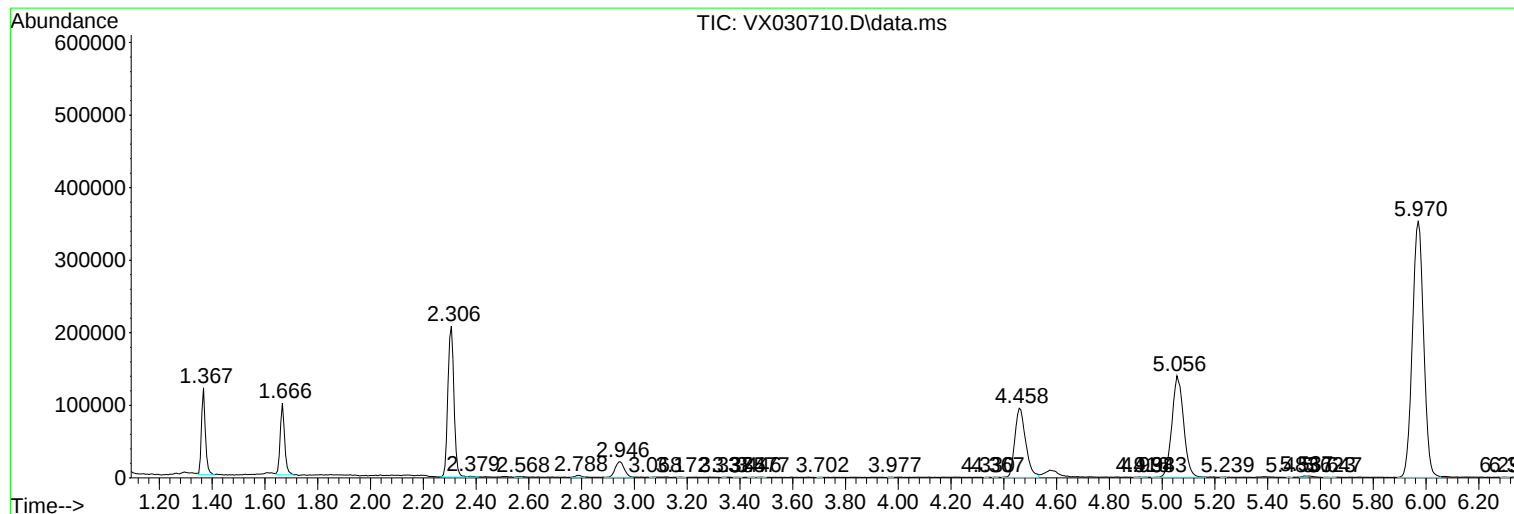

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030710.D
Acq On : 22 Aug 2022 12:28
Operator : JC/MD
Sample : N4221-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030710.D
Acq On : 22 Aug 2022 12:28
Operator : JC/MD
Sample : N4221-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc