

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030711.D
 Acq On : 22 Aug 2022 12:54
 Operator : JC/MD
 Sample : N4231-09DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KQ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030711.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	131285	137863	12.69%	1.550%
2	1.666	91	95	104	rVB	98403	129934	11.96%	1.461%
3	2.307	193	200	210	rVB	230027	363289	33.44%	4.085%
4	2.514	230	234	237	rVB3	735	1162	0.11%	0.013%
5	2.660	254	258	263	rVB3	525	955	0.09%	0.011%
6	2.703	263	265	268	rVB3	413	451	0.04%	0.005%
7	2.788	274	279	287	rVB2	2065	3556	0.33%	0.040%
8	2.947	297	305	315	rVB2	7638	18056	1.66%	0.203%
9	3.020	315	317	319	rBV2	467	484	0.04%	0.005%
10	3.081	325	327	328	rBV	581	344	0.03%	0.004%
11	3.209	346	348	350	rBV2	359	352	0.03%	0.004%
12	3.270	357	358	362	rBV2	450	552	0.05%	0.006%
13	3.349	370	371	374	rVV2	313	354	0.03%	0.004%
14	3.520	396	399	404	rBV2	266	534	0.05%	0.006%
15	3.587	409	410	412	rBV	409	420	0.04%	0.005%
16	3.611	412	414	415	rBV2	457	441	0.04%	0.005%
17	3.837	448	451	452	rVB2	391	354	0.03%	0.004%
18	3.855	452	454	455	rBV2	438	416	0.04%	0.005%
19	4.136	499	500	504	rBV2	359	499	0.05%	0.006%
20	4.270	520	522	524	rBV	293	357	0.03%	0.004%
21	4.465	545	554	570	rBV	102956	332938	30.65%	3.744%
22	4.977	636	638	639	rBV2	464	408	0.04%	0.005%
23	5.056	639	651	667	rVV	141728	447248	41.17%	5.029%
24	5.385	697	705	706	rBV5	2662	4938	0.45%	0.056%
25	5.513	723	726	727	rBV	381	357	0.03%	0.004%
26	5.550	727	732	741	rVB6	4280	10931	1.01%	0.123%
27	5.733	759	762	764	rVB	643	428	0.04%	0.005%
28	5.971	789	801	820	rBV2	374389	1086347	100.00%	12.216%
29	6.129	825	827	830	rVV2	494	613	0.06%	0.007%
30	6.178	833	835	836	rBV	510	372	0.03%	0.004%
31	6.458	879	881	885	rBV2	561	683	0.06%	0.008%
32	6.544	893	895	896	rBV2	415	356	0.03%	0.004%
33	6.696	919	920	922	rBV	317	343	0.03%	0.004%
34	6.763	922	931	945	rBV	314286	735921	67.74%	8.276%
35	6.989	966	968	972	rVB2	422	517	0.05%	0.006%
36	7.123	981	990	1001	rVB5	25123	68103	6.27%	0.766%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030711.D
 Acq On : 22 Aug 2022 12:54
 Operator : JC/MD
 Sample : N4231-09DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KQ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1038	rVB	230604	500074	46.03%	5.623%
38	7.476	1046	1048	1052	rBV3	908	1165	0.11%	0.013%
39	7.934	1117	1123	1129	rBV3	2429	4962	0.46%	0.056%
40	8.049	1140	1142	1143	rBV2	437	348	0.03%	0.004%
41	8.141	1155	1157	1159	rBV	629	545	0.05%	0.006%
42	8.177	1161	1163	1166	rVB	587	583	0.05%	0.007%
43	8.220	1166	1170	1171	rBV2	446	558	0.05%	0.006%
44	8.263	1175	1177	1180	rBV	534	559	0.05%	0.006%
45	8.324	1181	1187	1197	rBV	154340	256819	23.64%	2.888%
46	8.653	1233	1241	1250	rBV	553877	878830	80.90%	9.883%
47	8.885	1277	1279	1283	rVB2	390	372	0.03%	0.004%
48	8.952	1283	1290	1299	rBV	115366	170784	15.72%	1.920%
49	9.153	1319	1323	1326	rBV3	727	955	0.09%	0.011%
50	9.275	1337	1343	1351	rBV	81044	118872	10.94%	1.337%
51	9.385	1355	1361	1378	rBV	417128	609890	56.14%	6.858%
52	9.665	1405	1407	1410	rBV2	393	501	0.05%	0.006%
53	9.702	1410	1413	1418	rVV3	2670	3637	0.33%	0.041%
54	9.763	1421	1423	1424	rVB	550	362	0.03%	0.004%
55	9.842	1433	1436	1439	rVB	604	669	0.06%	0.008%
56	9.866	1439	1440	1443	rBV	492	460	0.04%	0.005%
57	9.939	1449	1452	1457	rBV	502	798	0.07%	0.009%
58	10.055	1465	1471	1485	rBV	626674	843429	77.64%	9.484%
59	10.189	1491	1493	1495	rBV2	547	481	0.04%	0.005%
60	10.269	1504	1506	1508	rBV2	429	360	0.03%	0.004%
61	10.640	1564	1567	1568	rBV2	552	655	0.06%	0.007%
62	10.878	1605	1606	1608	rBV	501	379	0.03%	0.004%
63	10.939	1612	1616	1617	rBV	526	680	0.06%	0.008%
64	11.128	1644	1647	1649	rBV2	398	457	0.04%	0.005%
65	11.195	1652	1658	1665	rBV	435314	555240	51.11%	6.244%
66	11.311	1675	1677	1678	rBV	421	440	0.04%	0.005%
67	11.366	1684	1686	1688	rBV	587	479	0.04%	0.005%
68	11.421	1692	1695	1696	rVB	572	396	0.04%	0.004%
69	11.854	1764	1766	1771	rVB2	427	435	0.04%	0.005%
70	11.939	1779	1780	1782	rBV	463	346	0.03%	0.004%
71	11.969	1782	1785	1788	rVV3	745	706	0.06%	0.008%
72	12.024	1788	1794	1801	rBV	667315	808317	74.41%	9.090%
73	12.152	1812	1815	1817	rVB2	358	344	0.03%	0.004%
74	12.201	1821	1823	1825	rBV	646	548	0.05%	0.006%
75	12.219	1825	1826	1830	rBV2	645	631	0.06%	0.007%
76	12.323	1837	1843	1848	rBV	602461	757672	69.74%	8.520%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030711.D
 Acq On : 22 Aug 2022 12:54
 Operator : JC/MD
 Sample : N4231-09DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KQ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.433	1860	1861	1863	rBV2	434	381	0.04%	0.004%
78	12.457	1863	1865	1868	rVV2	613	598	0.06%	0.007%
79	12.768	1911	1916	1919	rBV3	1227	1957	0.18%	0.022%
80	12.799	1919	1921	1924	rVV2	367	387	0.04%	0.004%
81	12.860	1930	1931	1936	rVB2	1170	1051	0.10%	0.012%
82	13.116	1971	1973	1974	rBV	669	452	0.04%	0.005%
83	13.414	2021	2022	2025	rBV	438	424	0.04%	0.005%
84	13.439	2025	2026	2029	rVB2	642	463	0.04%	0.005%
85	13.475	2029	2032	2034	rBV2	472	480	0.04%	0.005%
86	13.530	2038	2041	2042	rBV2	439	483	0.04%	0.005%
87	13.652	2059	2061	2064	rBV3	501	437	0.04%	0.005%
88	13.914	2102	2104	2106	rVB2	634	586	0.05%	0.007%
89	13.963	2110	2112	2116	rVB3	782	663	0.06%	0.007%
90	14.134	2135	2140	2145	rBV3	2395	3597	0.33%	0.040%
91	14.231	2153	2156	2158	rBV	657	694	0.06%	0.008%
92	14.439	2187	2190	2191	rBV	667	540	0.05%	0.006%
93	15.170	2309	2310	2313	rBV	664	577	0.05%	0.006%
94	15.292	2327	2330	2332	rBV3	734	1029	0.09%	0.012%
95	15.329	2334	2336	2338	rVV2	606	431	0.04%	0.005%
96	15.707	2396	2398	2399	rBV2	631	447	0.04%	0.005%
97	16.072	2456	2458	2461	rBV4	735	777	0.07%	0.009%
98	16.298	2493	2495	2496	rBV	669	400	0.04%	0.004%
99	16.463	2520	2522	2523	rBV	616	366	0.03%	0.004%
100	16.652	2551	2553	2555	rBV	803	927	0.09%	0.010%




Sum of corrected areas: 8892761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030711.D
Acq On : 22 Aug 2022 12:54
Operator : JC/MD
Sample : N4231-09DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KQ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

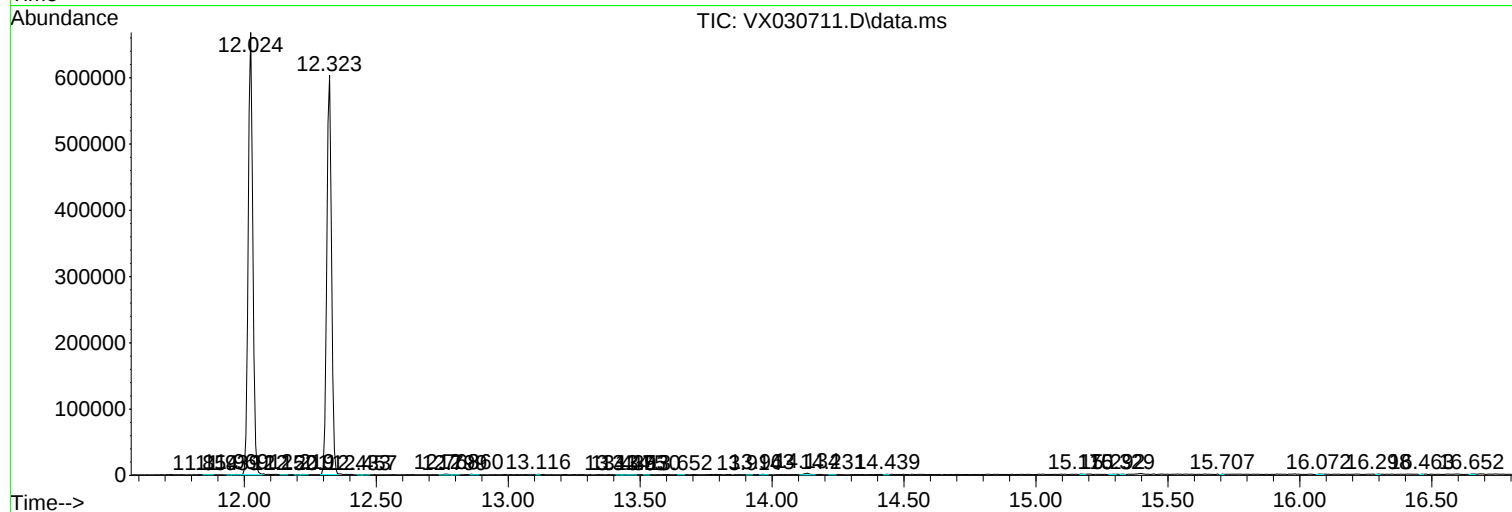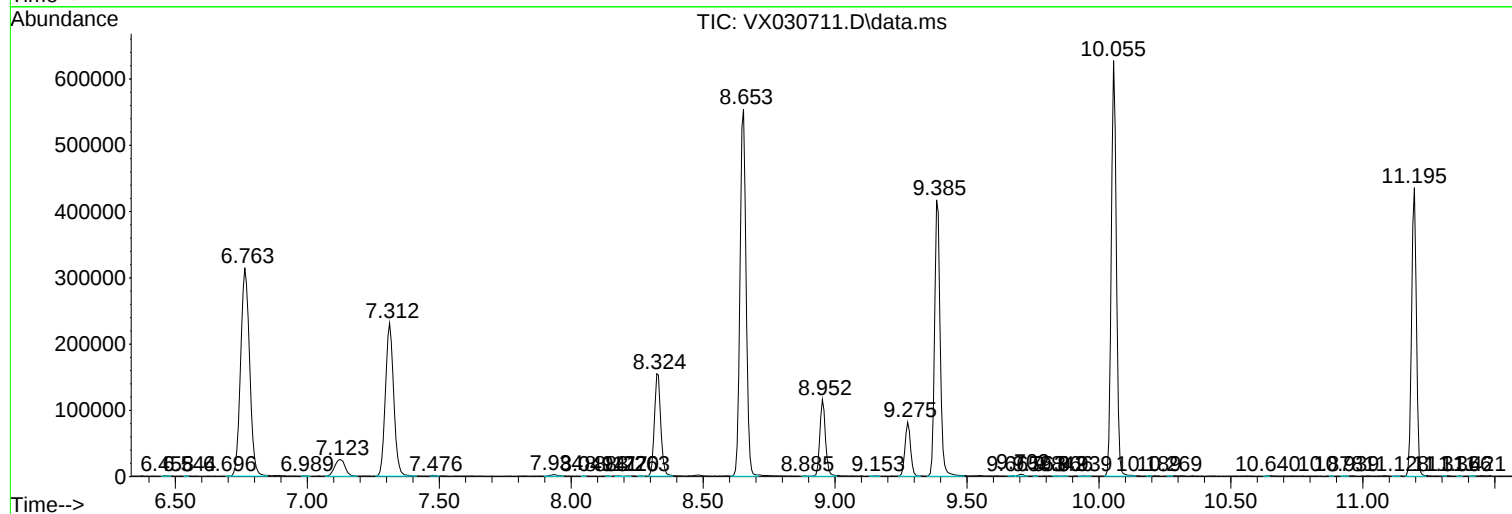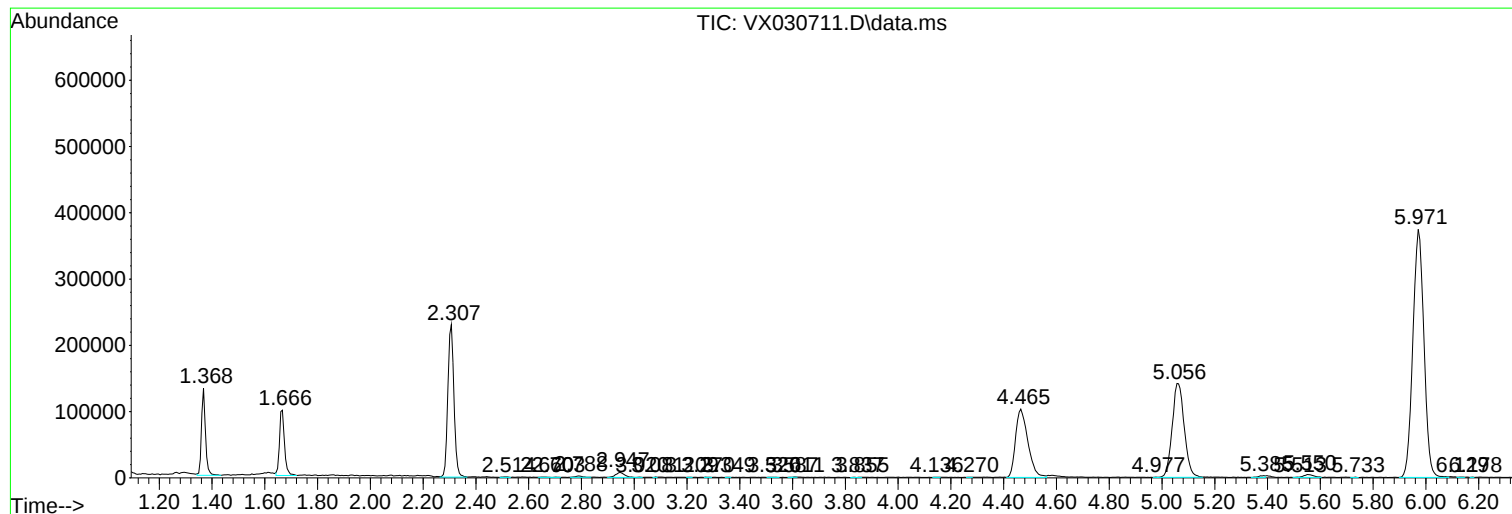

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030711.D
Acq On : 22 Aug 2022 12:54
Operator : JC/MD
Sample : N4231-09DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KQ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030711.D
Acq On : 22 Aug 2022 12:54
Operator : JC/MD
Sample : N4231-09DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KQ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc