

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030713.D
 Acq On : 22 Aug 2022 14:08
 Operator : JC/MD
 Sample : N4231-09DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KQ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	28124	33940	23.61%	3.073%
2	1.666	92	95	100	rVB	19757	22730	15.81%	2.058%
3	2.057	155	159	163	rBV5	1028	1297	0.90%	0.117%
4	2.252	188	191	194	rVB2	374	398	0.28%	0.036%
5	2.313	194	201	211	rBV2	44694	78835	54.84%	7.138%
6	2.428	217	220	223	rBV	449	630	0.44%	0.057%
7	2.477	227	228	231	rBV2	379	409	0.28%	0.037%
8	2.502	231	232	234	rBV	445	339	0.24%	0.031%
9	2.788	277	279	284	rVB3	857	1074	0.75%	0.097%
10	2.886	293	295	298	rBV	453	510	0.35%	0.046%
11	3.288	359	361	364	rVB2	477	355	0.25%	0.032%
12	3.319	364	366	367	rBV2	501	517	0.36%	0.047%
13	3.489	392	394	397	rBV2	347	411	0.29%	0.037%
14	3.575	405	408	411	rBV	401	364	0.25%	0.033%
15	3.617	413	415	419	rVB	637	518	0.36%	0.047%
16	3.831	448	450	453	rBV2	364	485	0.34%	0.044%
17	3.861	453	455	459	rVV2	523	541	0.38%	0.049%
18	3.898	459	461	462	rVV	429	348	0.24%	0.032%
19	4.190	505	509	510	rBV2	393	415	0.29%	0.038%
20	4.422	545	547	548	rBV2	481	377	0.26%	0.034%
21	4.465	548	554	568	rVV5	6827	23258	16.18%	2.106%
22	4.617	578	579	583	rVB2	618	499	0.35%	0.045%
23	4.660	583	586	589	rVB3	543	756	0.53%	0.068%
24	4.696	589	592	593	rBV	467	472	0.33%	0.043%
25	4.818	609	612	615	rBV2	324	368	0.26%	0.033%
26	4.885	622	623	626	rVB	470	433	0.30%	0.039%
27	4.922	626	629	632	rBV2	395	679	0.47%	0.061%
28	5.062	640	652	664	rBV2	20420	63647	44.27%	5.763%
29	5.239	678	681	682	rBV2	360	363	0.25%	0.033%
30	5.367	699	702	703	rBV	534	466	0.32%	0.042%
31	5.519	724	727	728	rBV2	291	358	0.25%	0.032%
32	5.544	728	731	734	rBV3	646	980	0.68%	0.089%
33	5.641	745	747	749	rBV2	538	413	0.29%	0.037%
34	5.684	751	754	757	rBV2	482	802	0.56%	0.073%
35	5.830	776	778	780	rBV	415	389	0.27%	0.035%
36	5.970	789	801	817	rVV3	48065	143763	100.00%	13.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030713.D
 Acq On : 22 Aug 2022 14:08
 Operator : JC/MD
 Sample : N4231-09DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KQ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.080	817	819	822	rBV2	302	390	0.27%	0.035%
38	6.397	867	871	873	rVV2	359	506	0.35%	0.046%
39	6.440	875	878	880	rVV3	612	664	0.46%	0.060%
40	6.464	880	882	886	rVV	506	615	0.43%	0.056%
41	6.537	893	894	898	rVV2	394	432	0.30%	0.039%
42	6.574	898	900	904	rVV	514	398	0.28%	0.036%
43	6.696	912	920	922	rBV2	299	597	0.42%	0.054%
44	6.763	922	931	947	rBV2	41755	102414	71.24%	9.273%
45	7.129	983	991	999	rBV5	8698	21233	14.77%	1.922%
46	7.214	1002	1005	1007	rBV2	481	511	0.36%	0.046%
47	7.312	1012	1021	1033	rBV2	27030	62779	43.67%	5.684%
48	7.452	1042	1044	1047	rBV2	384	475	0.33%	0.043%
49	7.495	1049	1051	1054	rBV	490	658	0.46%	0.060%
50	7.549	1059	1060	1062	rBV2	622	452	0.31%	0.041%
51	7.775	1096	1097	1101	rBV2	504	547	0.38%	0.050%
52	7.879	1112	1114	1119	rVB	534	468	0.33%	0.042%
53	8.098	1148	1150	1153	rBV	330	400	0.28%	0.036%
54	8.202	1166	1167	1170	rBV	615	654	0.45%	0.059%
55	8.281	1178	1180	1183	rBV2	387	424	0.29%	0.038%
56	8.330	1183	1188	1195	rVV	15975	27246	18.95%	2.467%
57	8.470	1208	1211	1212	rBV	642	479	0.33%	0.043%
58	8.586	1227	1230	1232	rBV2	534	481	0.33%	0.044%
59	8.653	1235	1241	1249	rVV	72551	113550	78.98%	10.281%
60	8.830	1266	1270	1273	rBV2	608	792	0.55%	0.072%
61	8.921	1282	1285	1286	rBV2	503	574	0.40%	0.052%
62	8.952	1286	1290	1296	rVB2	8951	14558	10.13%	1.318%
63	9.141	1318	1321	1324	rVB2	465	410	0.29%	0.037%
64	9.189	1327	1329	1332	rVB	411	393	0.27%	0.036%
65	9.275	1339	1343	1350	rVB3	11759	18462	12.84%	1.672%
66	9.336	1350	1353	1355	rBV	394	454	0.32%	0.041%
67	9.391	1357	1362	1373	rVB2	17575	30818	21.44%	2.790%
68	9.586	1393	1394	1397	rBV	373	360	0.25%	0.033%
69	9.659	1404	1406	1408	rVB	415	387	0.27%	0.035%
70	9.866	1437	1440	1442	rBV2	353	392	0.27%	0.035%
71	9.927	1446	1450	1453	rBV2	274	421	0.29%	0.038%
72	9.976	1456	1458	1461	rBV2	387	342	0.24%	0.031%
73	10.055	1466	1471	1479	rBV	73910	99322	69.09%	8.993%
74	10.159	1485	1488	1489	rBV3	374	378	0.26%	0.034%
75	10.226	1496	1499	1502	rBV2	375	612	0.43%	0.055%
76	10.543	1548	1551	1553	rBV	510	567	0.39%	0.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030713.D
 Acq On : 22 Aug 2022 14:08
 Operator : JC/MD
 Sample : N4231-09DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KQ6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	10.793	1589	1592	1594	rVB2	454	516	0.36%	0.047%
78	10.982	1621	1623	1625	rVB	595	404	0.28%	0.037%
79	11.006	1625	1627	1630	rBV	306	363	0.25%	0.033%
80	11.195	1653	1658	1663	rBV	29986	39117	27.21%	3.542%
81	11.457	1698	1701	1703	rBV2	587	603	0.42%	0.055%
82	11.500	1706	1708	1711	rBV3	358	460	0.32%	0.042%
83	11.591	1721	1723	1725	rVB	409	349	0.24%	0.032%
84	11.622	1725	1728	1730	rBV	521	514	0.36%	0.047%
85	12.024	1789	1794	1800	rBV	67616	86340	60.06%	7.817%
86	12.116	1807	1809	1812	rBV2	629	681	0.47%	0.062%
87	12.323	1838	1843	1850	rBV	60531	79026	54.97%	7.155%
88	12.518	1873	1875	1876	rBV	755	455	0.32%	0.041%
89	12.853	1929	1930	1934	rVB2	512	623	0.43%	0.056%
90	12.890	1934	1936	1937	rBV	584	367	0.26%	0.033%
91	12.908	1937	1939	1942	rVV2	484	469	0.33%	0.042%
92	13.658	2060	2062	2063	rBV	527	399	0.28%	0.036%
93	14.091	2129	2133	2135	rBV	752	725	0.50%	0.066%
94	14.195	2148	2150	2153	rVB2	524	395	0.27%	0.036%
95	14.701	2229	2233	2236	rBV	1020	1939	1.35%	0.176%
96	14.859	2258	2259	2262	rBV3	805	901	0.63%	0.082%
97	15.603	2379	2381	2383	rVB2	765	519	0.36%	0.047%
98	16.072	2457	2458	2459	rBV	993	484	0.34%	0.044%
99	16.322	2497	2499	2501	rBV2	761	421	0.29%	0.038%
100	16.719	2562	2564	2565	rBV2	785	639	0.44%	0.058%




Sum of corrected areas: 1104463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030713.D
Acq On : 22 Aug 2022 14:08
Operator : JC/MD
Sample : N4231-09DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KQ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

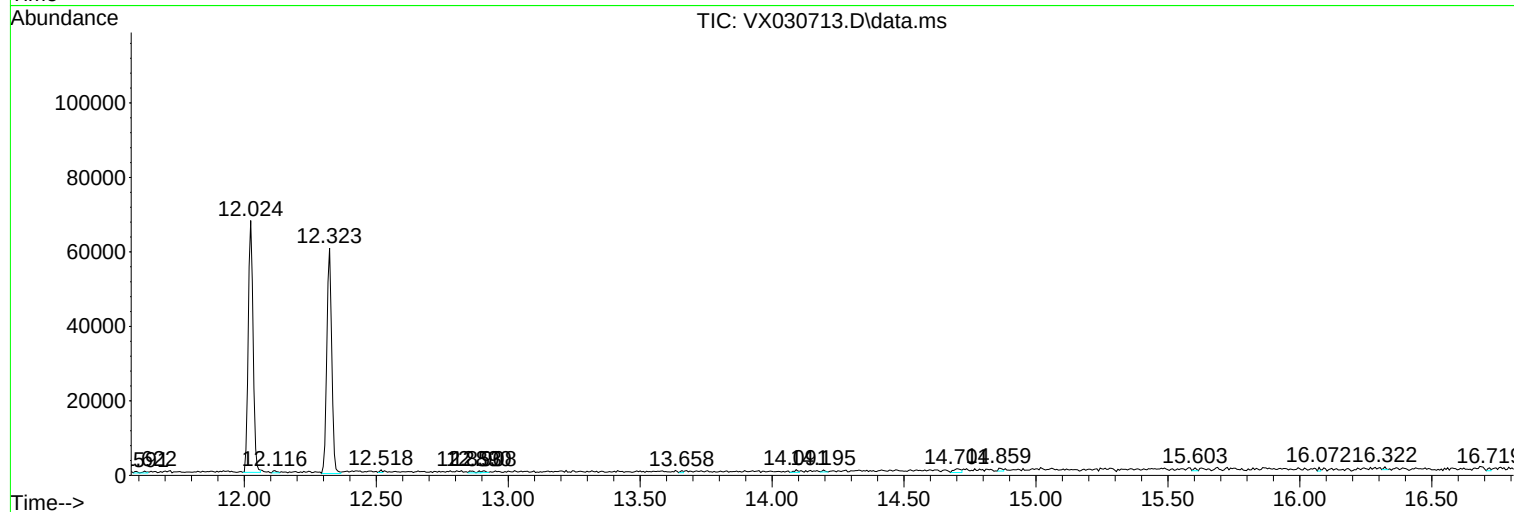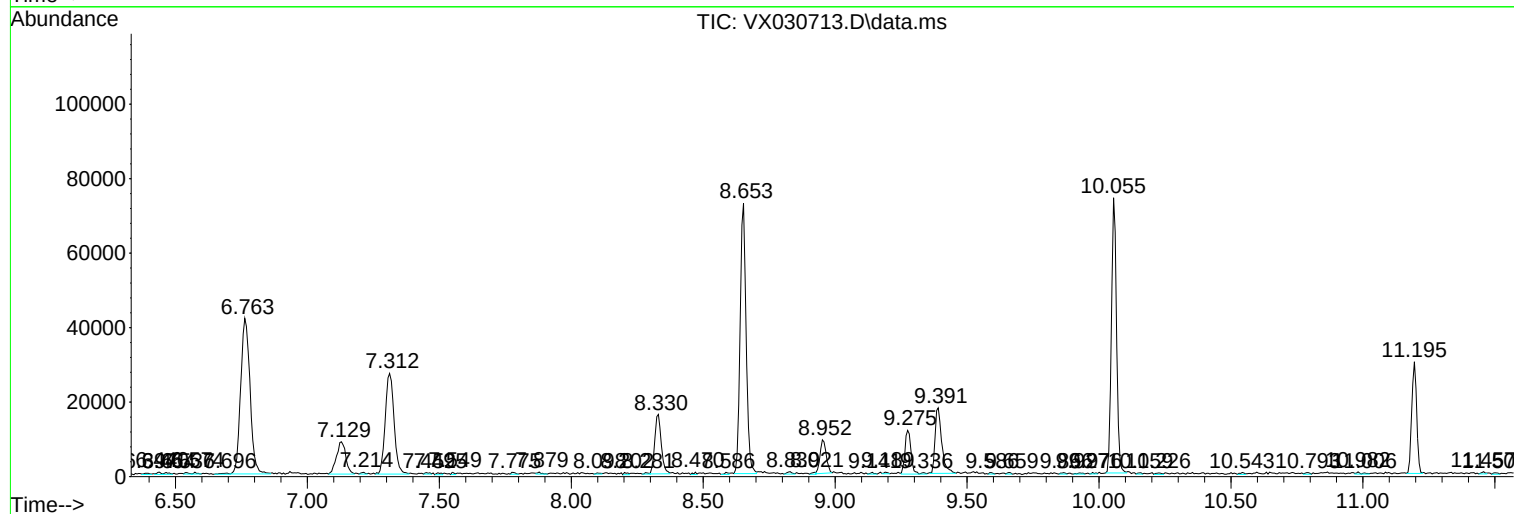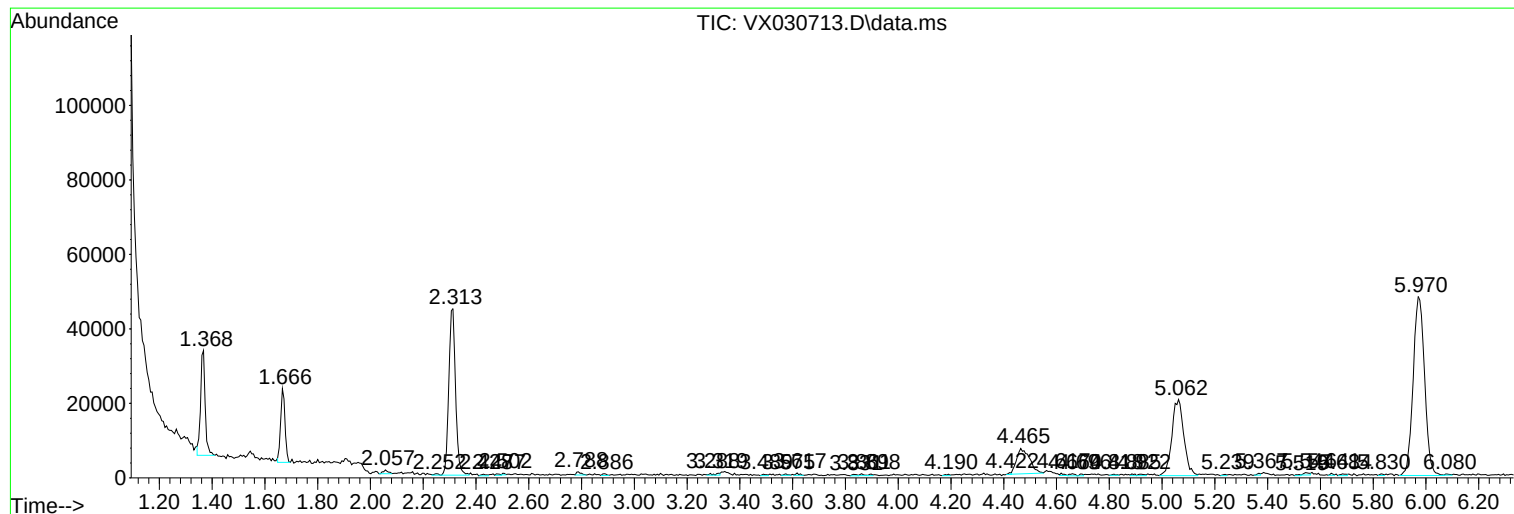

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030713.D
Acq On : 22 Aug 2022 14:08
Operator : JC/MD
Sample : N4231-09DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KQ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030713.D
Acq On : 22 Aug 2022 14:08
Operator : JC/MD
Sample : N4231-09DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KQ6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc