

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030716.D
 Acq On : 22 Aug 2022 15:49
 Operator : JC/MD
 Sample : N4231-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	124665	131152	11.97%	1.517%
2	1.666	91	95	105	rVB	101374	127181	11.61%	1.471%
3	2.307	194	200	208	rVB	220933	348946	31.85%	4.037%
4	2.428	218	220	221	rVB2	682	408	0.04%	0.005%
5	2.642	251	255	256	rBV2	433	459	0.04%	0.005%
6	2.788	274	279	286	rBV3	4174	7459	0.68%	0.086%
7	2.941	296	304	314	rVB	11140	24538	2.24%	0.284%
8	3.136	334	336	339	rVB2	589	523	0.05%	0.006%
9	3.166	339	341	343	rBV	462	398	0.04%	0.005%
10	3.282	357	360	361	rVB2	401	337	0.03%	0.004%
11	3.404	379	380	384	rVB2	398	478	0.04%	0.006%
12	3.703	427	429	432	rVB	424	467	0.04%	0.005%
13	3.885	456	459	460	rBV2	347	421	0.04%	0.005%
14	4.324	529	531	534	rBV2	414	600	0.05%	0.007%
15	4.459	544	553	567	rBV	94222	268880	24.55%	3.110%
16	4.739	597	599	602	rVB3	671	531	0.05%	0.006%
17	5.056	638	651	673	rVV	142496	450285	41.10%	5.209%
18	5.221	677	678	680	rBV	443	373	0.03%	0.004%
19	5.544	725	731	732	rBV2	1635	2134	0.19%	0.025%
20	5.763	766	767	771	rVB	390	401	0.04%	0.005%
21	5.970	789	801	816	rBV2	371912	1095456	100.00%	12.672%
22	6.147	827	830	831	rBV	461	402	0.04%	0.005%
23	6.190	835	837	840	rBV2	506	561	0.05%	0.006%
24	6.464	877	882	888	rVB3	747	1511	0.14%	0.017%
25	6.525	888	892	893	rBV	560	653	0.06%	0.008%
26	6.763	922	931	943	rBV	302184	713960	65.17%	8.259%
27	7.111	980	988	997	rVB2	12299	28576	2.61%	0.331%
28	7.184	997	1000	1002	rBV2	531	544	0.05%	0.006%
29	7.312	1011	1021	1037	rBV	228001	508810	46.45%	5.886%
30	7.421	1037	1039	1043	rVB4	797	1030	0.09%	0.012%
31	7.531	1055	1057	1060	rVB2	588	562	0.05%	0.007%
32	7.684	1080	1082	1084	rVV	411	356	0.03%	0.004%
33	7.842	1106	1108	1110	rVB2	507	488	0.04%	0.006%
34	7.860	1110	1111	1112	rBV	584	365	0.03%	0.004%
35	7.934	1118	1123	1130	rVB5	2279	5205	0.48%	0.060%
36	7.988	1130	1132	1135	rBV2	432	513	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030716.D
 Acq On : 22 Aug 2022 15:49
 Operator : JC/MD
 Sample : N4231-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	8.208	1165	1168	1170	rVB2	376	457	0.04%	0.005%
38	8.244	1170	1174	1179	rVB2	528	765	0.07%	0.009%
39	8.324	1179	1187	1196	rBV	153604	258911	23.63%	2.995%
40	8.476	1208	1212	1222	rVB4	1509	3411	0.31%	0.039%
41	8.580	1227	1229	1232	rBV3	751	685	0.06%	0.008%
42	8.653	1234	1241	1251	rBV	543415	874248	79.81%	10.113%
43	8.885	1277	1279	1283	rBV	397	577	0.05%	0.007%
44	8.952	1285	1290	1302	rVV	114733	171259	15.63%	1.981%
45	9.159	1320	1324	1328	rBV2	592	813	0.07%	0.009%
46	9.232	1335	1336	1339	rVB2	476	338	0.03%	0.004%
47	9.275	1340	1343	1346	rVV2	1619	1662	0.15%	0.019%
48	9.324	1350	1351	1356	rBV	548	738	0.07%	0.009%
49	9.384	1356	1361	1377	rVV	413298	599971	54.77%	6.940%
50	9.702	1410	1413	1419	rVB4	1663	2361	0.22%	0.027%
51	9.775	1422	1425	1426	rBV2	447	474	0.04%	0.005%
52	9.848	1434	1437	1442	rBV2	552	776	0.07%	0.009%
53	9.945	1451	1453	1455	rVB2	444	359	0.03%	0.004%
54	10.055	1465	1471	1483	rBV	634132	827248	75.52%	9.569%
55	10.208	1494	1496	1499	rVB3	872	635	0.06%	0.007%
56	10.311	1510	1513	1514	rVV2	571	529	0.05%	0.006%
57	10.348	1517	1519	1522	rVB	444	348	0.03%	0.004%
58	10.409	1525	1529	1531	rBV2	485	691	0.06%	0.008%
59	10.494	1542	1543	1546	rVB2	501	505	0.05%	0.006%
60	10.525	1546	1548	1550	rBV2	479	481	0.04%	0.006%
61	10.622	1561	1564	1566	rVB2	415	413	0.04%	0.005%
62	10.640	1566	1567	1570	rBV2	717	708	0.06%	0.008%
63	10.878	1602	1606	1608	rBV2	350	453	0.04%	0.005%
64	10.963	1618	1620	1625	rBB3	655	597	0.05%	0.007%
65	11.195	1652	1658	1665	rBV	448294	568242	51.87%	6.573%
66	11.311	1674	1677	1681	rVB3	620	938	0.09%	0.011%
67	11.341	1681	1682	1684	rBV2	621	480	0.04%	0.006%
68	11.366	1684	1686	1691	rVB2	540	644	0.06%	0.007%
69	11.451	1699	1700	1703	rVB	534	429	0.04%	0.005%
70	11.476	1703	1704	1706	rBV	455	388	0.04%	0.004%
71	11.555	1712	1717	1719	rVB2	378	457	0.04%	0.005%
72	11.585	1719	1722	1724	rBV	453	409	0.04%	0.005%
73	11.677	1735	1737	1740	rVV2	391	387	0.04%	0.004%
74	11.854	1764	1766	1770	rVB2	335	372	0.03%	0.004%
75	11.927	1775	1778	1780	rBV	646	518	0.05%	0.006%
76	11.975	1782	1786	1788	rVB2	667	867	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030716.D
 Acq On : 22 Aug 2022 15:49
 Operator : JC/MD
 Sample : N4231-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1801	rBV	647857	801395	73.16%	9.270%
78	12.164	1814	1817	1820	rVB2	658	885	0.08%	0.010%
79	12.323	1837	1843	1849	rBV	618794	775979	70.84%	8.976%
80	12.488	1869	1870	1873	rBV2	355	394	0.04%	0.005%
81	12.603	1886	1889	1891	rBV2	328	365	0.03%	0.004%
82	12.628	1891	1893	1897	rVV2	435	624	0.06%	0.007%
83	12.713	1905	1907	1908	rVB	629	351	0.03%	0.004%
84	12.762	1911	1915	1919	rBV3	1878	2827	0.26%	0.033%
85	12.927	1938	1942	1945	rVB2	596	720	0.07%	0.008%
86	12.981	1948	1951	1953	rBV2	354	360	0.03%	0.004%
87	13.451	2026	2028	2029	rBV	615	536	0.05%	0.006%
88	13.628	2054	2057	2060	rBV2	433	753	0.07%	0.009%
89	13.774	2080	2081	2090	rVV3	713	1054	0.10%	0.012%
90	13.920	2103	2105	2109	rVB	634	738	0.07%	0.009%
91	13.957	2109	2111	2112	rBV	465	372	0.03%	0.004%
92	14.091	2131	2133	2134	rBV2	458	390	0.04%	0.005%
93	14.140	2135	2141	2146	rVV3	1670	3327	0.30%	0.038%
94	14.335	2171	2173	2176	rVB2	480	490	0.04%	0.006%
95	14.408	2183	2185	2188	rVB2	595	567	0.05%	0.007%
96	14.481	2195	2197	2198	rBV	609	355	0.03%	0.004%
97	14.823	2249	2253	2254	rBV2	821	1051	0.10%	0.012%
98	14.841	2254	2256	2257	rVB2	946	502	0.05%	0.006%
99	15.237	2319	2321	2323	rBV2	668	465	0.04%	0.005%
100	16.060	2454	2456	2457	rBV2	1160	716	0.07%	0.008%


Sum of corrected areas: 8644723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030716.D
Acq On : 22 Aug 2022 15:49
Operator : JC/MD
Sample : N4231-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

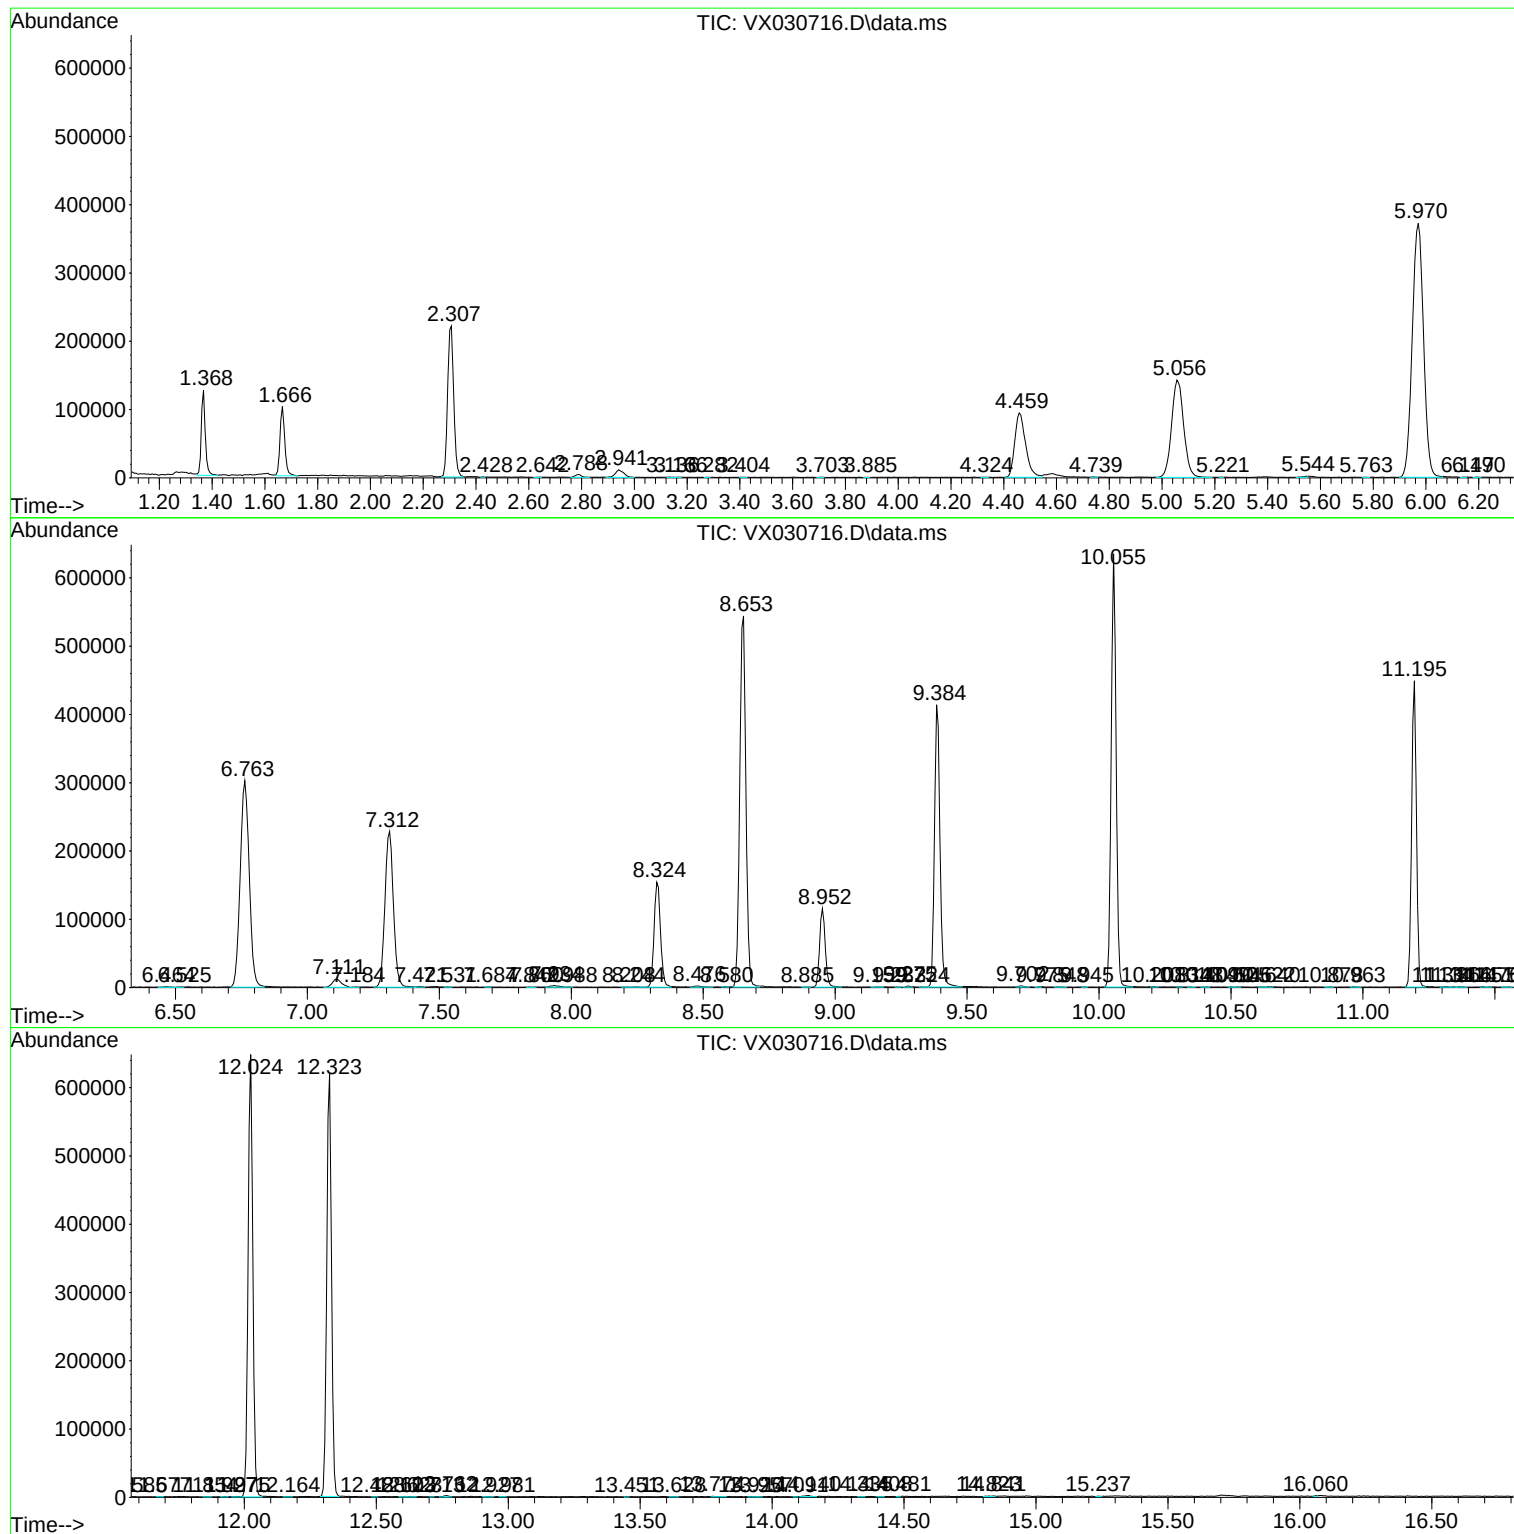

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030716.D
Acq On : 22 Aug 2022 15:49
Operator : JC/MD
Sample : N4231-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030716.D
Acq On : 22 Aug 2022 15:49
Operator : JC/MD
Sample : N4231-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc